

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
 Data File : PD051590.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2019 18:48
 Operator : AJ\SJ
 Sample : K1661-16
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF874

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:38:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	29741090	627.6E6	20.696	20.313
2)	SA Decachlor...	7.825	9.160	48538157	699.7E6	40.360	36.910
Target Compounds							
6)	B beta-BHC	0.000	4.941f	0 50238708	N.D.		2.532
8)	B Heptachlo...	0.000	5.920	0 14372567	N.D.		0.401


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030419\
Data File : PD051590.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2019 18:48
Operator : AJ\SJ
Sample : K1661-16
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:38:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

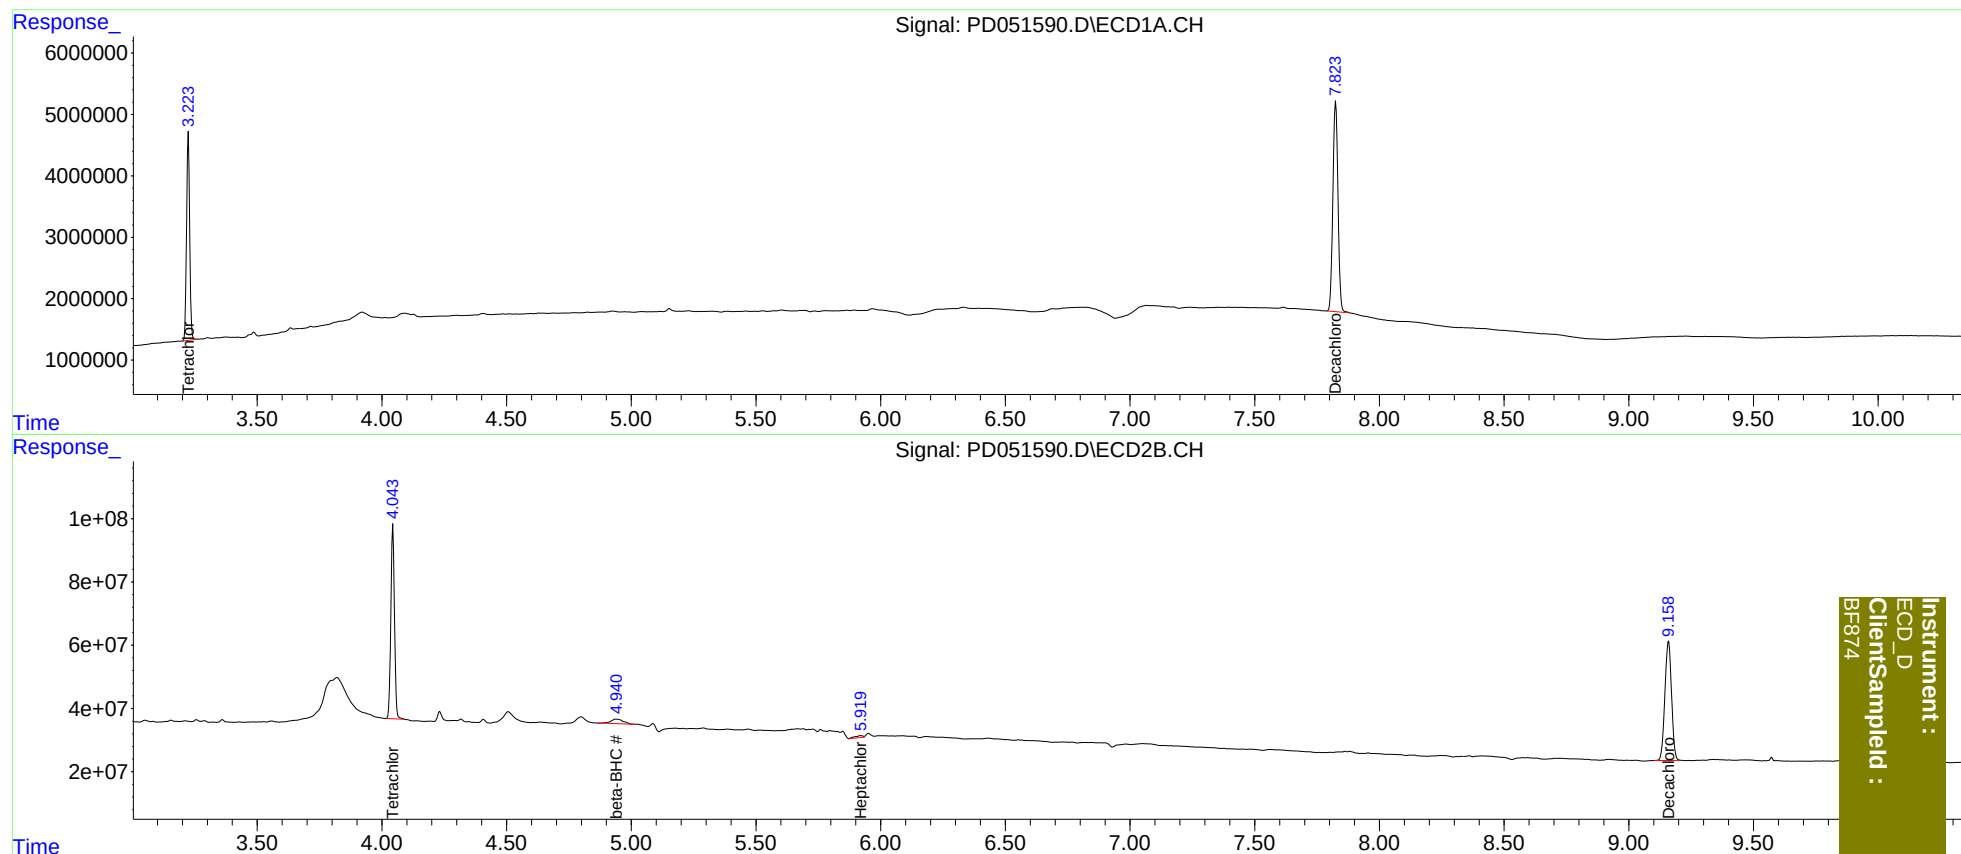


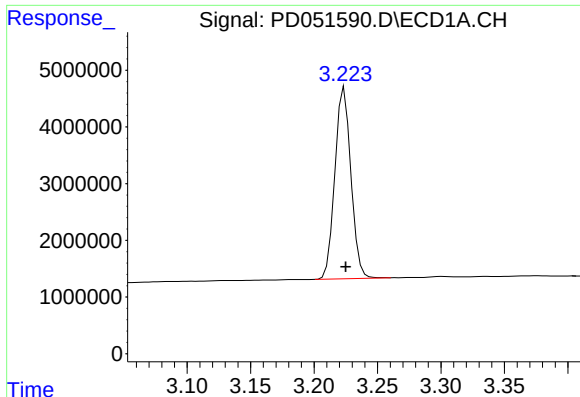

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 29741090
Conc: 20.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF874

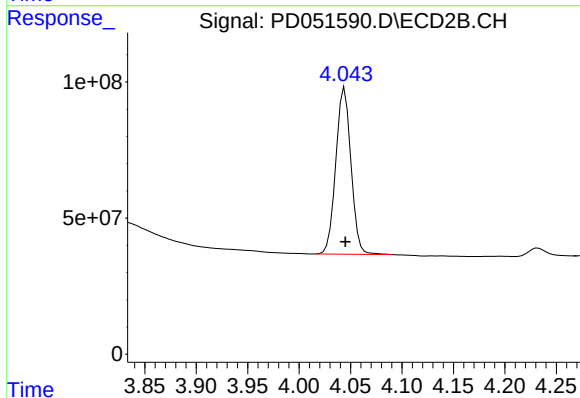


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 627595307
Conc: 20.31 ng/ml

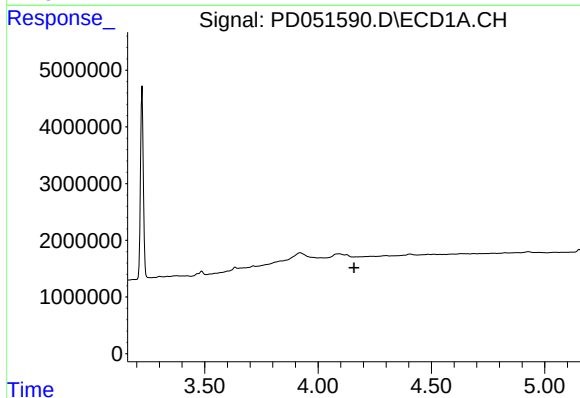


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

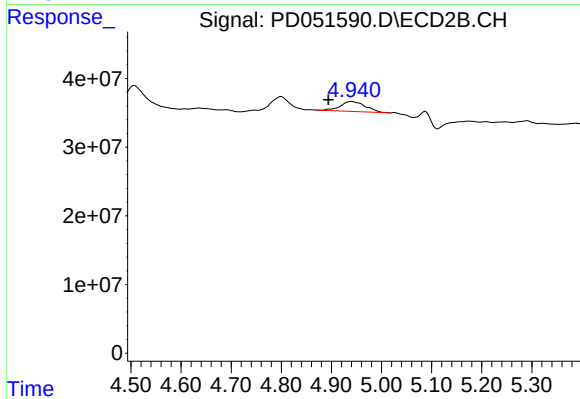

#6 beta-BHC


R.T.: 4.941 min
Delta R.T.: 0.047 min
Response: 50238708
Conc: 2.53 ng/ml

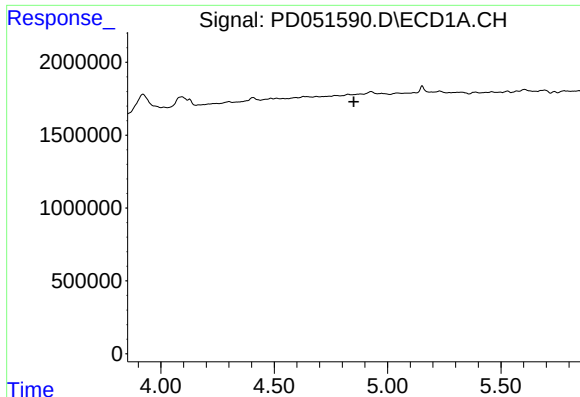

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF874

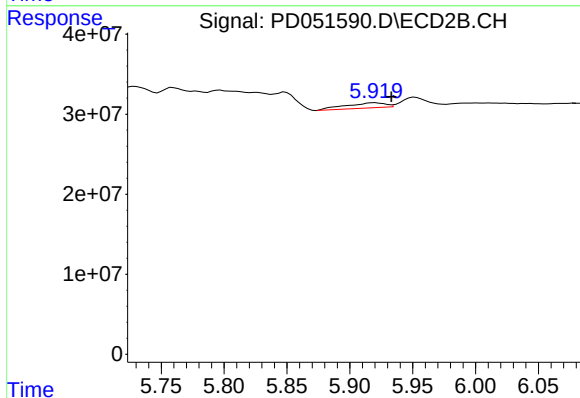


#8 Heptachlor epoxide

R.T.: 5.920 min
Delta R.T.: -0.013 min
Response: 14372567
Conc: 0.40 ng/ml

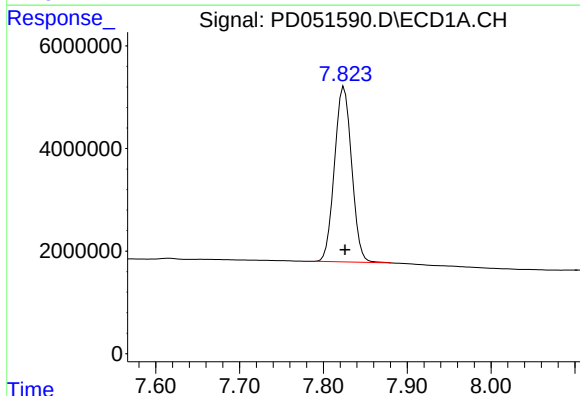

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.001 min
Response: 48538157
Conc: 40.36 ng/ml

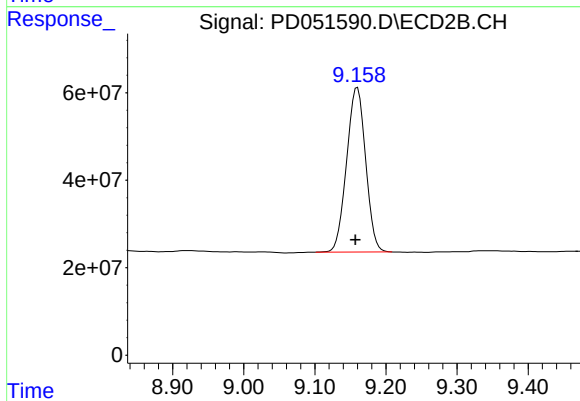

#27 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: 0.003 min
Response: 699714054
Conc: 36.91 ng/ml