

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
 Data File : PD061425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 18:42
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 05:43:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:43:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	4702638	49333945	5.099	5.174
27)	SA Decachlor...	8.261	9.042	15411326	107.7E6	11.736	11.494
Target Compounds							
2)	A alpha-BHC	3.926	4.371	6328236	76530229	4.793	5.237
3)	MA gamma-BHC...	4.211	4.656	6554698	69877838	5.048	5.212
4)	MA Heptachlor	4.516	5.164	6827771	74057156	5.046	5.416
9)	A Endosulfan I	5.551	6.211	6170099	61154268	5.113	5.325
13)	MA Dieldrin	5.795	6.468	12985788	129.1E6	9.806	10.553
14)	MA Endrin	6.053	6.686	11875905	112.1E6	10.329	11.127
16)	A 4,4'-DDD	6.177	6.808	10014760	101.4E6	9.572	10.448
17)	MA 4,4'-DDT	6.419	7.107	10732988	99995363	9.685	10.306
20)	A Methoxychlor	6.966	7.564	33246293	260.4E6	54.713	57.033


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
Data File : PD061425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 18:42
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 05:43:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:43:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

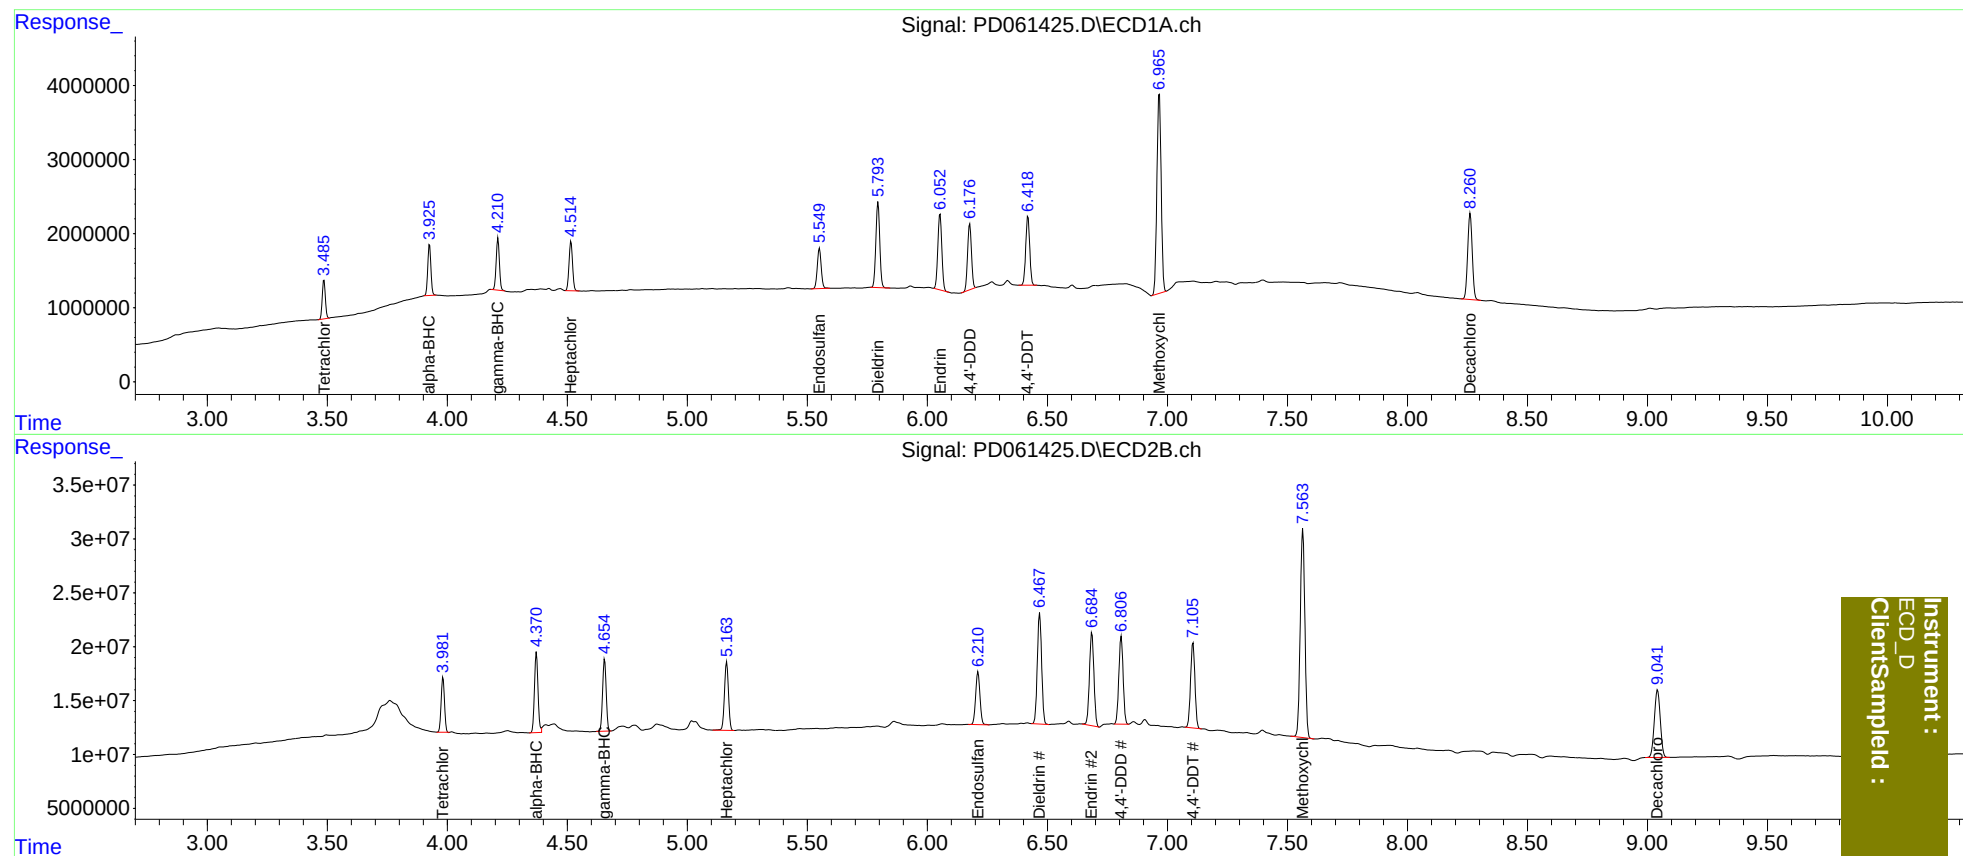


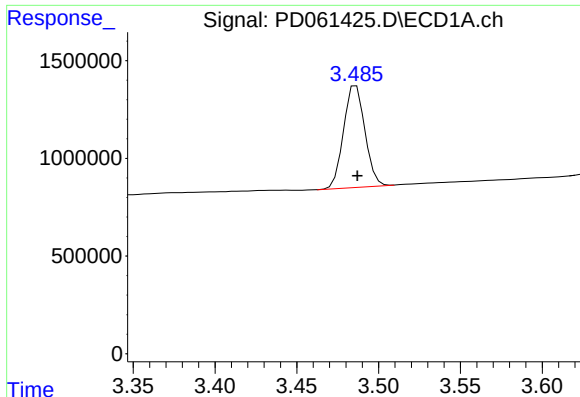

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 4702638
Conc: 5.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

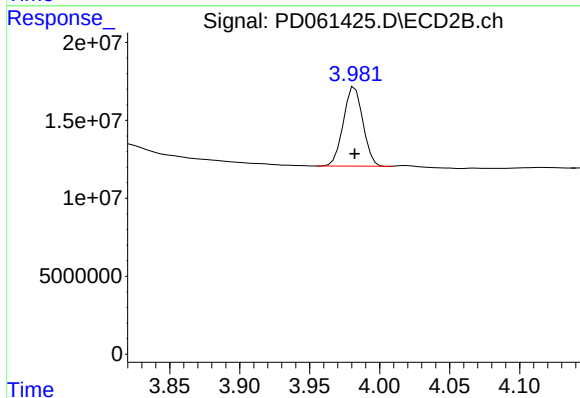


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 49333945
Conc: 5.17 ng/ml

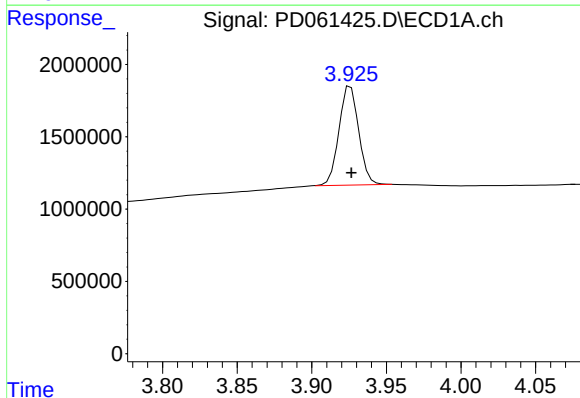


#2 alpha-BHC

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 6328236
Conc: 4.79 ng/ml

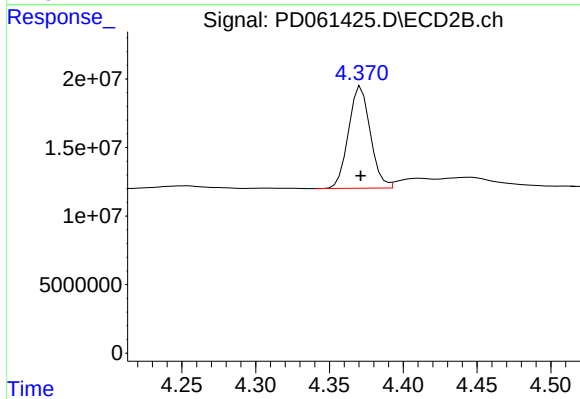

#2 alpha-BHC


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 76530229
Conc: 5.24 ng/ml

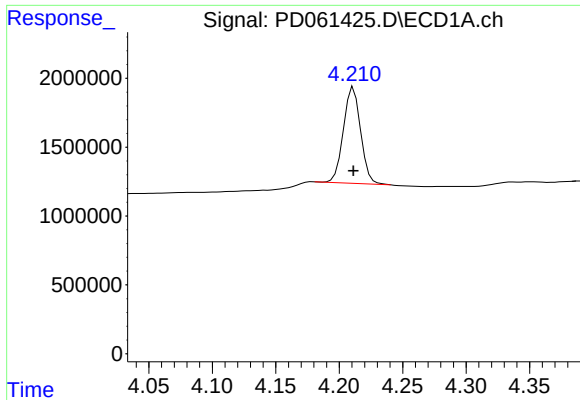

#3 gamma-BHC (Lindane)


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 6554698
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

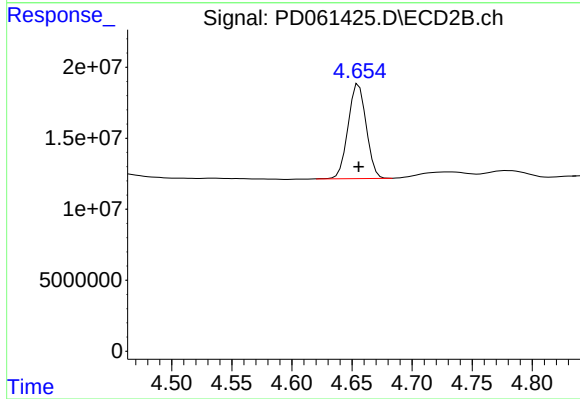


#3 gamma-BHC (Lindane)

R.T.: 4.656 min
Delta R.T.: 0.000 min
Response: 69877838
Conc: 5.21 ng/ml

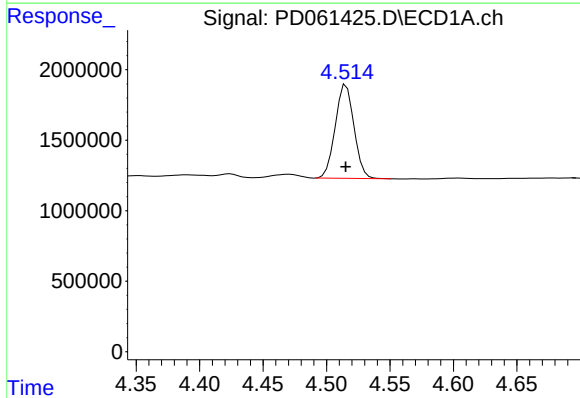


#4 Heptachlor

R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 6827771
Conc: 5.05 ng/ml

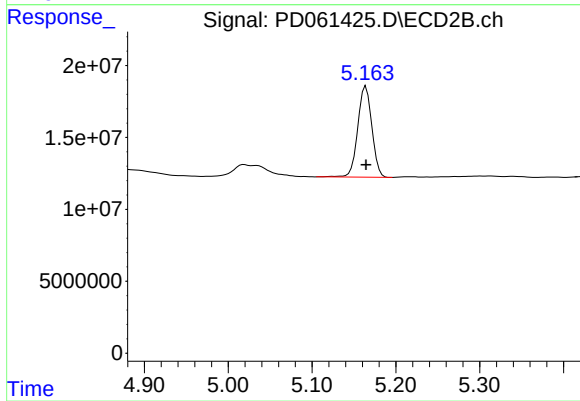

#4 Heptachlor


R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 74057156
Conc: 5.42 ng/ml

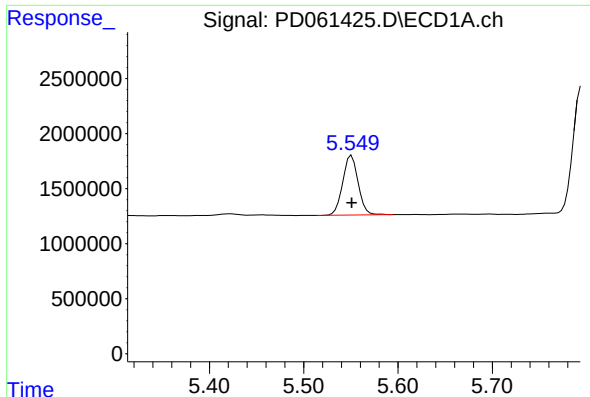

#9 Endosulfan I


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 6170099
Conc: 5.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

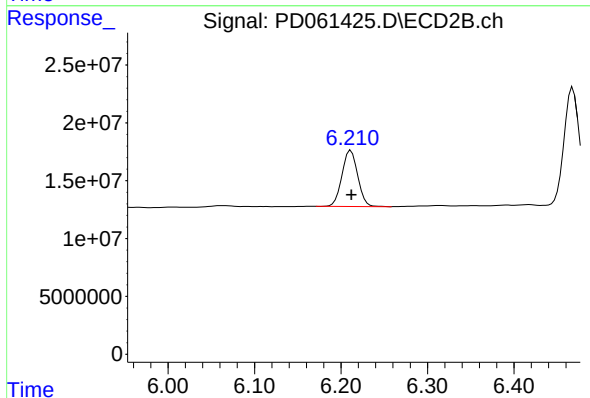


#9 Endosulfan I

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 61154268
Conc: 5.33 ng/ml

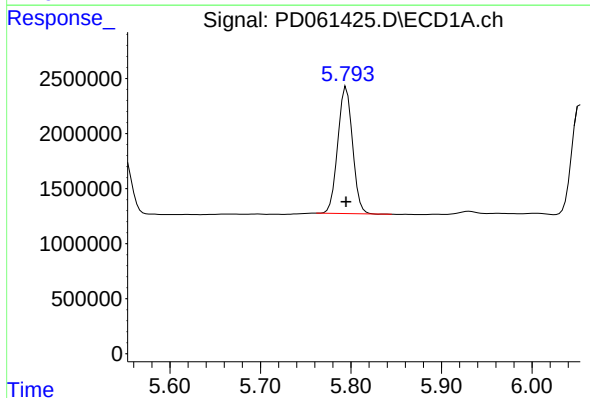


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 12985788
Conc: 9.81 ng/ml

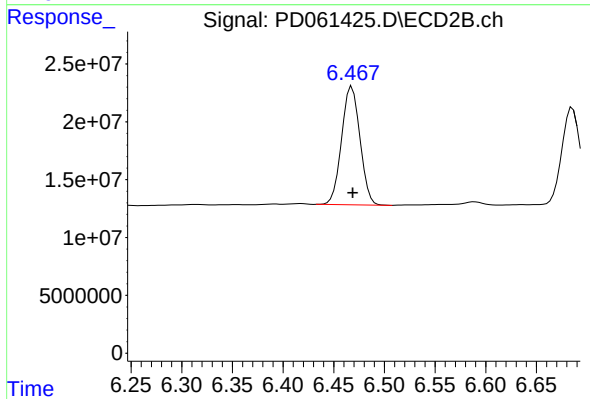

#13 Dieldrin


R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 129127788
Conc: 10.55 ng/ml

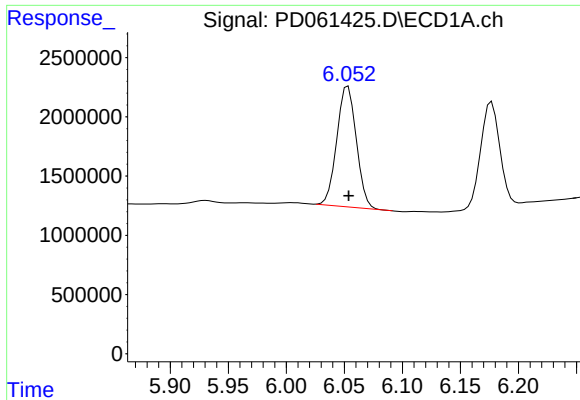

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 11875905
Conc: 10.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

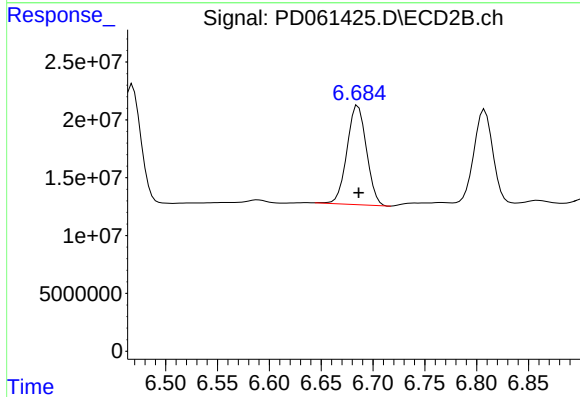


#14 Endrin

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 112145652
Conc: 11.13 ng/ml

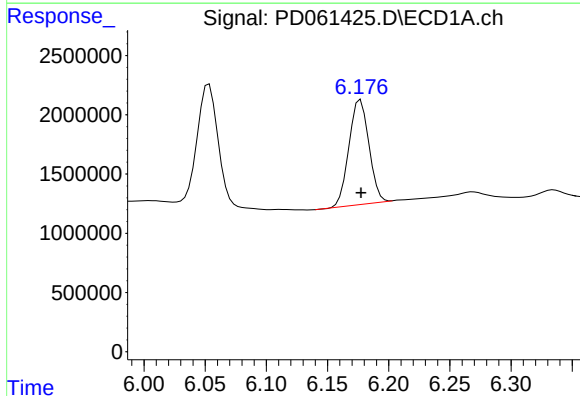


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 10014760
Conc: 9.57 ng/ml

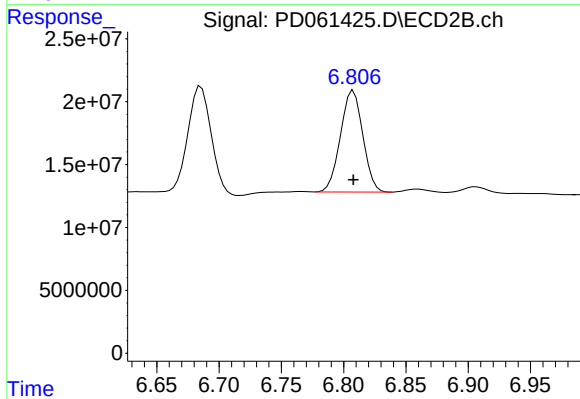

#16 4,4'-DDD


R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 101422467
Conc: 10.45 ng/ml

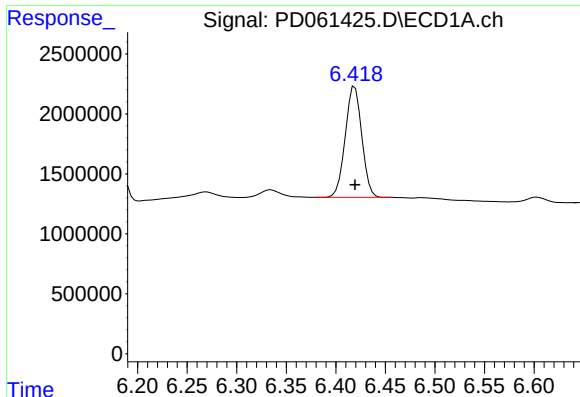

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 10732988
Conc: 9.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

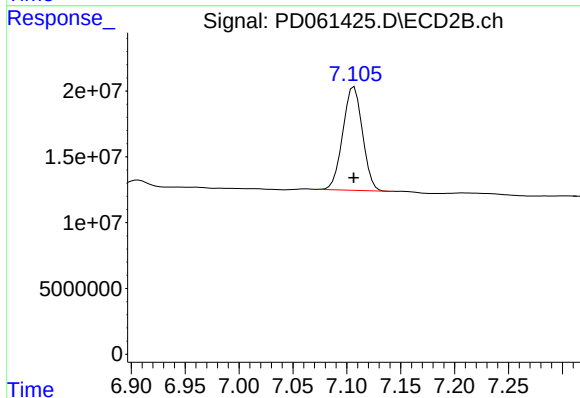


#17 4,4'-DDT

R.T.: 7.107 min
Delta R.T.: 0.000 min
Response: 99995363
Conc: 10.31 ng/ml

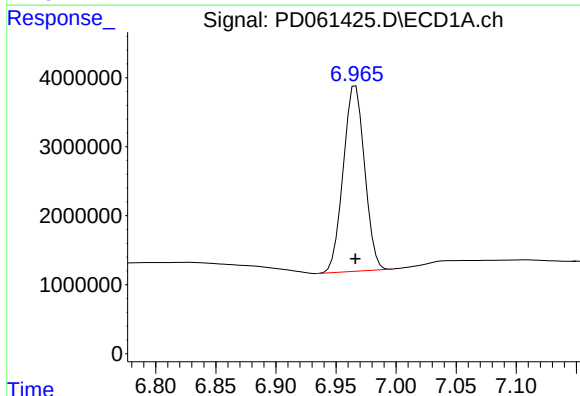


#20 Methoxychlor

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 33246293
Conc: 54.71 ng/ml

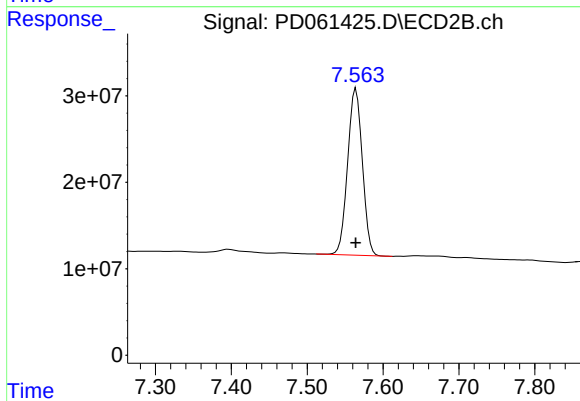

#20 Methoxychlor


R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 260374970
Conc: 57.03 ng/ml

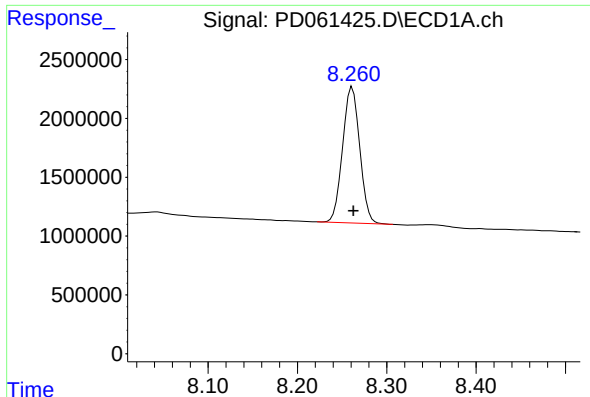

#27 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: -0.001 min
Response: 15411326
Conc: 11.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

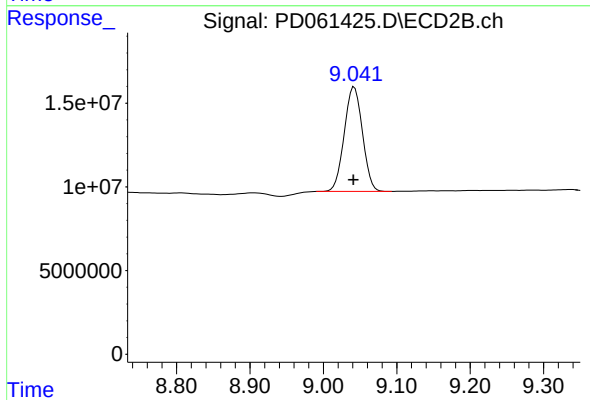

#27 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 107718531
Conc: 11.49 ng/ml