

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
 Data File : PD061427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 19:10
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 05:43:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:43:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	9429380	96110081	10.224	10.080
27)	SA Decachlor...	8.262	9.043	28645001	199.1E6	21.813	21.242
Target Compounds							
2)	A alpha-BHC	3.926	4.371	12927830	145.8E6	9.791	9.977
3)	MA gamma-BHC...	4.211	4.655	13013233	133.4E6	10.021	9.954
4)	MA Heptachlor	4.515	5.164	13575974	137.0E6	10.033	10.018
9)	A Endosulfan I	5.551	6.211	12431142	117.6E6	10.301	10.242
13)	MA Dieldrin	5.795	6.468	26274803	249.8E6	19.840	20.411
14)	MA Endrin	6.054	6.686	22982554	208.3E6	19.989	20.669
16)	A 4,4'-DDD	6.178	6.807	20569407	197.4E6	19.660	20.337
17)	MA 4,4'-DDT	6.419	7.106	21483777	202.9E6	19.386	20.915
20)	A Methoxychlor	6.966	7.564	63180006	483.6E6	103.974	105.930

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
Data File : PD061427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 19:10
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 05:43:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:43:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

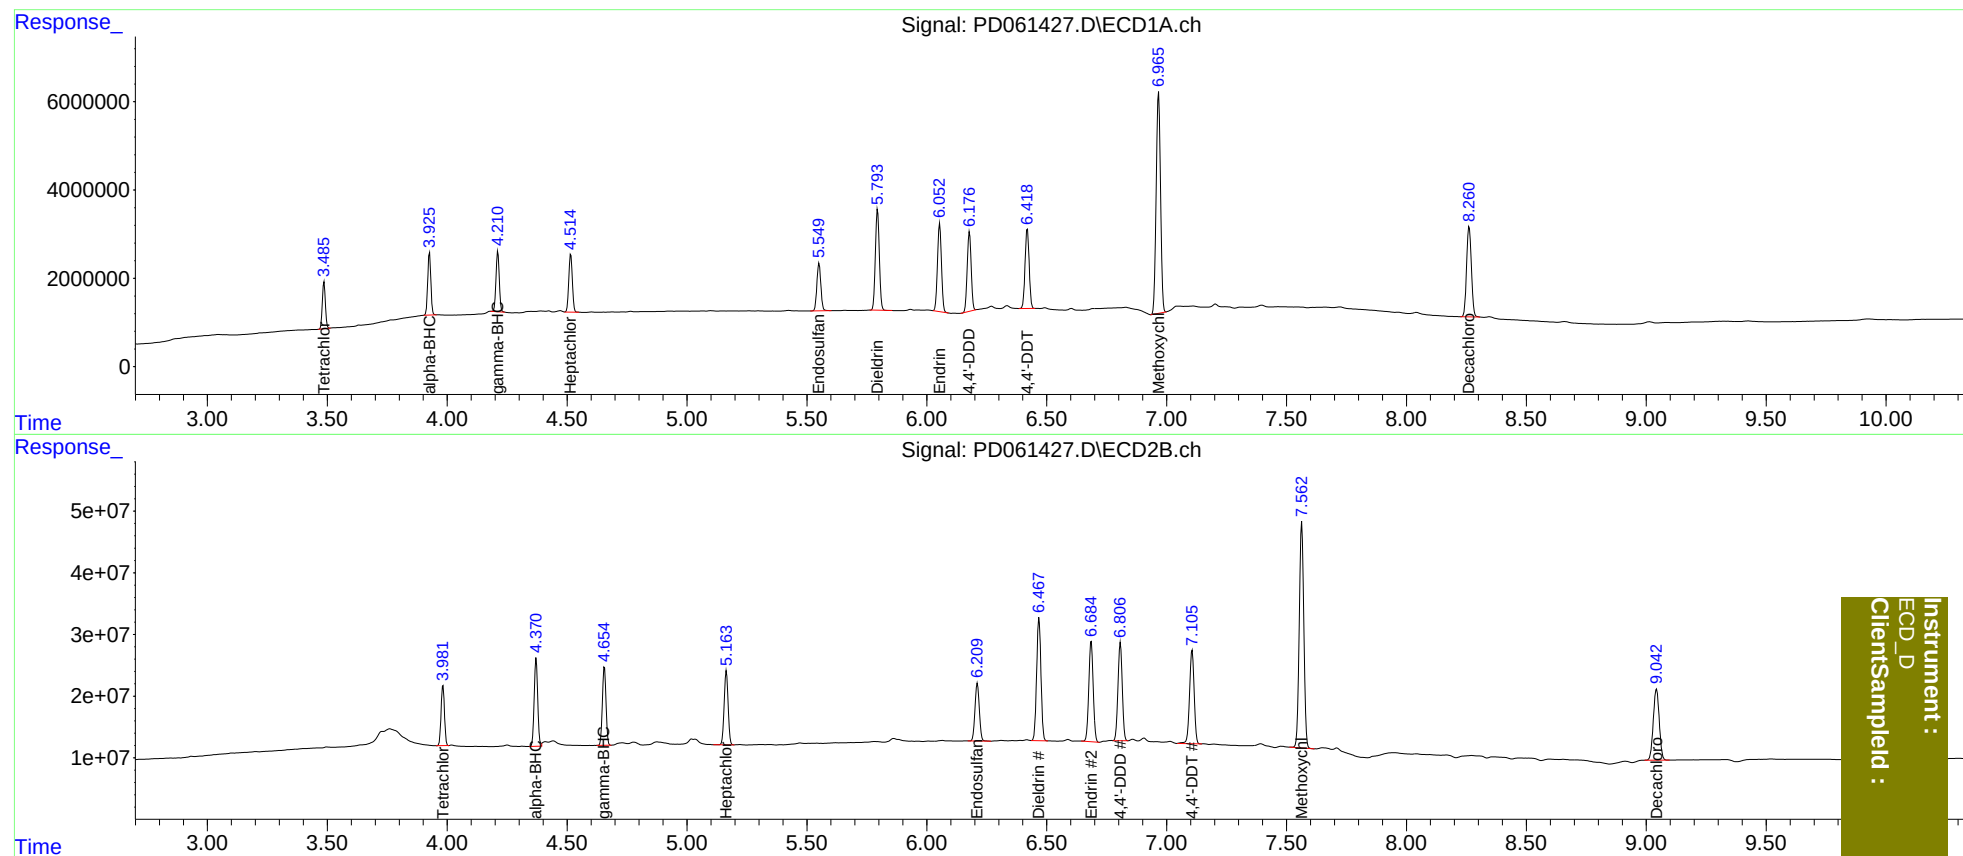


Instrument :
ECD_D
ClientSampled :

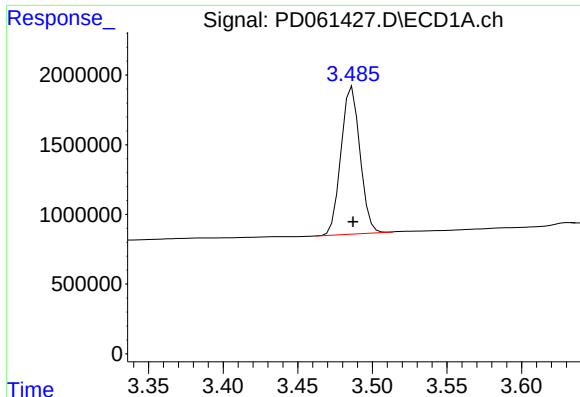

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 9429380
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

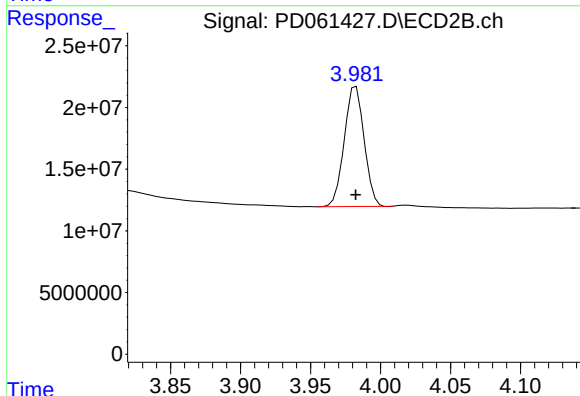


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 96110081
Conc: 10.08 ng/ml

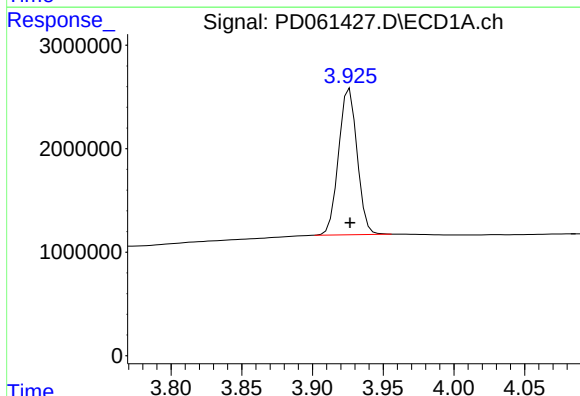


#2 alpha-BHC

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 12927830
Conc: 9.79 ng/ml

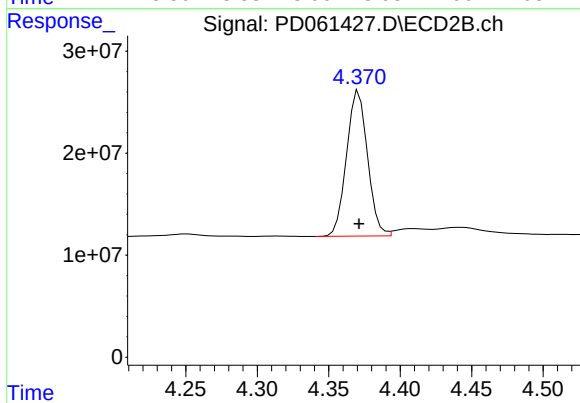

#2 alpha-BHC


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 145788125
Conc: 9.98 ng/ml

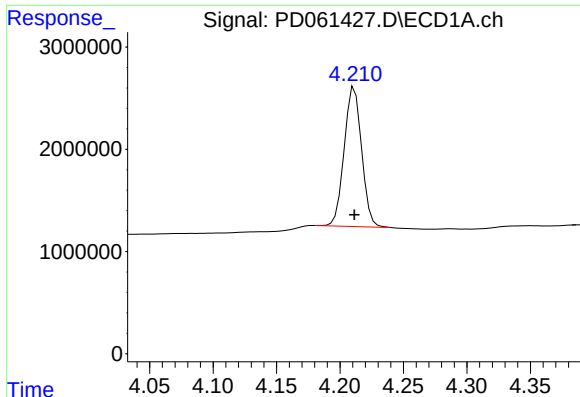

#3 gamma-BHC (Lindane)


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 13013233
Conc: 10.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

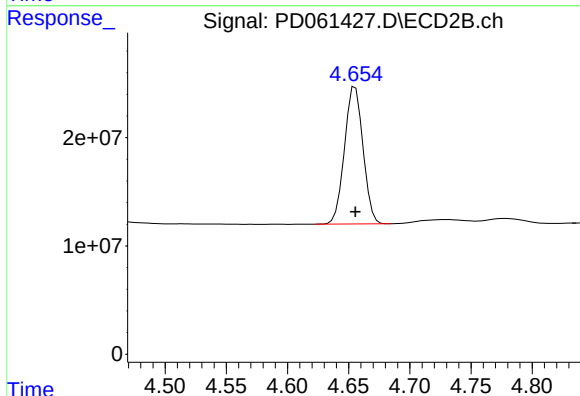


#3 gamma-BHC (Lindane)

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 133442379
Conc: 9.95 ng/ml

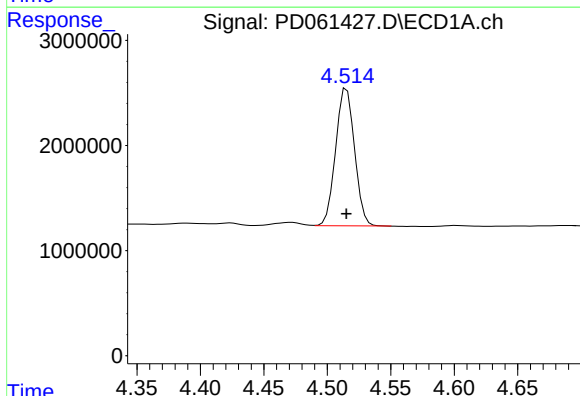


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 13575974
Conc: 10.03 ng/ml

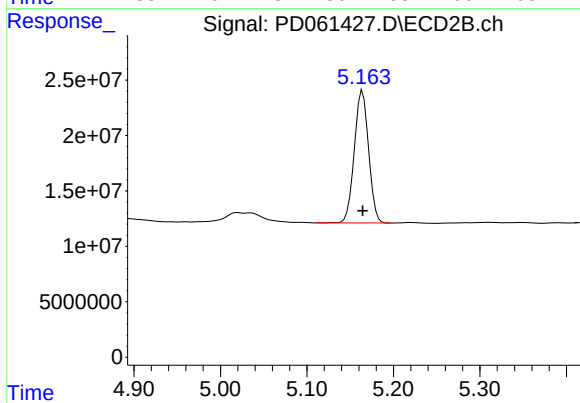

#4 Heptachlor


R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 136983557
Conc: 10.02 ng/ml

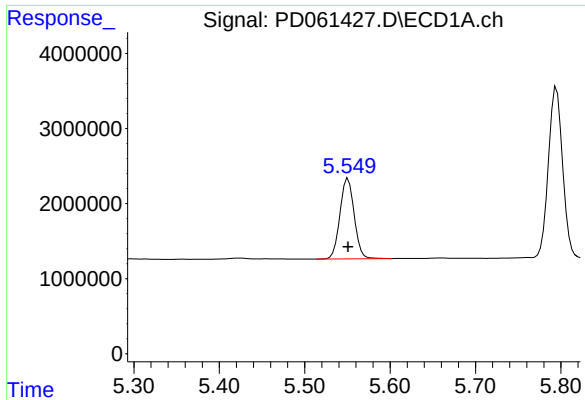

#9 Endosulfan I


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 12431142
Conc: 10.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

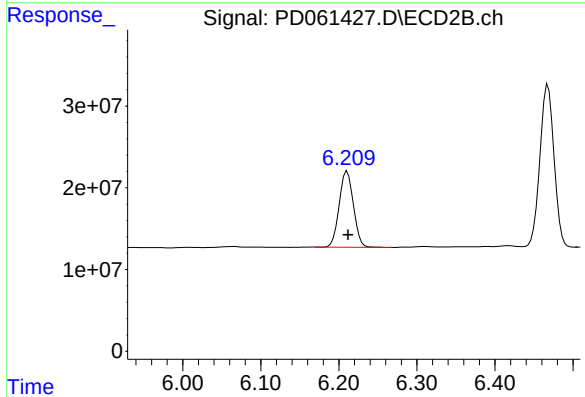


#9 Endosulfan I

R.T.: 6.211 min
Delta R.T.: -0.001 min
Response: 117614575
Conc: 10.24 ng/ml

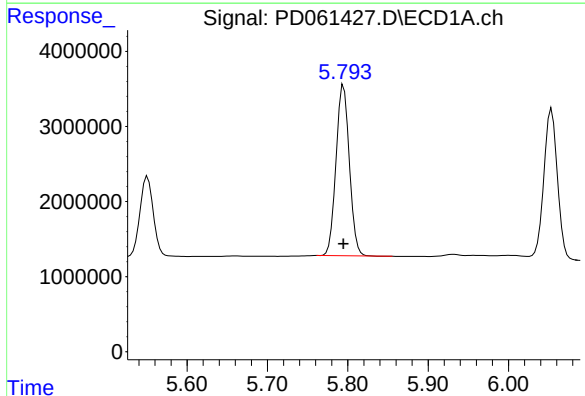


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 26274803
Conc: 19.84 ng/ml

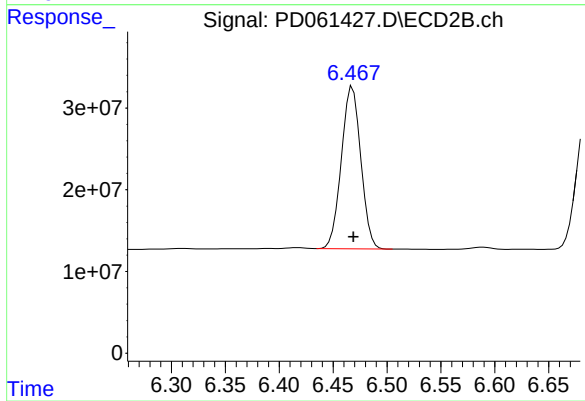

#13 Dieldrin


R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 249751758
Conc: 20.41 ng/ml

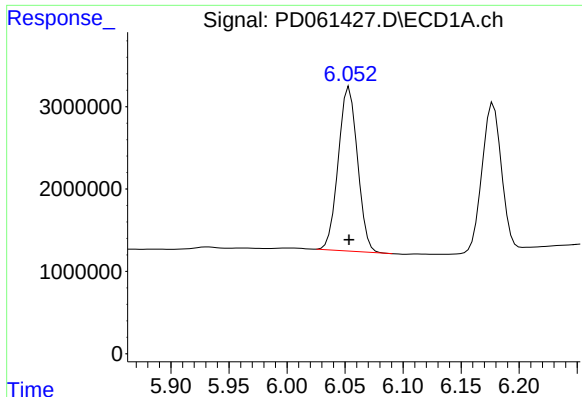

#14 Endrin


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 22982554
Conc: 19.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

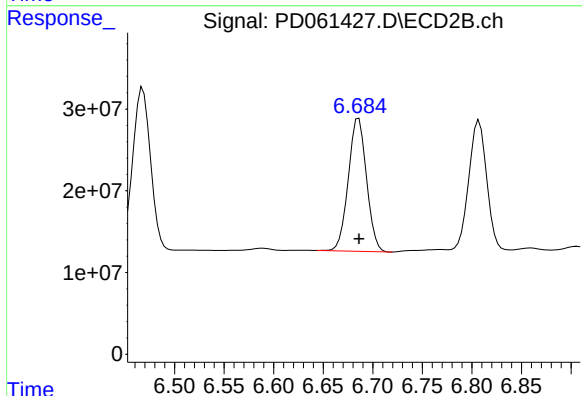


#14 Endrin

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 208316445
Conc: 20.67 ng/ml

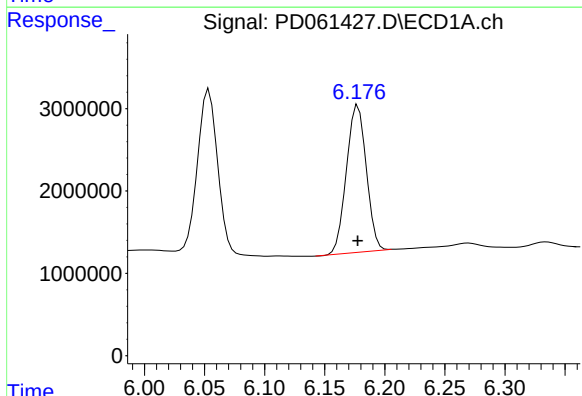


#16 4,4'-DDD

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 20569407
Conc: 19.66 ng/ml

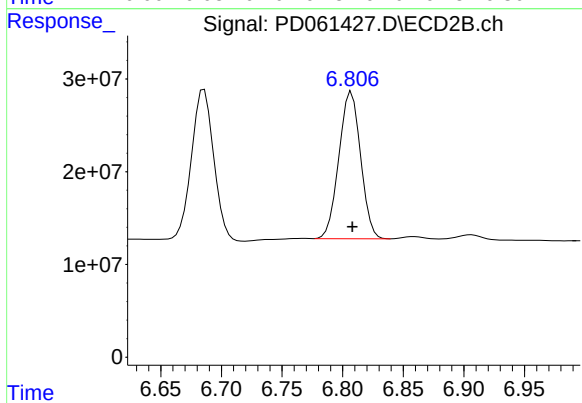

#16 4,4'-DDD


R.T.: 6.807 min
Delta R.T.: 0.000 min
Response: 197414913
Conc: 20.34 ng/ml

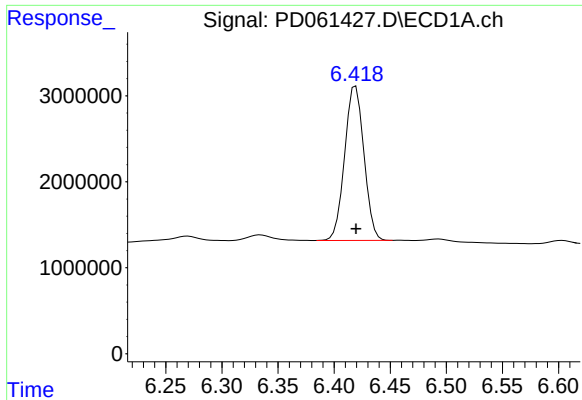

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 21483777
Conc: 19.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

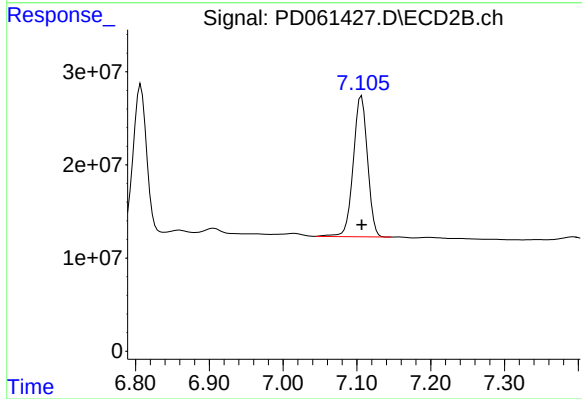


#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 202941555
Conc: 20.92 ng/ml

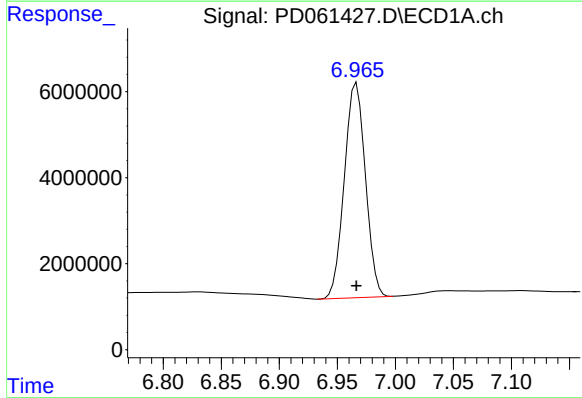


#20 Methoxychlor

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 63180006
Conc: 103.97 ng/ml

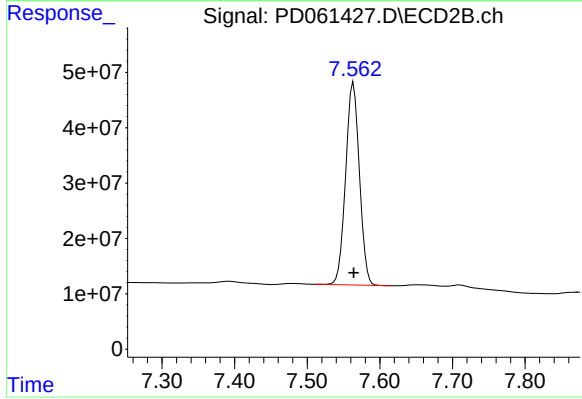

#20 Methoxychlor

R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 483605241
Conc: 105.93 ng/ml

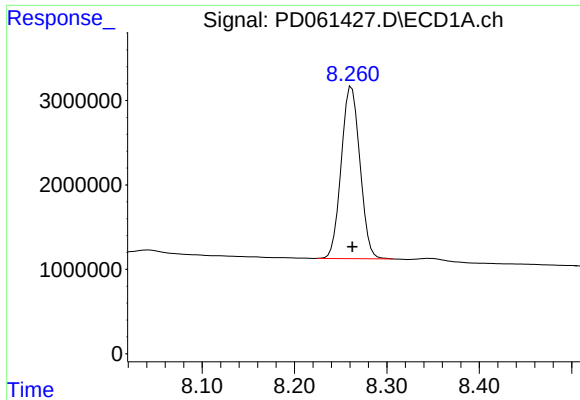

#27 Decachlorobiphenyl


R.T.: 8.262 min

Delta R.T.: 0.000 min

Response: 28645001

Conc: 21.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

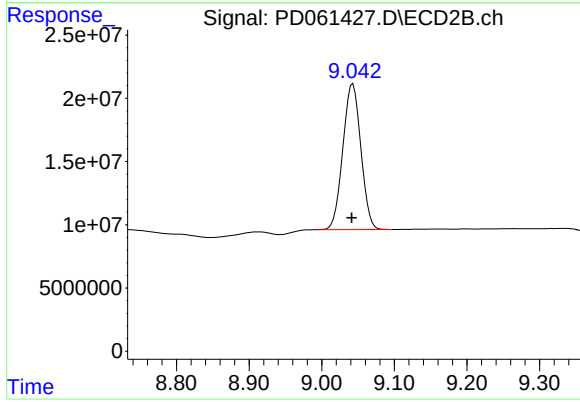

#27 Decachlorobiphenyl

R.T.: 9.043 min

Delta R.T.: 0.002 min

Response: 199074747

Conc: 21.24 ng/ml