

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
 Data File : PD061429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 19:38
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 05:44:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:43:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.487	3.982	18445215	190.7E6	20.000	20.000
27)	SA Decachlor...	8.263	9.041	52528415	374.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.927	4.371	26407327	292.2E6	20.000	20.000
3)	MA gamma-BHC...	4.211	4.656	25972002	268.1E6	20.000	20.000
4)	MA Heptachlor	4.515	5.165	27063251	273.5E6	20.000	20.000
9)	A Endosulfan I	5.551	6.212	24135538	229.7E6	20.000	20.000
13)	MA Dieldrin	5.795	6.469	52973475	489.4E6	40.000	40.000
14)	MA Endrin	6.054	6.686	45989452	403.2E6	40.000	40.000
16)	A 4,4'-DDD	6.177	6.808	41849808	388.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.419	7.106	44328545	388.1E6	40.000	40.000
20)	A Methoxychlor	6.966	7.564	121.5E6	913.1E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
Data File : PD061429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 19:38
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 05:44:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:43:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

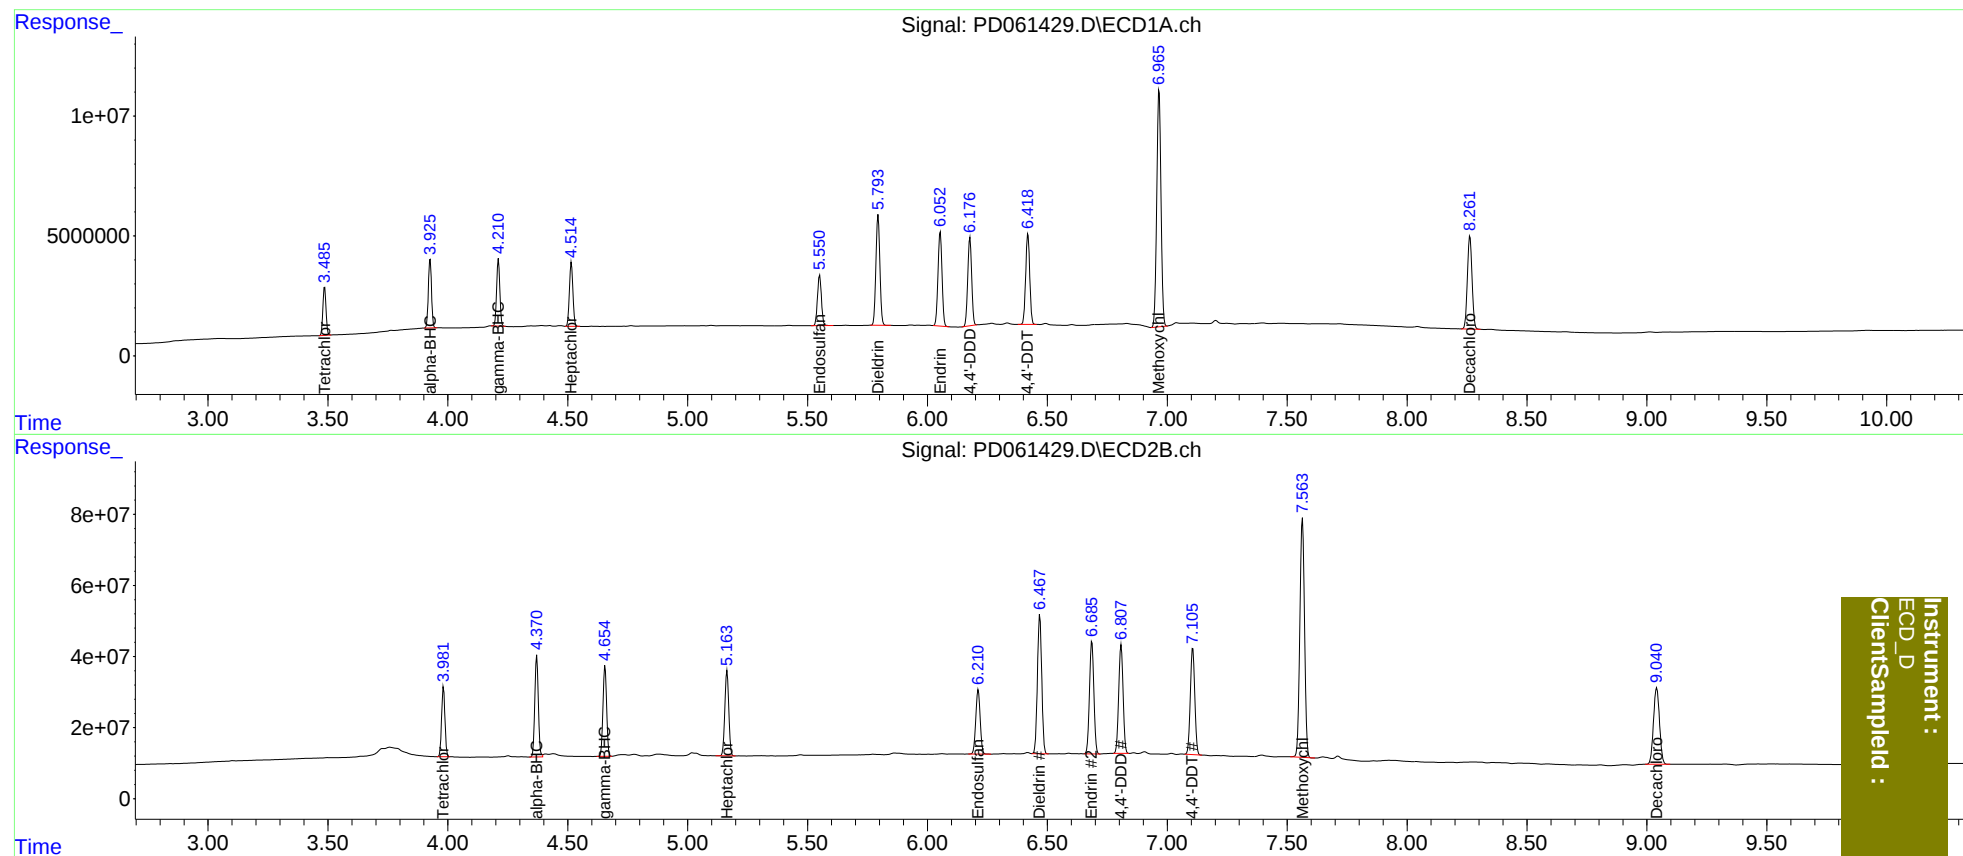


Instrument :
ECD_D
ClientSampled :

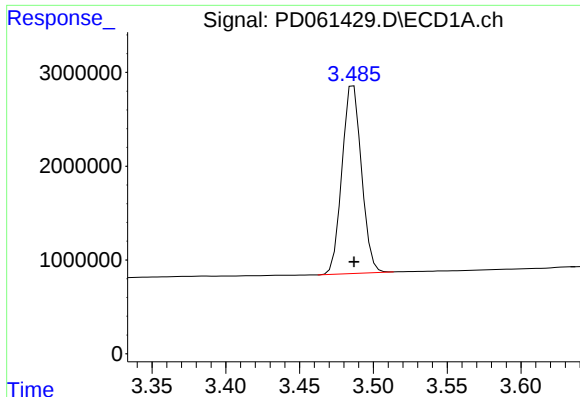

#1 Tetrachloro-m-xylene


R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 18445215
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

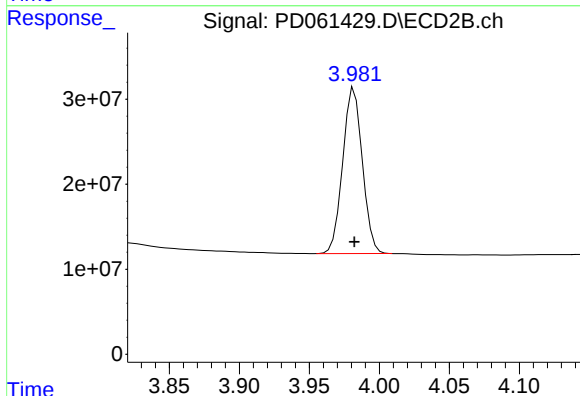


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 190687816
Conc: 20.00 ng/ml

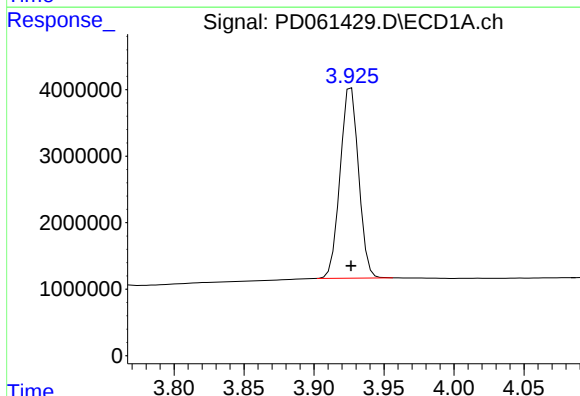


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 26407327
Conc: 20.00 ng/ml

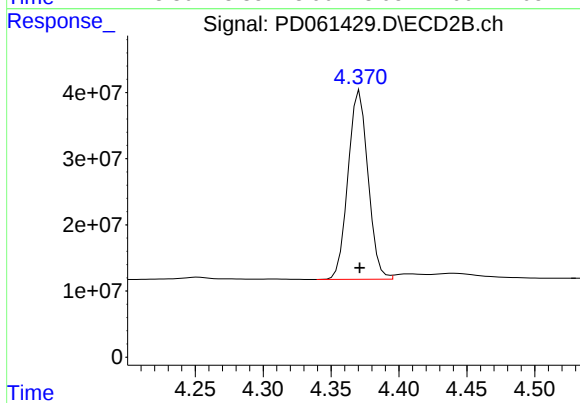

#2 alpha-BHC


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 292243480
Conc: 20.00 ng/ml

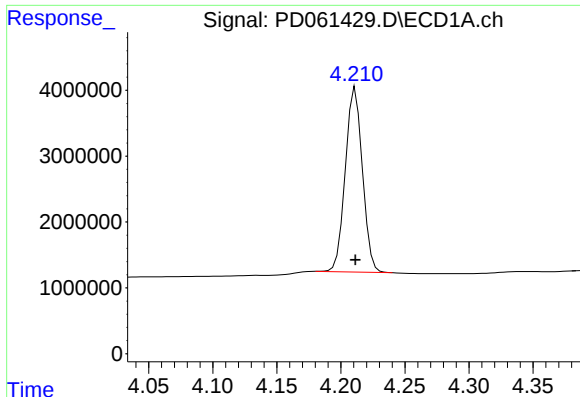

#3 gamma-BHC (Lindane)


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 25972002
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

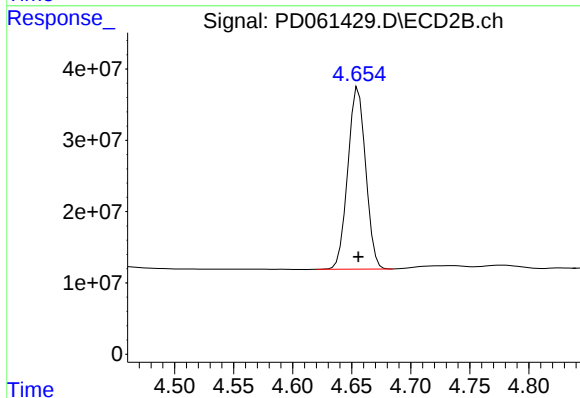


#3 gamma-BHC (Lindane)

R.T.: 4.656 min
Delta R.T.: 0.000 min
Response: 268123669
Conc: 20.00 ng/ml

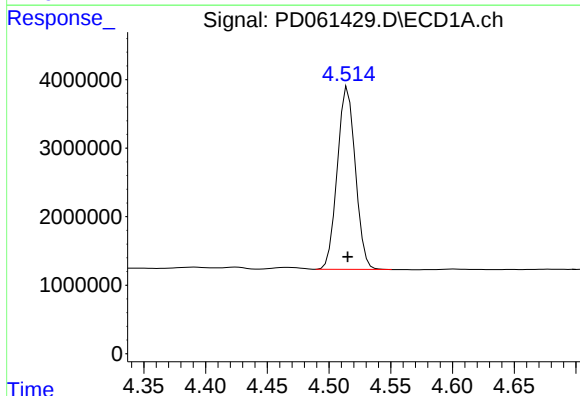


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 27063251
Conc: 20.00 ng/ml

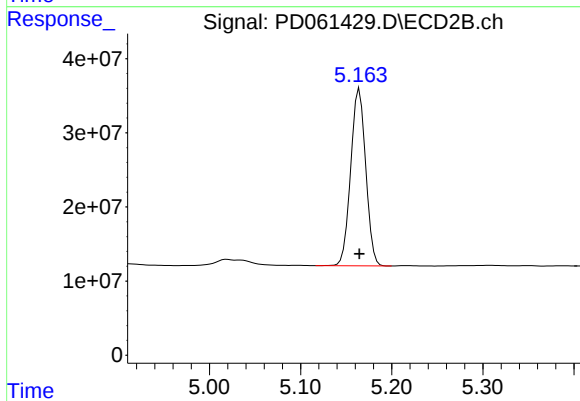

#4 Heptachlor


R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 273466166
Conc: 20.00 ng/ml

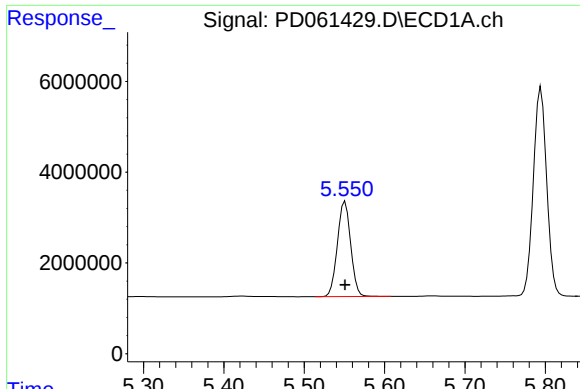

#9 Endosulfan I


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 24135538
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

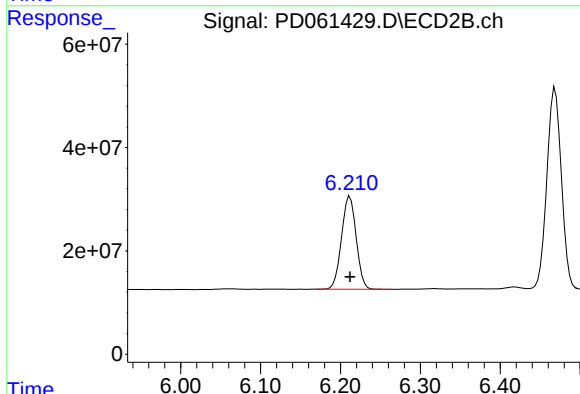


#9 Endosulfan I

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 229666579
Conc: 20.00 ng/ml

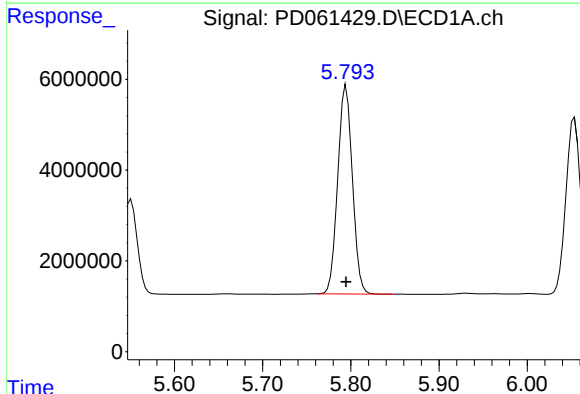


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 52973475
Conc: 40.00 ng/ml

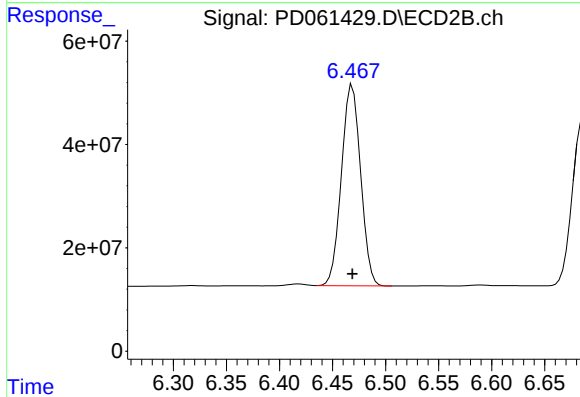

#13 Dieldrin


R.T.: 6.469 min
Delta R.T.: 0.000 min
Response: 489439952
Conc: 40.00 ng/ml

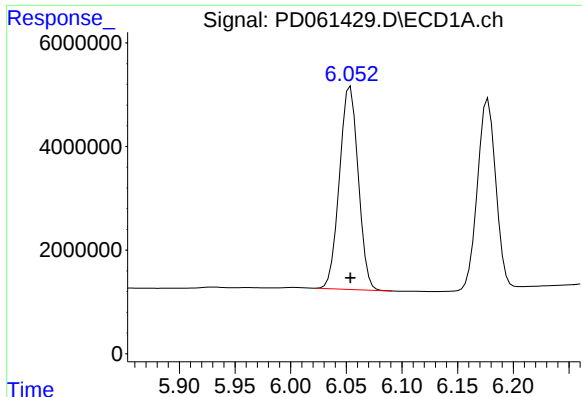

#14 Endrin


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 45989452
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

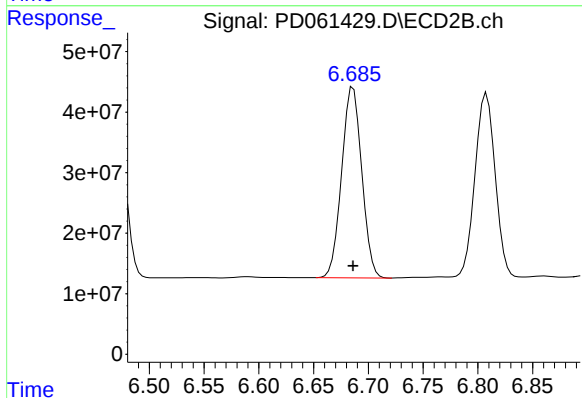


#14 Endrin

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 403153298
Conc: 40.00 ng/ml

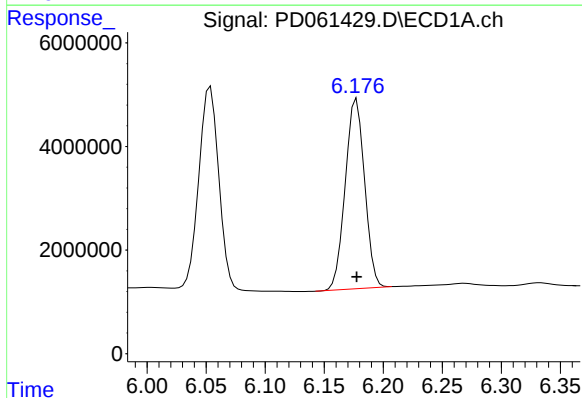


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 41849808
Conc: 40.00 ng/ml

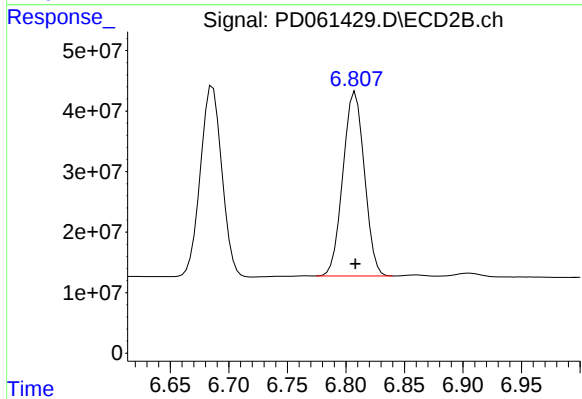

#16 4,4'-DDD


R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 388290169
Conc: 40.00 ng/ml

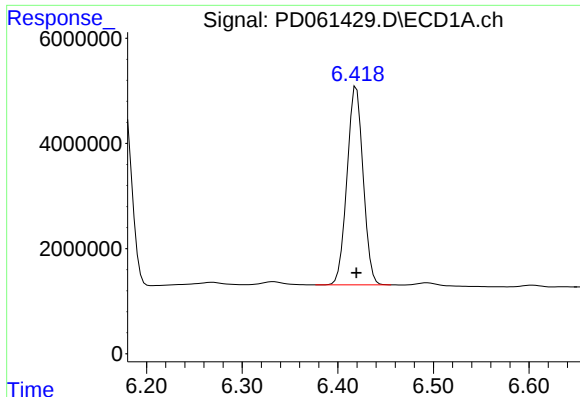

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 44328545
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

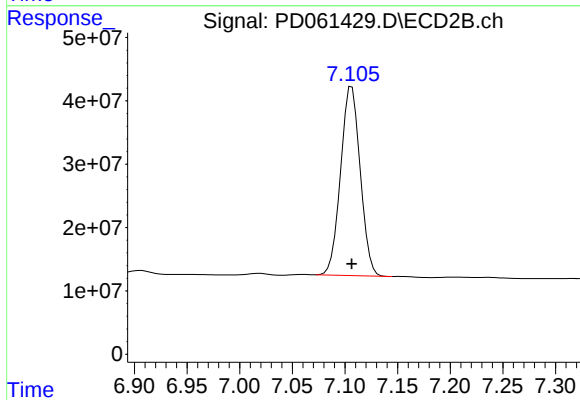


#17 4,4'-DDT

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 388121149
Conc: 40.00 ng/ml

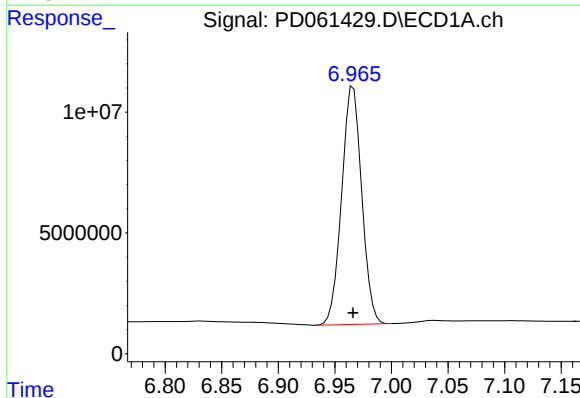


#20 Methoxychlor

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 121530570
Conc: 200.00 ng/ml

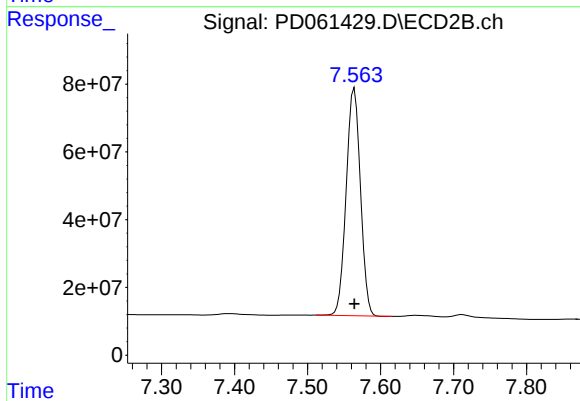

#20 Methoxychlor


R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 913069887
Conc: 200.00 ng/ml

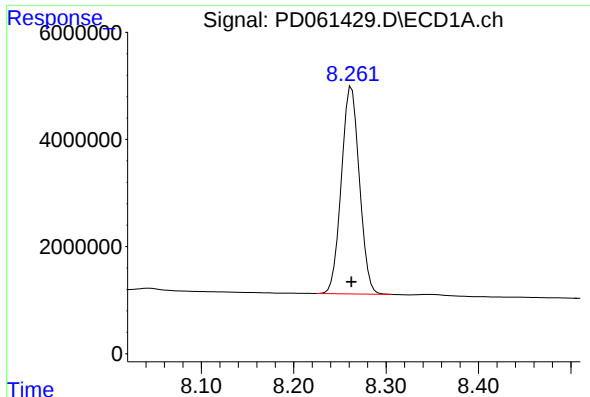

#27 Decachlorobiphenyl

R.T.: 8.263 min
Delta R.T.: 0.000 min
Response: 52528415
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

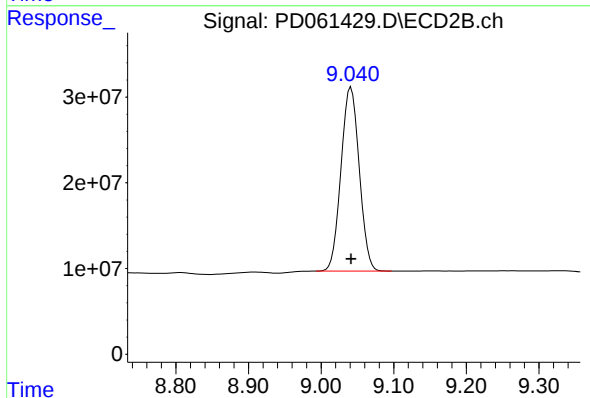

#27 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 374877621
Conc: 40.00 ng/ml