

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
 Data File : PD061431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 20:06
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 05:44:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:43:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.983	35220615	361.8E6	38.189	37.942
27)	SA Decachlor...	8.262	9.042	98944722	692.2E6	75.346	73.855
Target Compounds							
2)	A alpha-BHC	3.927	4.372	53310181	562.5E6	40.375	38.493
3)	MA gamma-BHC...	4.212	4.655	51407082	516.4E6	39.587	38.517
4)	MA Heptachlor	4.515	5.165	53247130	526.1E6	39.350	38.475
9)	A Endosulfan I	5.551	6.211	47039811	438.8E6	38.980	38.214
13)	MA Dieldrin	5.795	6.467	106.6E6	945.8E6	80.522	77.292
14)	MA Endrin	6.053	6.685	91845272	779.1E6	79.884	77.297
16)	A 4,4'-DDD	6.177	6.807	84892626	752.9E6	81.140	77.561
17)	MA 4,4'-DDT	6.419	7.105	91005069	762.0E6	82.119	78.537
20)	A Methoxychlor	6.966	7.563	234.6E6	1708.3E6	386.115	374.198

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
Data File : PD061431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 20:06
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 05:44:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:43:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

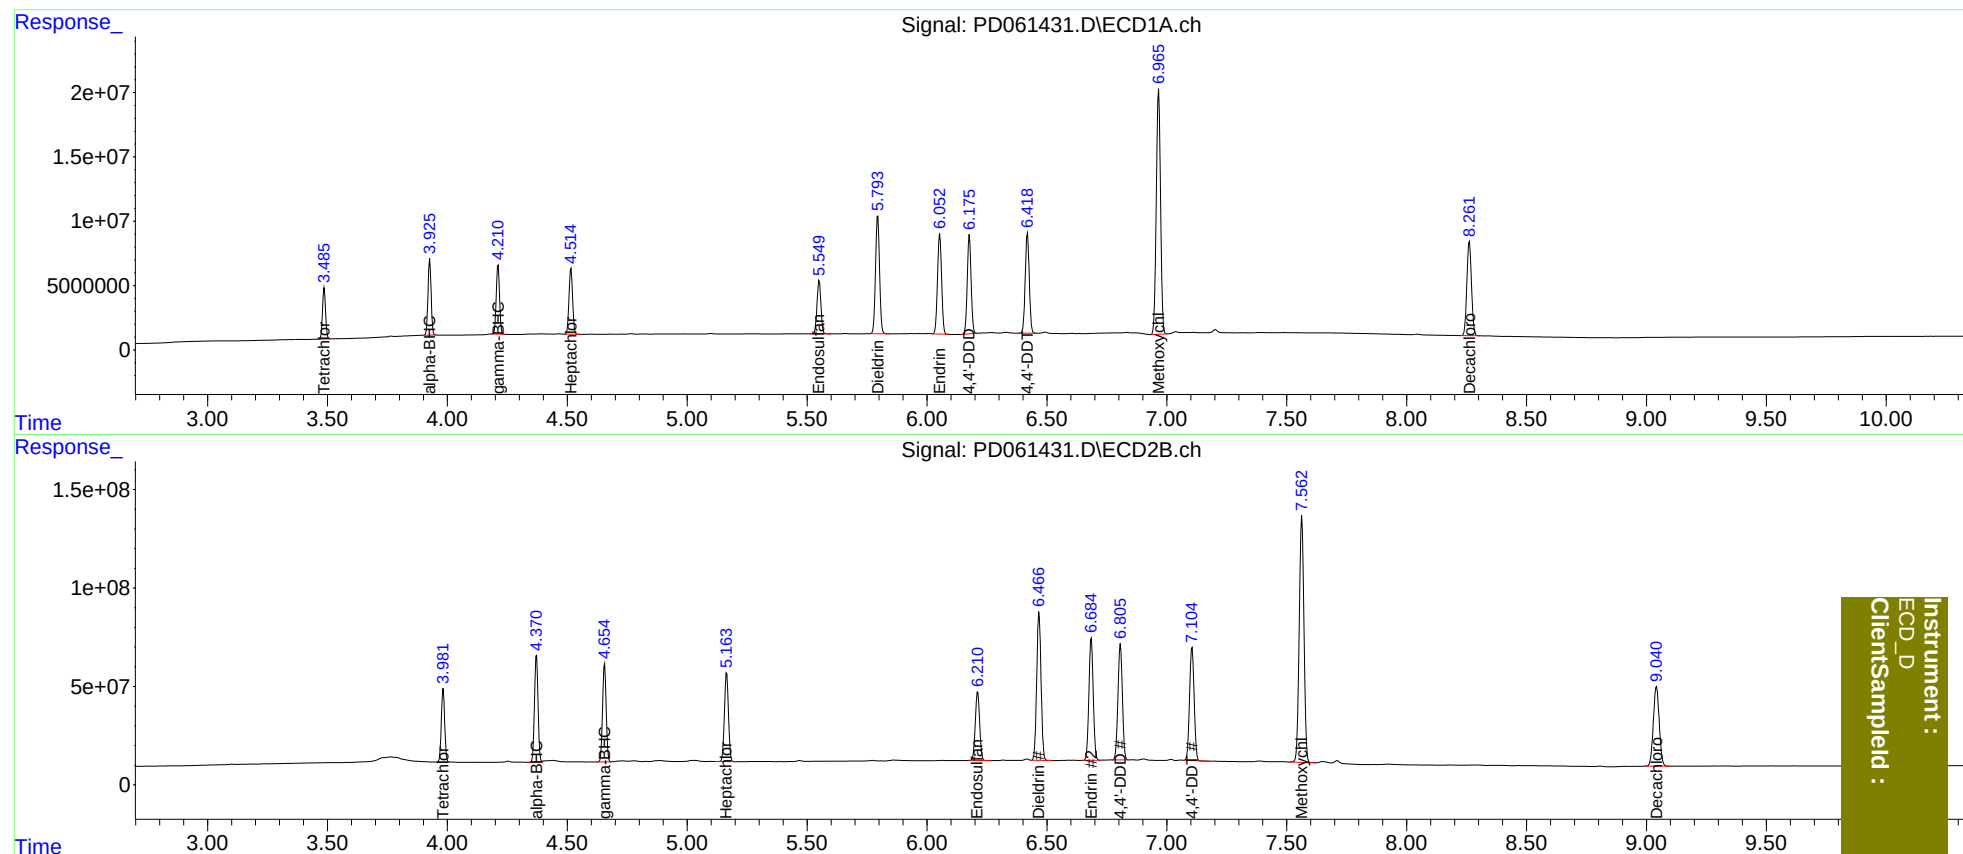


Instrument :
ECD_D
ClientSampled :

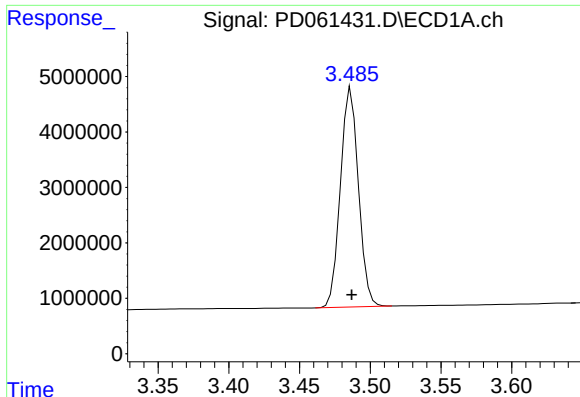

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 35220615
Conc: 38.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

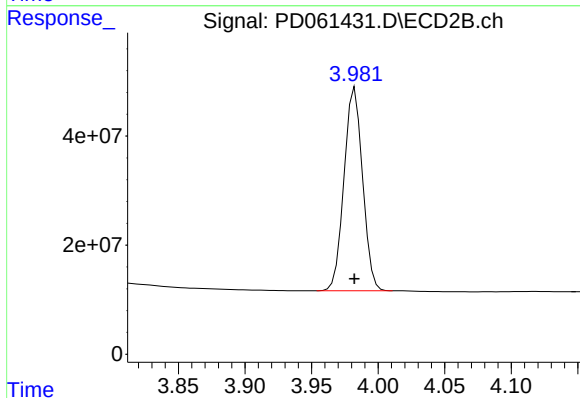


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 361757262
Conc: 37.94 ng/ml

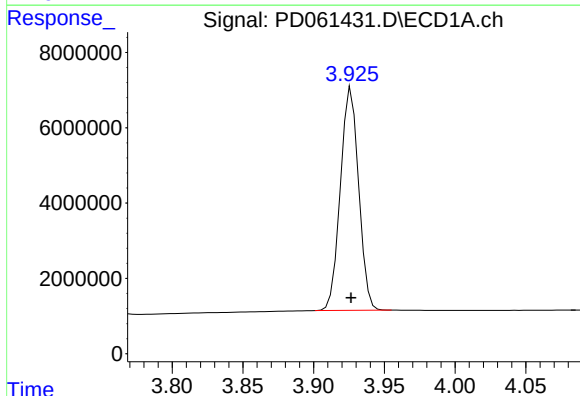


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 53310181
Conc: 40.38 ng/ml

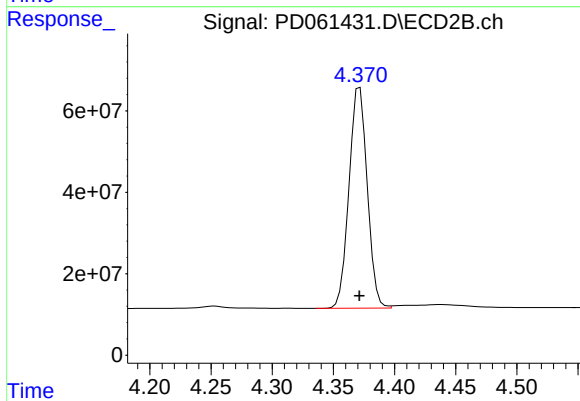

#2 alpha-BHC


R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 562460143
Conc: 38.49 ng/ml

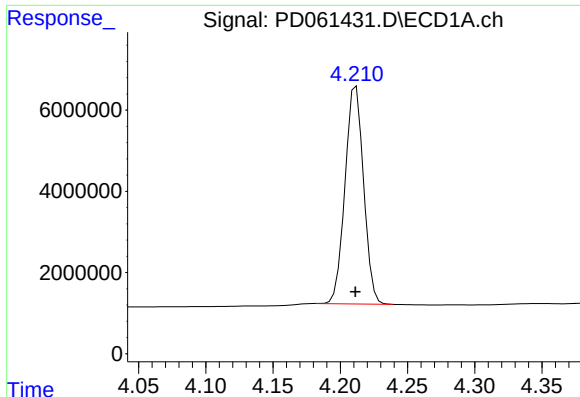

#3 gamma-BHC (Lindane)


R.T.: 4.212 min
Delta R.T.: 0.000 min
Response: 51407082
Conc: 39.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

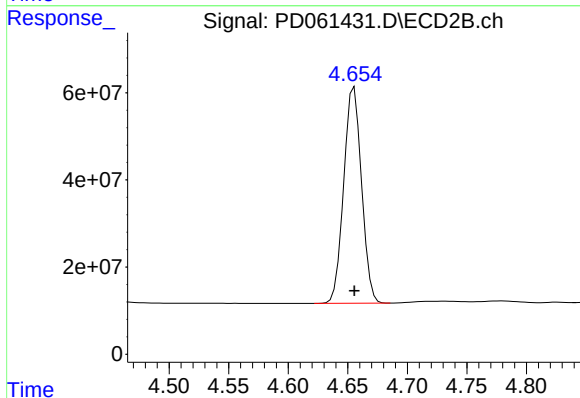


#3 gamma-BHC (Lindane)

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 516360279
Conc: 38.52 ng/ml

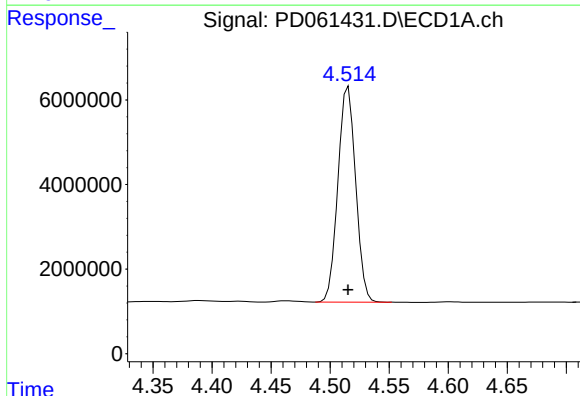


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 53247130
Conc: 39.35 ng/ml

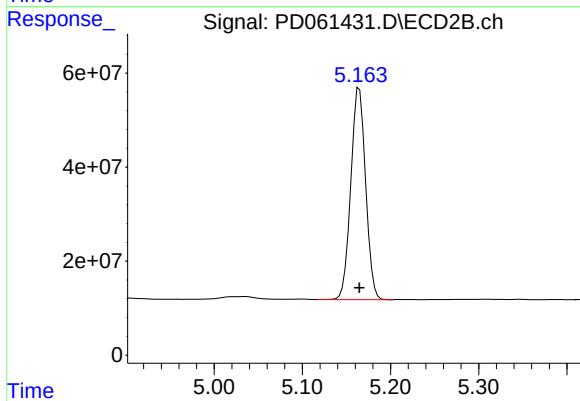

#4 Heptachlor


R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 526079826
Conc: 38.47 ng/ml

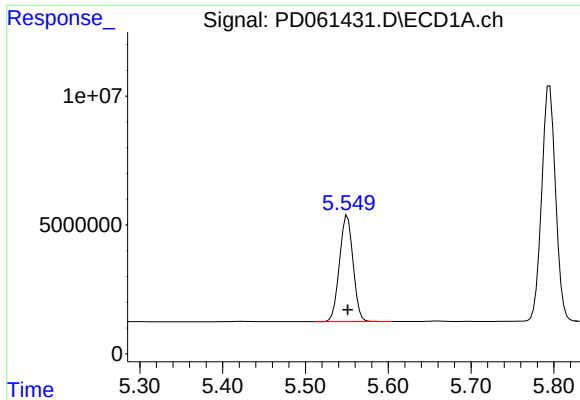

#9 Endosulfan I


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 47039811
Conc: 38.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

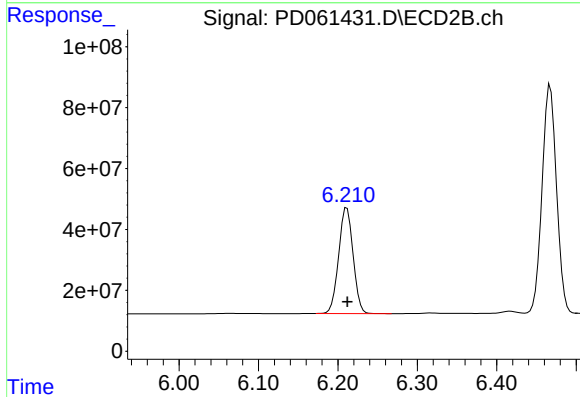


#9 Endosulfan I

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 438818200
Conc: 38.21 ng/ml

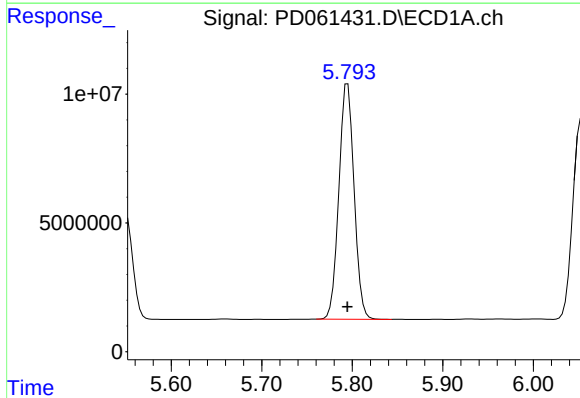


#13 Dieldrin

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 106638588
Conc: 80.52 ng/ml

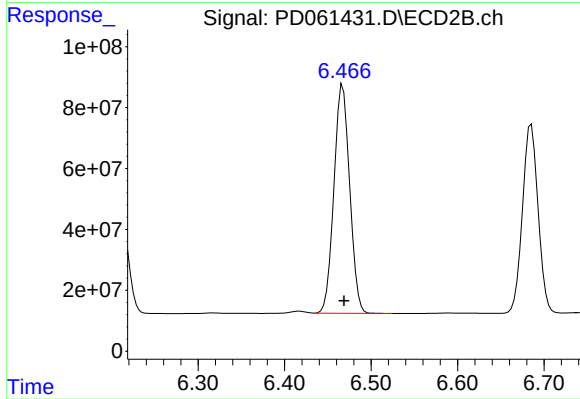

#13 Dieldrin


R.T.: 6.467 min
Delta R.T.: -0.001 min
Response: 945750915
Conc: 77.29 ng/ml

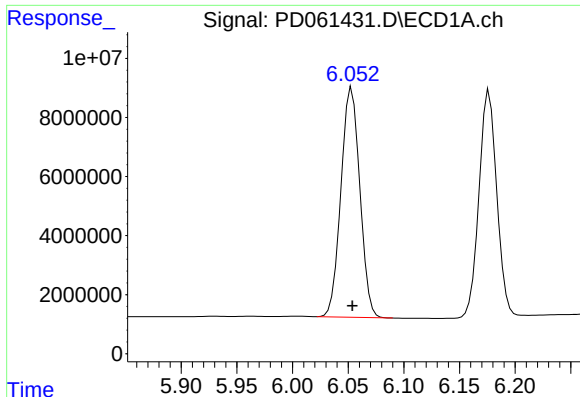

#14 Endrin


R.T.: 6.053 min
Delta R.T.: 0.000 min
Response: 91845272
Conc: 79.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

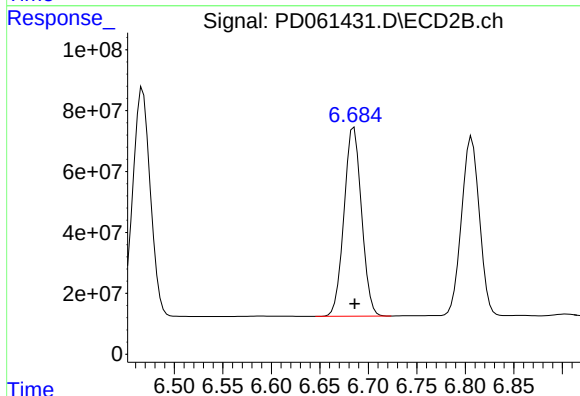


#14 Endrin

R.T.: 6.685 min
Delta R.T.: 0.000 min
Response: 779065985
Conc: 77.30 ng/ml

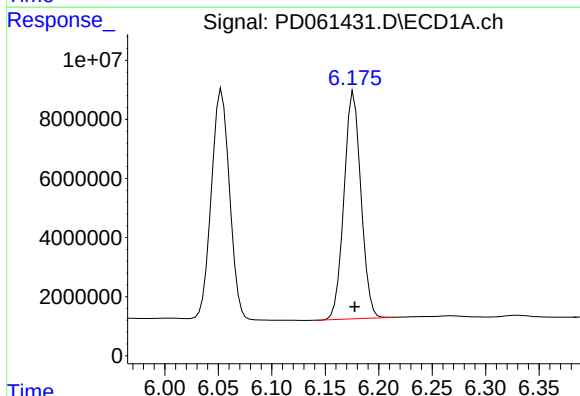


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 84892626
Conc: 81.14 ng/ml

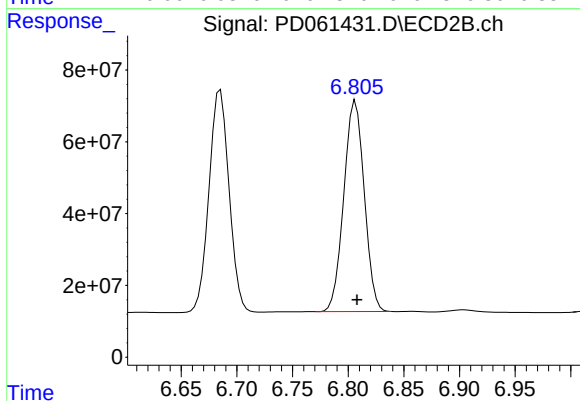

#16 4,4'-DDD


R.T.: 6.807 min
Delta R.T.: -0.001 min
Response: 752908914
Conc: 77.56 ng/ml

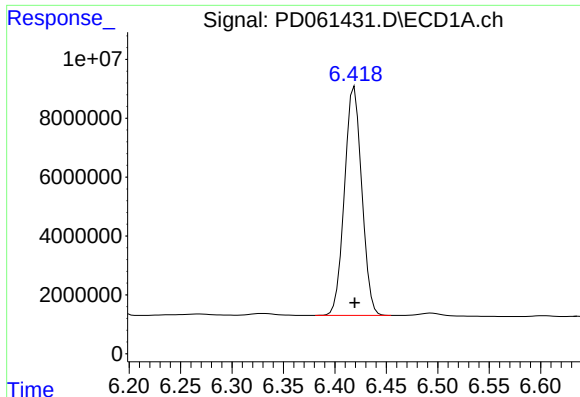

#17 4,4'-DDT


R.T.: 6.419 min
Delta R.T.: 0.000 min
Response: 91005069
Conc: 82.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

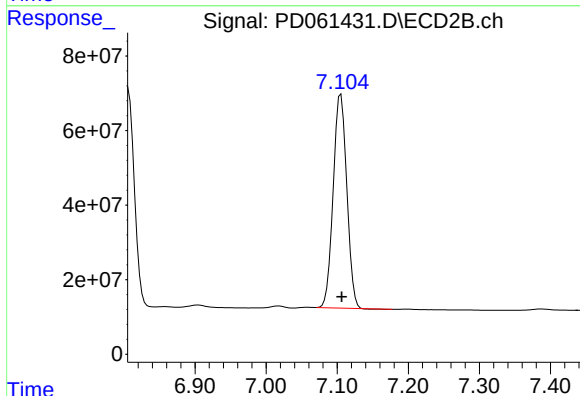


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: -0.001 min
Response: 762046621
Conc: 78.54 ng/ml

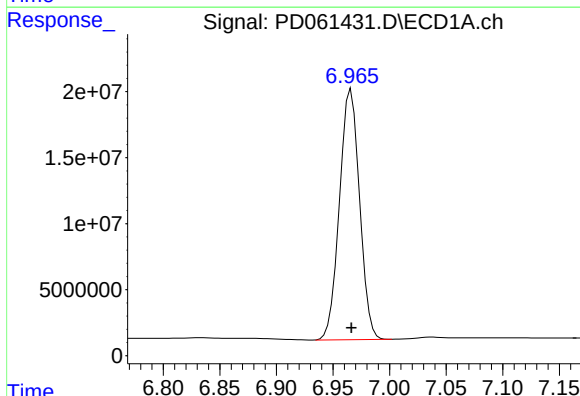


#20 Methoxychlor

R.T.: 6.966 min
Delta R.T.: 0.000 min
Response: 234623698
Conc: 386.11 ng/ml

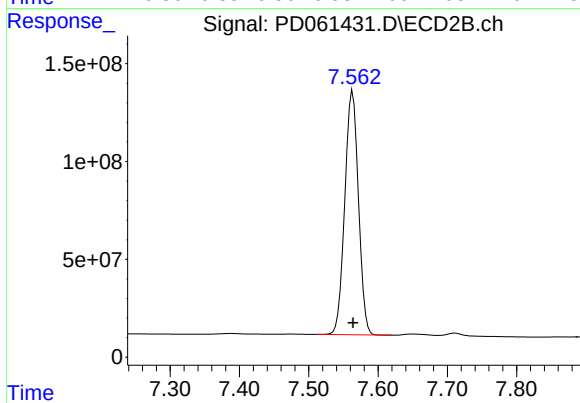

#20 Methoxychlor


R.T.: 7.563 min
Delta R.T.: 0.000 min
Response: 1708345333
Conc: 374.20 ng/ml

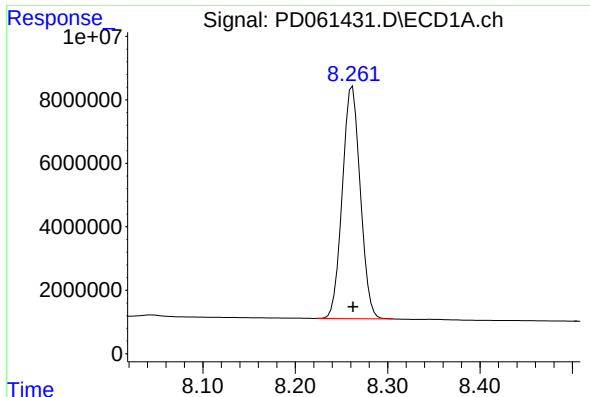

#27 Decachlorobiphenyl

R.T.: 8.262 min
Delta R.T.: 0.000 min
Response: 98944722
Conc: 75.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

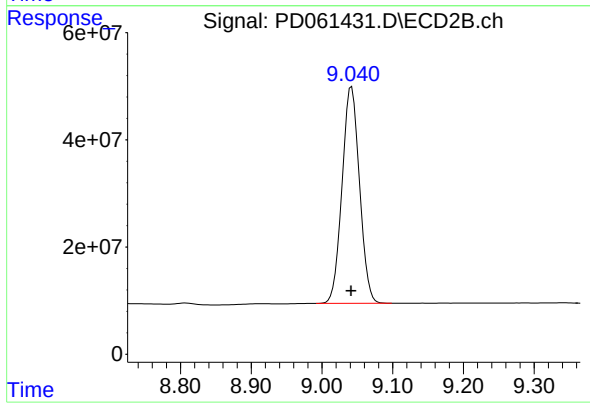

#27 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 692160271
Conc: 73.85 ng/ml