

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
 Data File : PD061432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 20:20
 Operator : DD\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 05:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:11:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.983	34814851	357.9E6	38.712	38.820
27)	SA Decachlor...	8.262	9.043	100.4E6	709.8E6	74.727	73.719
Target Compounds							
5)	MB Aldrin	4.765	5.469	51652973	514.8E6	40.066	38.733
6)	B beta-BHC	4.461	4.825	24089590	222.8E6	37.077	38.772
7)	B delta-BHC	4.667	5.042	53368146	508.8E6	40.350	38.486
8)	B Heptachlo...	5.209	5.855	49958226	457.2E6	39.231	38.535
10)	B trans-Chl...	5.437	6.088	52372461	496.0E6	39.450	38.642
11)	B cis-Chlor...	5.496	6.161	51140933	469.7E6	39.345	38.577
12)	B 4,4'-DDE	5.659	6.318	102.3E6	951.3E6	81.556	77.449
15)	B Endosulfa...	6.327	6.894	88260853	752.3E6	78.686	75.932
18)	B Endrin al...	6.495	7.018	75117646	645.4E6	77.673	76.381
19)	B Endosulfa...	6.709	7.241	88963113	749.8E6	78.171	76.492
21)	B Endrin ke...	7.203	7.712	103.7E6	736.0E6	78.712	75.676

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030421\
Data File : PD061432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 20:20
Operator : DD\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 05:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:11:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

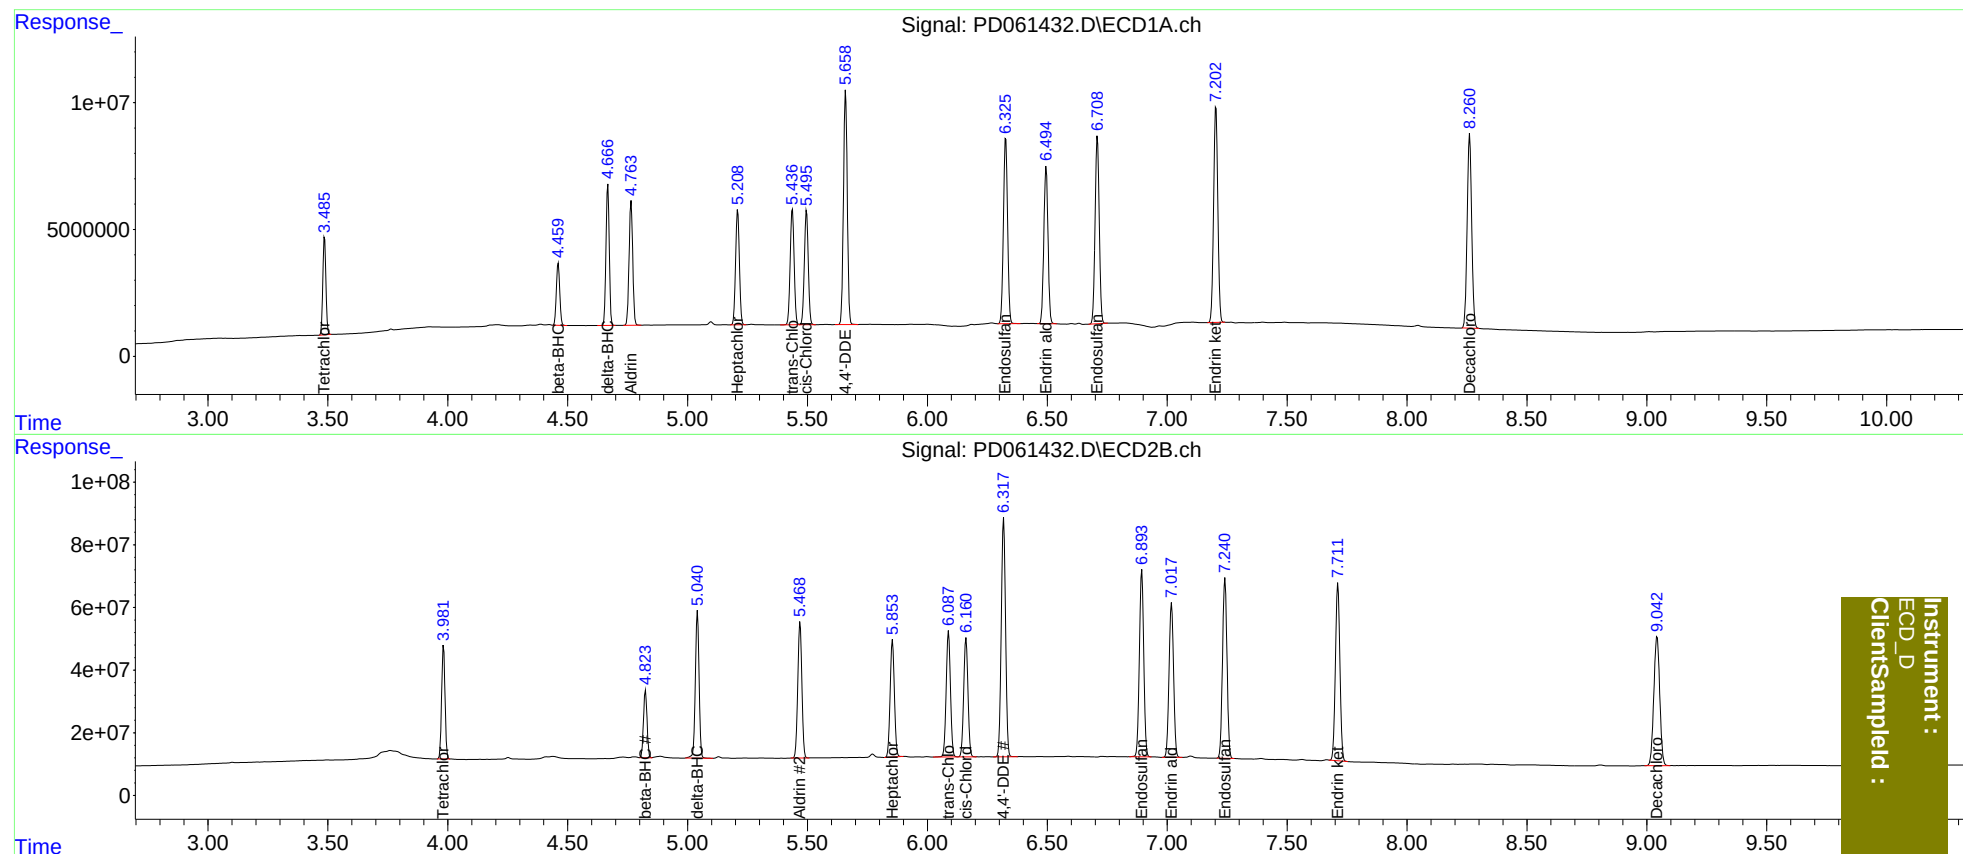


Instrument :
ECD_D
ClientSampled :

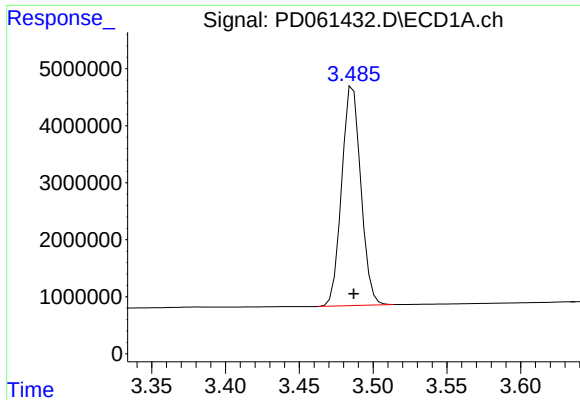

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 34814851
Conc: 38.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

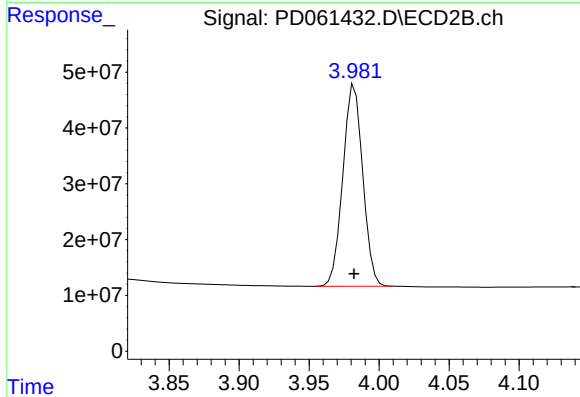


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 357919823
Conc: 38.82 ng/ml

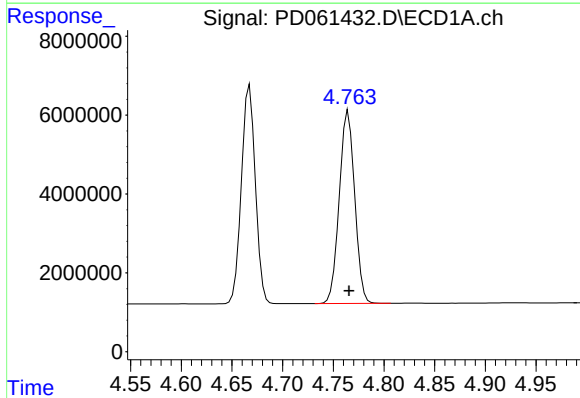


#5 Aldrin

R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 51652973
Conc: 40.07 ng/ml

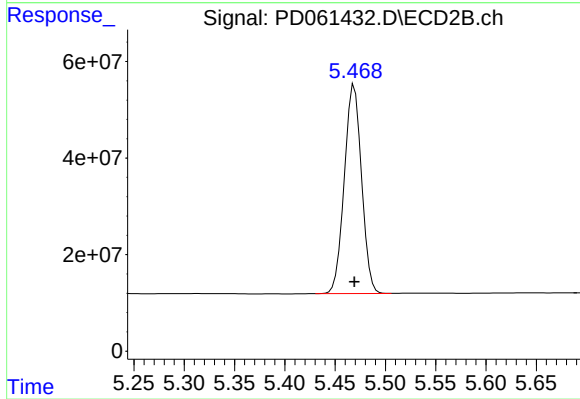

#5 Aldrin


R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 514799220
Conc: 38.73 ng/ml

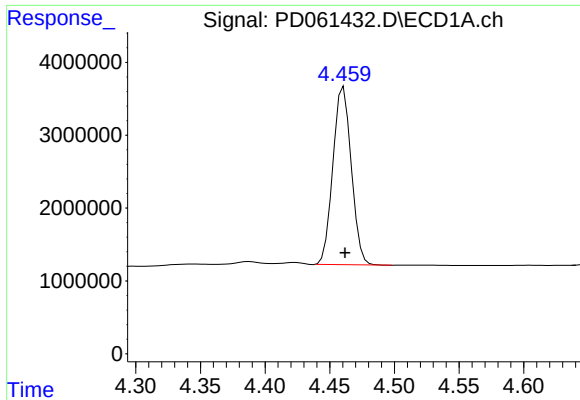

#6 beta-BHC


R.T.: 4.461 min
Delta R.T.: -0.001 min
Response: 24089590
Conc: 37.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

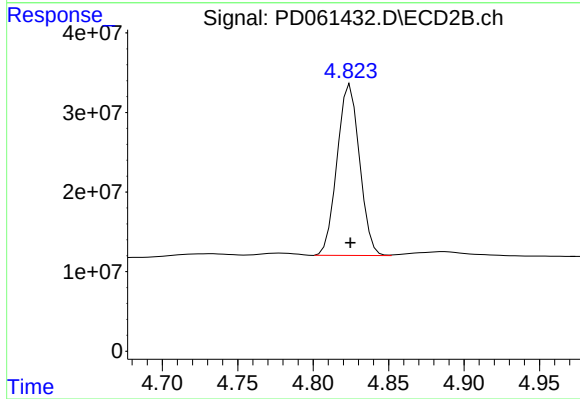


#6 beta-BHC

R.T.: 4.825 min
Delta R.T.: 0.000 min
Response: 222808624
Conc: 38.77 ng/ml

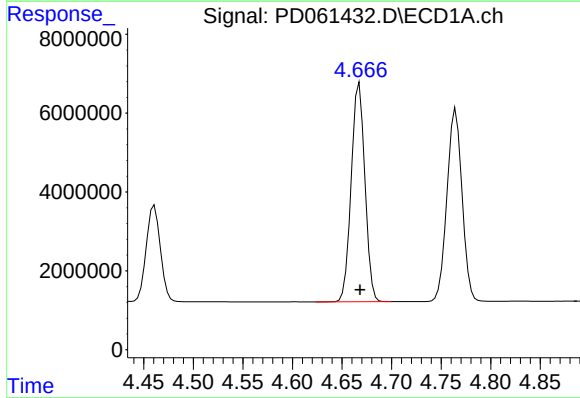


#7 delta-BHC

R.T.: 4.667 min
Delta R.T.: 0.000 min
Response: 53368146
Conc: 40.35 ng/ml

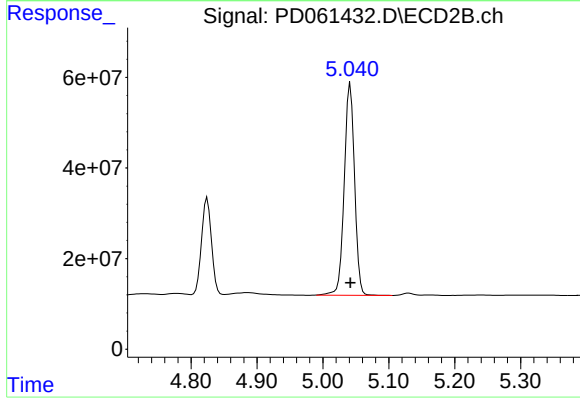

#7 delta-BHC


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 508838509
Conc: 38.49 ng/ml

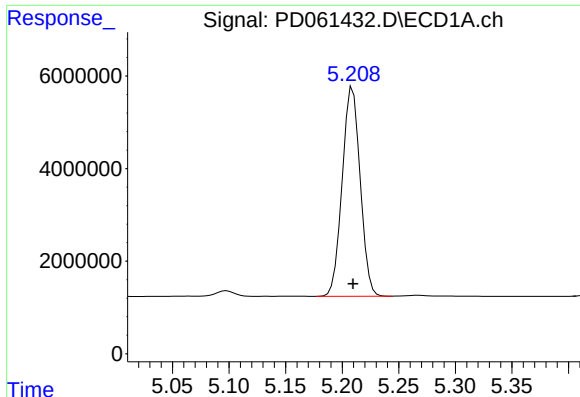

#8 Heptachlor epoxide


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 49958226
Conc: 39.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

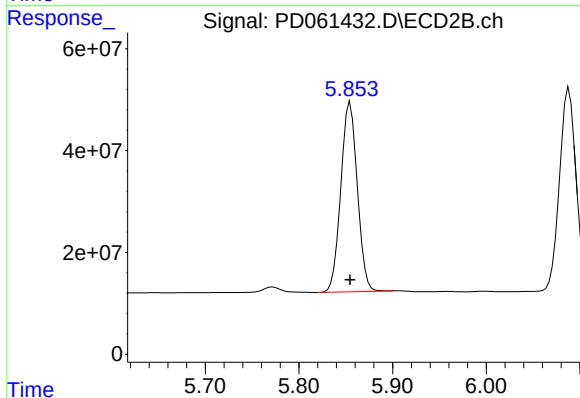


#8 Heptachlor epoxide

R.T.: 5.855 min
Delta R.T.: 0.000 min
Response: 457197732
Conc: 38.54 ng/ml

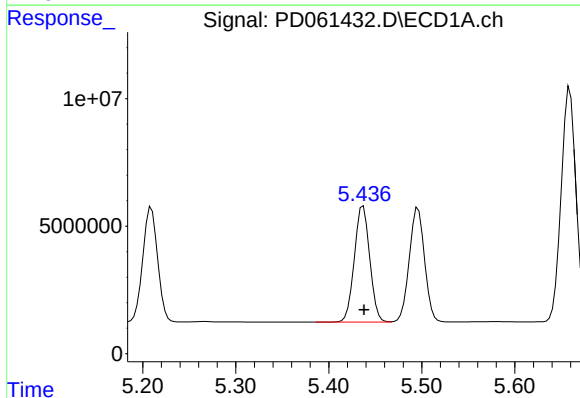


#10 trans-Chlordane

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 52372461
Conc: 39.45 ng/ml

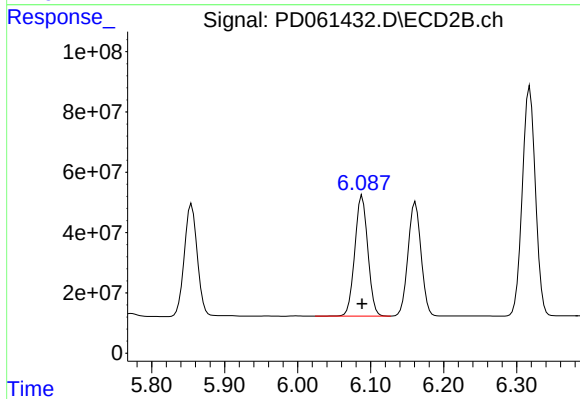

#10 trans-Chlordane


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 496009667
Conc: 38.64 ng/ml

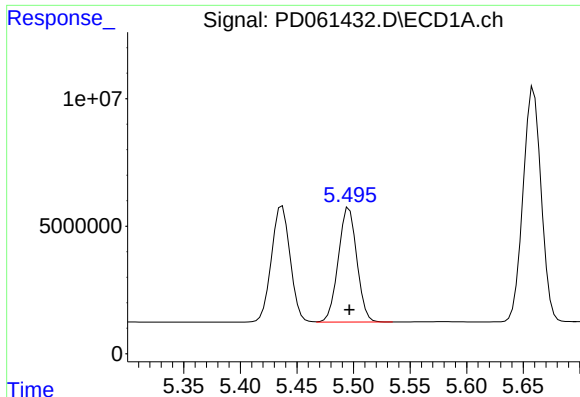

#11 cis-Chlordane


R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 51140933
Conc: 39.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

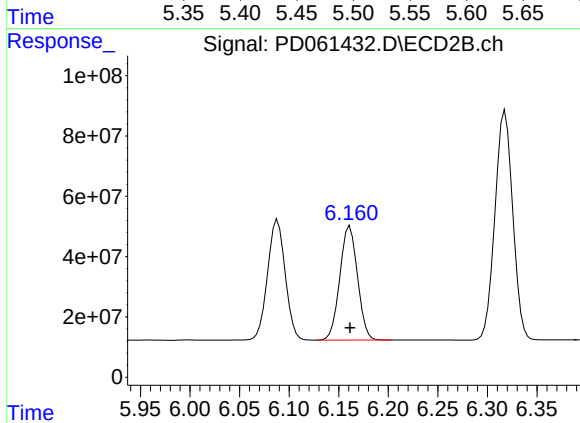


#11 cis-Chlordane

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 469659537
Conc: 38.58 ng/ml

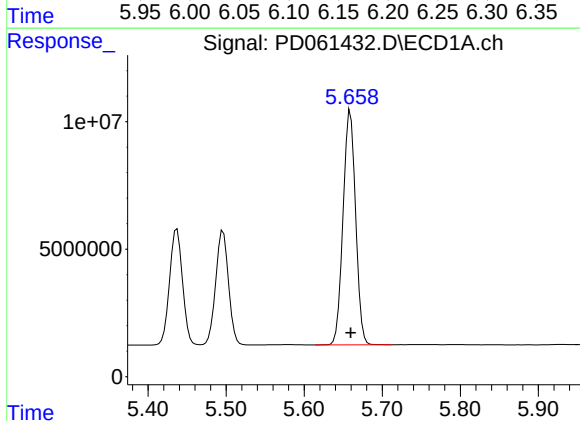


#12 4,4'-DDE

R.T.: 5.659 min
Delta R.T.: 0.000 min
Response: 102313944
Conc: 81.56 ng/ml

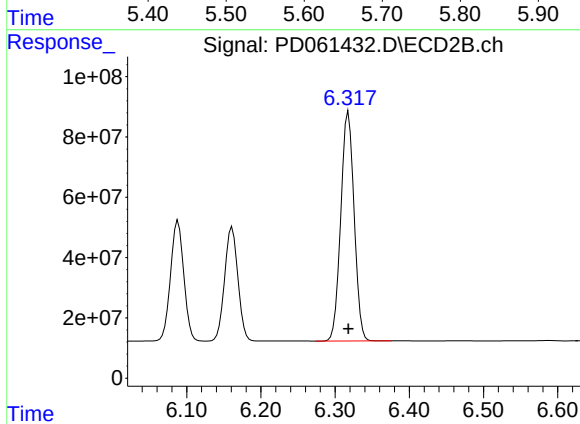

#12 4,4'-DDE


R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 951299811
Conc: 77.45 ng/ml

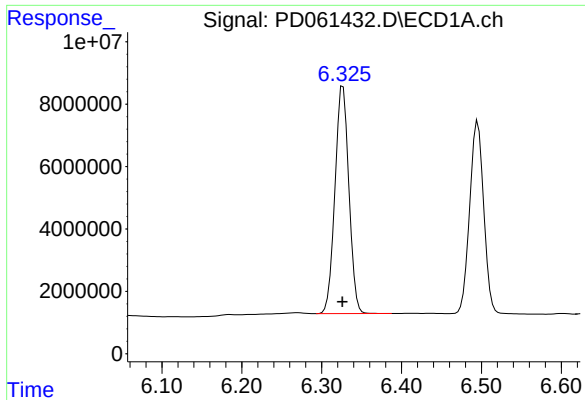

#15 Endosulfan II


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 88260853
Conc: 78.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

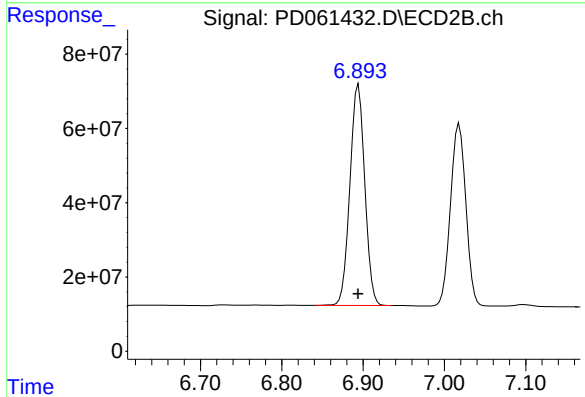


#15 Endosulfan II

R.T.: 6.894 min
Delta R.T.: 0.000 min
Response: 752260825
Conc: 75.93 ng/ml

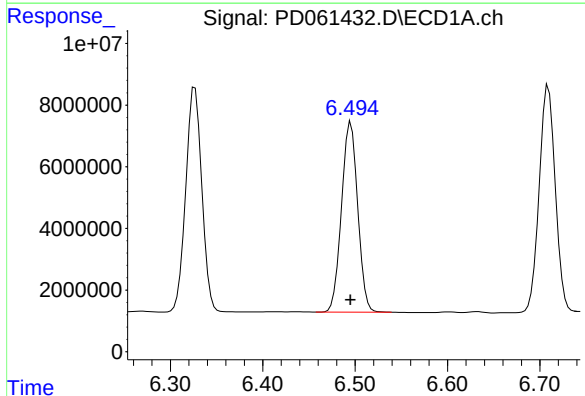


#18 Endrin aldehyde

R.T.: 6.495 min
Delta R.T.: 0.000 min
Response: 75117646
Conc: 77.67 ng/ml

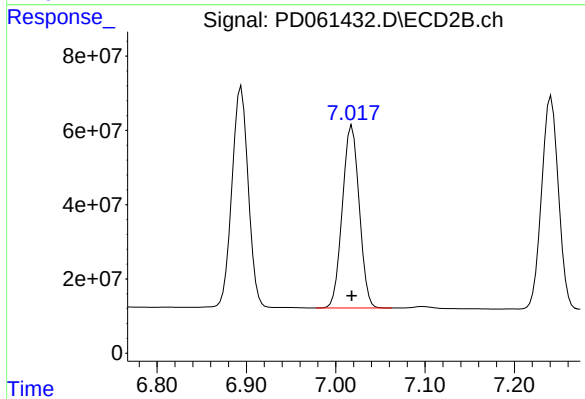

#18 Endrin aldehyde


R.T.: 7.018 min
Delta R.T.: 0.000 min
Response: 645373998
Conc: 76.38 ng/ml

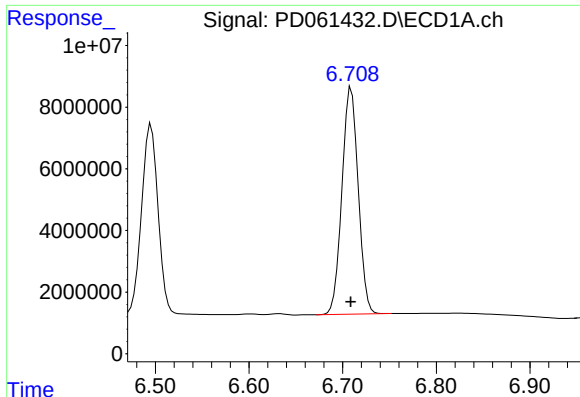

#19 Endosulfan Sulfate


R.T.: 6.709 min
Delta R.T.: 0.000 min
Response: 88963113
Conc: 78.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

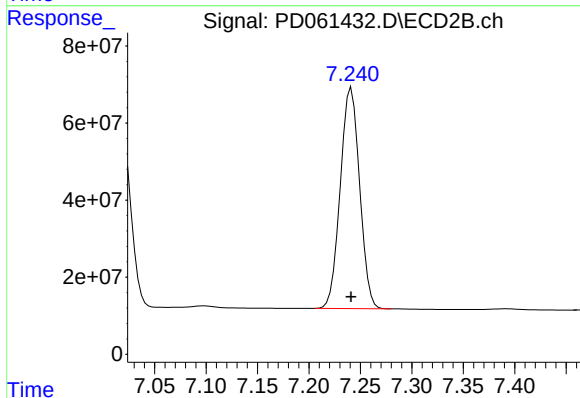


#19 Endosulfan Sulfate

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 749767859
Conc: 76.49 ng/ml

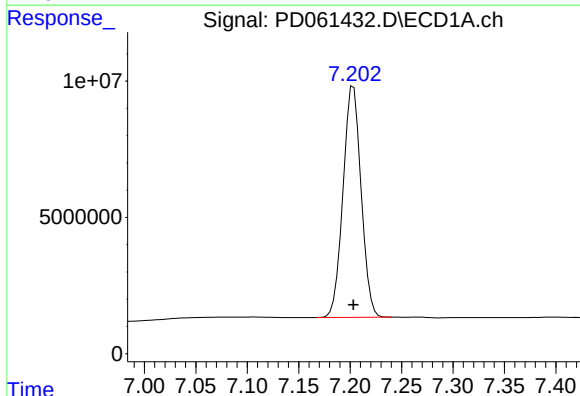


#21 Endrin ketone

R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 103749575
Conc: 78.71 ng/ml

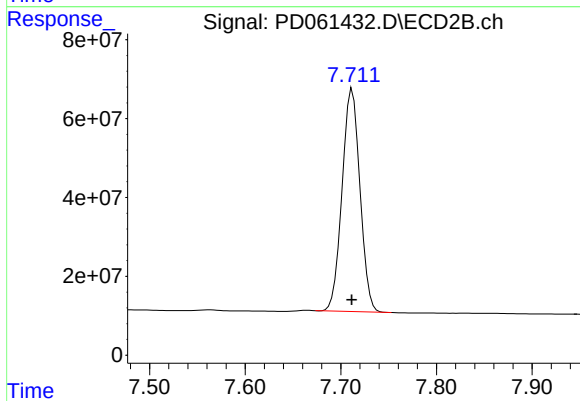

#21 Endrin ketone


R.T.: 7.712 min
Delta R.T.: 0.000 min
Response: 736019836
Conc: 75.68 ng/ml

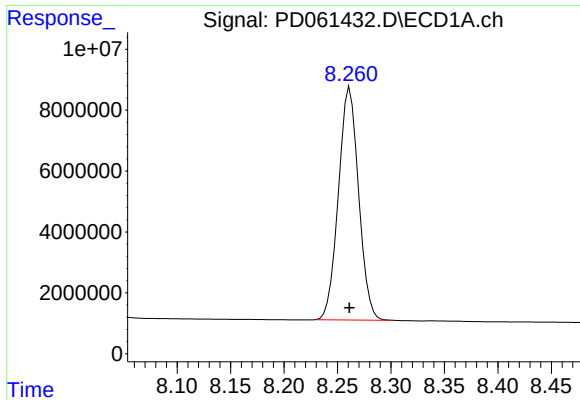

#27 Decachlorobiphenyl

R.T.: 8.262 min
Delta R.T.: 0.000 min
Response: 100351348
Conc: 74.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

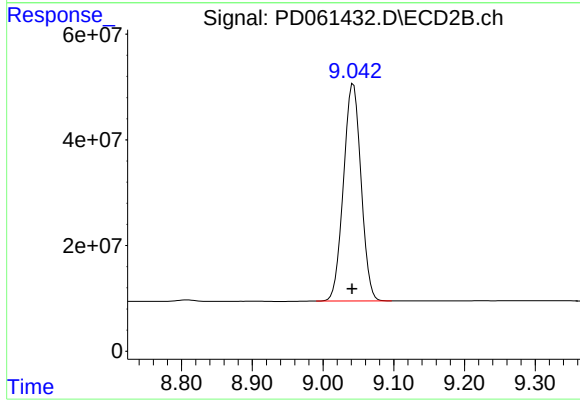

#27 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.002 min
Response: 709818220
Conc: 73.72 ng/ml