

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030422\
 Data File : PD068324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 18:19
 Operator : AR\AJ
 Sample : N1746-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/04/2022
 Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:12:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.177	16947950	94879302	14.458	9.885 #
28)	SA Decachlor...	8.205	9.372	20642090	50305985	17.738	8.485m#
Target Compounds							
10)	B gamma-Chl...	5.395	6.325	15837969	46826371	10.639m	4.428m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030422\
Data File : PD068324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 18:19
Operator : AR\AJ
Sample : N1746-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:12:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

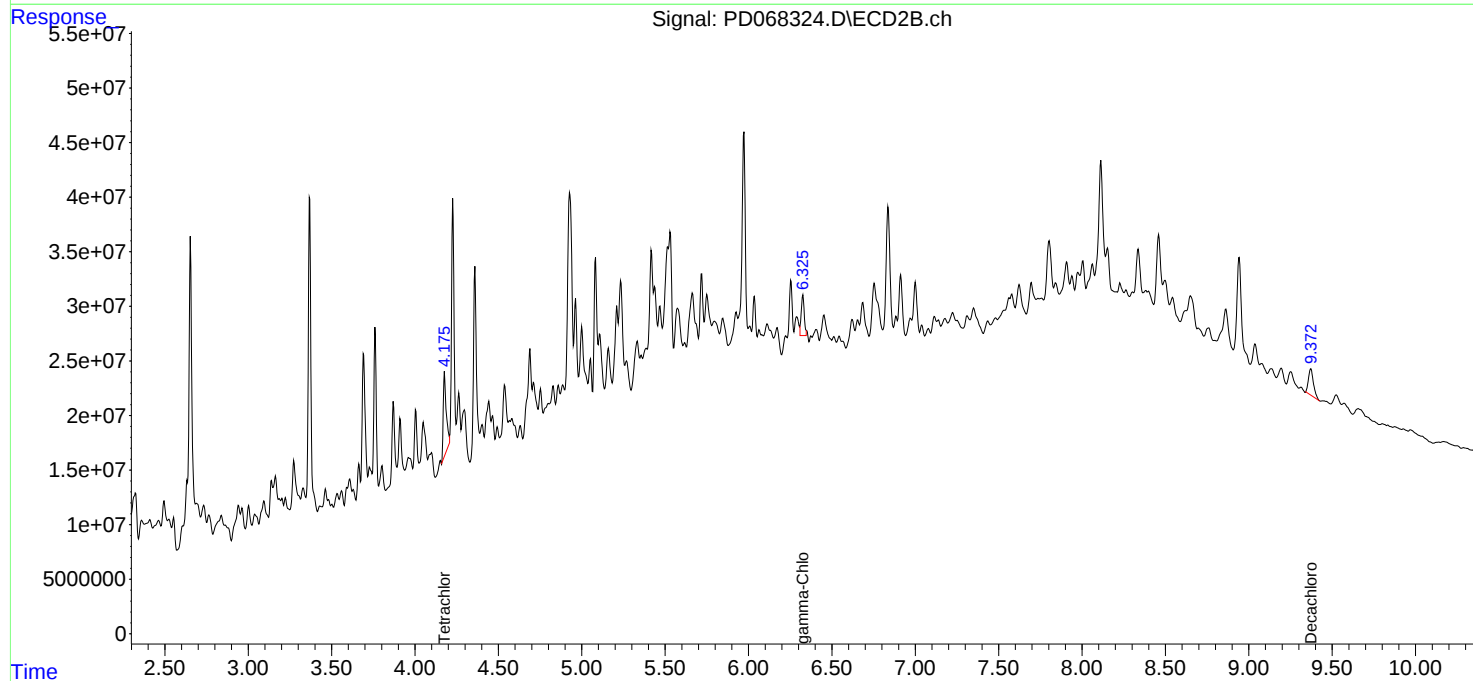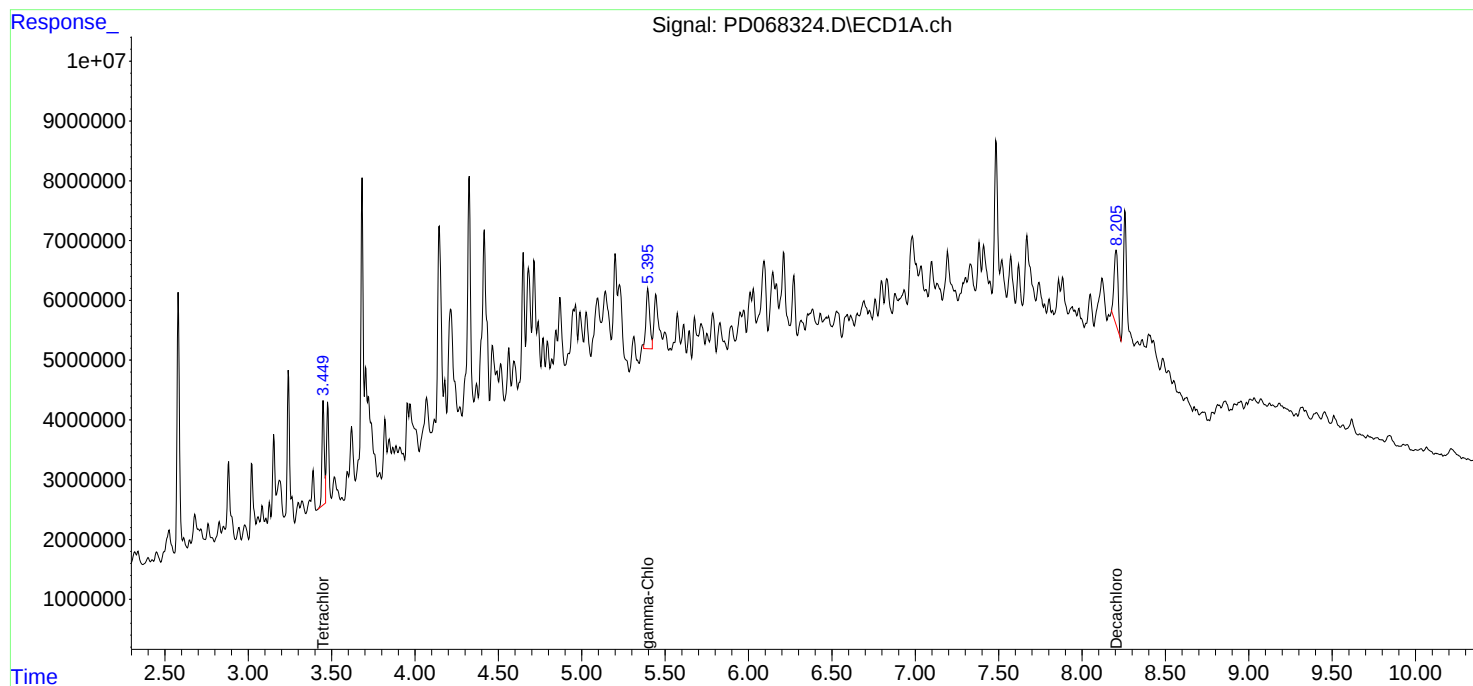

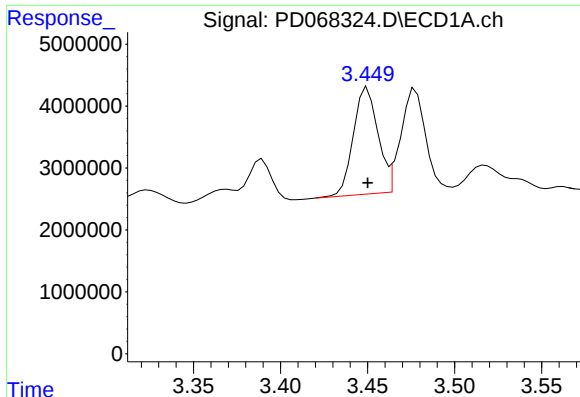


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 16947950
Conc: 14.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

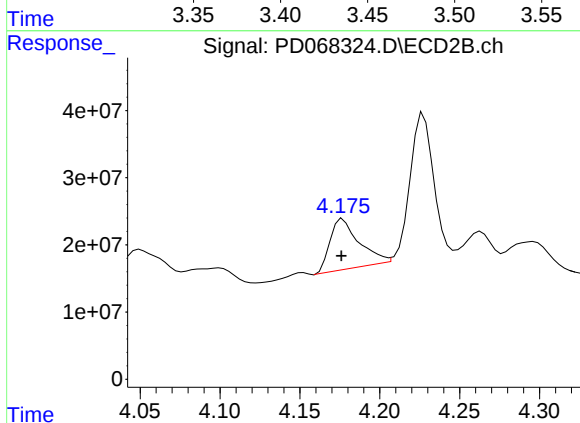


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: 0.001 min
Response: 94879302
Conc: 9.89 ng/ml

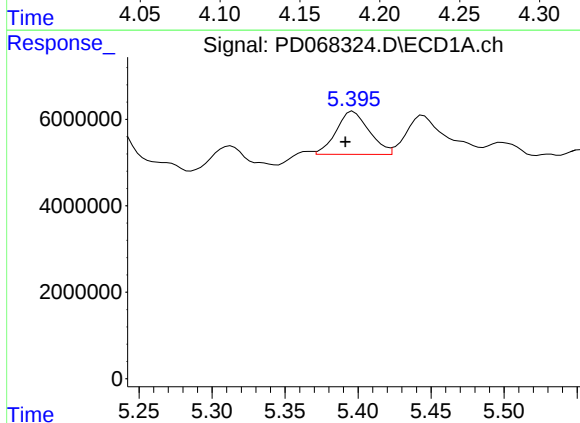


#10 gamma-Chlordane

R.T.: 5.395 min
Delta R.T.: 0.004 min
Response: 15837969
Conc: 10.64 ng/ml m

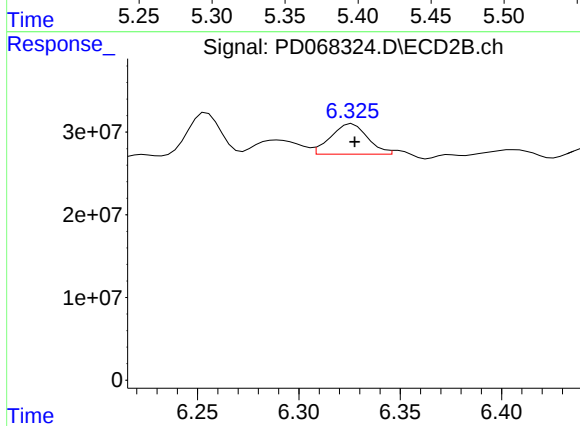

#10 gamma-Chlordane

R.T.: 6.325 min
Delta R.T.: -0.003 min
Response: 46826371
Conc: 4.43 ng/ml m

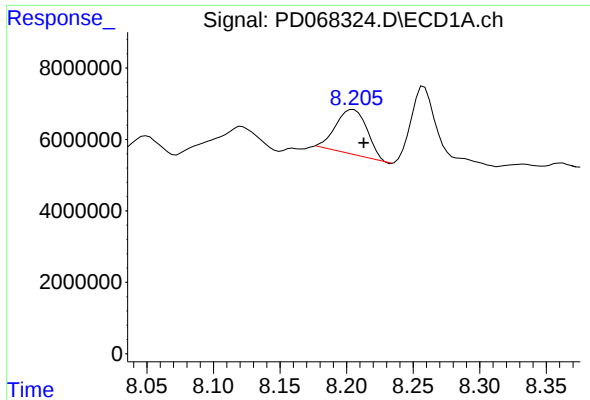


#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.008 min
Response: 20642090
Conc: 17.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

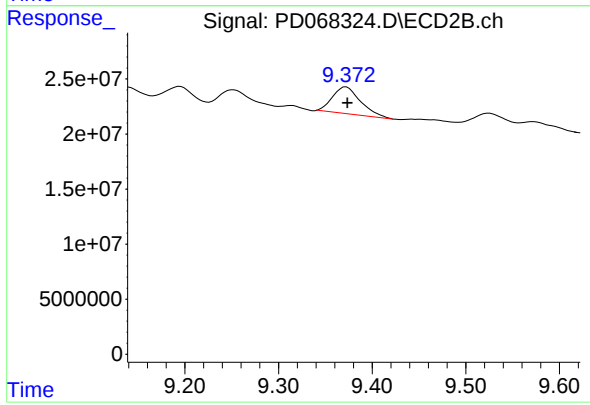

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.001 min
Response: 50305985
Conc: 8.49 ng/ml m