

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030424\
 Data File : PD081902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2024 11:30
 Operator : AR\AJ
 Sample : P1667-03MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSJ6MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/05/2024
 Supervised By :Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 11:59:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.792	17103595	29998556	12.510	12.237
27)	SA Decachlor...	9.106	7.925	22142842	31033222	11.477	12.510
Target Compounds							
2)	A alpha-BHC	4.021	3.293	126.8E6	204.4E6	54.312	53.163
3)	MA gamma-BHC...	4.354	3.622	118.4E6	182.7E6	51.255	50.439
4)	MA Heptachlor	4.947	3.962	124.5E6	179.1E6	50.757	50.491
5)	MB Aldrin	5.290	4.242	121.4E6	179.1E6	51.353	52.869
6)	B beta-BHC	4.549	3.917	52464004	79450465	50.484	47.021
7)	B delta-BHC	4.798	4.148	125.4E6	189.9E6	52.929	50.724
8)	B Heptachlo...	5.716	4.743	108.3E6	161.1E6	47.838	50.204
9)	A Endosulfan I	6.103	5.113	104.6E6	152.9E6	49.677	51.051
10)	B trans-Chl...	5.972	4.993	106.9E6	158.9E6	48.808	50.906
11)	B cis-Chlor...	6.052	5.057	109.8E6	159.1E6	48.742	49.670
12)	B 4,4'-DDE	6.223	5.244	214.1E6	308.8E6	99.720	104.424m
13)	MA Dieldrin	6.378	5.377	225.6E6	331.2E6	101.584	100.845
14)	MA Endrin	6.609	5.650	185.6E6	286.7E6	98.903	99.800m
15)	B Endosulfa...	6.827	5.945	193.7E6	286.9E6	100.333	101.632
16)	A 4,4'-DDD	6.740	5.798	167.9E6	252.6E6	101.112	100.242
17)	MA 4,4'-DDT	7.055	6.050	182.5E6	262.7E6	105.049	101.740
18)	B Endrin al...	6.957	6.124	132.9E6	194.8E6	88.991	89.912
19)	B Endosulfa...	7.191	6.345	184.1E6	268.2E6	100.548	99.967m
20)	A Methoxychlor	7.529	6.624	453.0E6	613.6E6	493.847	459.288
21)	B Endrin ke...	7.677	6.852	204.6E6	305.2E6	105.821	101.791

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030424\
Data File : PD081902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2024 11:30
Operator : AR\AJ
Sample : P1667-03MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 11:59:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

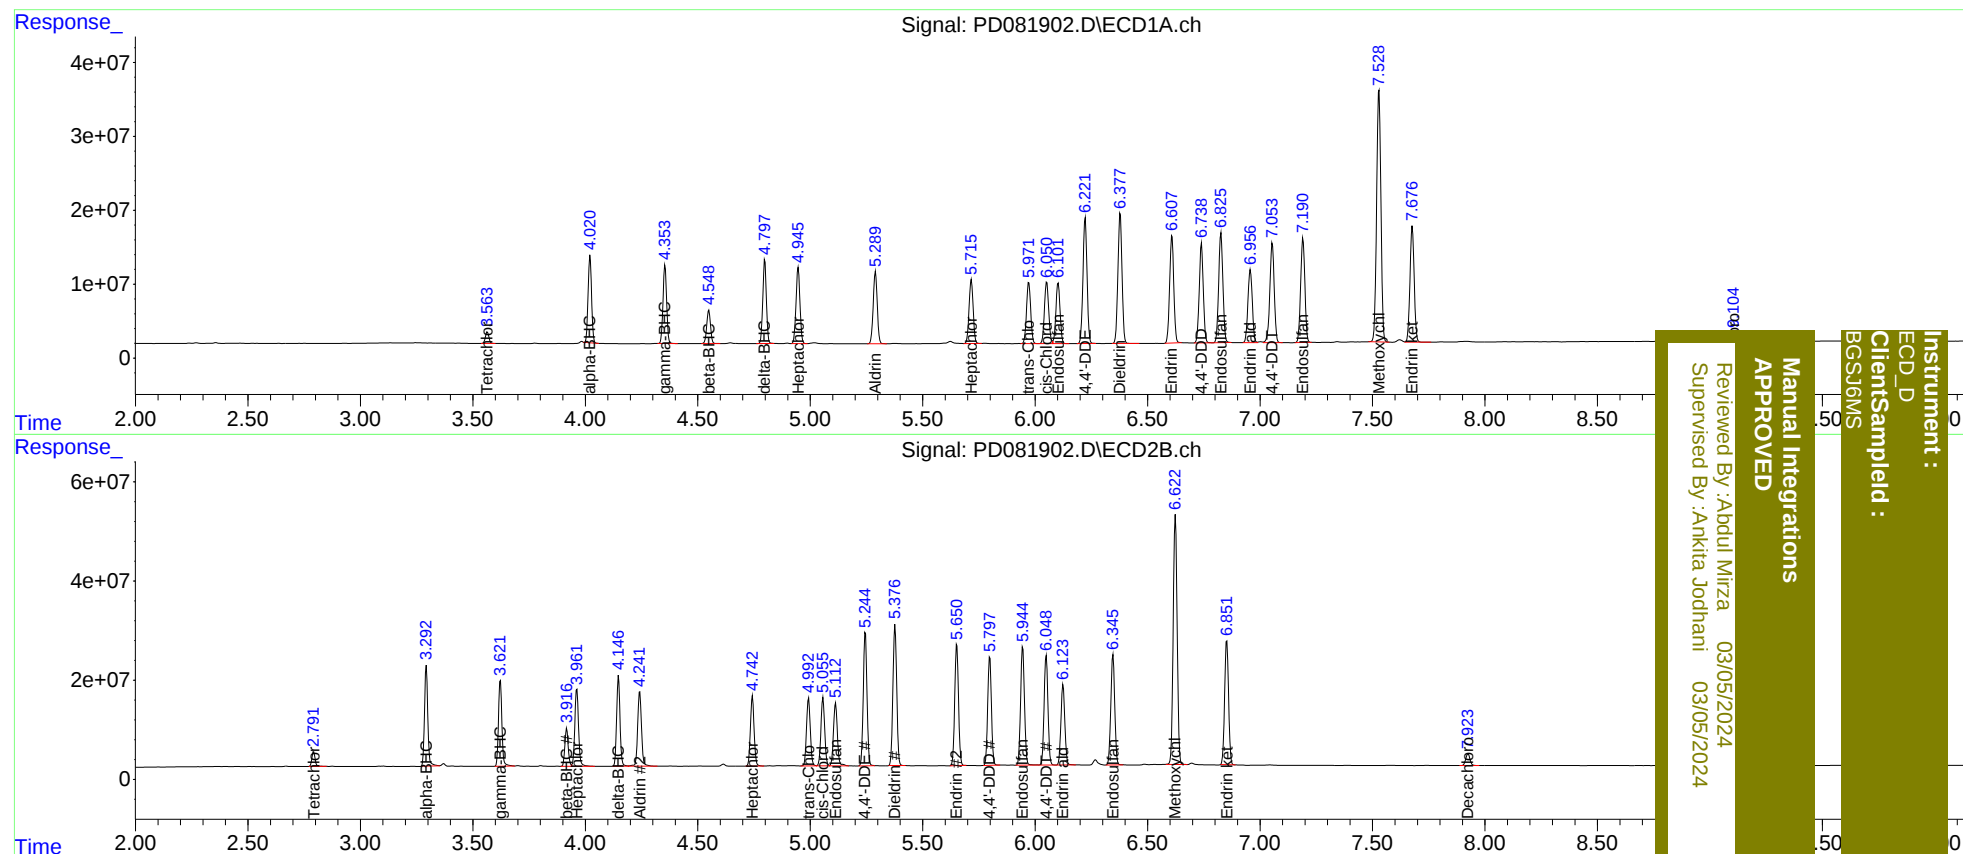

Instrument :
ECD_D
ClientSampled :
BGSJ6MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024