

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030519\
 Data File : PD051607.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2019 14:21
 Operator : AJ\SJ
 Sample : K1626-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 04:15:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	7963244	174.5E6	5.541	5.646
27)	SA Decachlor...	7.824	9.159	8524624	130.5E6	7.088	6.883
Target Compounds							
6)	B beta-BHC	0.000	4.939f	0 62882804	N.D.		3.169
8)	B Heptachlo...	0.000	5.918	0 57459023	N.D.		1.605
15)	B Endosulfa...	0.000	6.982	0 15485506	N.D.		0.564

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030519\
Data File : PD051607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2019 14:21
Operator : AJ\SJ
Sample : K1626-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 04:15:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

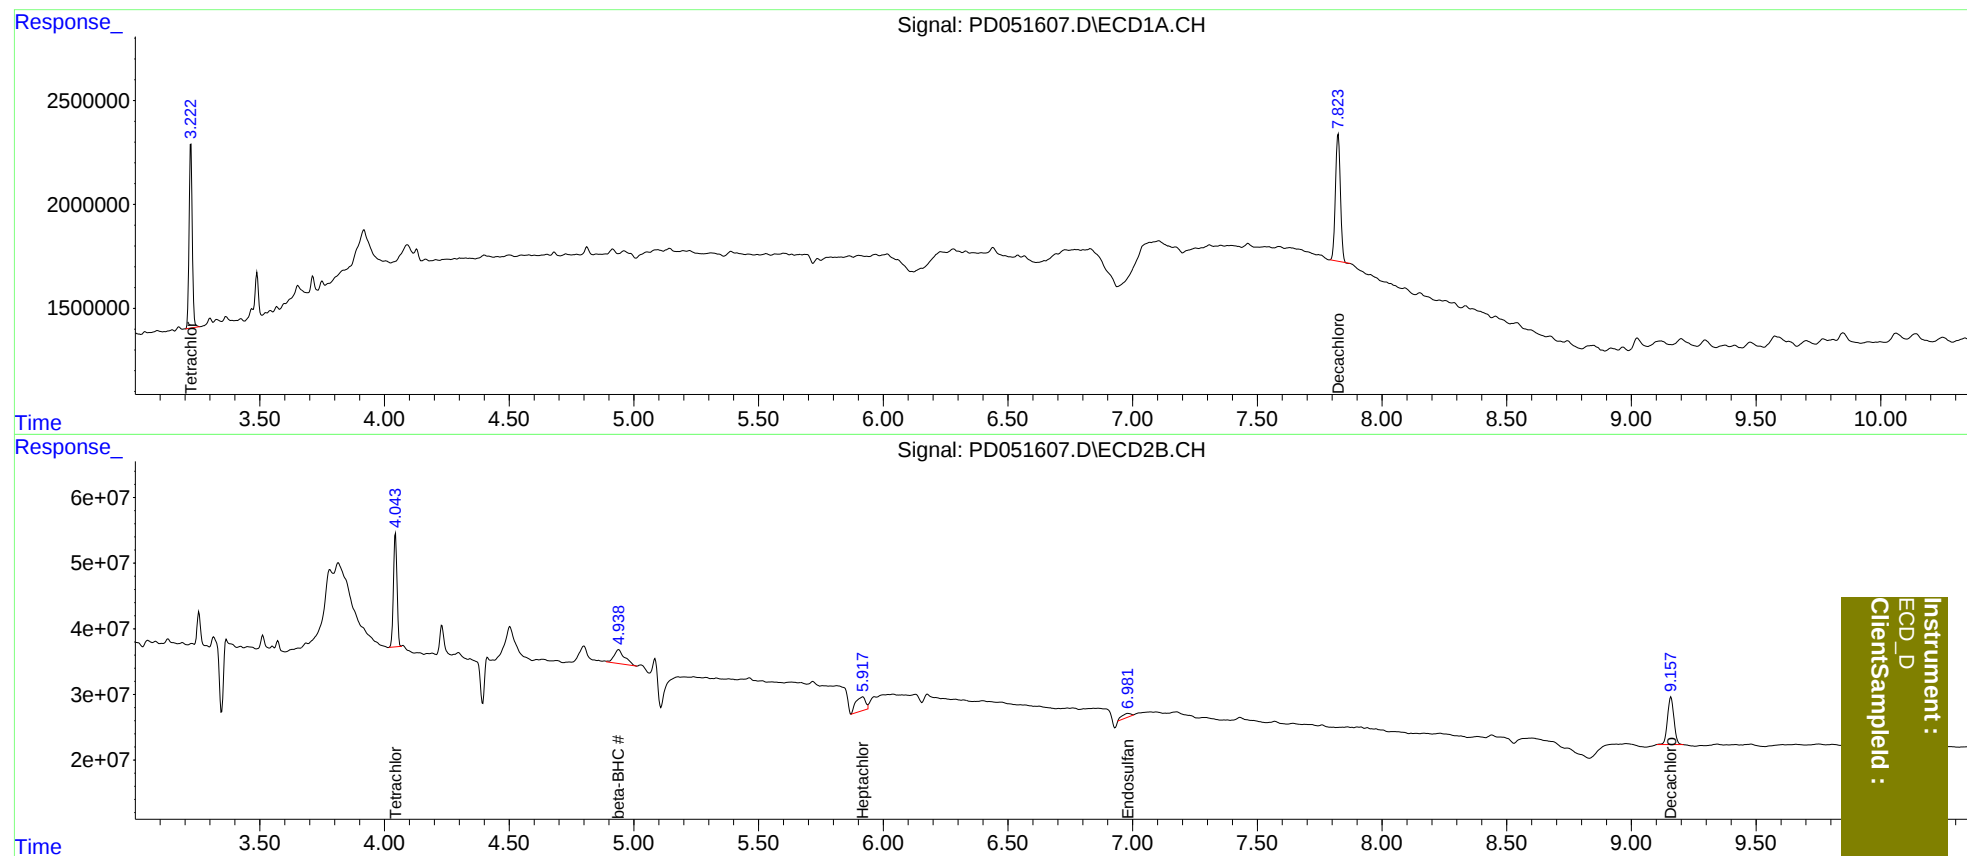


Instrument :
ECD_D
ClientSampled :

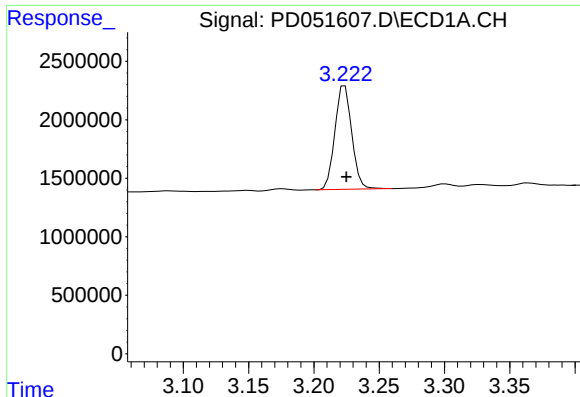

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 7963244
Conc: 5.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

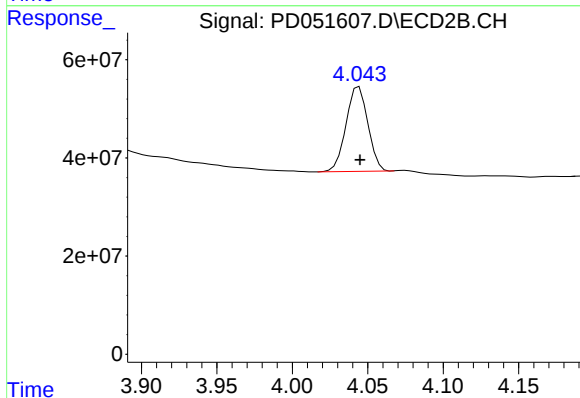


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 174451059
Conc: 5.65 ng/ml

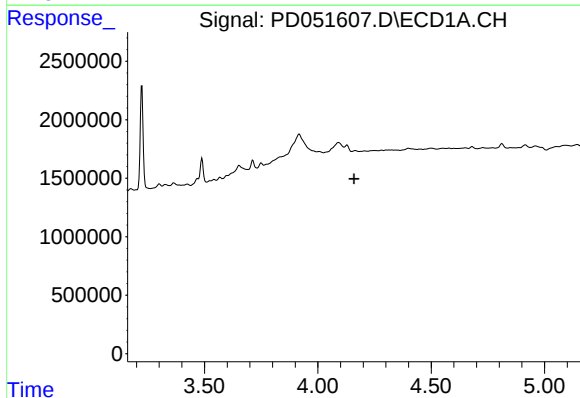


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

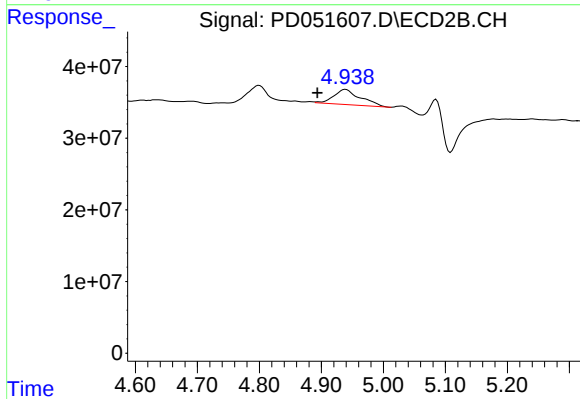

#6 beta-BHC


R.T.: 4.939 min
Delta R.T.: 0.045 min
Response: 62882804
Conc: 3.17 ng/ml

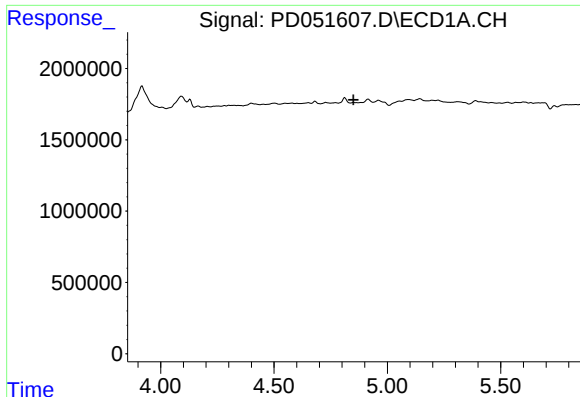

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

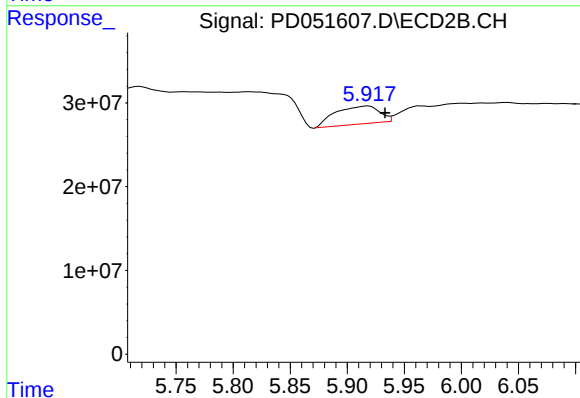


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.015 min
Response: 57459023
Conc: 1.60 ng/ml

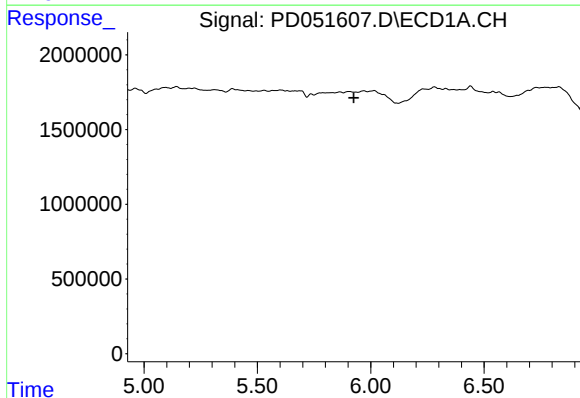


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

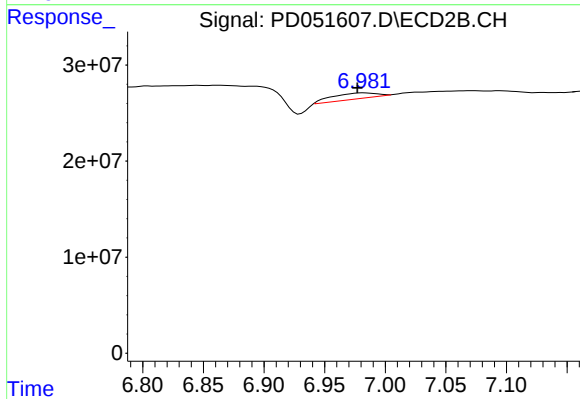

#15 Endosulfan II


R.T.: 6.982 min
Delta R.T.: 0.005 min
Response: 15485506
Conc: 0.56 ng/ml

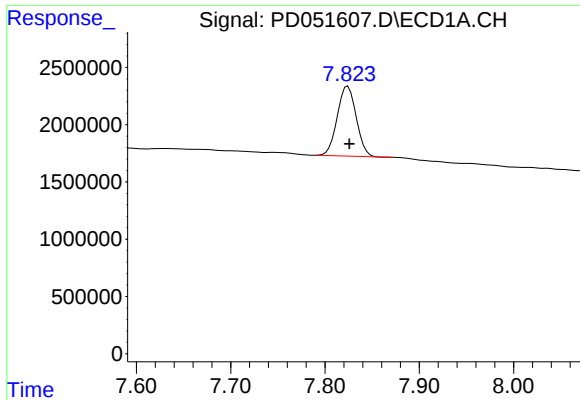

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: -0.002 min
Response: 8524624
Conc: 7.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

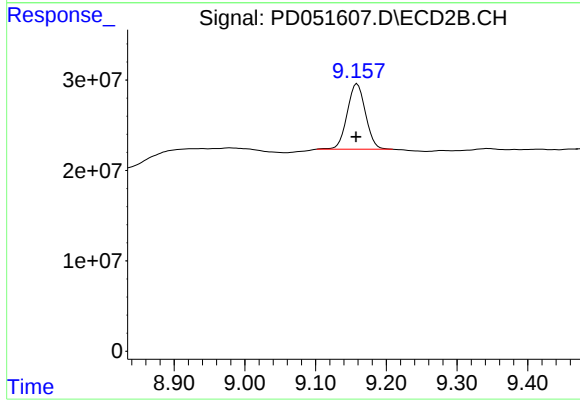

#27 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.002 min
Response: 130483415
Conc: 6.88 ng/ml