

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030521\
 Data File : PD061444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 11:21
 Operator : AR\AJ
 Sample : M1344-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:09:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 06:01:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:53:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.983	18107665	188.9E6	19.932	20.225
27)	SA Decachlor...	8.265	9.044	52720045	375.5E6	39.363	40.151
Target Compounds							
2)	A alpha-BHC	3.929	4.370	1316783	26267109	1.002	1.817m#
3)	MA gamma-BHC...	4.214	4.656	1577254	14112082	1.215	1.065
4)	MA Heptachlor	4.518	5.165	1055129	12743567	0.783	0.936
5)	MB Aldrin	4.768	5.470	1063654	13113798	0.824	0.989
6)	B beta-BHC	4.463	4.826	613628	4951987	0.929m	0.879
7)	B delta-BHC	4.671	5.042	1047743	16318578	0.790	1.162 #
8)	B Heptachlo...	5.213	5.855	1121647	16621994	0.878	1.367m#
9)	A Endosulfan I	5.554	6.212	1353849	10661224	1.125	0.936
10)	B trans-Chl...	5.440	6.090	1307033	11384896	0.972	0.882
11)	B cis-Chlor...	5.500	6.162	1179420	10873648	0.904	0.895
12)	B 4,4'-DDE	5.662	6.318	1111337	11237706	0.885	0.922
13)	MA Dieldrin	5.798	6.469	1025225	12620733	0.776	1.038 #
14)	MA Endrin	6.055	6.688	989857	9429681	0.856	0.928
15)	B Endosulfa...	6.330	6.895	1272801	15100768	1.115	1.541m#
16)	A 4,4'-DDD	6.181	6.807	863918	8510637	0.830	0.883m
17)	MA 4,4'-DDT	6.423	7.107	742916	11722363	0.669	1.204 #
18)	B Endrin al...	6.498	7.019	988468	9340472	1.016	1.104
19)	B Endosulfa...	6.713	7.242	1087500	8477500	0.943	0.867
20)	A Methoxychlor	6.969	7.563	387921	4321846	0.636m	0.948m#
21)	B Endrin ke...	7.206	7.712	1171136	12386551	0.887	1.292 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030521\
Data File : PD061444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 11:21
Operator : AR\AJ
Sample : M1344-01
Misc : PEST MDL 1 PPB
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 06:01:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:53:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

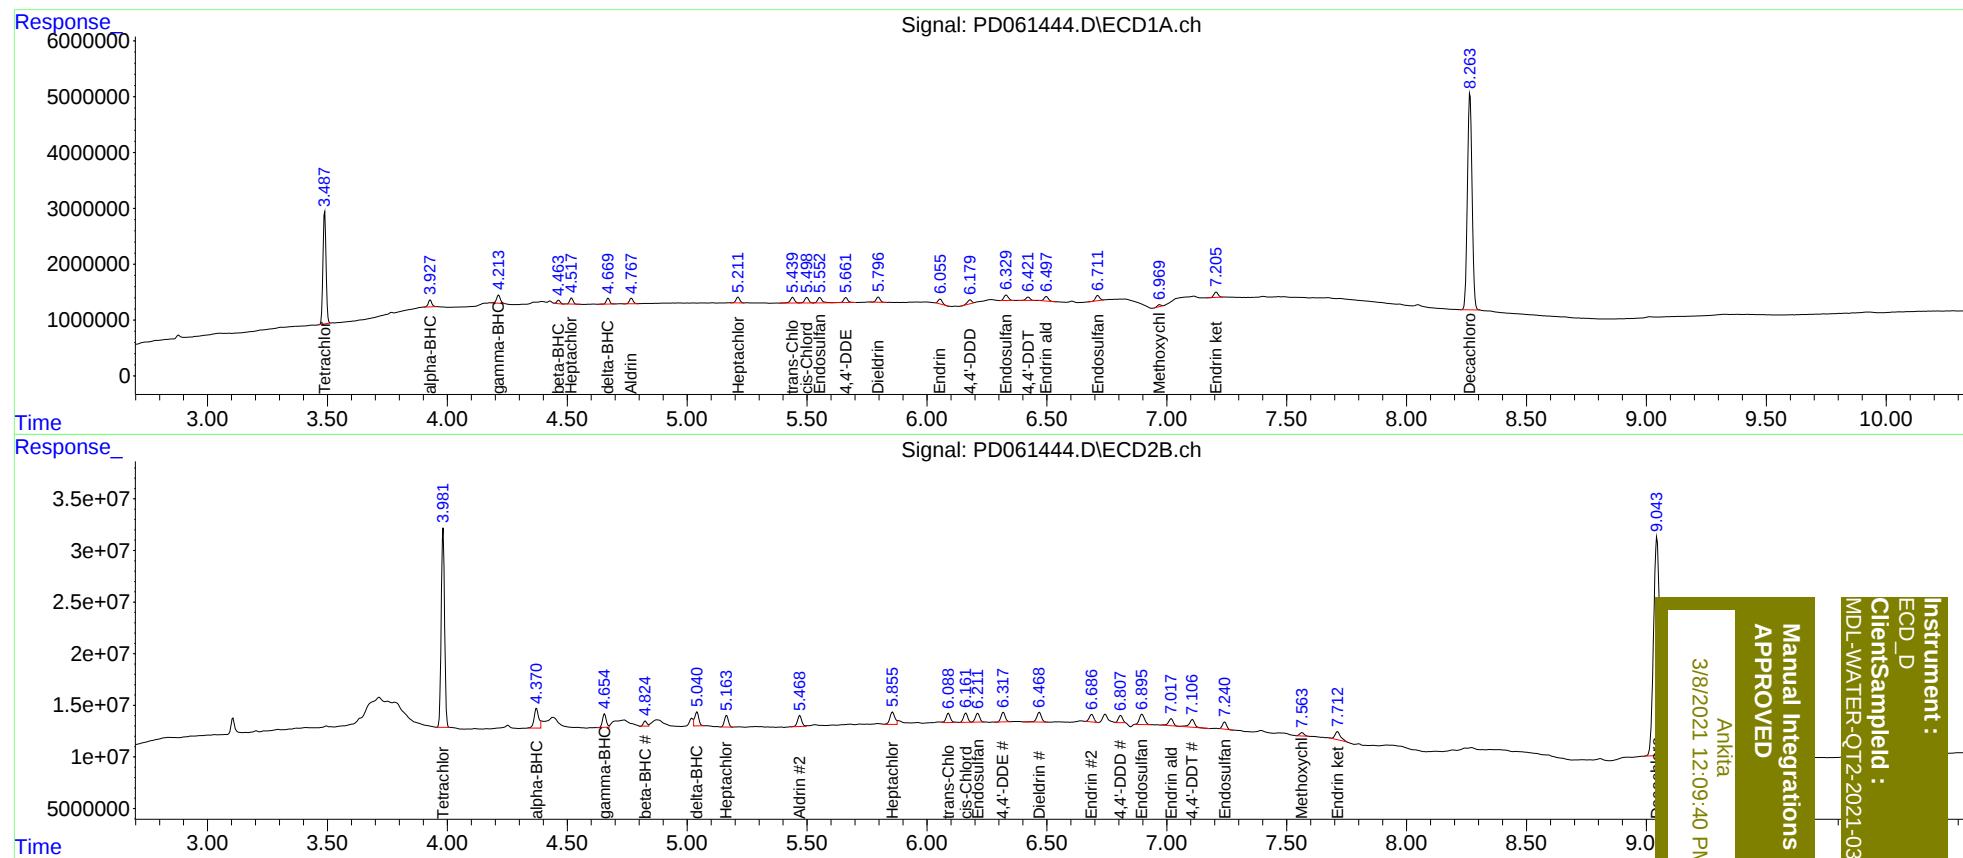

Manual Integrations
APPROVED

Ankita
3/8/2021 12:09:40 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT2-2021-03