

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030521\
 Data File : PD061445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 11:39
 Operator : AR\AJ
 Sample : M1344-01
 Misc : TOX MDL 100 PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 00:52:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:53:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	3.982	17346787	181.6E6	19.094	19.446
27)	SA Decachlor...	8.267	9.045	51144423	365.6E6	38.186	39.089
Target Compounds							
22)	Toxaphene-1	5.761	6.370	754175	5603272	83.403	95.466
23)	Toxaphene-2	5.923	6.659	662979	8617537	71.095	118.386 #
24)	Toxaphene-3	6.246	7.066	849348	9538131	78.449	92.841
25)	Toxaphene-4	6.365	7.143	1770591	26039649	75.827	92.291
26)	Toxaphene-5	7.100	7.642	3226094	10284101	122.163	84.497 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030521\
Data File : PD061445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 11:39
Operator : AR\AJ
Sample : M1344-01
Misc : TOX MDL 100 PPB
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 00:52:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:53:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

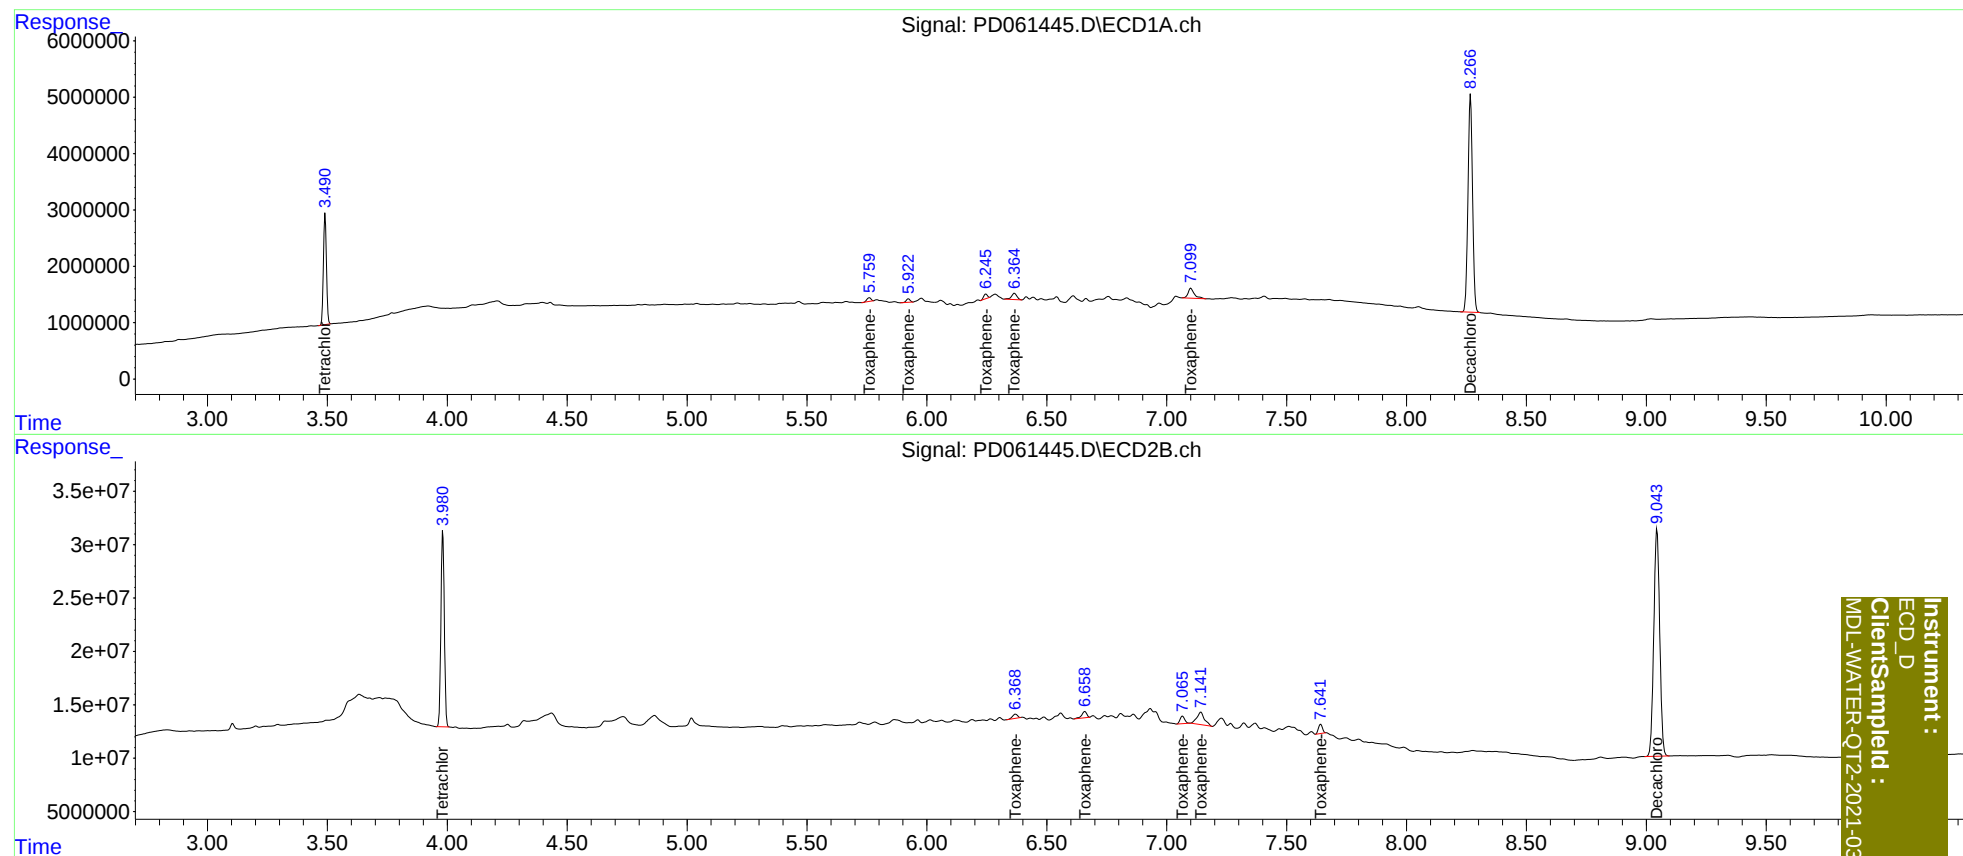

Instrument :
ECD_D
ClientSample :
MDL-WATER-QT2-2021-03