

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030524\
 Data File : PD081946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2024 10:39
 Operator : AR\AJ
 Sample : PB1594289BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK428

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 21:28:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.788	27988622	56962162	20.472	23.235
27)	SA Decachlor...	9.119	7.926	46269885	68715896	23.982	27.700
Target Compounds							
3)	MA gamma-BHC...	0.000	3.635	0	226498	N.D.	<MDL
4)	MA Heptachlor	0.000	3.954	0	66140	N.D.	<MDL
5)	MB Aldrin	0.000	4.257	0	66130	N.D.	<MDL
6)	B beta-BHC	0.000	3.954f	0	66140	N.D.	<MDL
7)	B delta-BHC	4.800	0.000	1257284	0	0.531	N.D. #
14)	MA Endrin	0.000	5.624	0	83639	N.D.	<MDL
15)	B Endosulfa...	0.000	5.905f	0	320814	N.D.	0.114
17)	MA 4,4'-DDT	0.000	6.047	0	34920	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030524\
Data File : PD081946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2024 10:39
Operator : AR\AJ
Sample : PB1594289BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 21:28:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

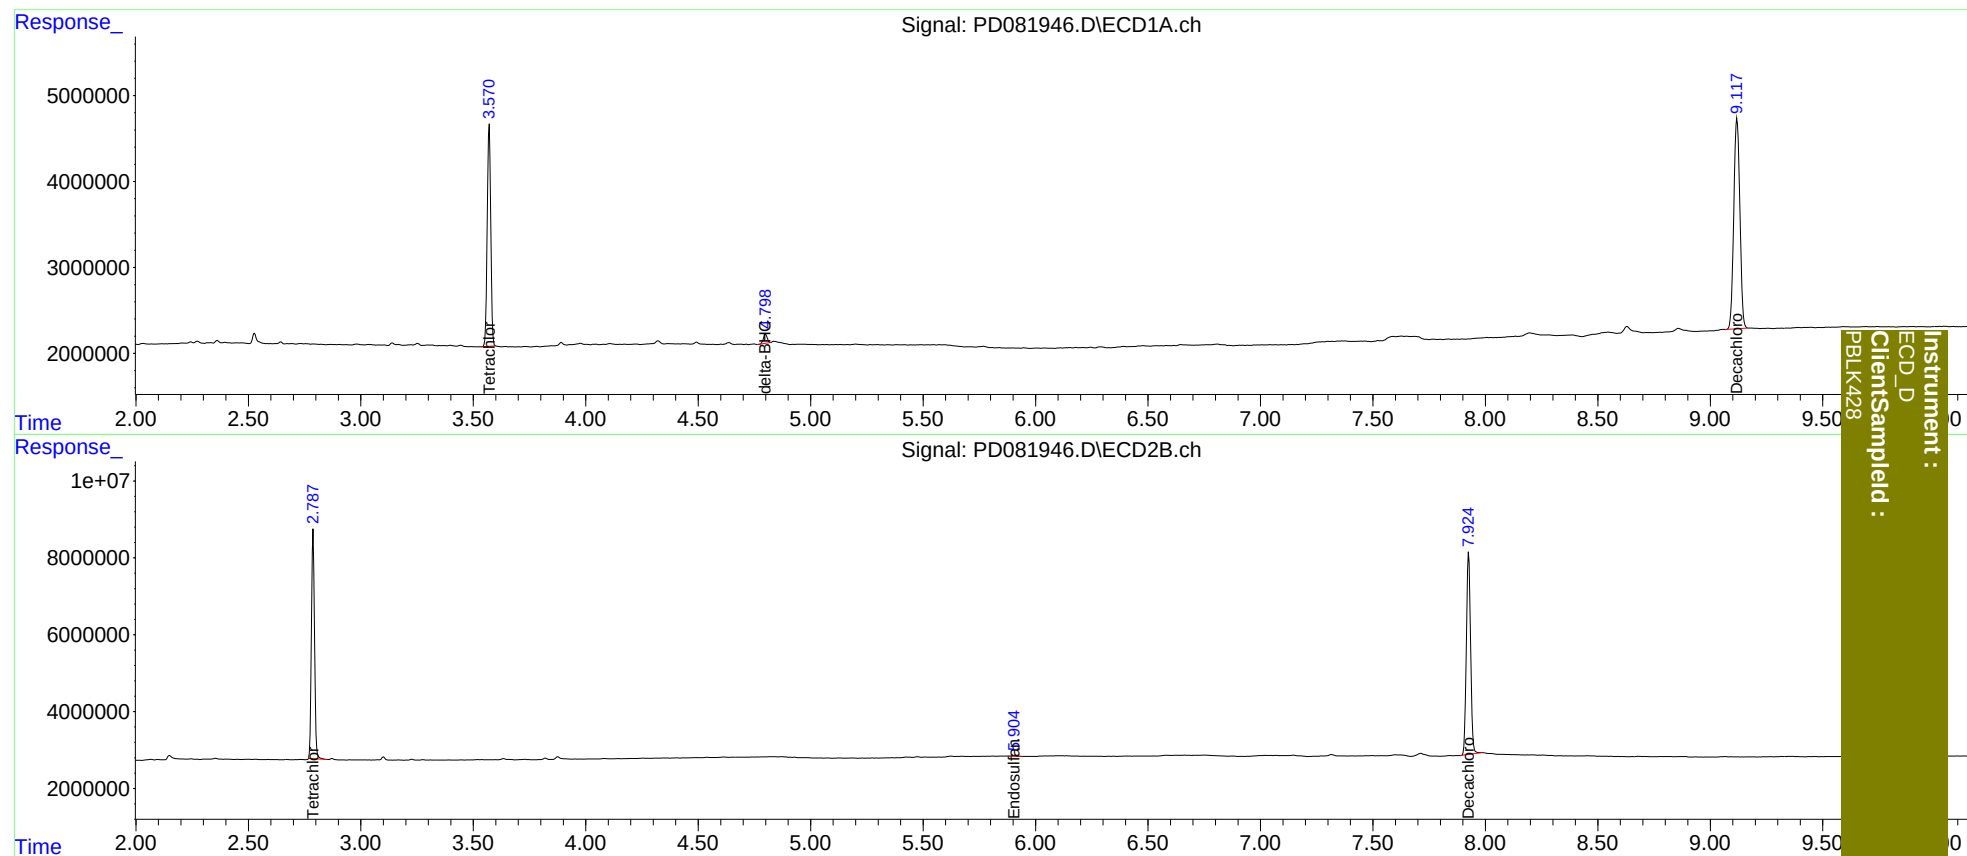


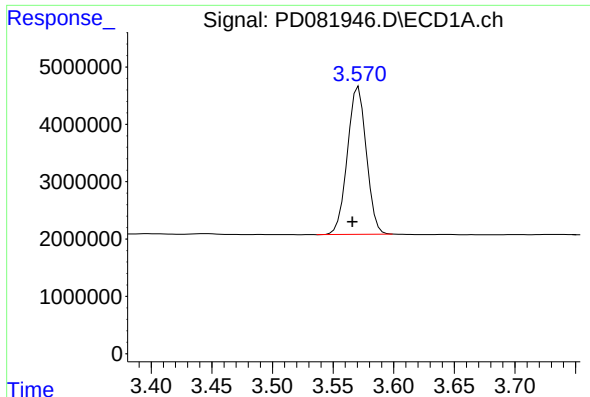

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.005 min
Response: 27988622
Conc: 20.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK428

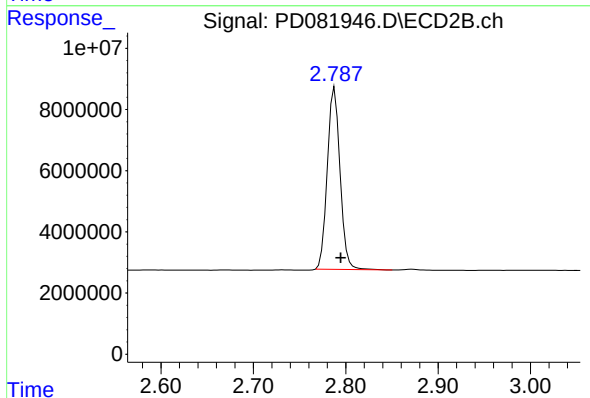


#1 Tetrachloro-m-xylene

R.T.: 2.788 min
Delta R.T.: -0.006 min
Response: 56962162
Conc: 23.24 ng/ml

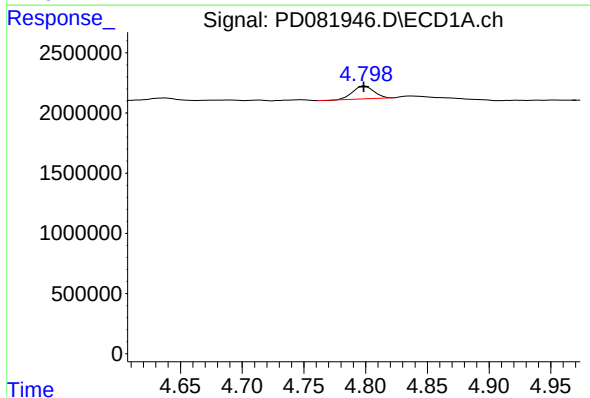


#7 delta-BHC

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1257284
Conc: 0.53 ng/ml

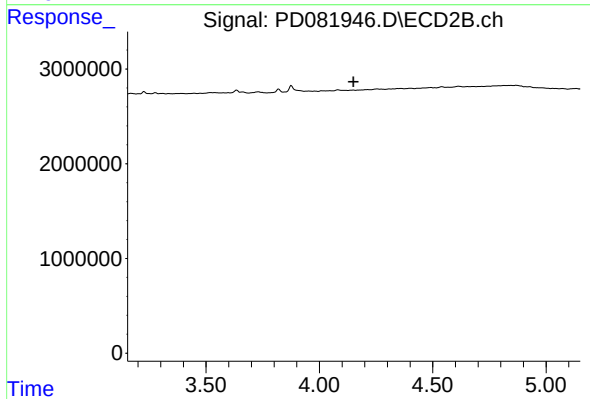

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.151 min
Response: 0
Conc: N.D.

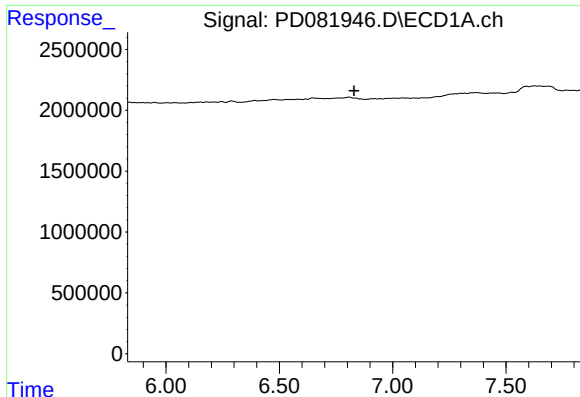

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK428

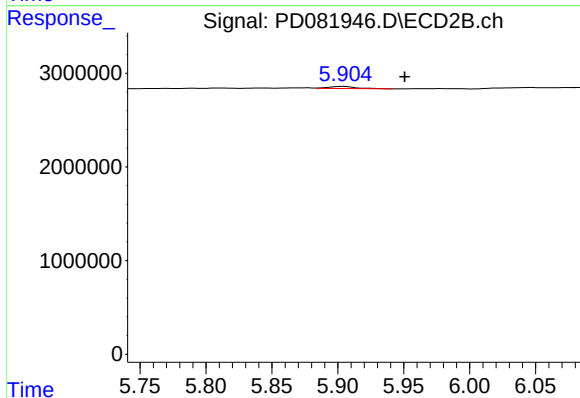


#15 Endosulfan II

R.T.: 5.905 min
Delta R.T.: -0.046 min
Response: 320814
Conc: 0.11 ng/ml

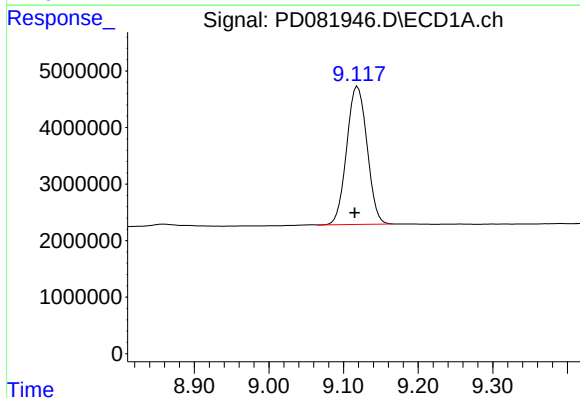

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.004 min
Response: 46269885
Conc: 23.98 ng/ml

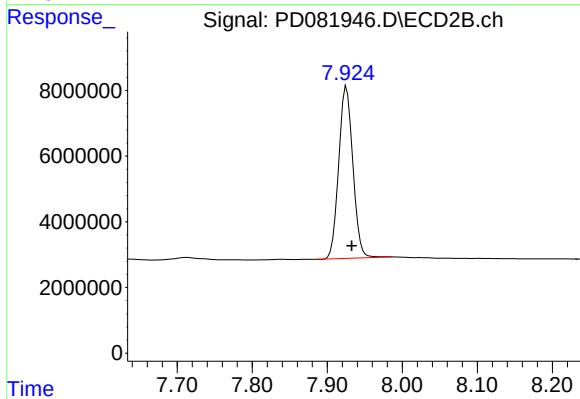

#27 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.007 min
Response: 68715896
Conc: 27.70 ng/ml