

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030620\
 Data File : PD057508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 19:13
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA101

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 05:31:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 09 05:31:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.228	3.898	5329510	12116645	5.139	5.067
27)	SA Decachlor...	7.870	8.900	13437091	28521628	11.111	11.104
Target Compounds							
2)	A alpha-BHC	3.651	4.281	7208187	16461724	4.694	4.630
3)	MA gamma-BHC...	3.923	4.562	7946160	16750558	5.301	4.772
4)	MA Heptachlor	4.203	5.063	6839226	18267220	4.914	5.033
9)	A Endosulfan I	5.198	6.100	6240000	16525054	5.031	5.046
13)	MA Dieldrin	5.436	6.355	13573782	34703499	9.574	9.707
14)	MA Endrin	5.688	6.571	11942120	28409634	9.801	9.571
16)	A 4,4'-DDD	5.825	6.697	10789135	27401868	9.667	9.747
17)	MA 4,4'-DDT	6.058	6.994	10956397	27067720	9.457	9.599
20)	A Methoxychlor	6.607	7.453	30492119	77227318	51.721	52.876


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030620\
Data File : PD057508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 19:13
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA101

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 05:31:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 09 05:31:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

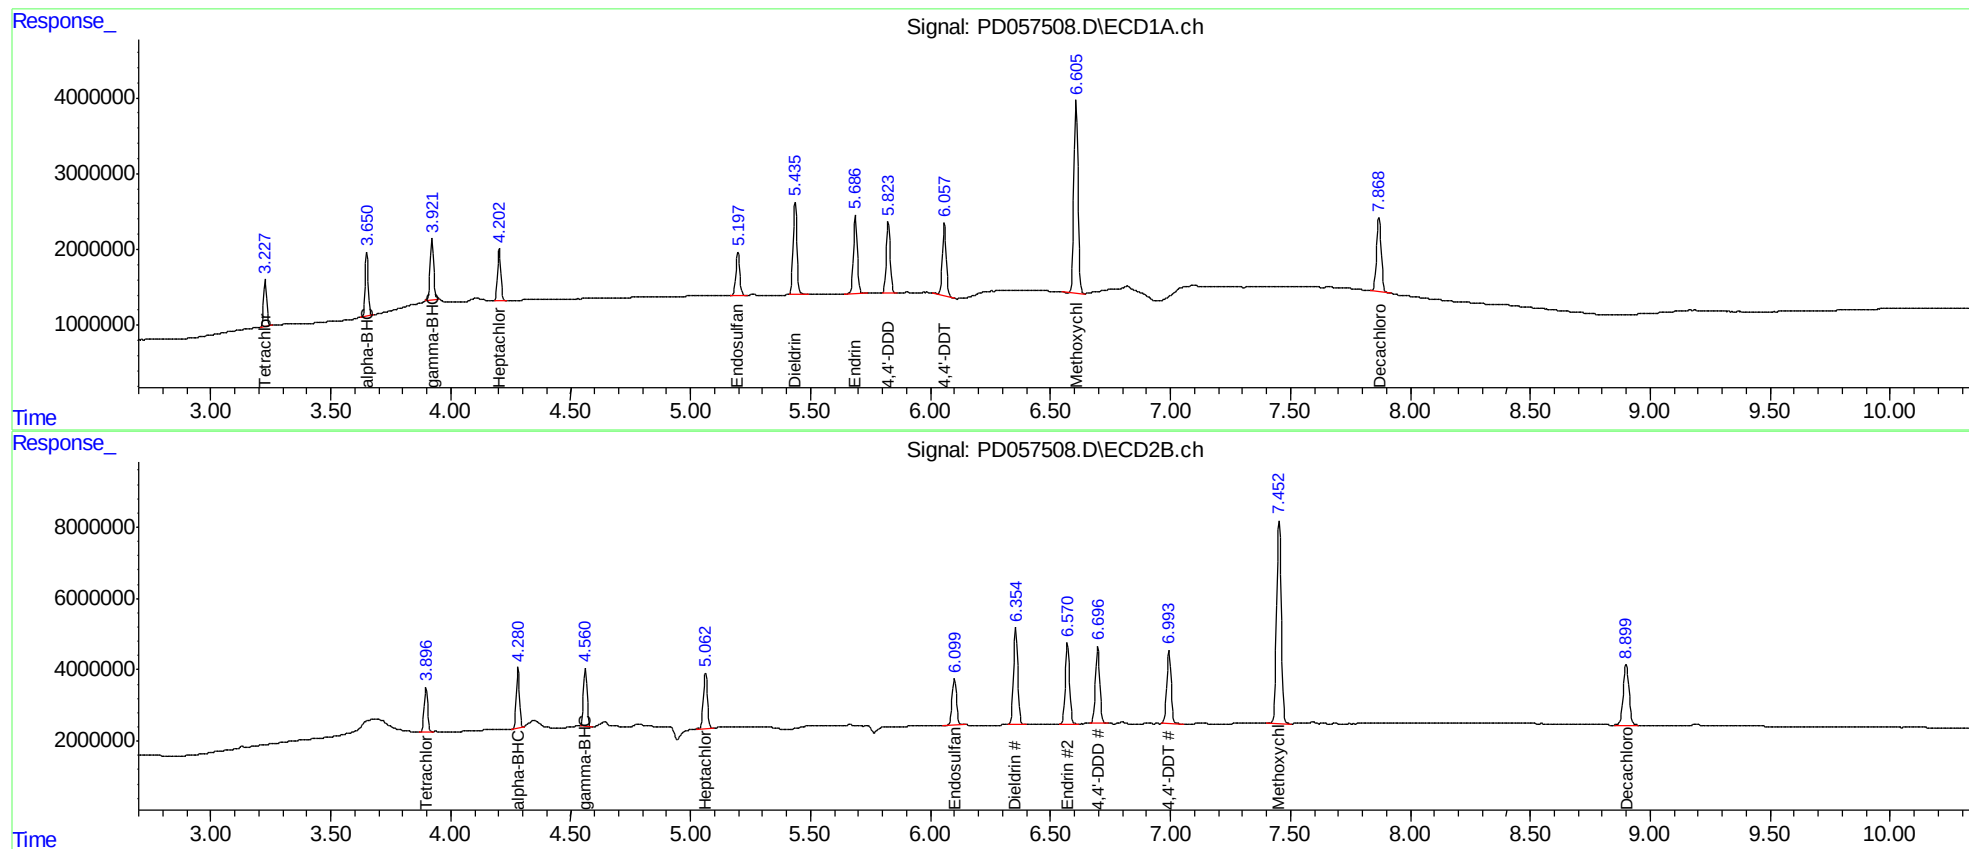


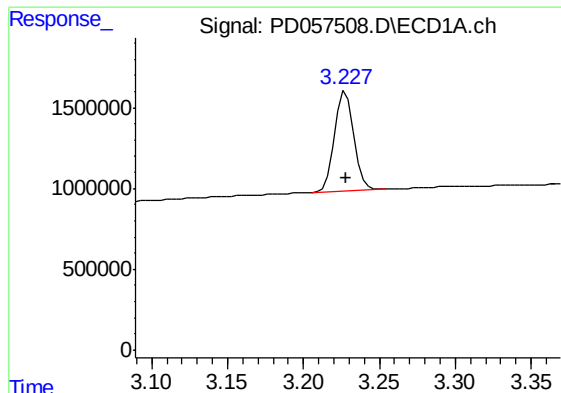

#1 Tetrachloro-m-xylene


R.T.: 3.228 min
Delta R.T.: 0.000 min
Response: 5329510
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

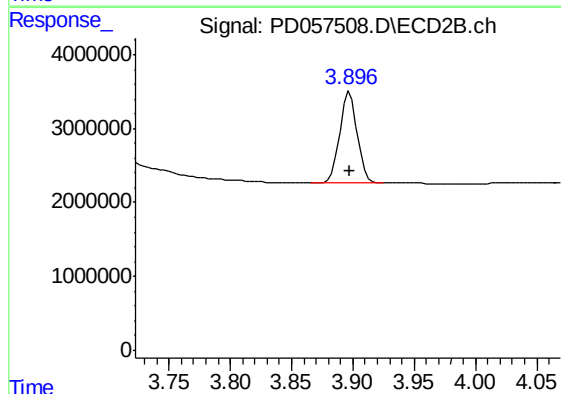


#1 Tetrachloro-m-xylene

R.T.: 3.898 min
Delta R.T.: 0.000 min
Response: 12116645
Conc: 5.07 ng/ml

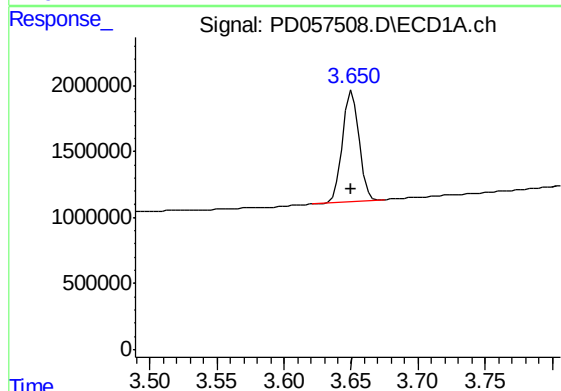


#2 alpha-BHC

R.T.: 3.651 min
Delta R.T.: 0.000 min
Response: 7208187
Conc: 4.69 ng/ml

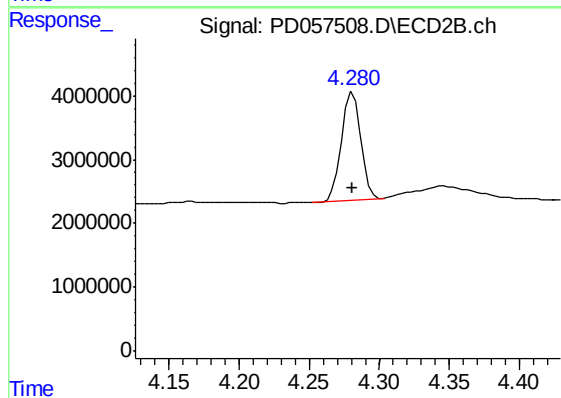

#2 alpha-BHC


R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 16461724
Conc: 4.63 ng/ml

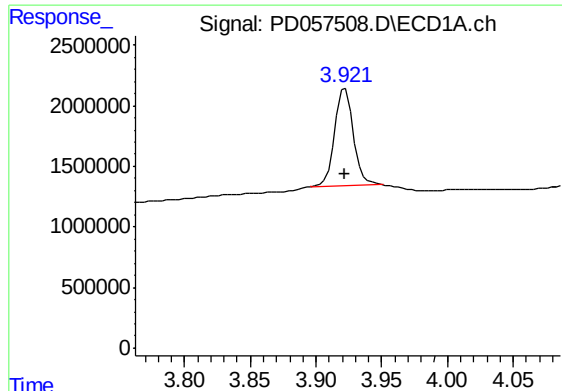

#3 gamma-BHC (Lindane)


R.T.: 3.923 min
Delta R.T.: 0.000 min
Response: 7946160
Conc: 5.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

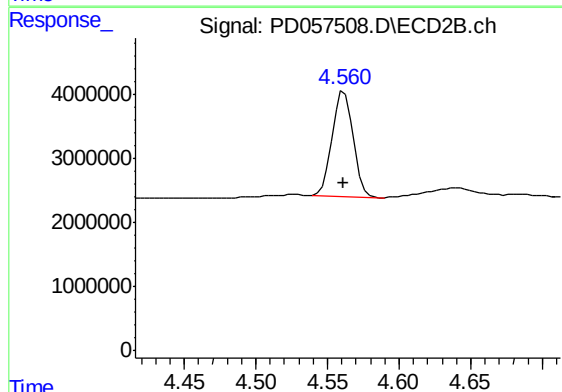


#3 gamma-BHC (Lindane)

R.T.: 4.562 min
Delta R.T.: 0.000 min
Response: 16750558
Conc: 4.77 ng/ml

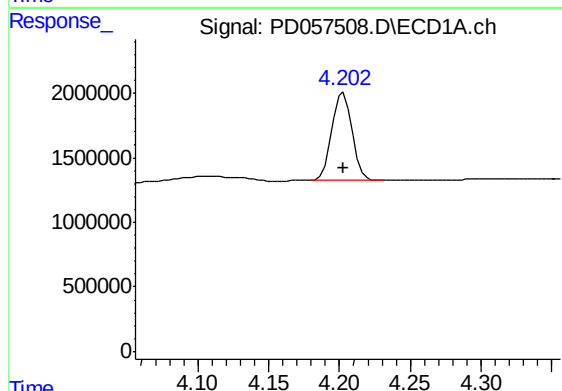


#4 Heptachlor

R.T.: 4.203 min
Delta R.T.: 0.000 min
Response: 6839226
Conc: 4.91 ng/ml

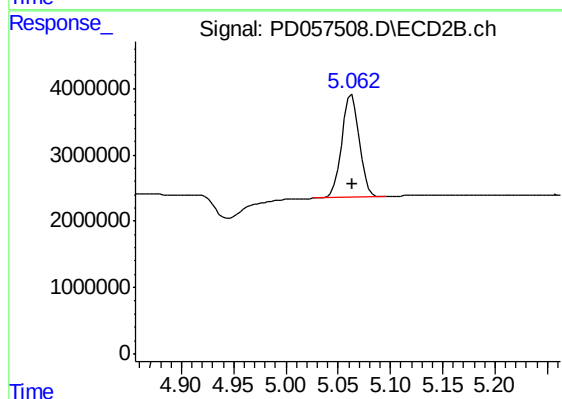

#4 Heptachlor


R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 18267220
Conc: 5.03 ng/ml

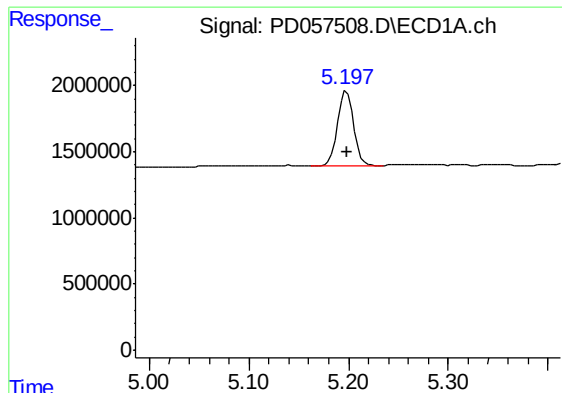

#9 Endosulfan I


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 6240000
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

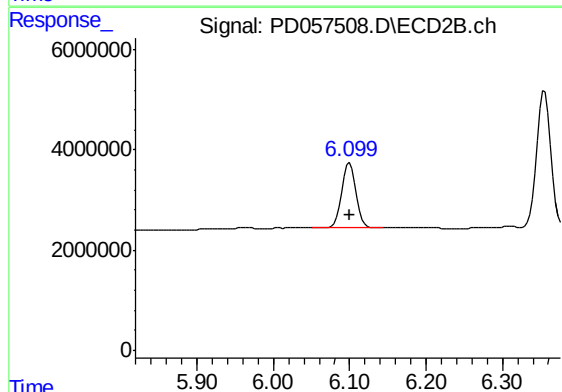


#9 Endosulfan I

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 16525054
Conc: 5.05 ng/ml

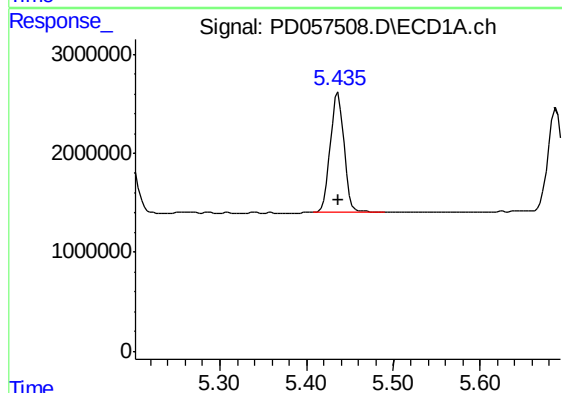


#13 Dieldrin

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 13573782
Conc: 9.57 ng/ml

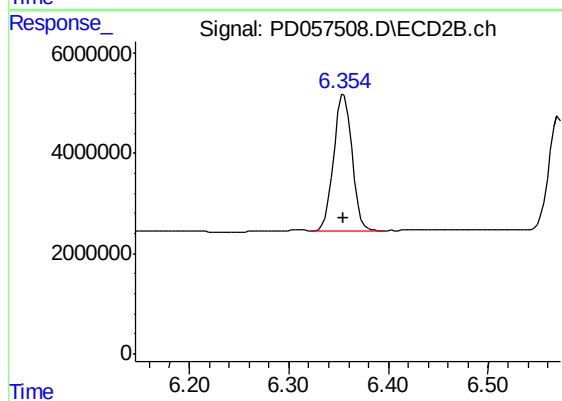

#13 Dieldrin


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 34703499
Conc: 9.71 ng/ml

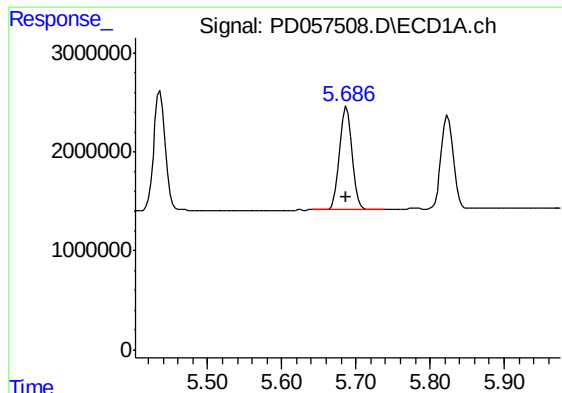

#14 Endrin


R.T.: 5.688 min
Delta R.T.: 0.000 min
Response: 11942120
Conc: 9.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

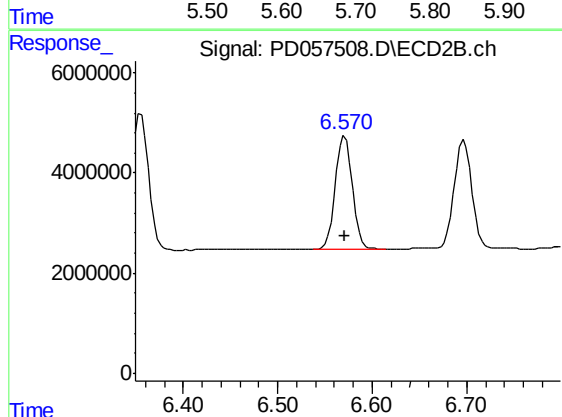


#14 Endrin

R.T.: 6.571 min
Delta R.T.: 0.000 min
Response: 28409634
Conc: 9.57 ng/ml

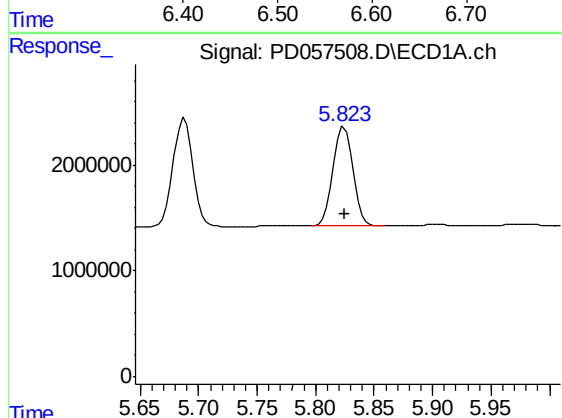


#16 4,4'-DDD

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 10789135
Conc: 9.67 ng/ml

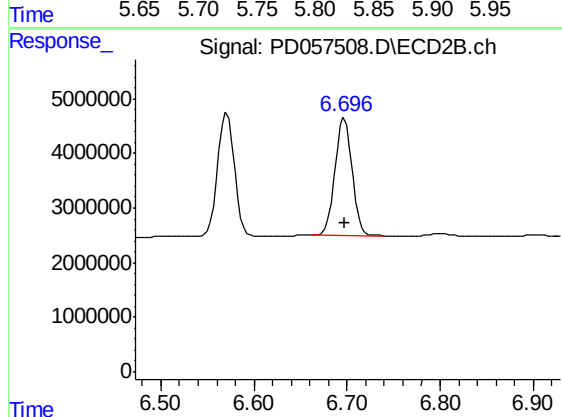

#16 4,4'-DDD


R.T.: 6.697 min
Delta R.T.: 0.000 min
Response: 27401868
Conc: 9.75 ng/ml

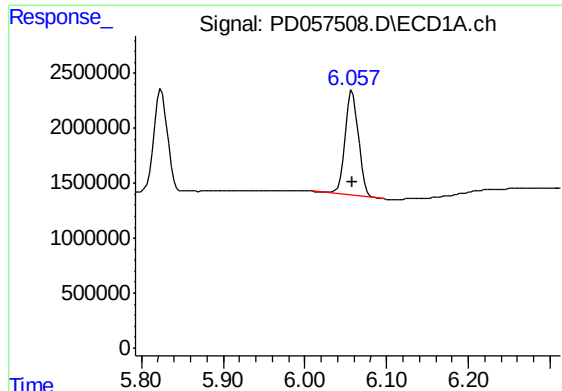

#17 4,4'-DDT


R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 10956397
Conc: 9.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

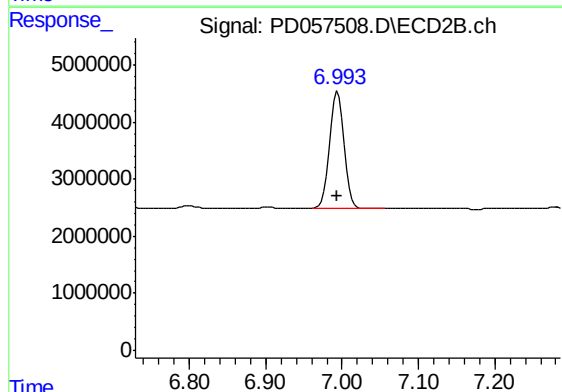


#17 4,4'-DDT

R.T.: 6.994 min
Delta R.T.: 0.000 min
Response: 27067720
Conc: 9.60 ng/ml

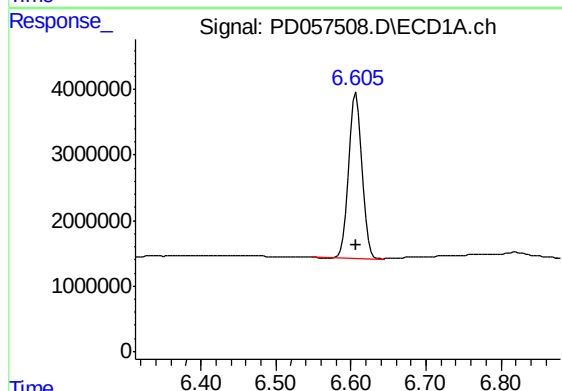


#20 Methoxychlor

R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 30492119
Conc: 51.72 ng/ml

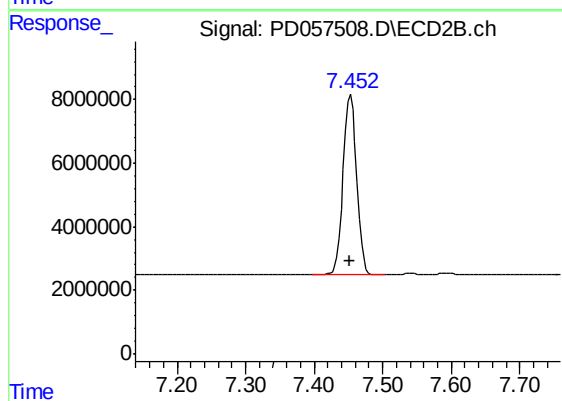

#20 Methoxychlor


R.T.: 7.453 min
Delta R.T.: 0.001 min
Response: 77227318
Conc: 52.88 ng/ml

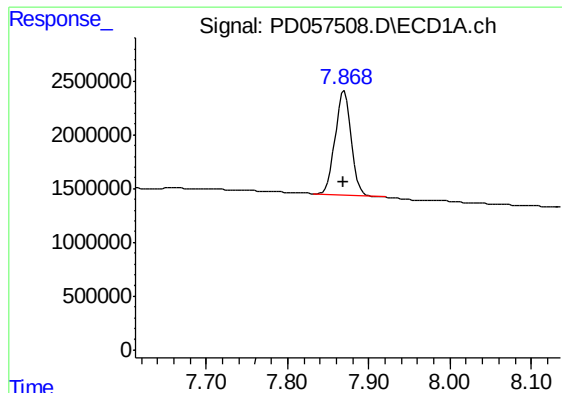

#27 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.000 min
Response: 13437091
Conc: 11.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

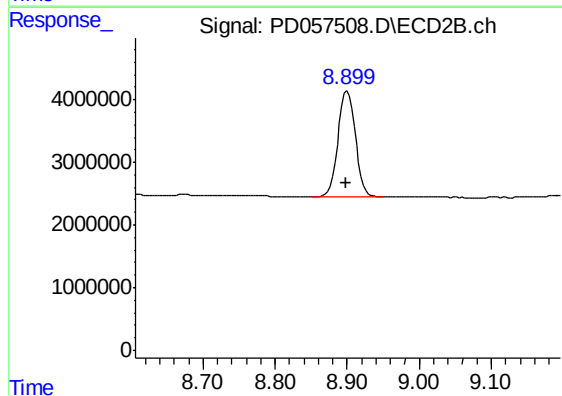

#27 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.001 min
Response: 28521628
Conc: 11.10 ng/ml