

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD030620\  
 Data File : PD057516.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Mar 2020 21:07  
 Operator : AJ\MA  
 Sample : INDA501  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA501

Manual Integrations  
 APPROVED

mohammad  
 3/10/2020 12:44:44 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 09 05:40:40 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD030620CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Mar 09 05:31:06 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml    | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|----------|---------|
| -----                       |                 |       |       |          |          |          |         |
| System Monitoring Compounds |                 |       |       |          |          |          |         |
| 1)                          | SA Tetrachlo... | 3.247 | 3.898 | 86140724 | 192.8E6  | 83.057m  | 80.607  |
| 27)                         | SA Decachlor... | 7.889 | 8.900 | 185.1E6  | 382.8E6  | 153.088  | 149.037 |
| Target Compounds            |                 |       |       |          |          |          |         |
| 2)                          | A alpha-BHC     | 3.672 | 4.282 | 139.6E6  | 310.6E6  | 90.893   | 87.356  |
| 3)                          | MA gamma-BHC... | 3.941 | 4.562 | 130.4E6  | 298.7E6  | 86.976m  | 85.092  |
| 4)                          | MA Heptachlor   | 4.222 | 5.064 | 120.1E6  | 298.5E6  | 86.268m  | 82.234  |
| 9)                          | A Endosulfan I  | 5.219 | 6.101 | 104.0E6  | 263.9E6  | 83.836   | 80.578  |
| 13)                         | MA Dieldrin     | 5.456 | 6.356 | 242.8E6  | 588.0E6  | 171.260  | 164.474 |
| 14)                         | MA Endrin       | 5.708 | 6.572 | 203.3E6  | 483.8E6  | 166.850  | 162.977 |
| 16)                         | A 4,4'-DDD      | 5.845 | 6.698 | 191.8E6  | 463.7E6  | 171.836  | 164.958 |
| 17)                         | MA 4,4'-DDT     | 6.076 | 6.994 | 203.9E6  | 471.8E6  | 176.025m | 167.294 |
| 20)                         | A Methoxychlor  | 6.626 | 7.453 | 453.1E6  | 1075.7E6 | 768.470  | 736.479 |
| -----                       |                 |       |       |          |          |          |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD030620\  
Data File : PD057516.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Mar 2020 21:07  
Operator : AJ\MA  
Sample : INDA501  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 09 05:40:40 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD030620CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Mar 09 05:31:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

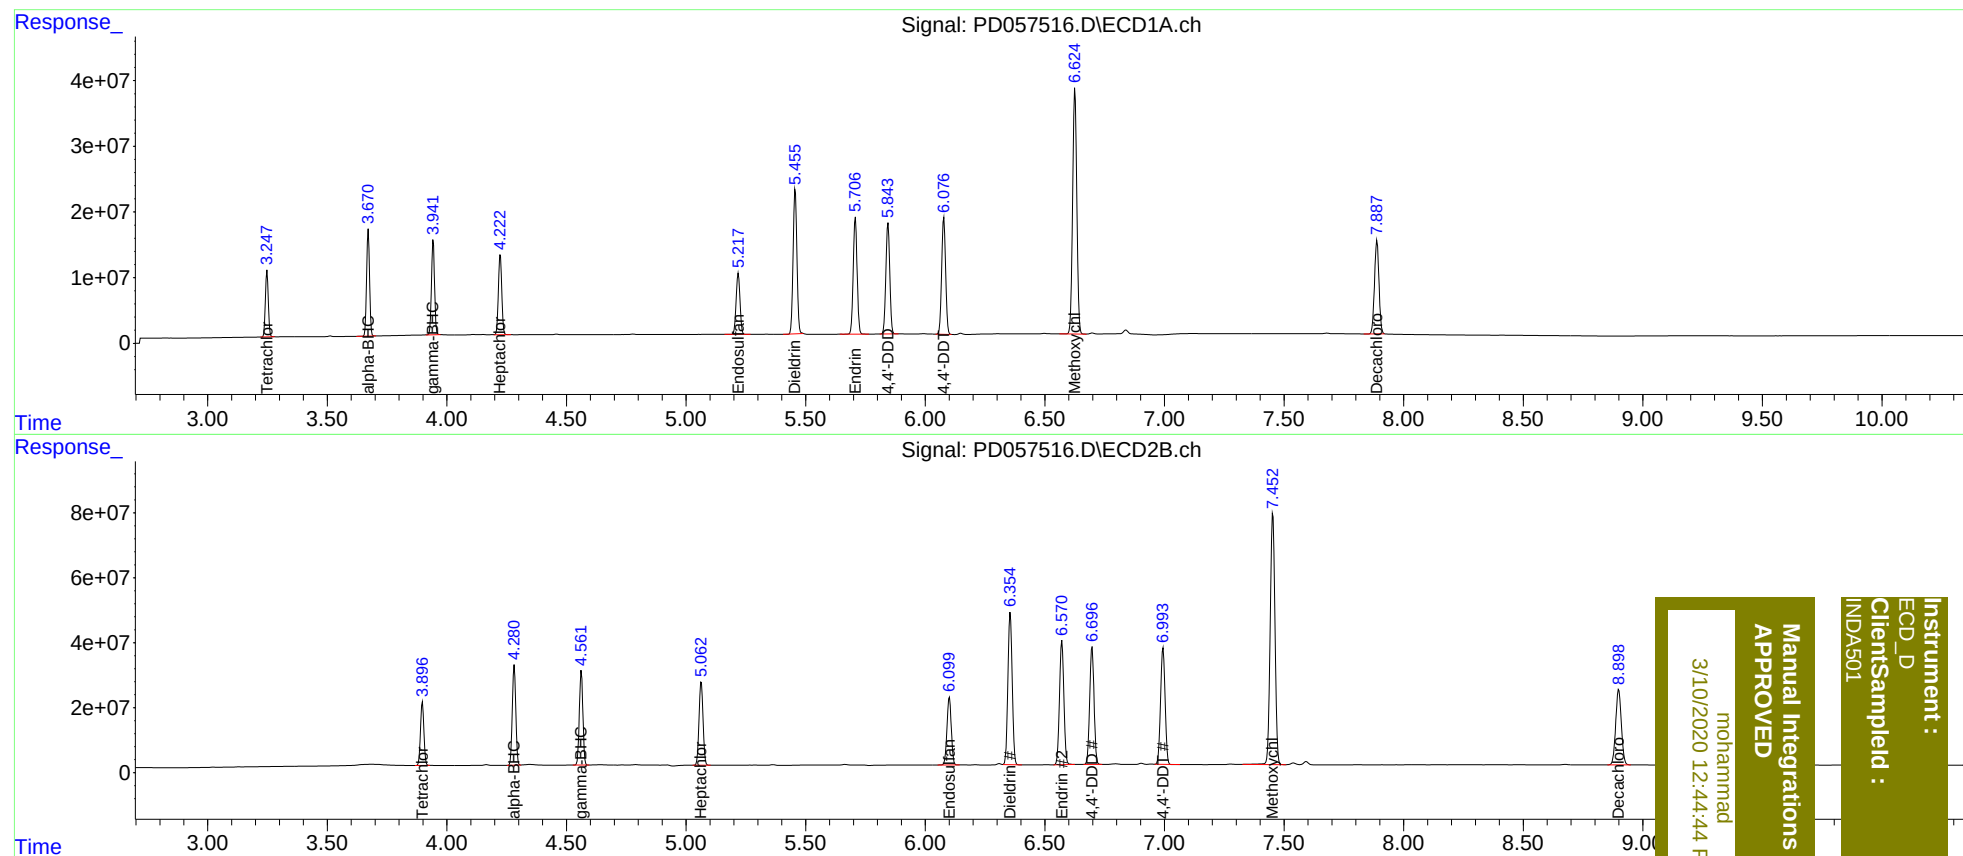

Manual Integrations  
APPROVED

mohammad  
3/10/2020 12:44:44 PM

Instrument :  
ECD\_D  
ClientSampled :  
INDA501