

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

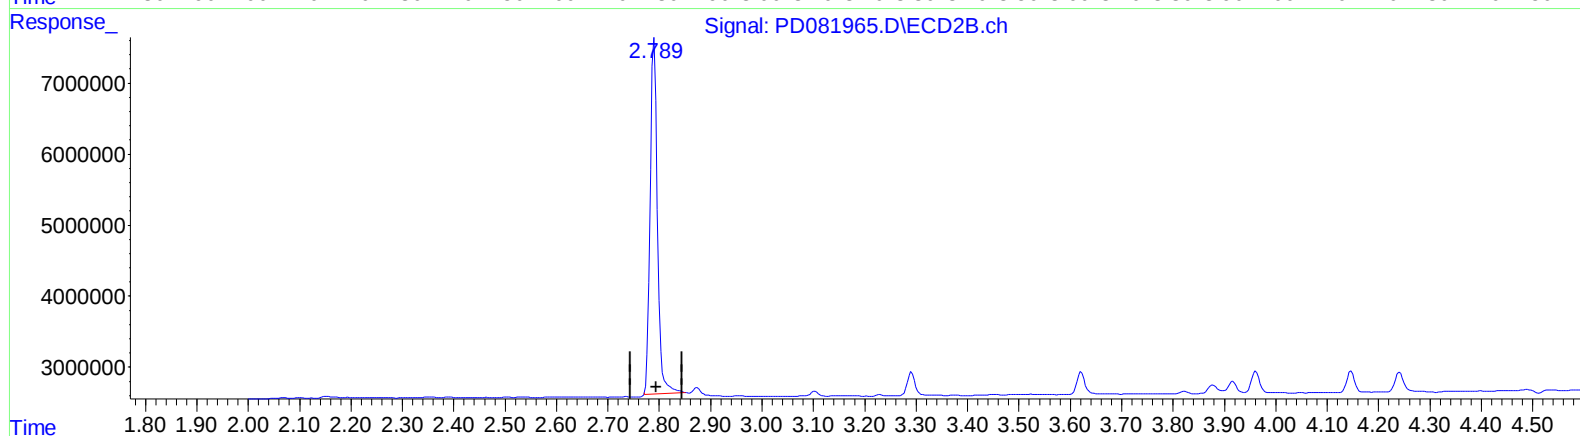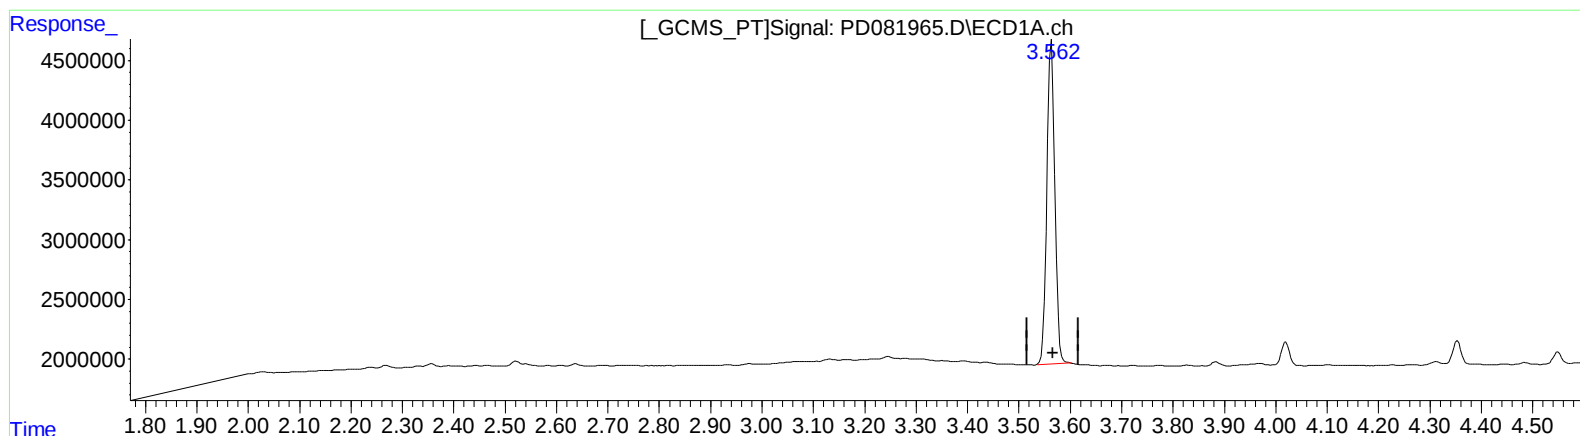

QEdit

(1) Tetrachloro-m-xylene (SA)

3.564min 21.279 ng/ml

response 29090800

(1) Tetrachloro-m-xylene #2 (SA)

2.790min 20.282 ng/ml

response 49723304

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

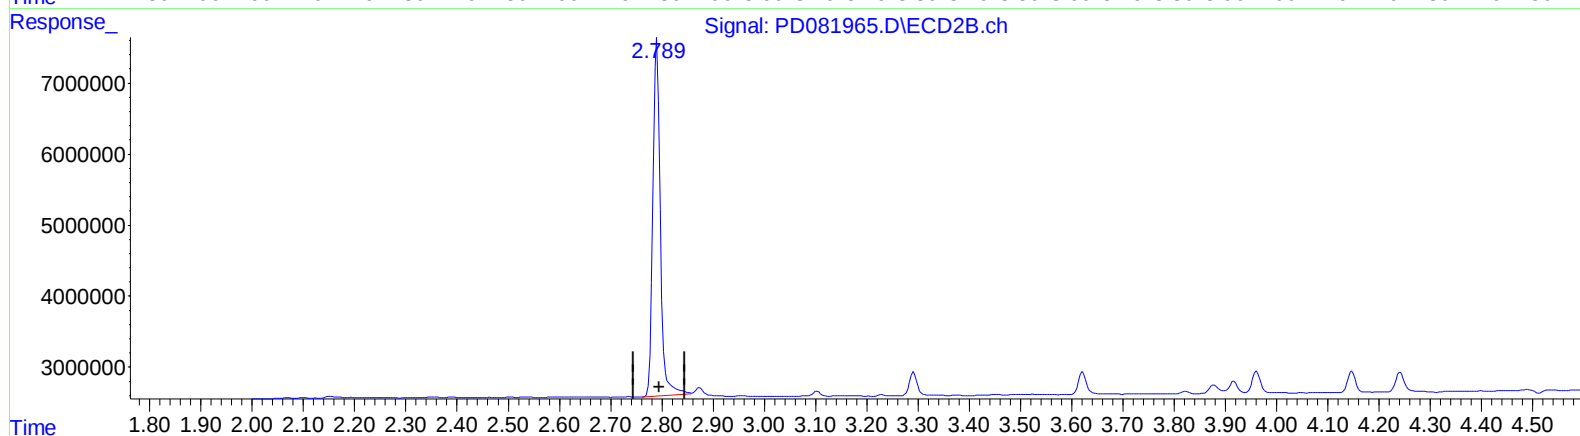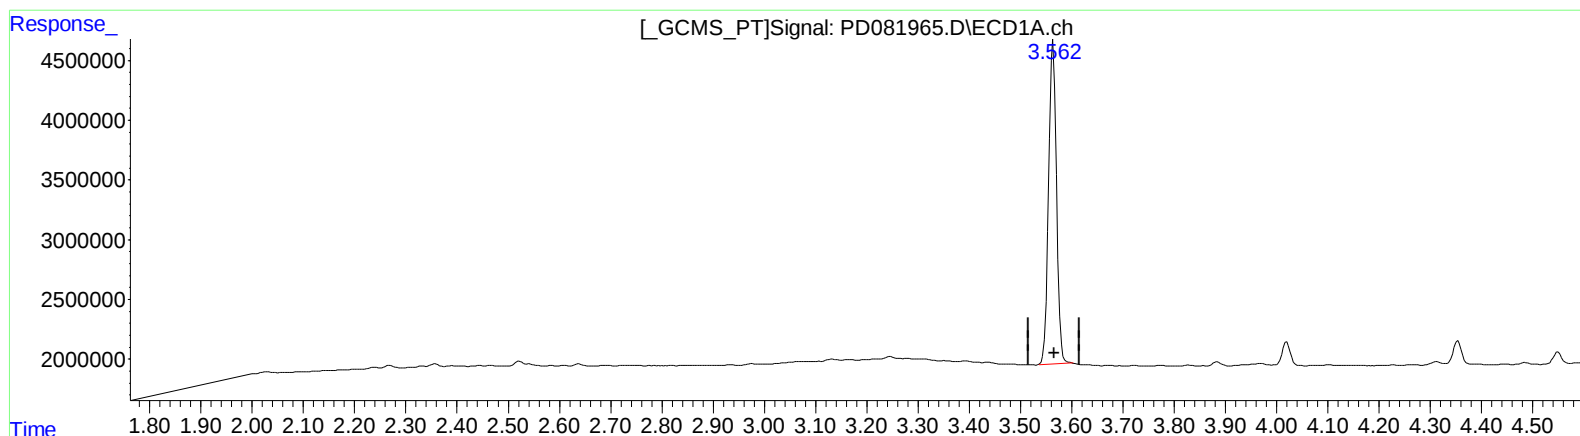

QEdit

(1) Tetrachloro-m-xylene (SA)

3.564min 21.279 ng/ml

response 29090800

(1) Tetrachloro-m-xylene #2 (SA)

2.789min 20.774 ng/ml m

response 50928689

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

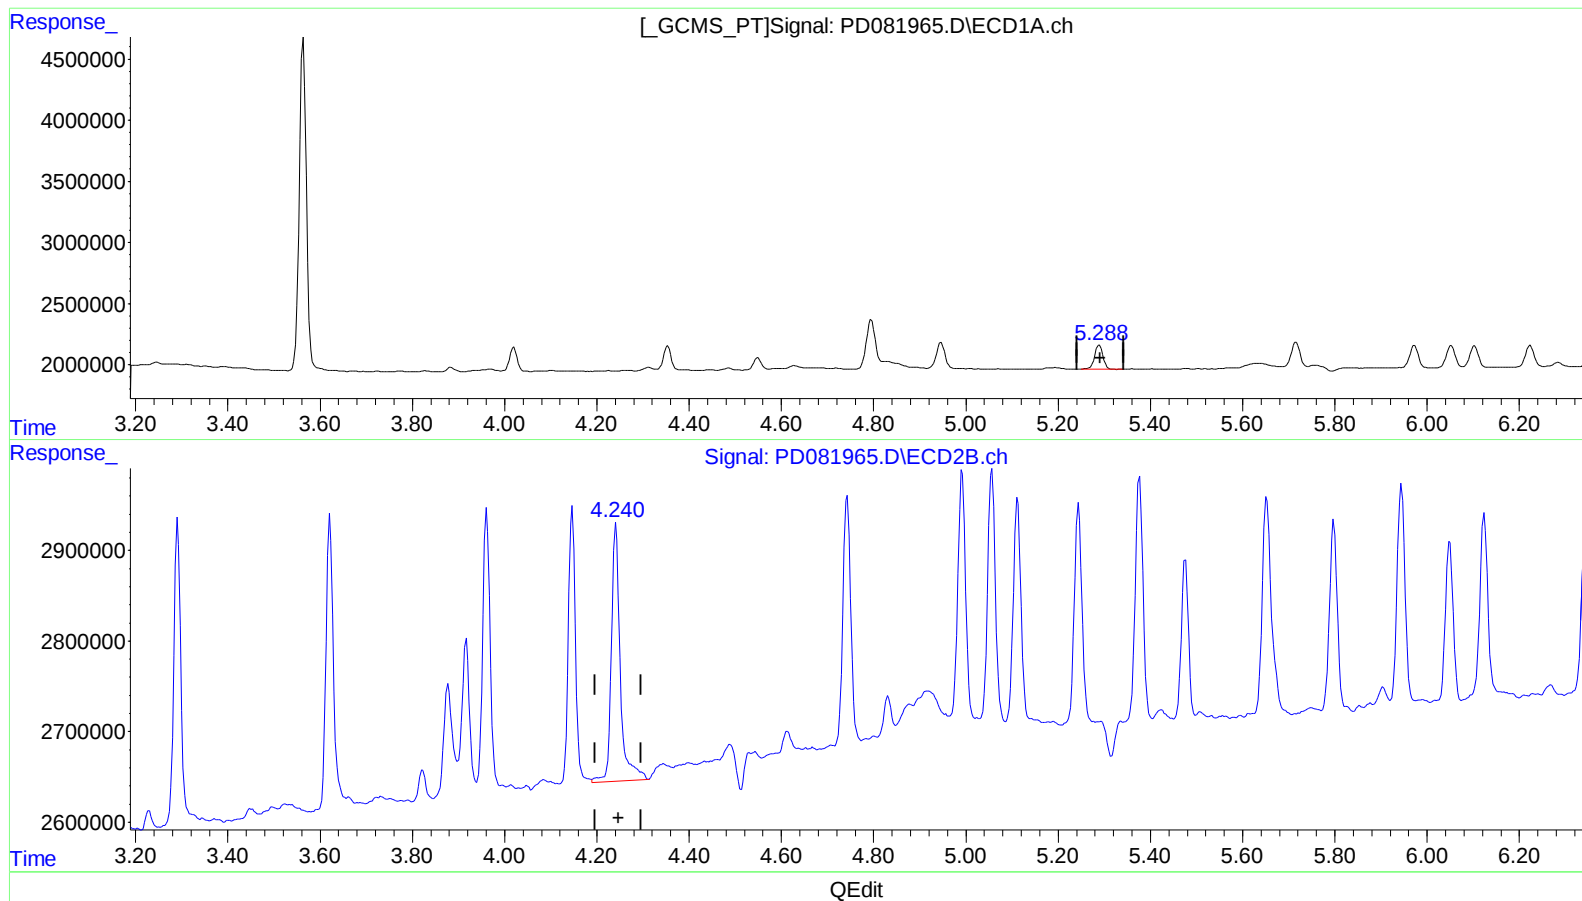

(5) Aldrin (MB)

5.289min 1.048 ng/ml

response 2479142

(5) Aldrin #2 (MB)

4.241min 1.133 ng/ml

response 3835999

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

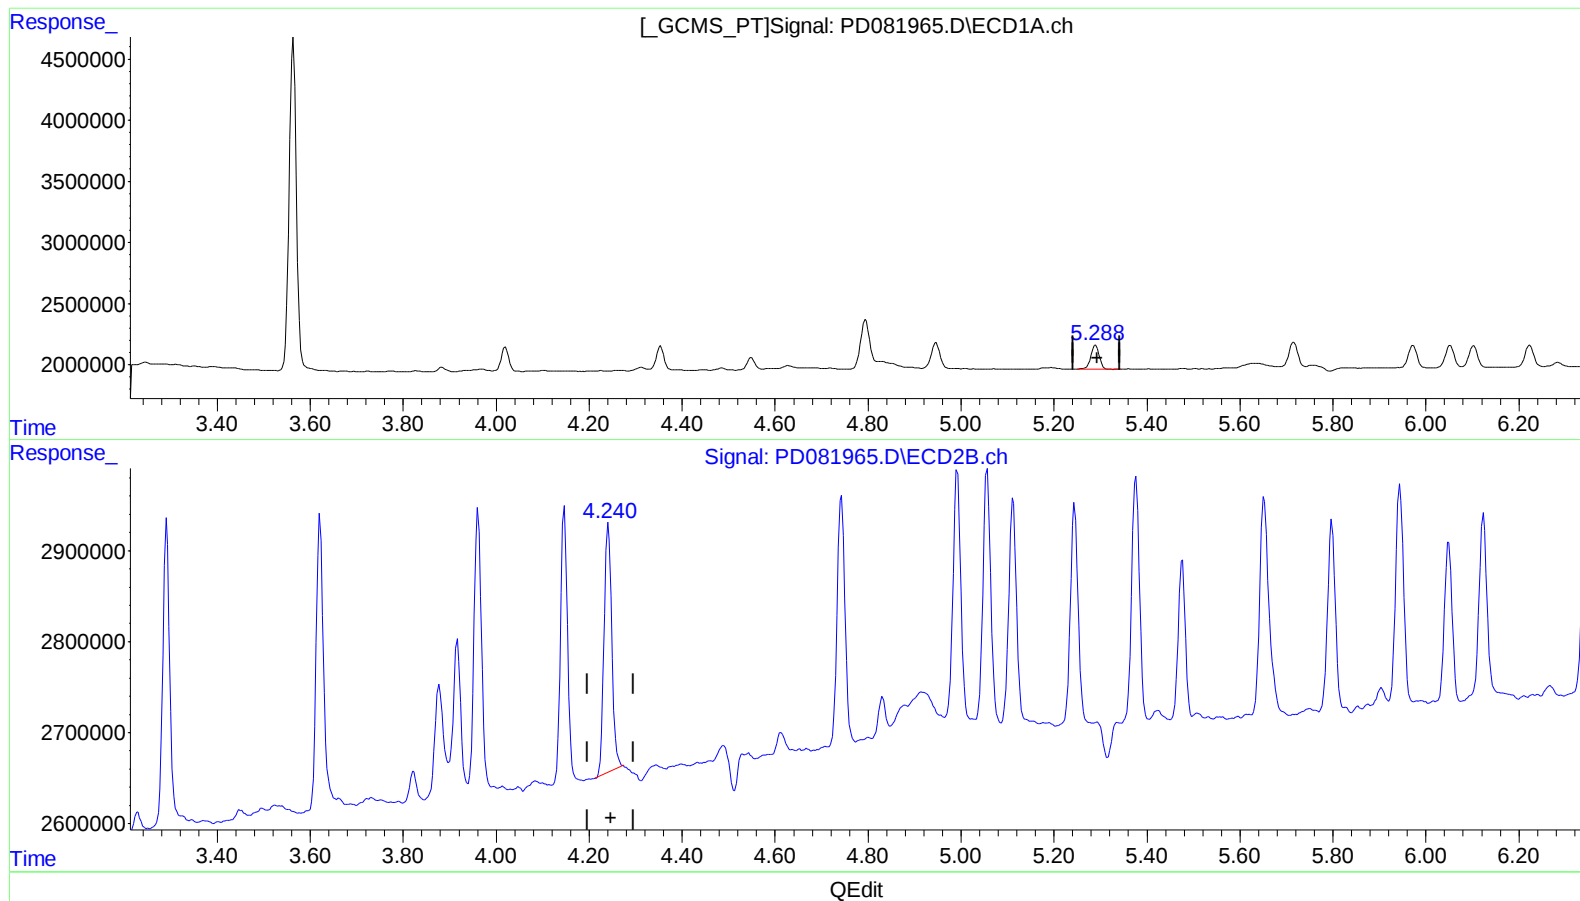

(5) Aldrin (MB)

5.289min 1.048 ng/ml

response 2479142

(5) Aldrin #2 (MB)

4.240min 0.924 ng/ml m

response 3130472

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

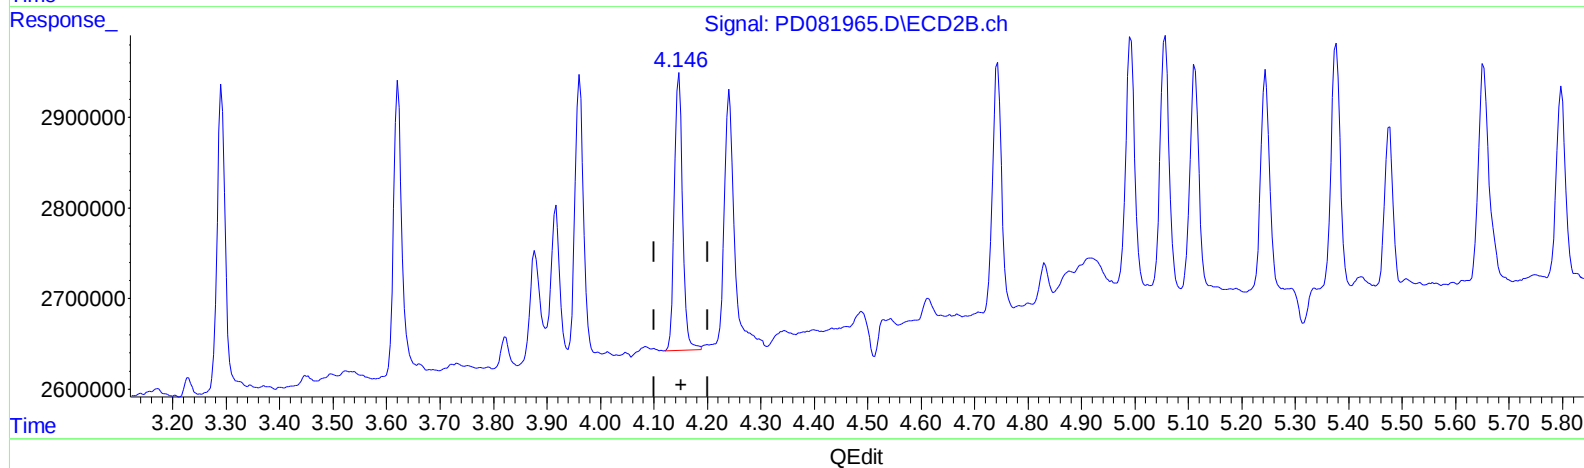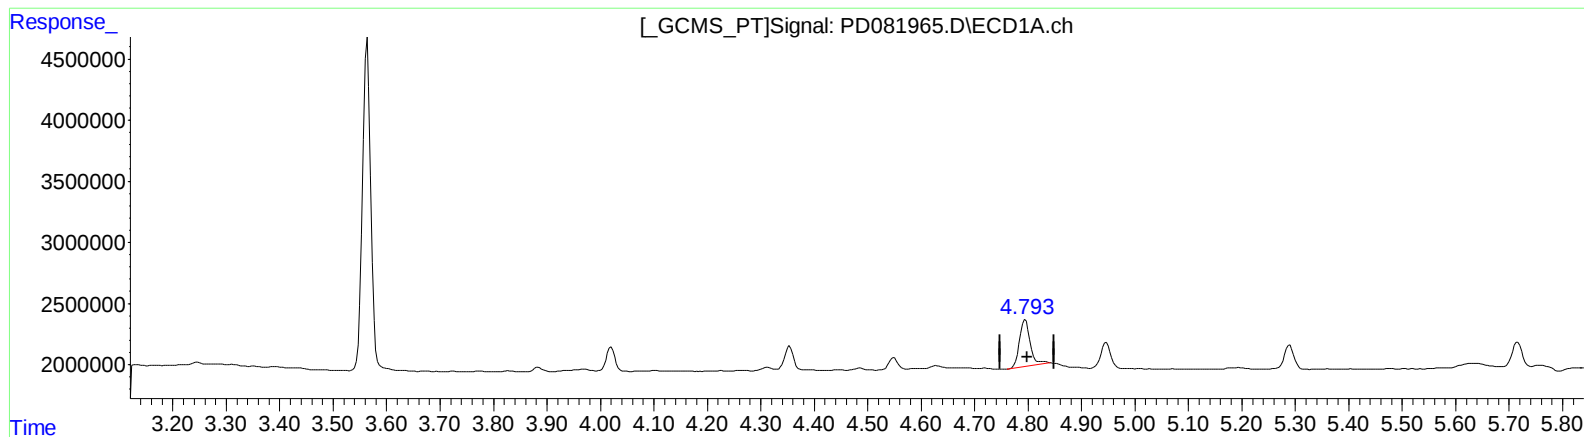

(7) delta-BHC (B)

4.795min 2.246 ng/ml

response 5320385

(7) delta-BHC #2 (B)

4.147min 0.872 ng/ml

response 3265228

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

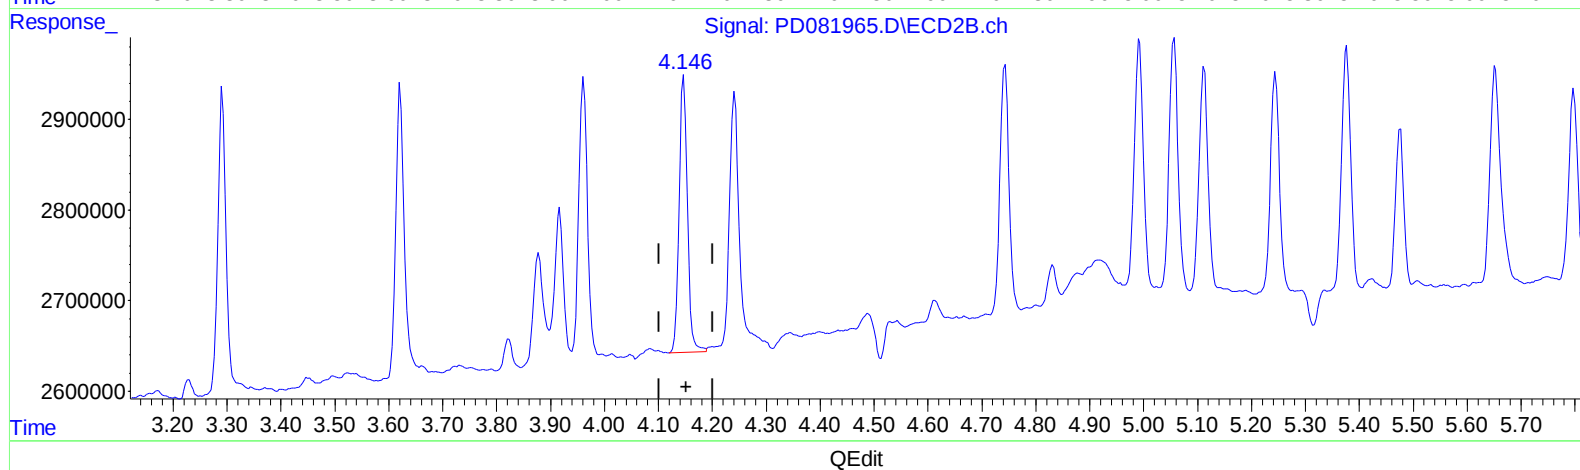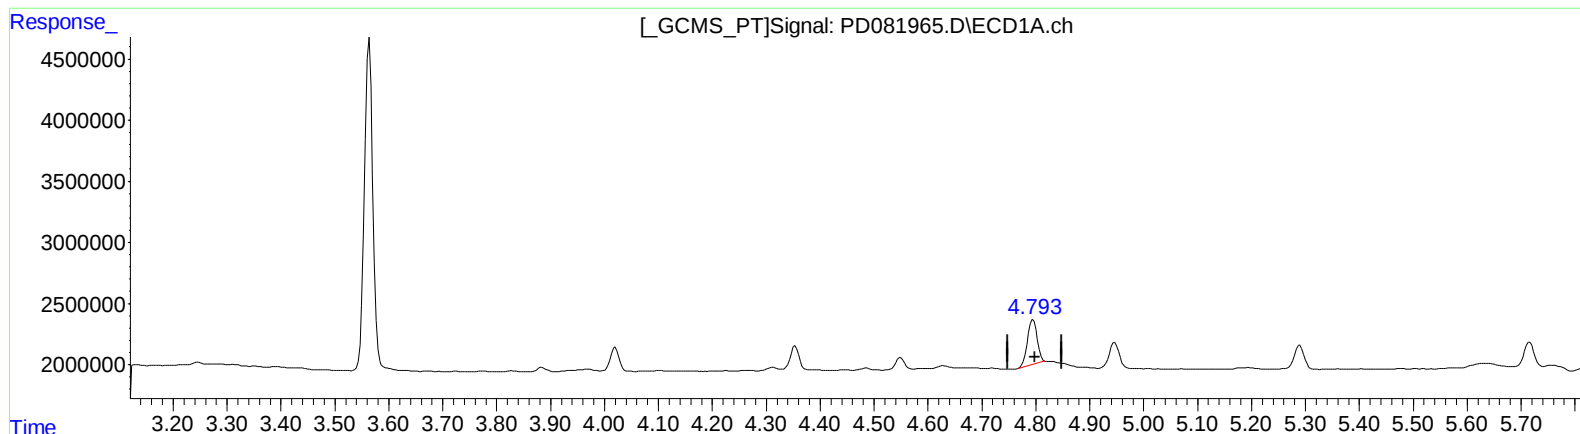

(7) delta-BHC (B)

4.793min 1.938 ng/ml m

response 4590029

(7) delta-BHC #2 (B)

4.147min 0.872 ng/ml

response 3265228

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

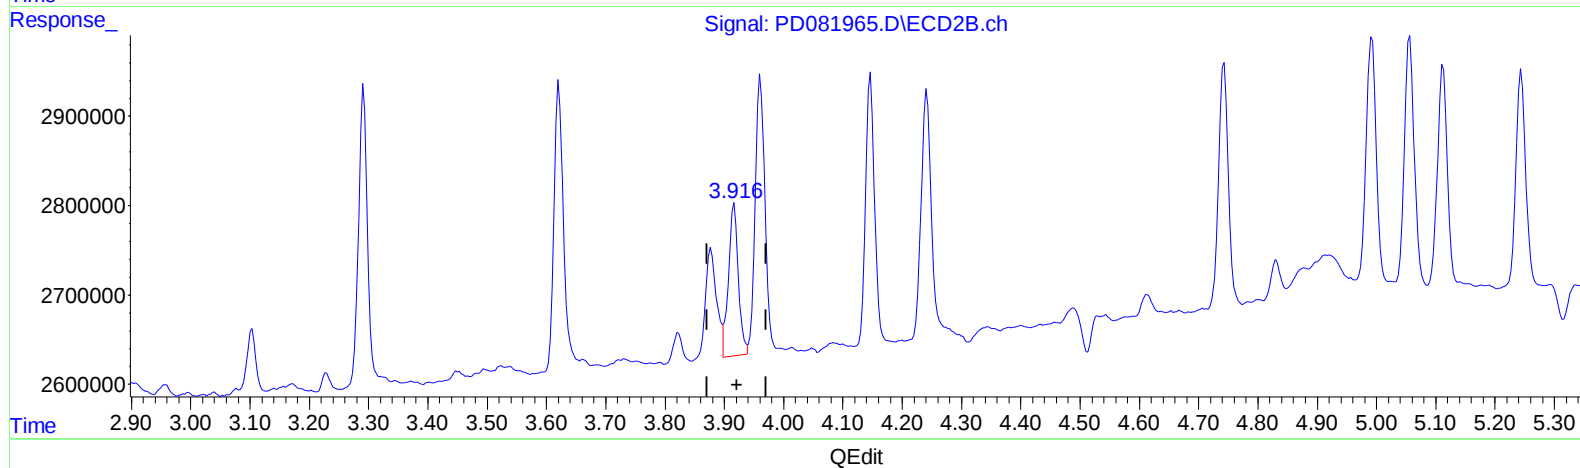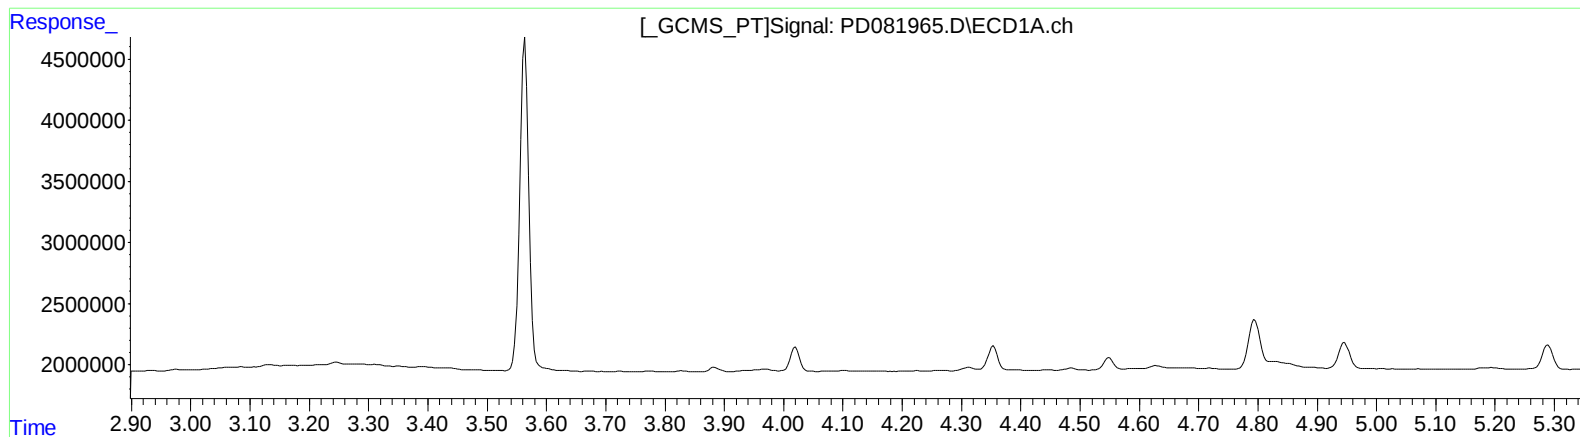

(6) beta-BHC (B)

0.000min 0.000 ng/ml

response 0

(6) beta-BHC #2 (B)

3.917min 1.179 ng/ml

response 1991480

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

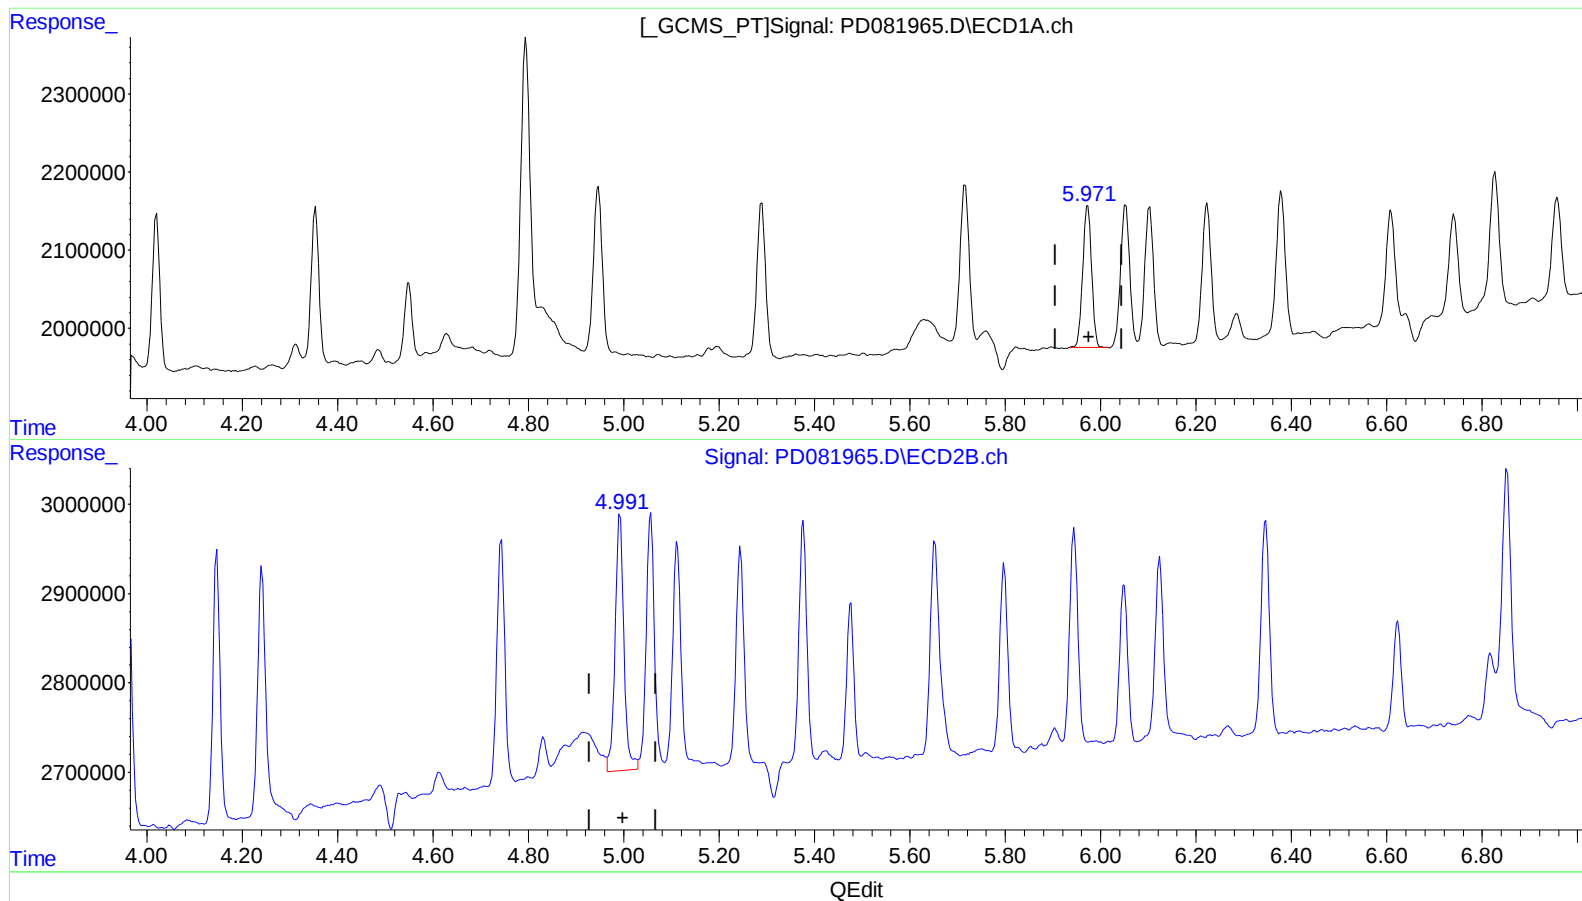

(10) trans-Chlordane (B)

5.973min 1.064 ng/ml

response 2329247

(10) trans-Chlordane #2 (B)

4.992min 1.166 ng/ml

response 3640024

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

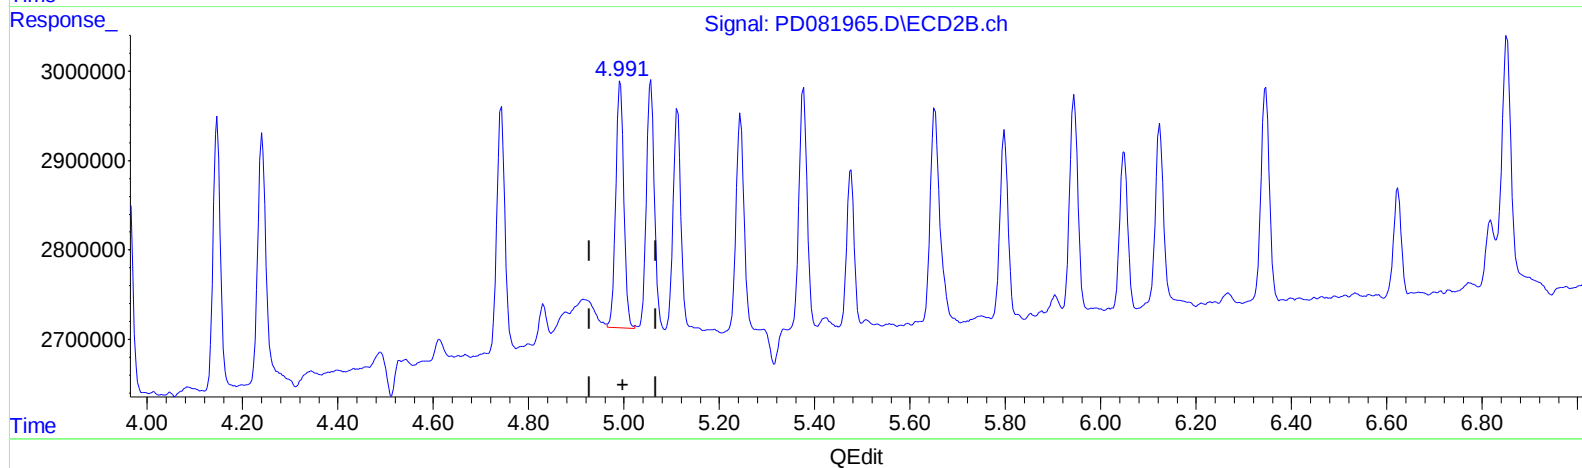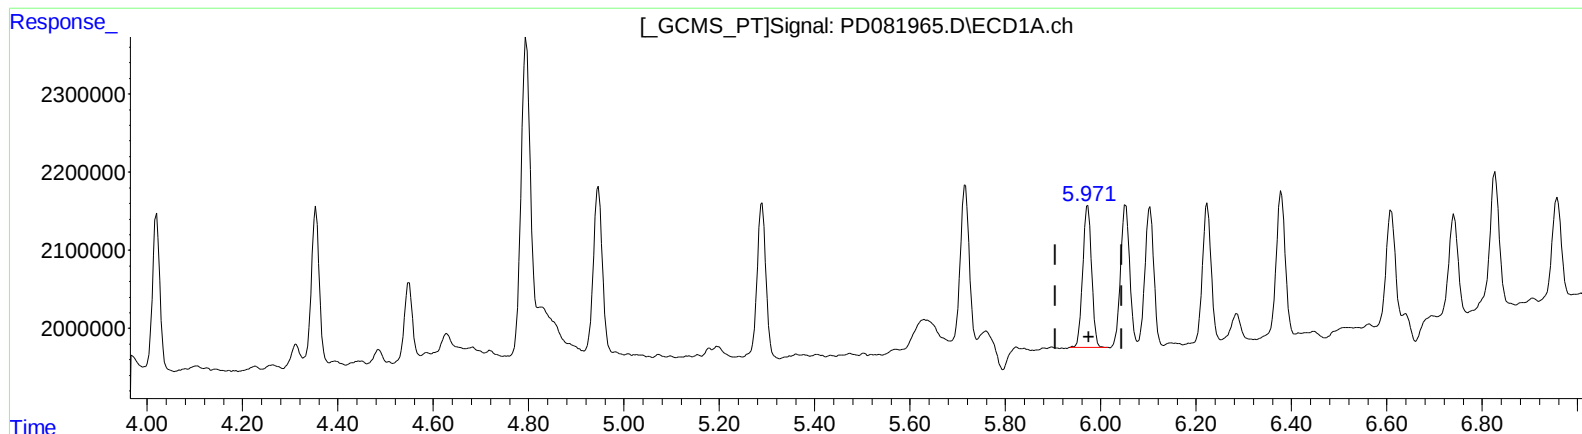

(10) trans-Chlordane (B)

5.973min 1.064 ng/ml

response 2329247

(10) trans-Chlordane #2 (B)

4.991min 1.035 ng/ml m

response 3230466

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

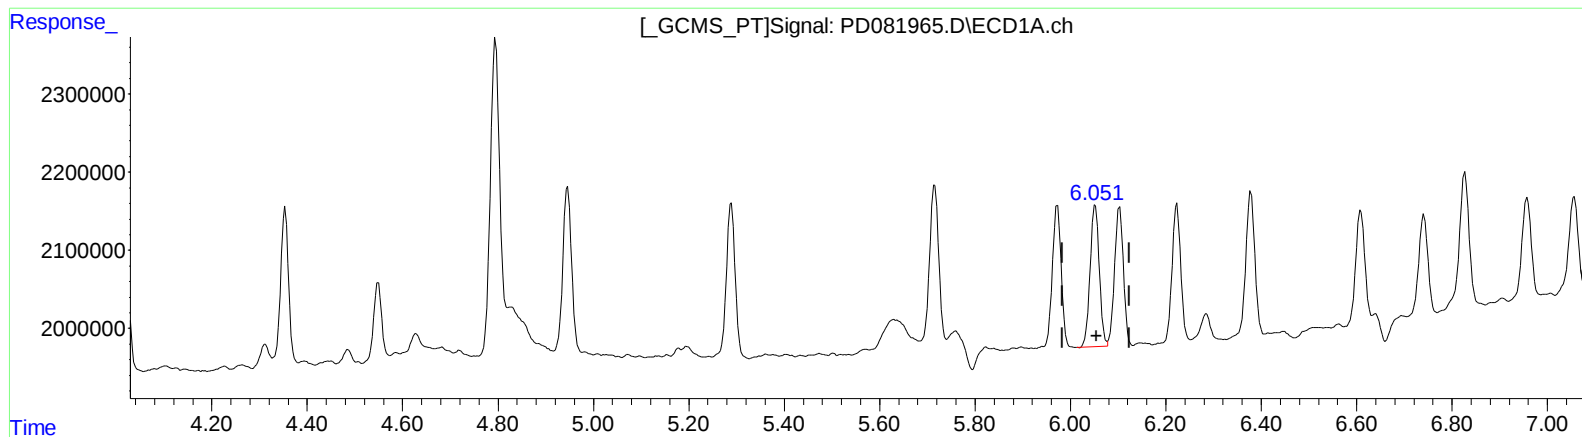

(11) cis-Chlordane (B)
6.052min 1.070 ng/ml
response 2410288

(11) cis-Chlordane #2 (B)
5.056min 1.075 ng/ml
response 3444616

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

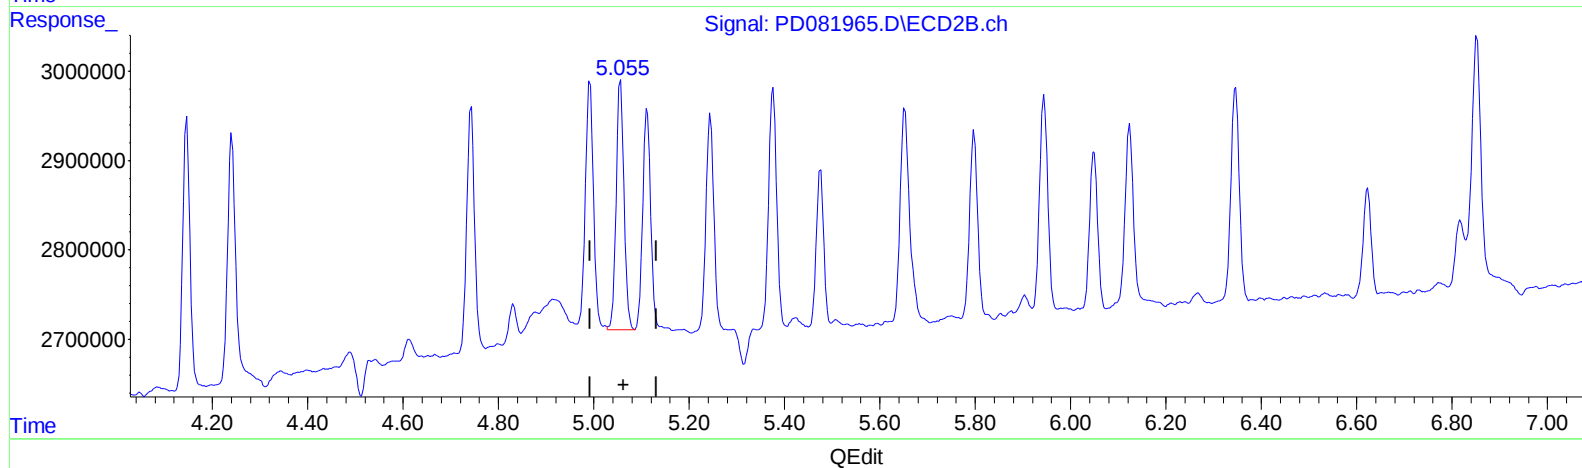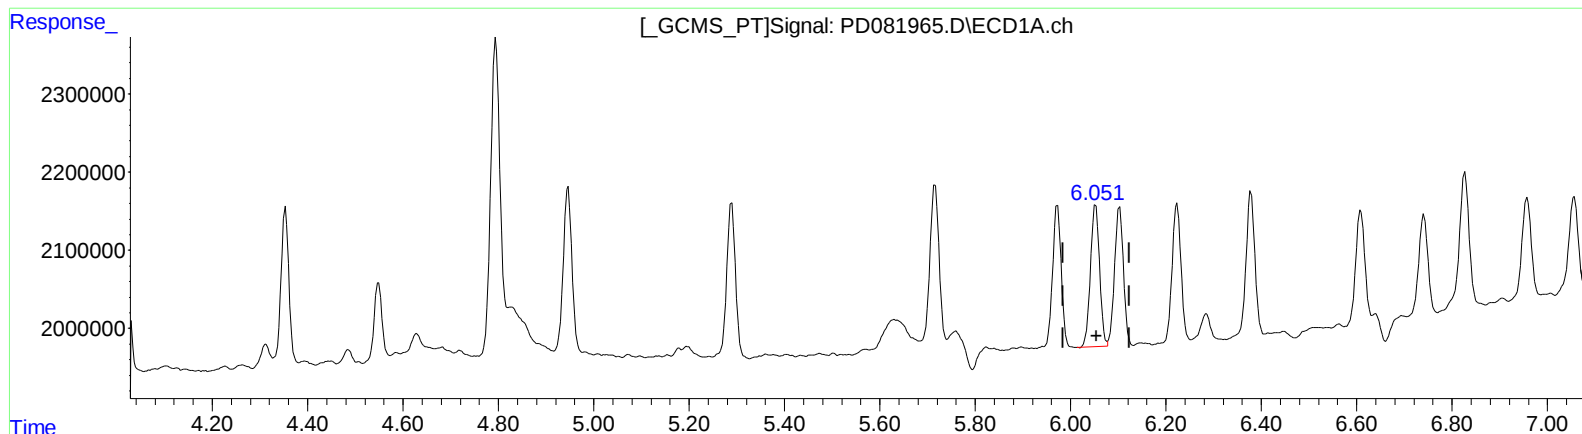

(11) cis-Chlordane (B)
6.052min 1.070 ng/ml
response 2410288

(11) cis-Chlordane #2 (B)
5.055min 1.012 ng/ml m
response 3243091

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

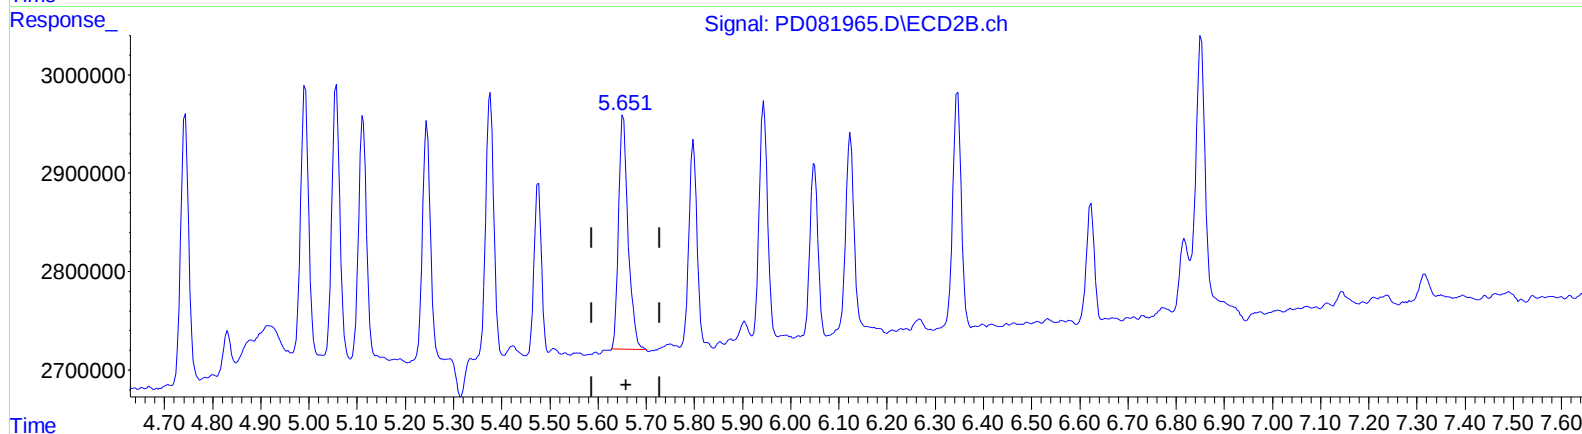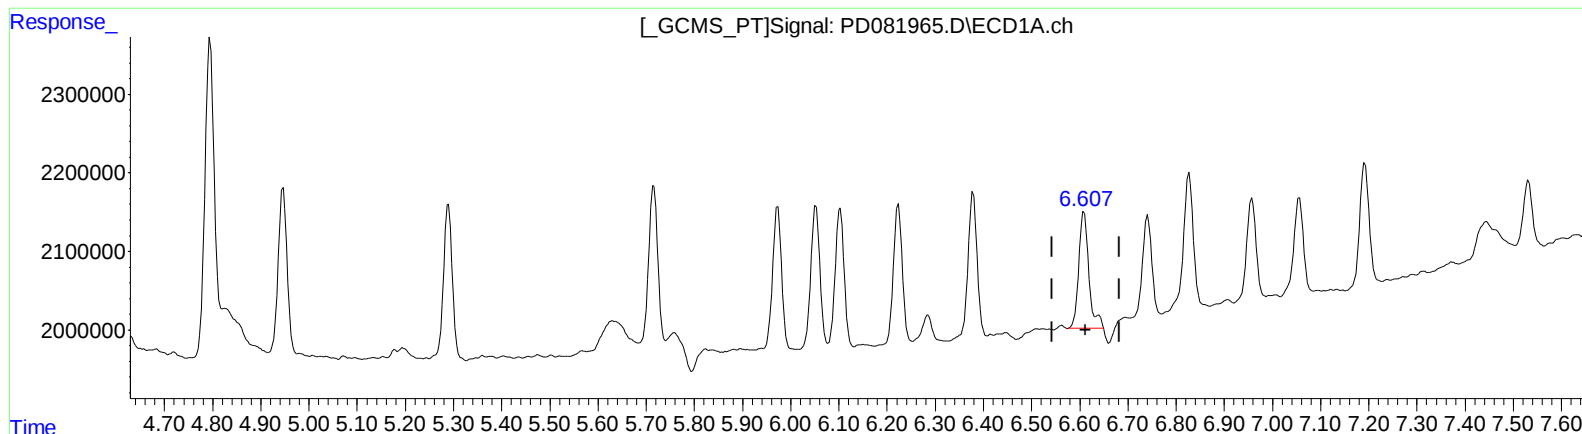

QEdit

(14) Endrin (MA)

6.609min 1.164 ng/ml

response 2183743

(14) Endrin #2 (MA)

5.652min 1.144 ng/ml

response 3287039

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

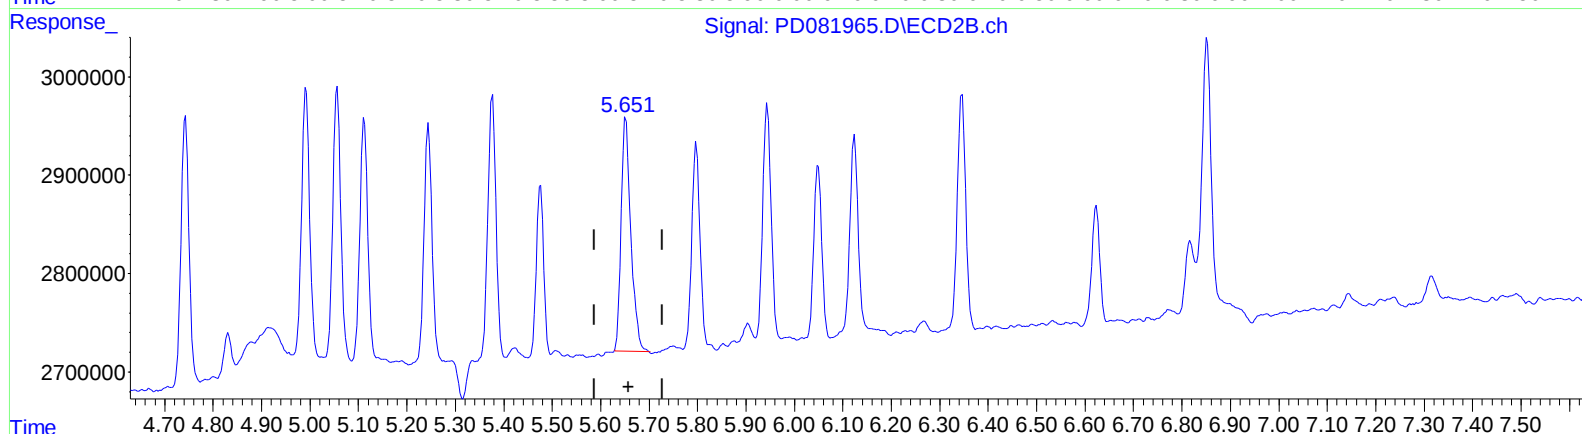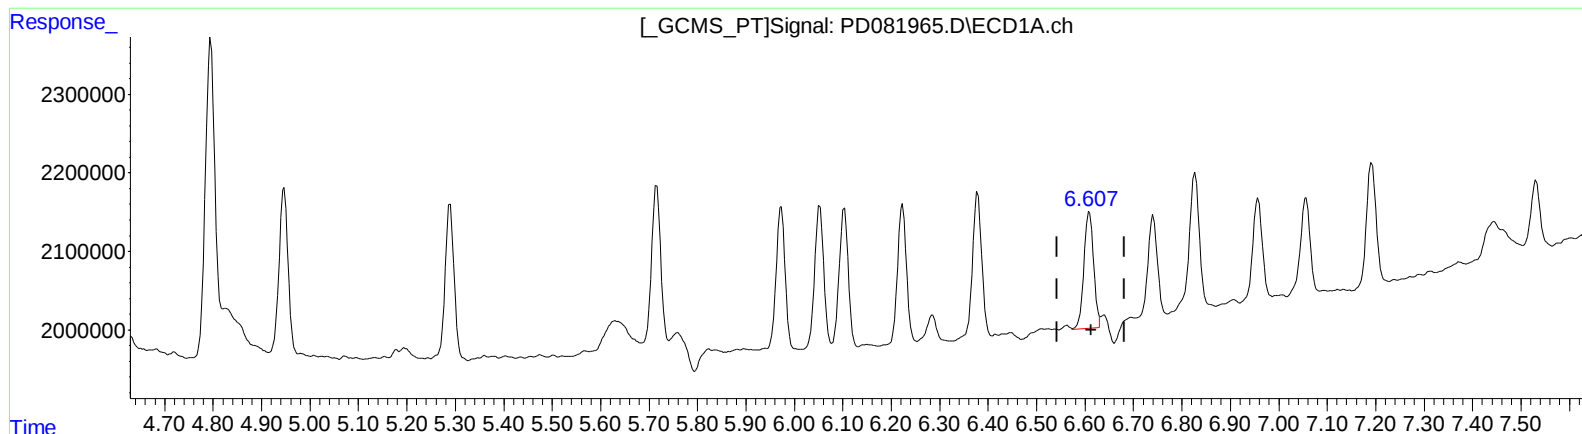

QEdit

(14) Endrin (MA)

6.607min 1.095 ng/ml m

response 2054504

(14) Endrin #2 (MA)

5.652min 1.144 ng/ml

response 3287039

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

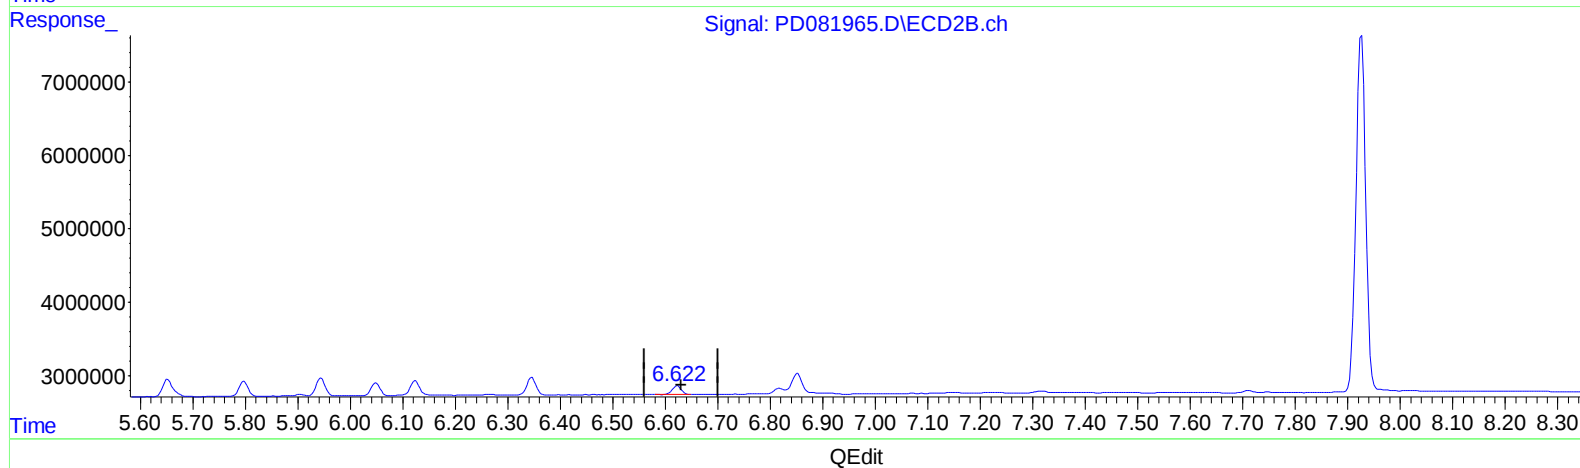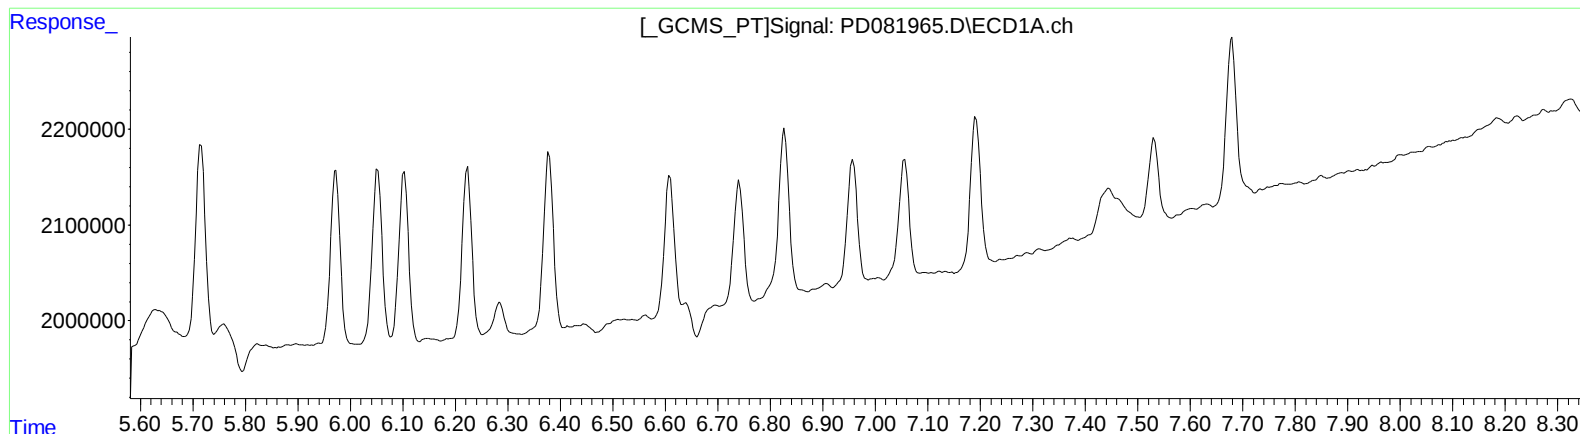

(20) Methoxychlor (A)

0.000min 0.000 ng/ml

response 0

(20) Methoxychlor #2 (A)

6.623min 0.986 ng/ml

response 1317385

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

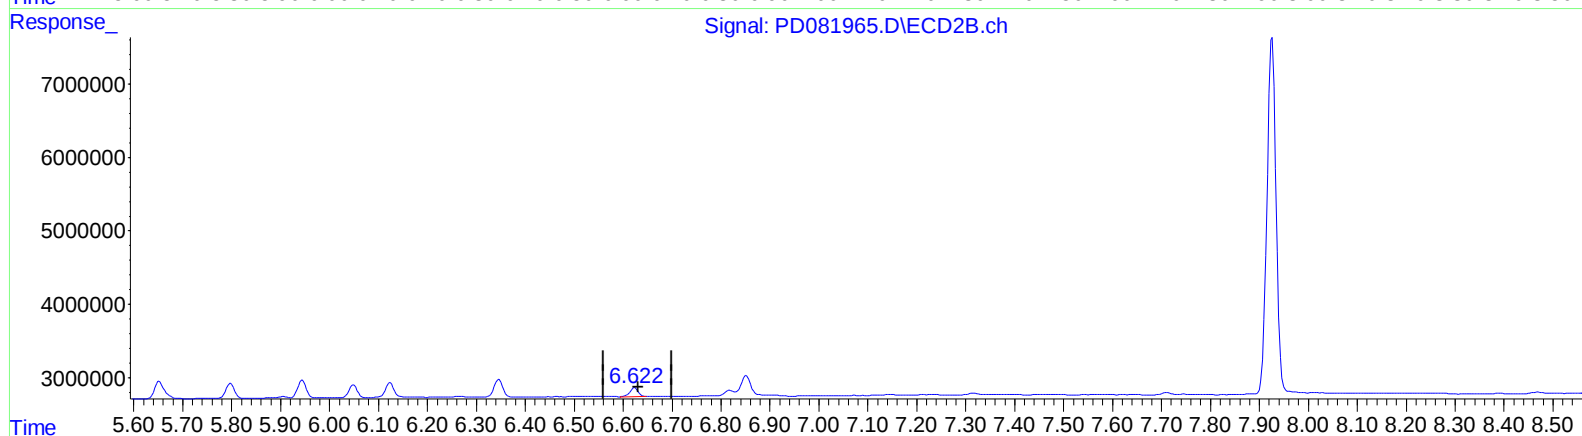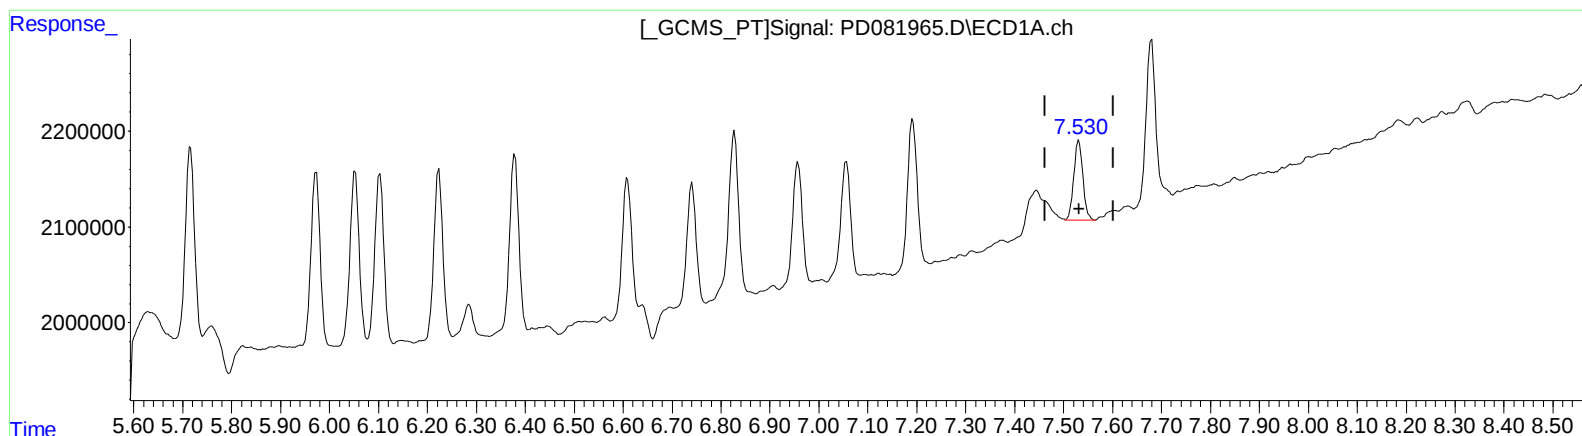

QEdit

(20) Methoxychlor (A)

7.530min 1.174 ng/ml m

response 1076710

(20) Methoxychlor #2 (A)

6.622min 1.034 ng/ml m

response 1381456

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

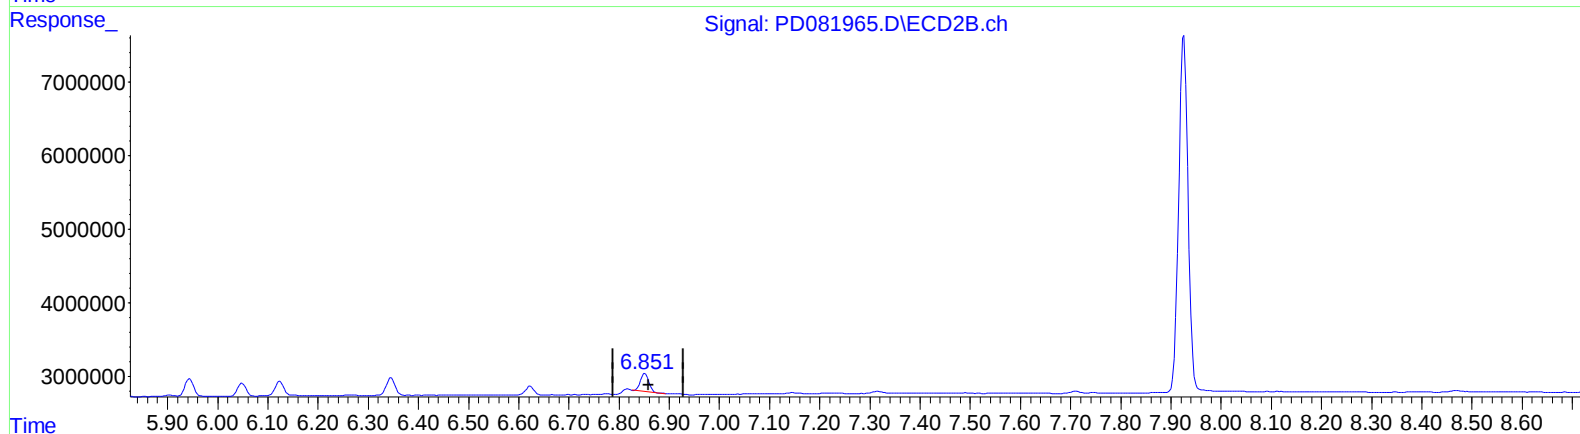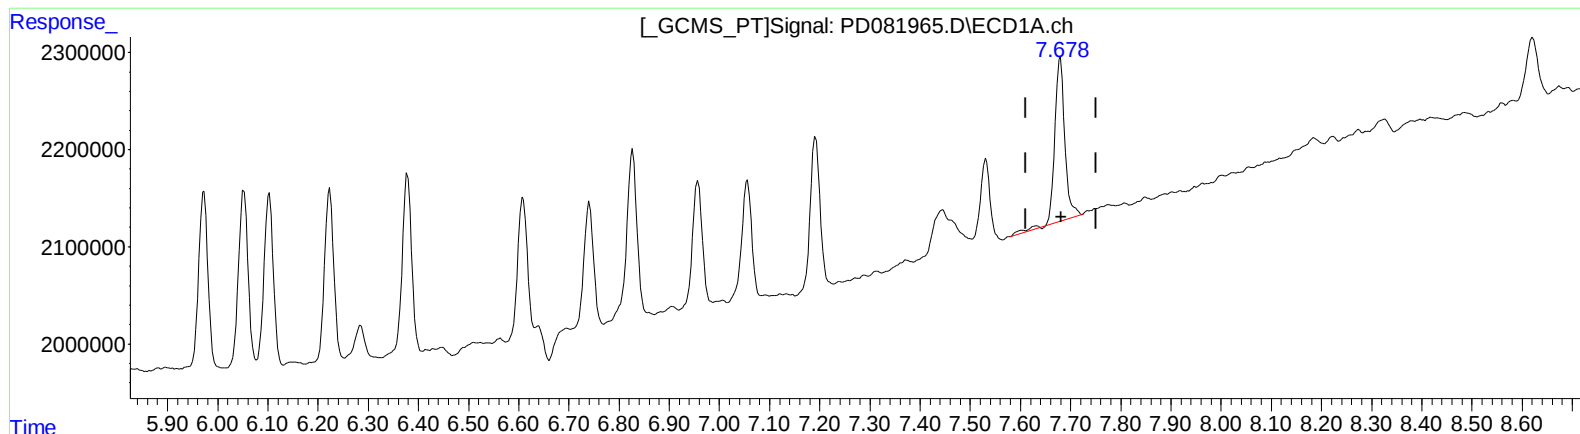

QEdit

(21) Endrin ketone (B)

7.680min 1.235 ng/ml

response 2389006

(21) Endrin ketone #2 (B)

6.852min 0.886 ng/ml

response 2656456

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030624\
Data File : PD081965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 11:32
Operator : AR\AJ
Sample : P1601-02
Misc : PEST MDL WATER 1PPB
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MDL-WATER-QT1-2024-02

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

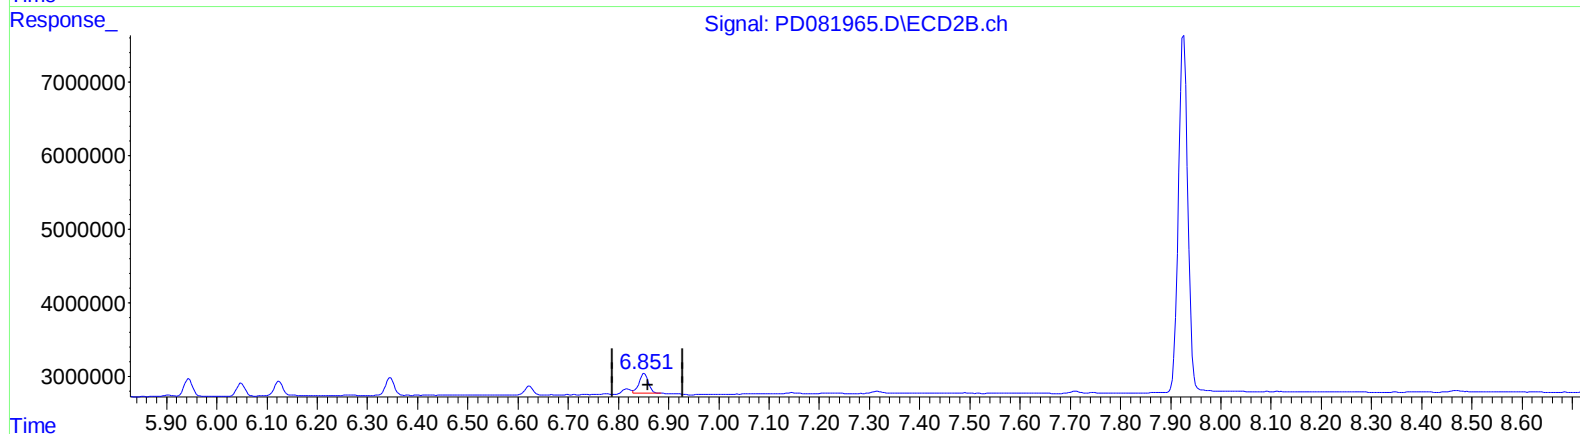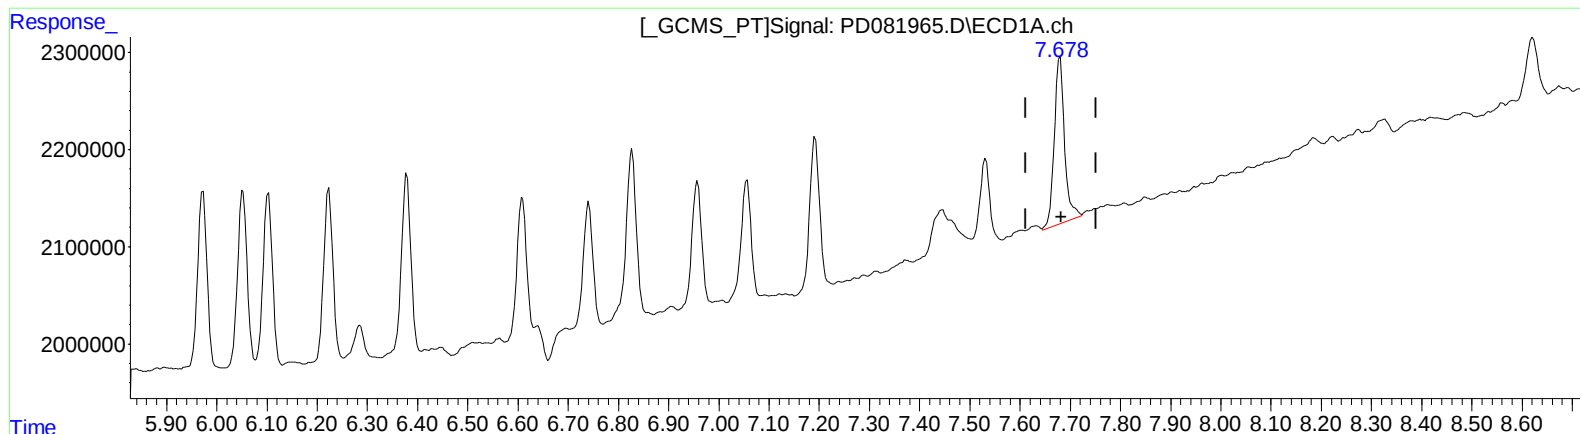

QEdit

(21) Endrin ketone (B)
7.678min 1.265 ng/ml m
response 2445920

(21) Endrin ketone #2 (B)
6.851min 1.135 ng/ml m
response 3404454