

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
 Data File : PD068361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 15:35
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/09/2022
 Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 15:47:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 07:11:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.451	4.177	64716170	499.8E6	51.208	50.414
7) SA Decachlor...	8.215	9.377	65892411	316.2E6	52.857	52.222
Target Compounds						
2) Toxaphene-1	5.708	6.197	5779427	15150742	543.360m	525.868
3) Toxaphene-2	5.927	6.801	8348786	59979721	535.771	510.131
4) Toxaphene-3	6.313	7.481	13298872	77389503	532.064	524.374
5) Toxaphene-4	6.561	7.621	14259725	30698712	513.375	523.458
6) Toxaphene-5	7.048	7.892	14750255	50935955	540.132	510.097m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
Data File : PD068361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 15:35
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 15:47:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 07:11:37 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

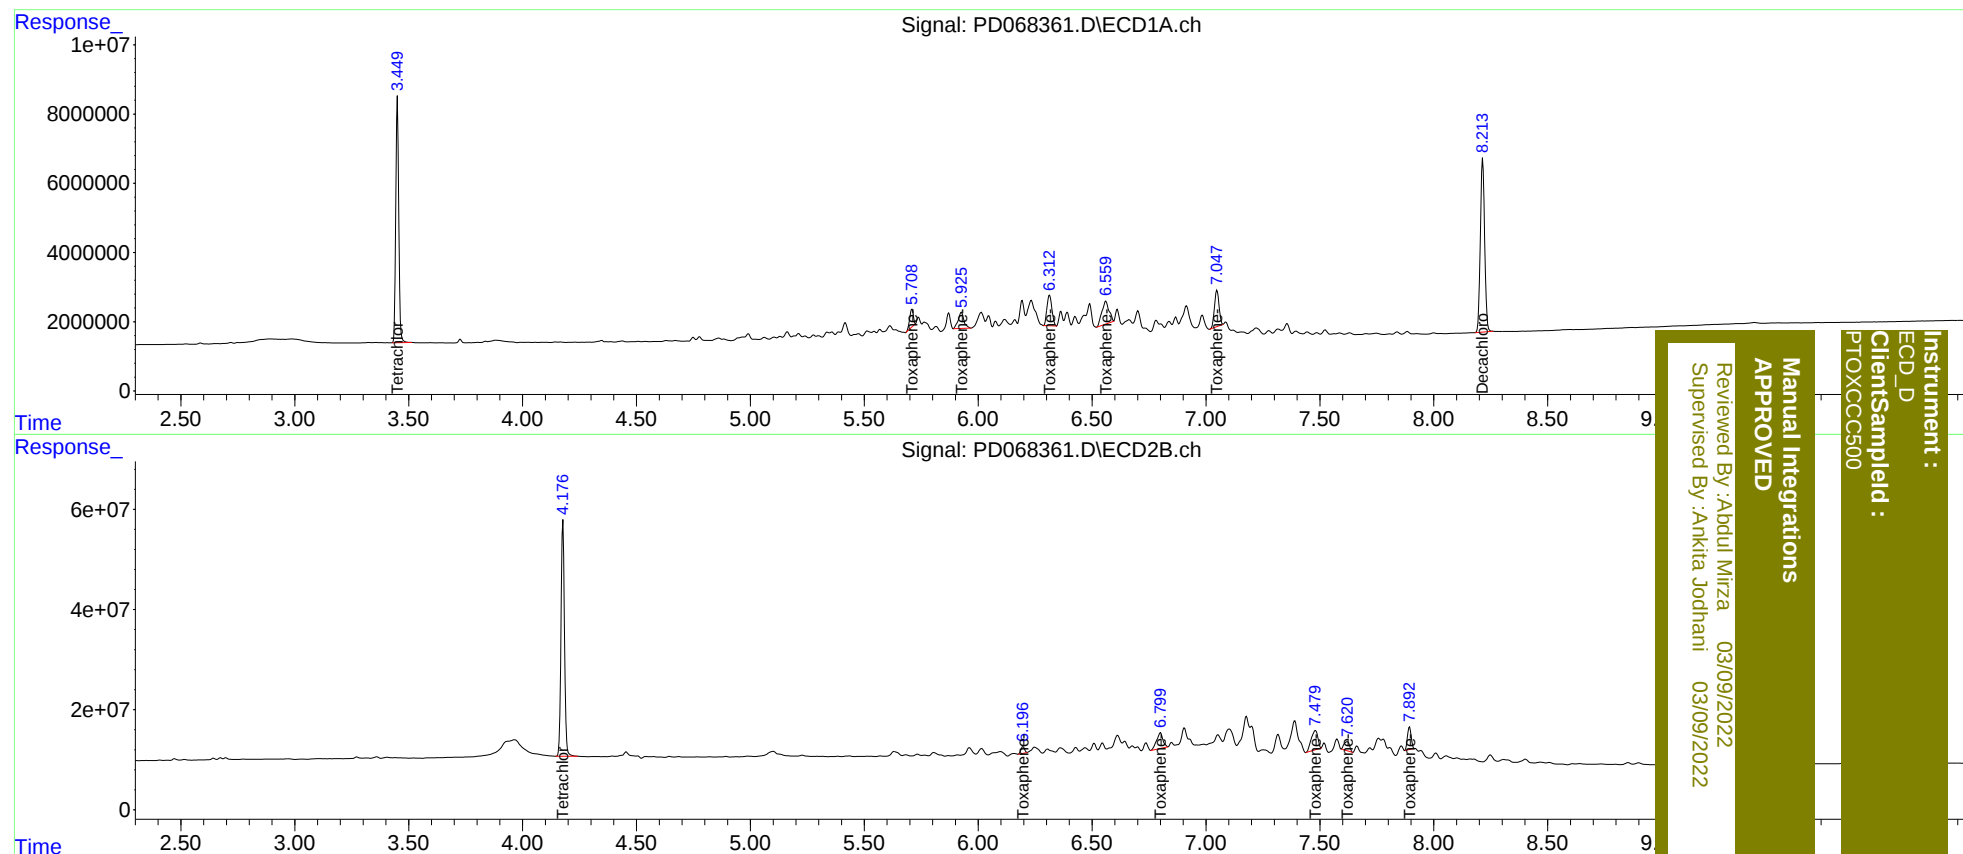

Instrument :
ECD_D
ClientSampled :
PTOXCCC500

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

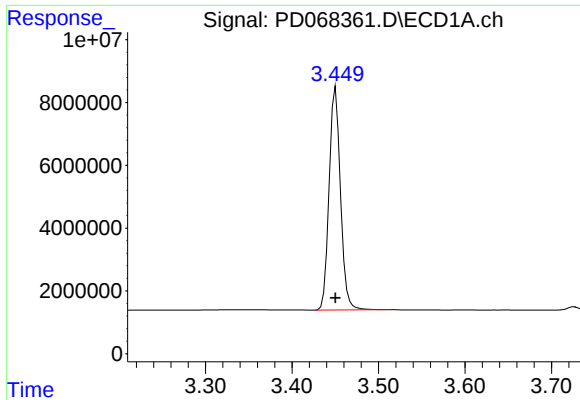


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 64716170
Conc: 51.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

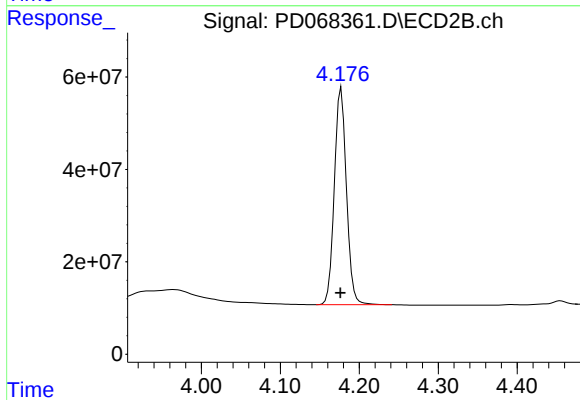


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: 0.001 min
Response: 499818059
Conc: 50.41 ng/ml

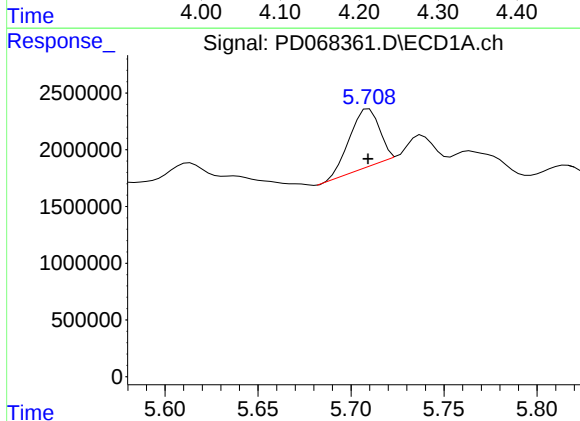


#2 Toxaphene-1

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 5779427
Conc: 543.36 ng/ml m

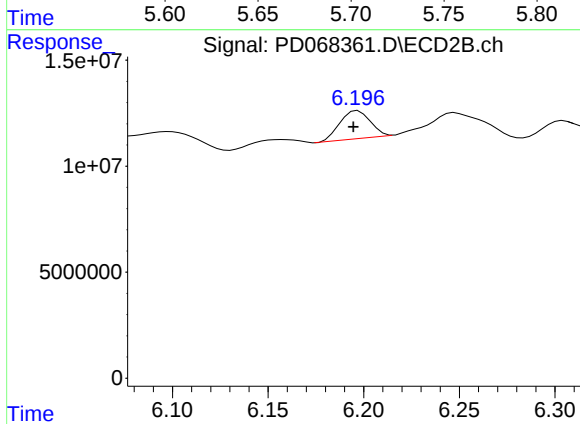

#2 Toxaphene-1

R.T.: 6.197 min
Delta R.T.: 0.002 min
Response: 15150742
Conc: 525.87 ng/ml

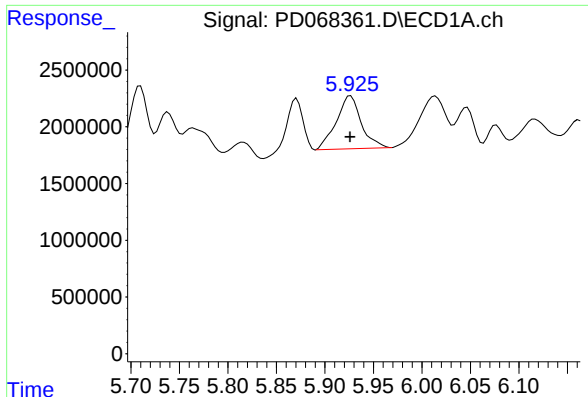


#3 Toxaphene-2

R.T.: 5.927 min
Delta R.T.: 0.000 min
Response: 8348786
Conc: 535.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

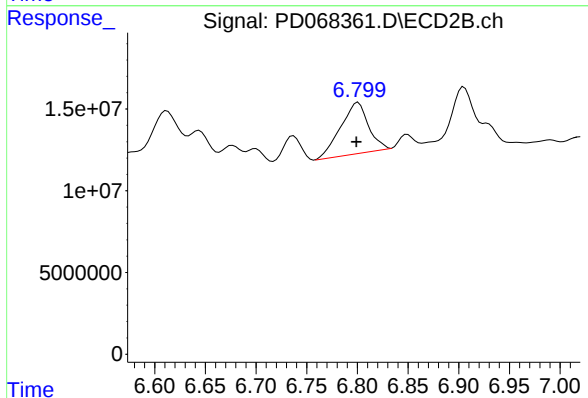


#3 Toxaphene-2

R.T.: 6.801 min
Delta R.T.: 0.002 min
Response: 59979721
Conc: 510.13 ng/ml

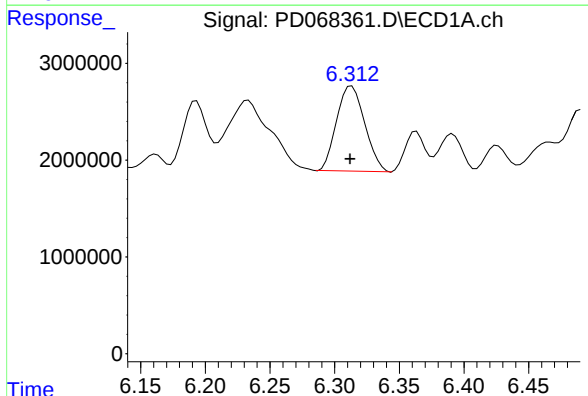


#4 Toxaphene-3

R.T.: 6.313 min
Delta R.T.: 0.001 min
Response: 13298872
Conc: 532.06 ng/ml

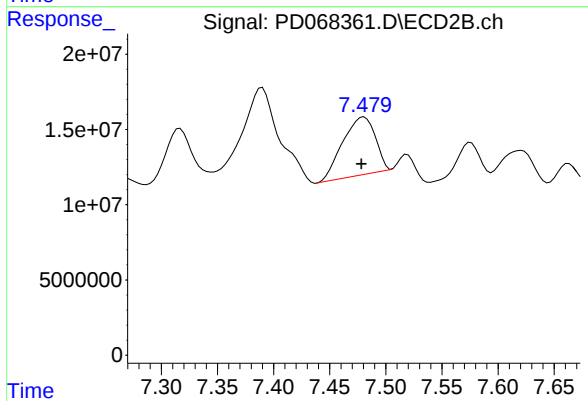

#4 Toxaphene-3

R.T.: 7.481 min
Delta R.T.: 0.002 min
Response: 77389503
Conc: 524.37 ng/ml

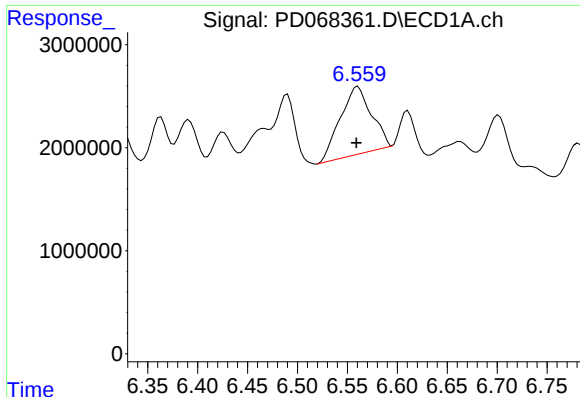


#5 Toxaphene-4

R.T.: 6.561 min
Delta R.T.: 0.002 min
Response: 14259725
Conc: 513.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

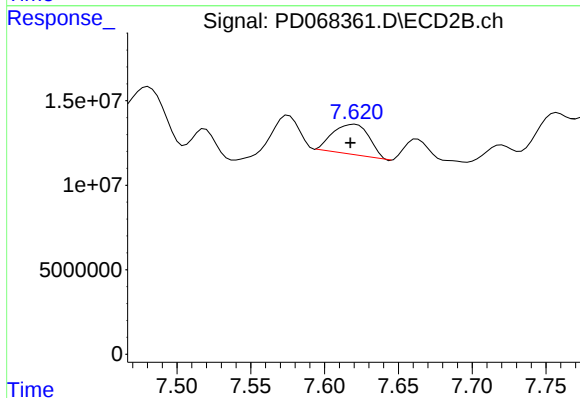


#5 Toxaphene-4

R.T.: 7.621 min
Delta R.T.: 0.003 min
Response: 30698712
Conc: 523.46 ng/ml

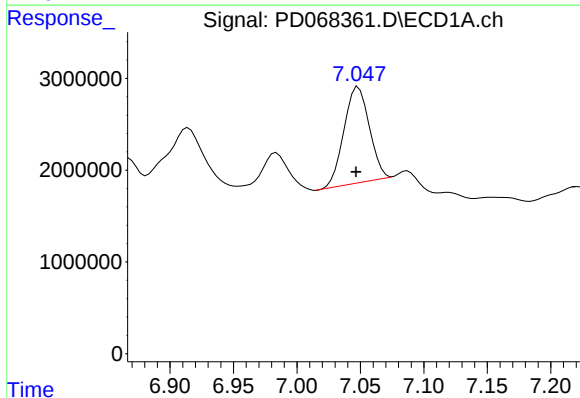


#6 Toxaphene-5

R.T.: 7.048 min
Delta R.T.: 0.002 min
Response: 14750255
Conc: 540.13 ng/ml

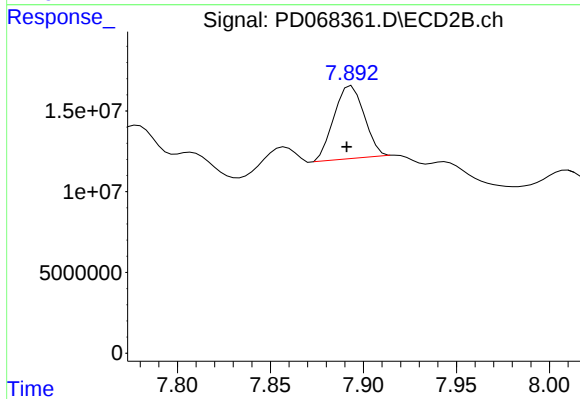

#6 Toxaphene-5

R.T.: 7.892 min
Delta R.T.: 0.001 min
Response: 50935955
Conc: 510.10 ng/ml m

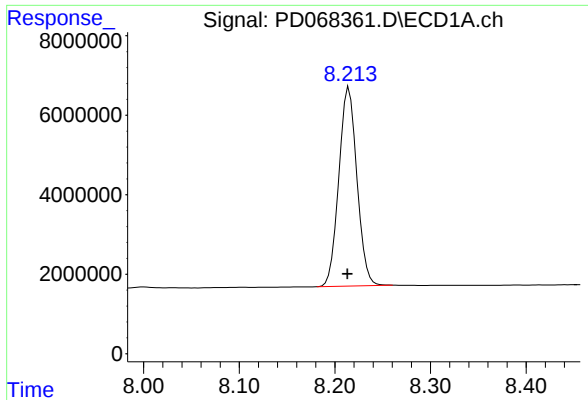


#7 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.002 min
Response: 65892411
Conc: 52.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PTOXCCC500

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

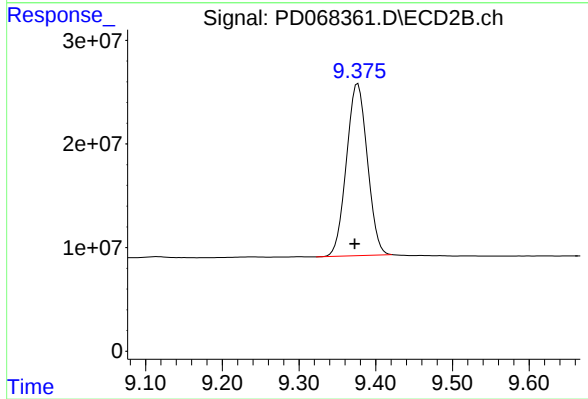

#7 Decachlorobiphenyl

R.T.: 9.377 min
Delta R.T.: 0.004 min
Response: 316169784
Conc: 52.22 ng/ml