

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
 Data File : PD068365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 16:41
 Operator : AR\AJ
 Sample : N1805-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NB-08-030422

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/09/2022
 Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 00:59:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	14011581	109.6E6	11.953m	11.415m
28)	SA Decachlor...	8.215	9.377	15387100	82740914	13.222	13.956

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
Data File : PD068365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 16:41
Operator : AR\AJ
Sample : N1805-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NB-08-030422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 00:59:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

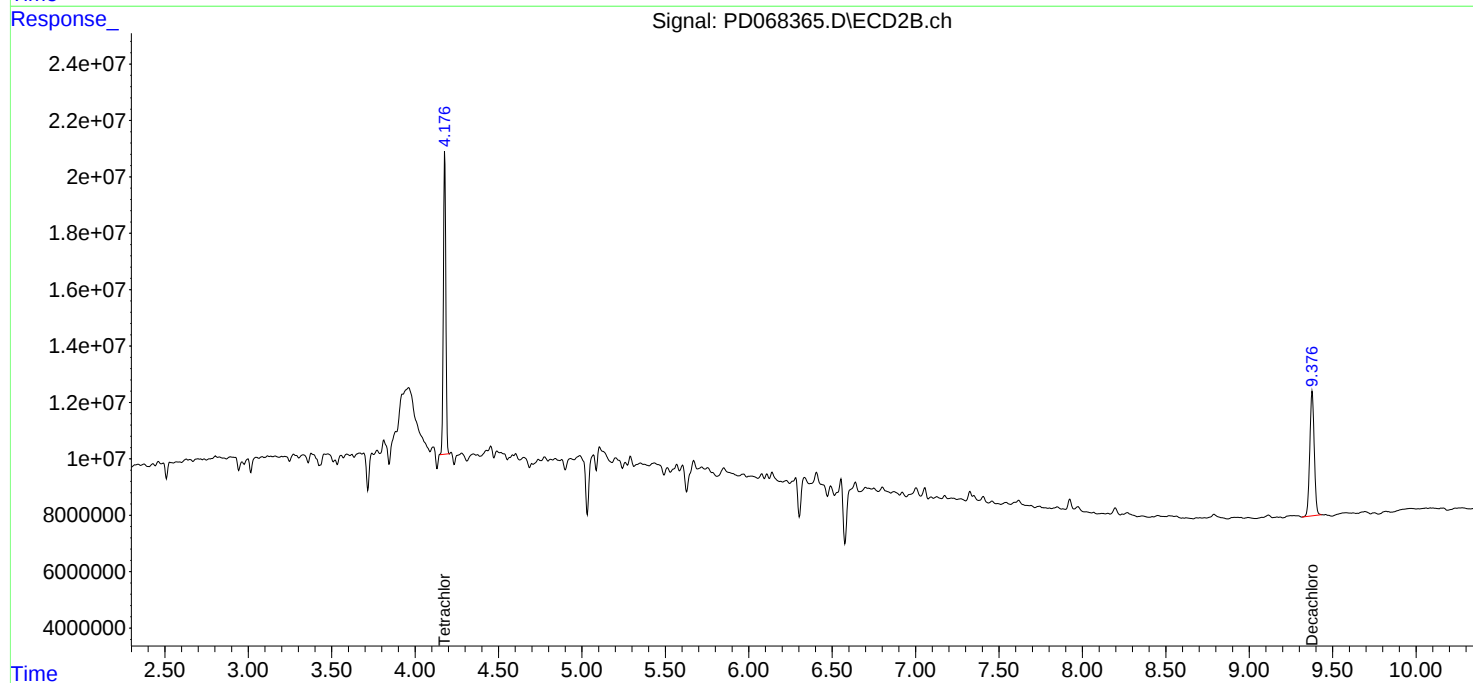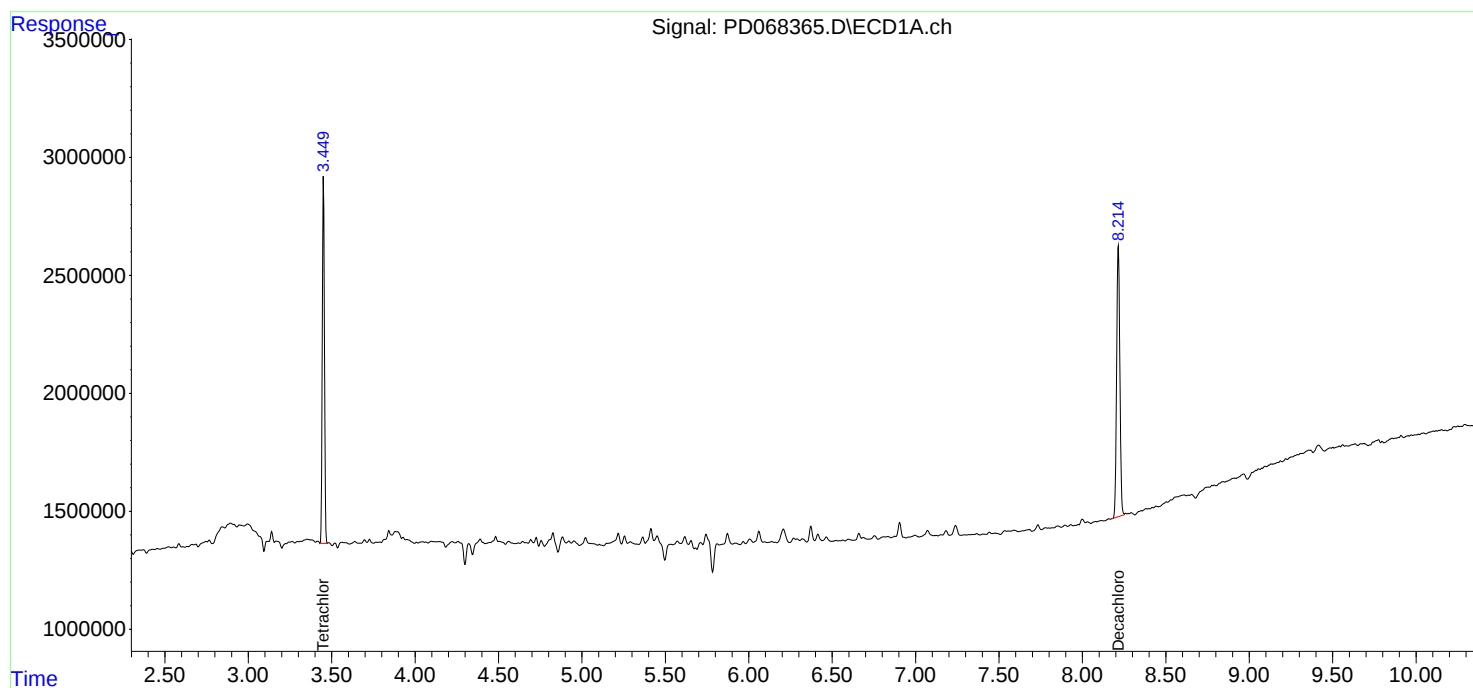

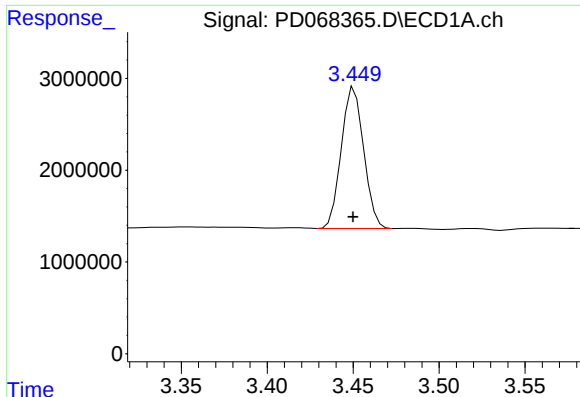

#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 14011581
Conc: 11.95 ng/ml

Instrument :

ECD_D


ClientSampleId :

NB-08-030422

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

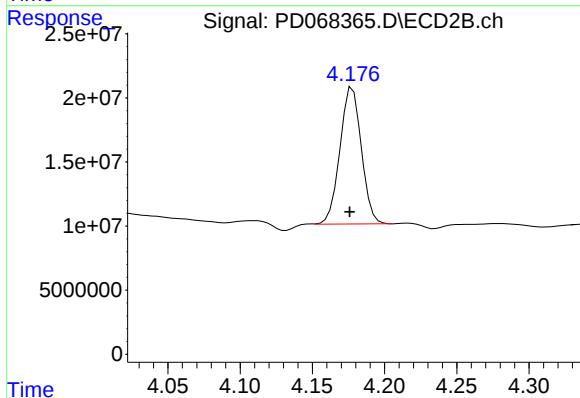


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 109563757
Conc: 11.42 ng/ml m

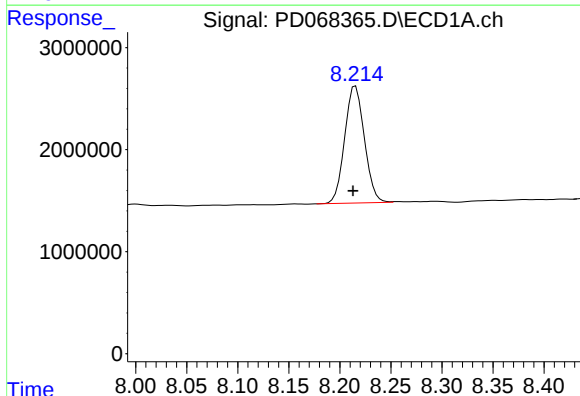

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: 0.003 min
Response: 15387100
Conc: 13.22 ng/ml

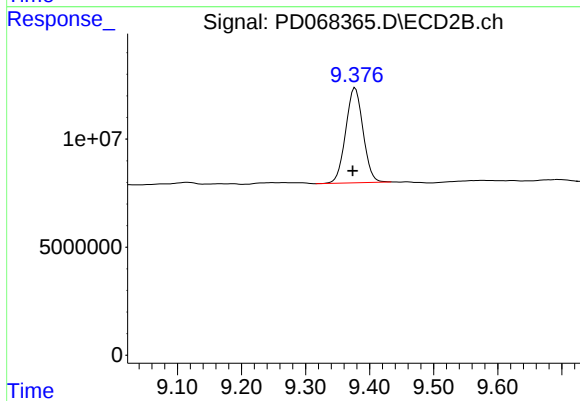

#28 Decachlorobiphenyl

R.T.: 9.377 min
Delta R.T.: 0.004 min
Response: 82740914
Conc: 13.96 ng/ml