

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
 Data File : PD068378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 20:56
 Operator : AR\AJ
 Sample : N1808-01 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CL-01-030422

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/09/2022
 Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 01:05:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.449	4.178	2061703	17515342	1.759m	1.825
2) SA Decachlor...	8.216	9.379	1985829	11373321	1.706	1.918

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030722\
Data File : PD068378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 20:56
Operator : AR\AJ
Sample : N1808-01 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CL-01-030422


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/09/2022
Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 01:05:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

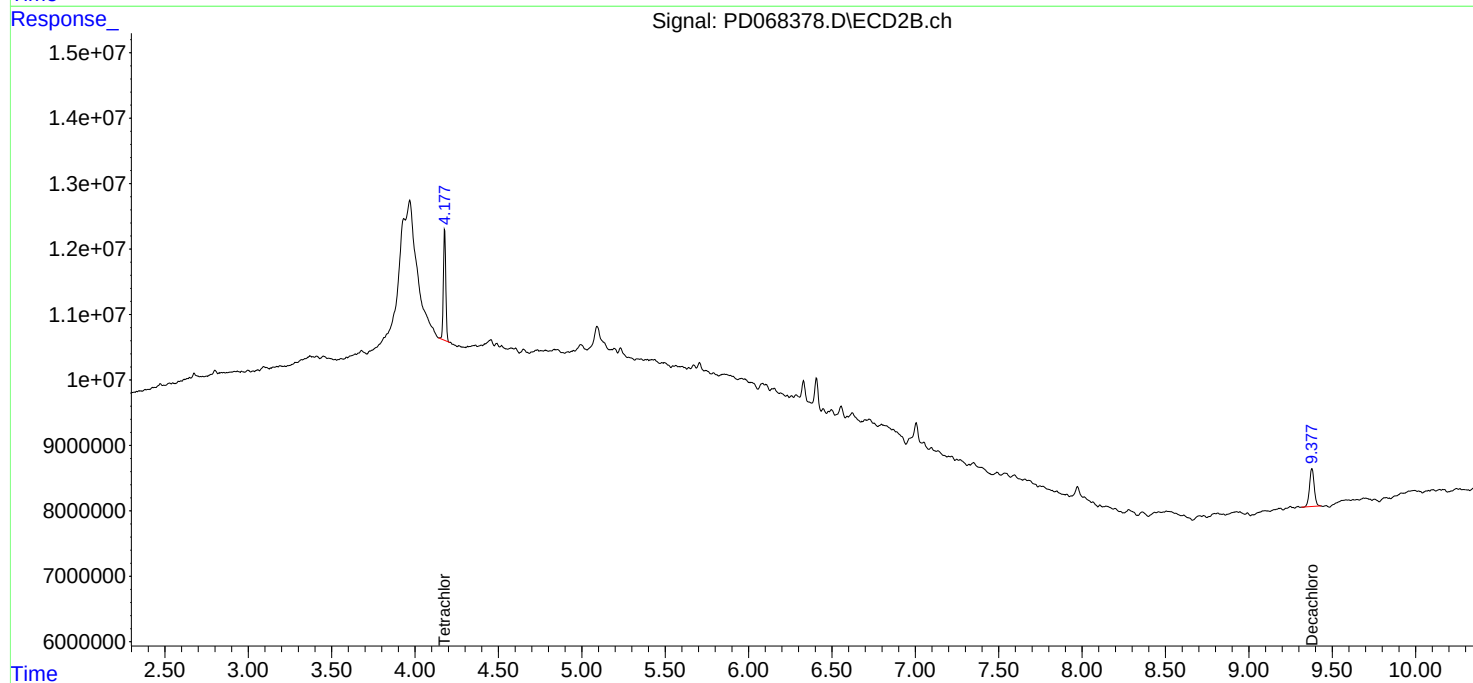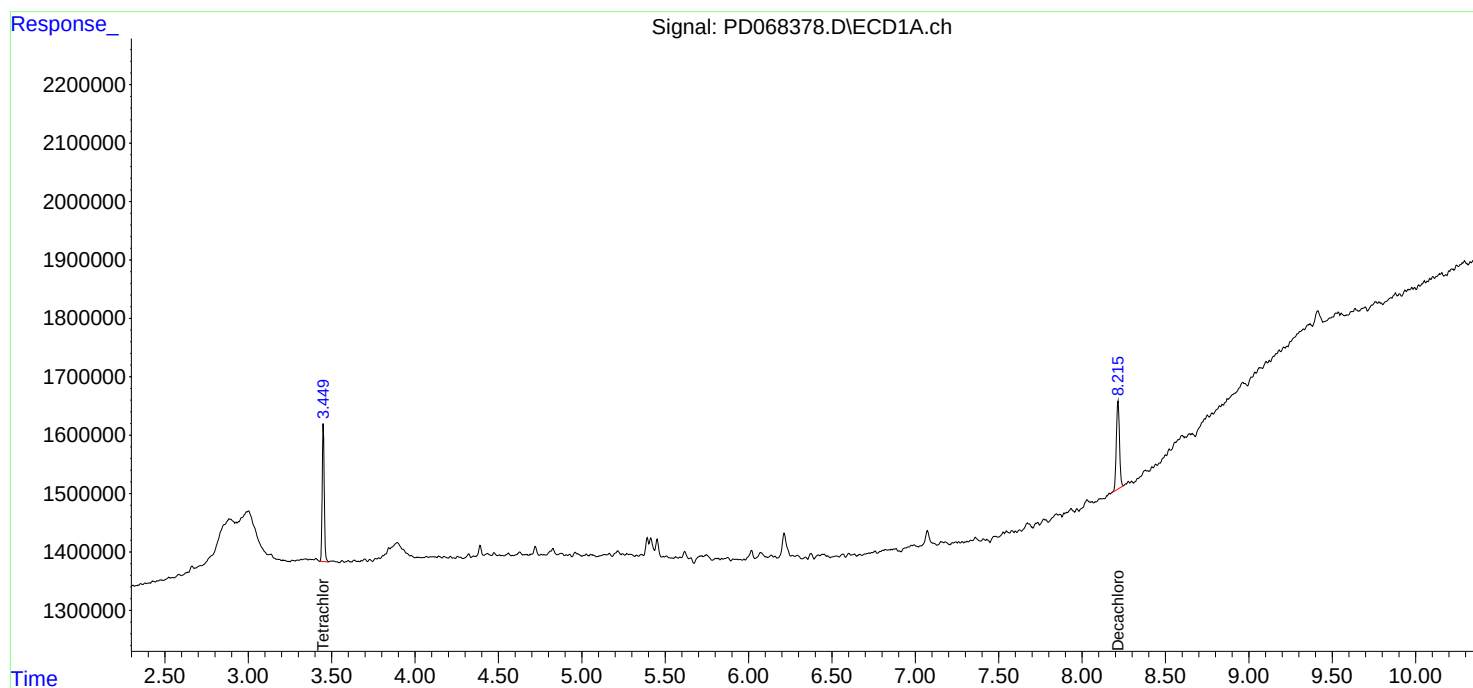

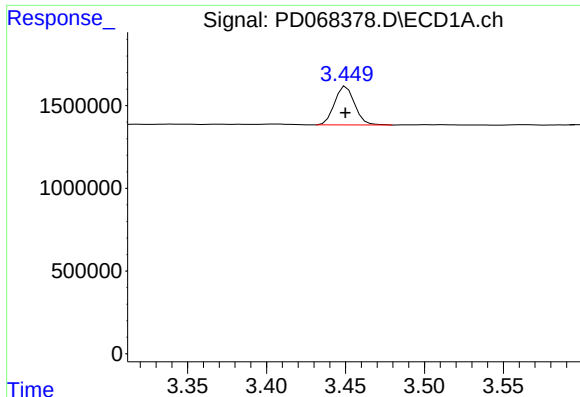


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: 0.000 min
Response: 2061703
Conc: 1.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
CL-01-030422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

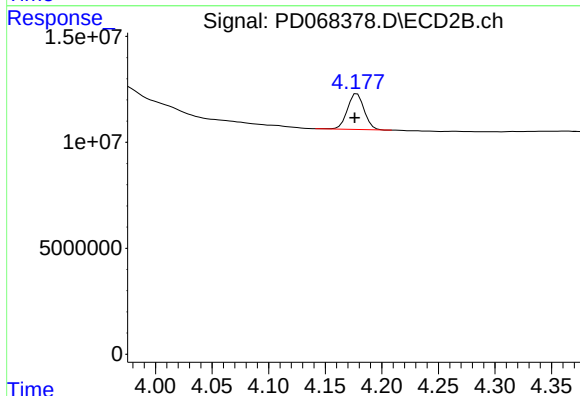


#1 Tetrachloro-m-xylene

R.T.: 4.178 min
Delta R.T.: 0.002 min
Response: 17515342
Conc: 1.82 ng/ml

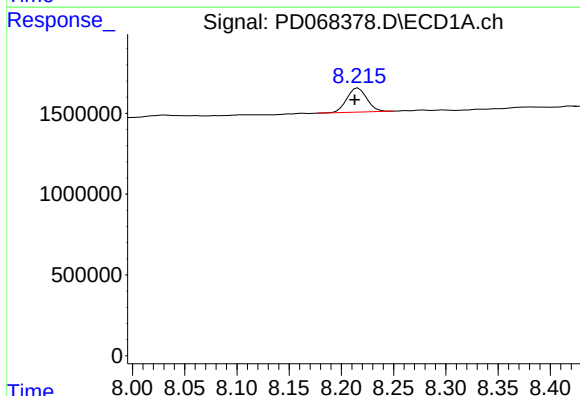

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: 0.003 min
Response: 1985829
Conc: 1.71 ng/ml

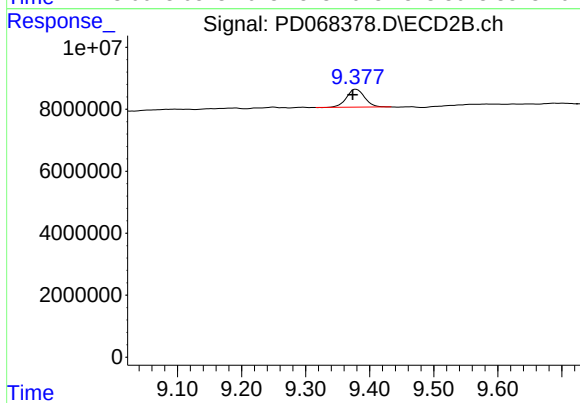

#28 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: 0.005 min
Response: 11373321
Conc: 1.92 ng/ml