

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
 Data File : PD082020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 18:18
 Operator : AR\AJ
 Sample : P1652-02MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRQ3MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/08/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 21:44:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.791	19537858	34393592	14.291	14.029
27)	SA Decachlor...	9.109	7.925	30204291	41726393	15.655	16.820
Target Compounds							
2)	A alpha-BHC	4.019	3.291	111.0E6	182.5E6	47.529m	47.474m
3)	MA gamma-BHC...	4.354	3.621	112.4E6	173.9E6	48.641	48.014
4)	MA Heptachlor	4.946	3.962	115.3E6	169.7E6	47.013	47.839
5)	MB Aldrin	5.289	4.240	108.0E6	146.6E6	45.684	43.284m
6)	B beta-BHC	4.549	3.917	48176138	73758917	46.358	43.652
7)	B delta-BHC	4.798	4.147	96386466	147.8E6	40.696	39.459
8)	B Heptachlo...	5.716	4.743	101.8E6	151.9E6	44.964	47.353
9)	A Endosulfan I	6.103	5.113	95613347	139.9E6	45.408	46.726
10)	B trans-Chl...	5.972	4.993	98642302	149.0E6	45.055	47.744
11)	B cis-Chlor...	6.052	5.057	102.9E6	152.6E6	45.669	47.620
12)	B 4,4'-DDE	6.223	5.244	196.7E6	288.3E6	91.650	97.505m
13)	MA Dieldrin	6.378	5.376	210.5E6	316.2E6	94.824	96.277m
14)	MA Endrin	6.608	5.651	173.5E6	278.8E6	92.471	97.030m
15)	B Endosulfa...	6.826	5.945	175.0E6	264.3E6	90.664	93.637
16)	A 4,4'-DDD	6.740	5.799	154.1E6	234.3E6	92.780	92.959
17)	MA 4,4'-DDT	7.055	6.049	165.6E6	248.2E6	95.334	96.109
18)	B Endrin al...	6.957	6.124	128.2E6	191.3E6	85.840	88.290
19)	B Endosulfa...	7.191	6.346	164.4E6	241.9E6	89.814	90.188
20)	A Methoxychlor	7.530	6.624	411.0E6	582.5E6	448.037	435.968
21)	B Endrin ke...	7.678	6.851	189.7E6	286.3E6	98.111	95.490m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
Data File : PD082020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 18:18
Operator : AR\AJ
Sample : P1652-02MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 21:44:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

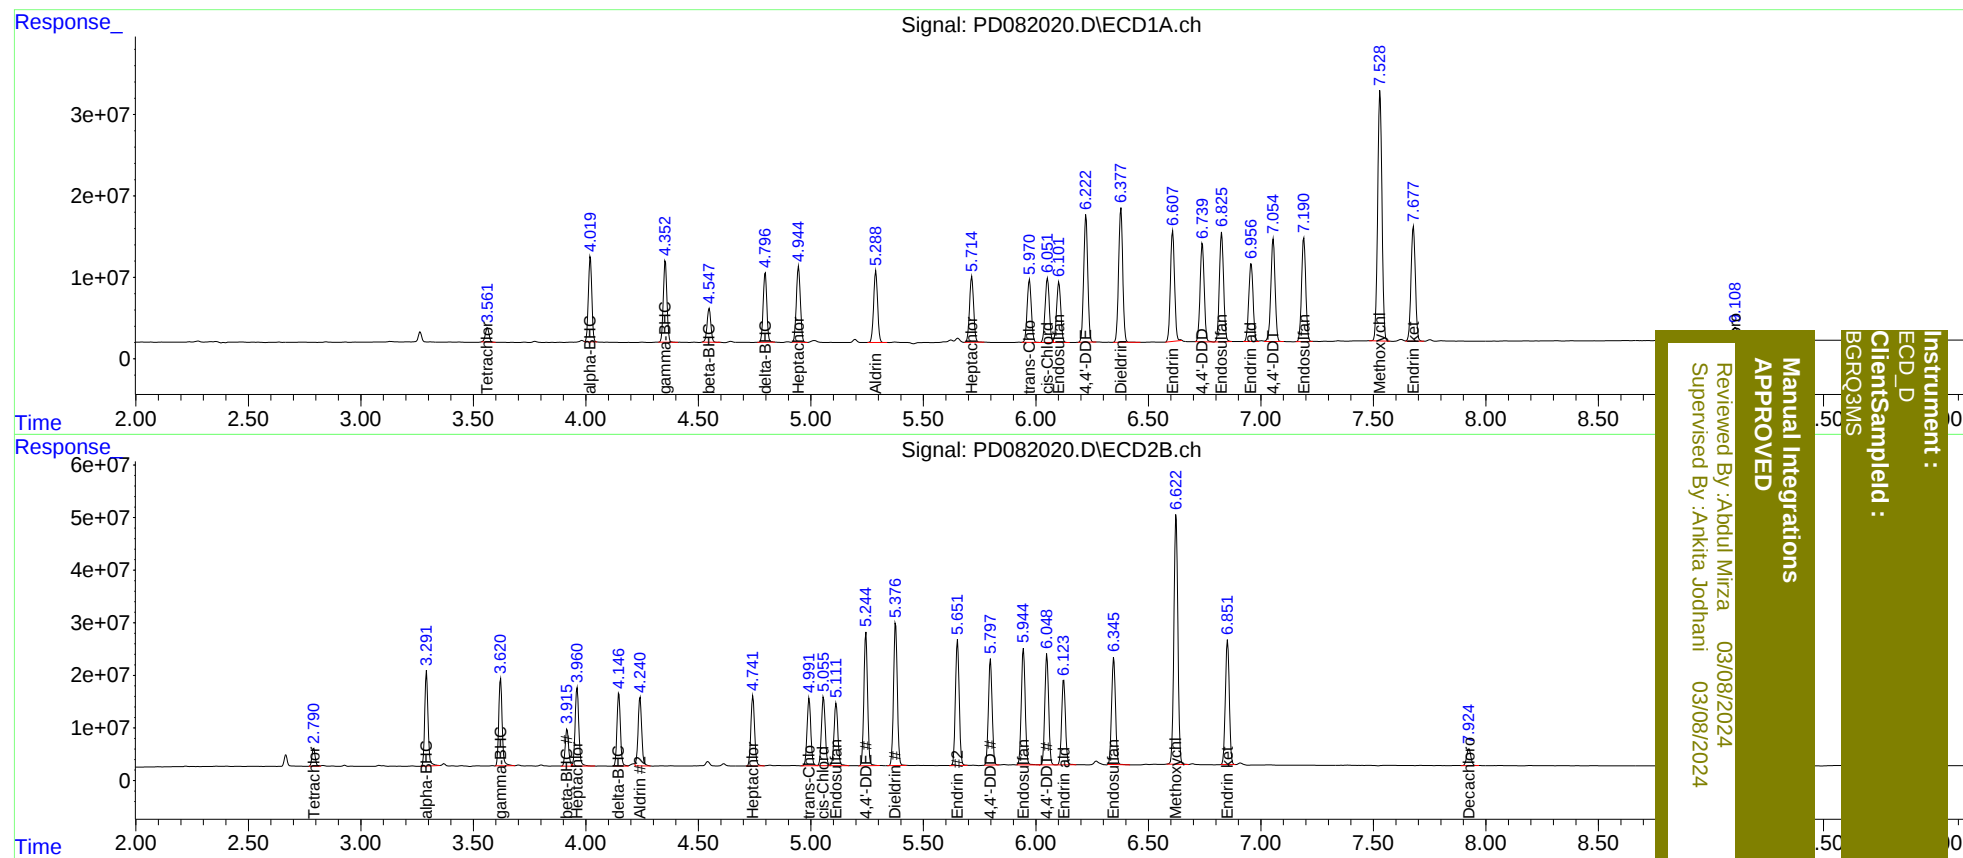

Reviewed By: Abdul Mirza 03/08/2024
Supervised By: Ankita Jodhani 03/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGRO3MS