

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
 Data File : PD082021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 18:32
 Operator : AR\AJ
 Sample : P1652-03MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRQ3MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/08/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 21:45:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.790	18563715	34003695	13.579	13.870
27)	SA Decachlor...	9.109	7.926	30550660	41516688	15.835	16.736
Target Compounds							
2)	A alpha-BHC	4.018	3.290	107.7E6	182.6E6	46.101m	47.503m
3)	MA gamma-BHC...	4.353	3.621	109.6E6	174.2E6	47.449	48.084
4)	MA Heptachlor	4.945	3.961	114.8E6	170.1E6	46.829	47.949
5)	MB Aldrin	5.289	4.239	108.0E6	149.9E6	45.673	44.261m
6)	B beta-BHC	4.548	3.916	47619611	73784999	45.822	43.668
7)	B delta-BHC	4.797	4.147	94551090	148.1E6	39.921	39.548
8)	B Heptachlo...	5.716	4.743	101.4E6	152.1E6	44.770	47.416
9)	A Endosulfan I	6.102	5.112	96771772	140.2E6	45.959	46.810
10)	B trans-Chl...	5.972	4.992	98501070	149.1E6	44.991	47.791
11)	B cis-Chlor...	6.051	5.056	103.3E6	152.7E6	45.870	47.672
12)	B 4,4'-DDE	6.223	5.243	198.4E6	287.1E6	92.420	97.106m
13)	MA Dieldrin	6.378	5.375	210.1E6	315.1E6	94.629	95.943m
14)	MA Endrin	6.609	5.650	172.2E6	278.4E6	91.743	96.911m
15)	B Endosulfa...	6.827	5.945	174.6E6	263.8E6	90.460	93.471
16)	A 4,4'-DDD	6.740	5.798	152.6E6	234.1E6	91.889	92.906
17)	MA 4,4'-DDT	7.055	6.049	166.5E6	246.6E6	95.828	95.489
18)	B Endrin al...	6.957	6.124	127.8E6	189.6E6	85.520	87.508
19)	B Endosulfa...	7.192	6.345	165.7E6	241.9E6	90.490	90.160m
20)	A Methoxychlor	7.530	6.624	412.3E6	579.1E6	449.519	433.436
21)	B Endrin ke...	7.678	6.851	188.7E6	285.5E6	97.567	95.206m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
Data File : PD082021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 18:32
Operator : AR\AJ
Sample : P1652-03MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 21:45:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

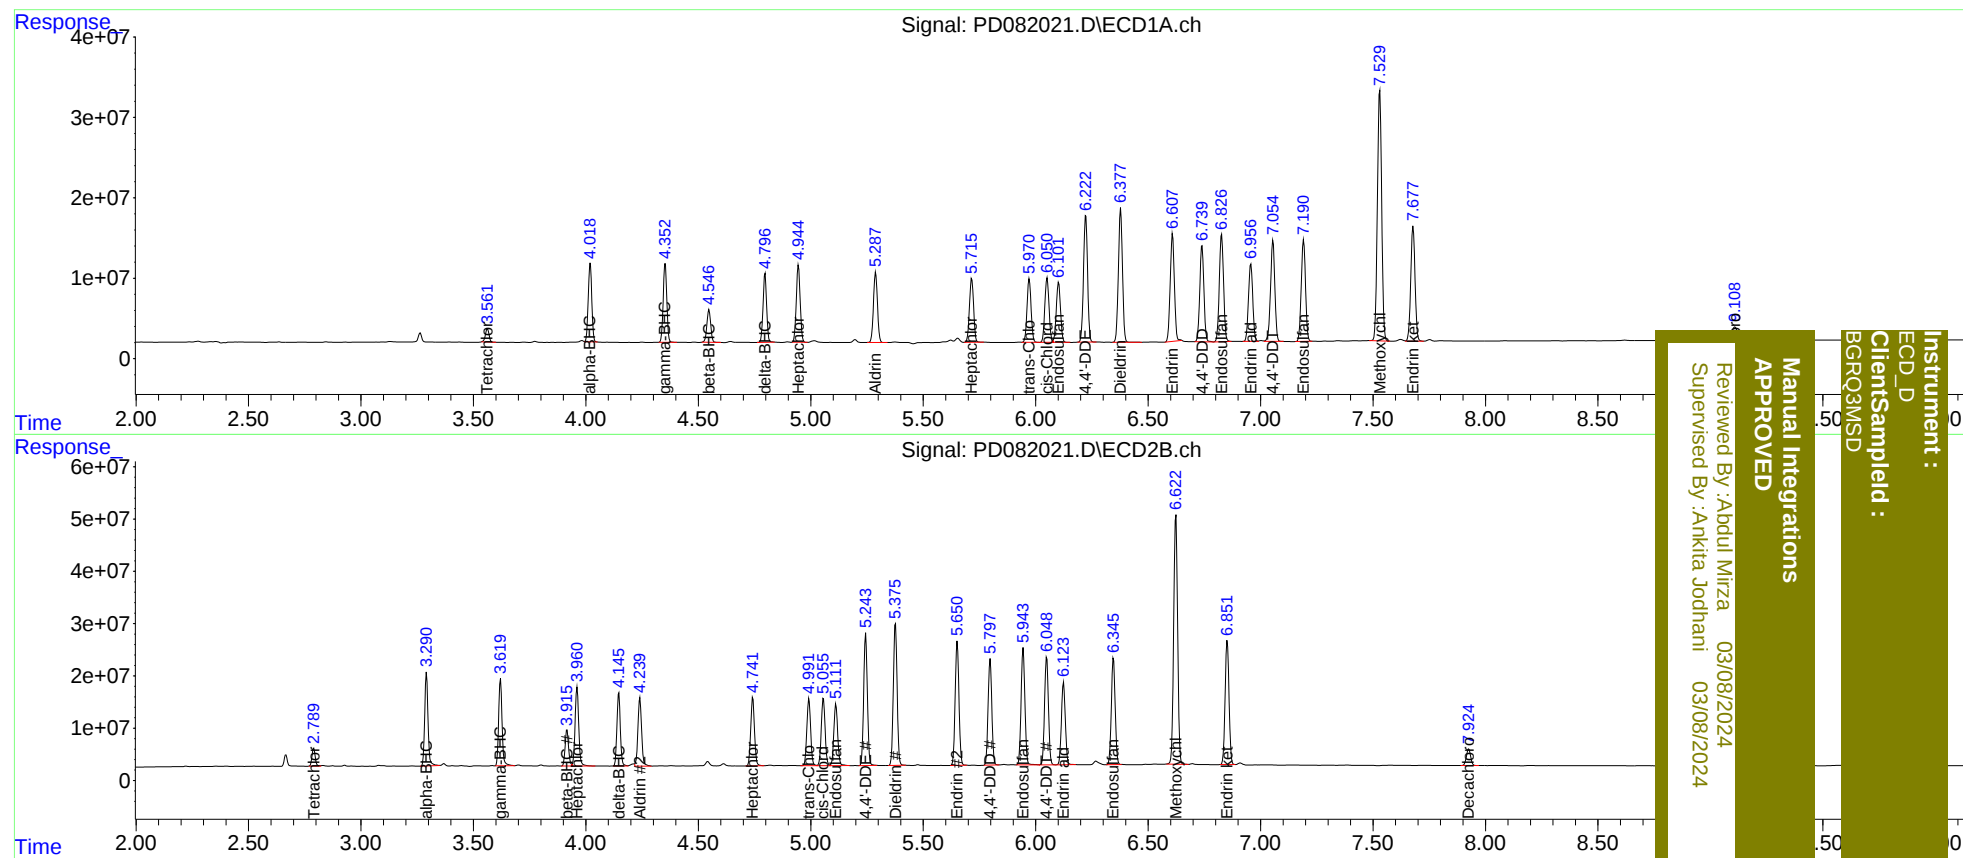

Reviewed By: Abdul Mirza 03/08/2024
Supervised By: Ankita Jodhani 03/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BGR03MSD