

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
 Data File : PD082033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 21:11
 Operator : AR\AJ
 Sample : P1652-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGR90

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/08/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 21:48:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 17:06:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.791	15242811	26980719	11.149	11.006
2)	SA Decachlor...	9.107	7.925	22740771	35395697	11.787m	14.268
Target Compounds							
13)	MA Dieldrin	6.378	5.376	302.9E6	447.6E6	136.419	136.273
16)	A 4,4'-DDD	6.746	5.807	1943340	1191844	1.170m	0.473m#
19)	B Endosulfa...	7.188	6.378	4267086	2604548	2.331	0.971m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030724\
Data File : PD082033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 21:11
Operator : AR\AJ
Sample : P1652-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 21:48:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD021224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 17:06:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

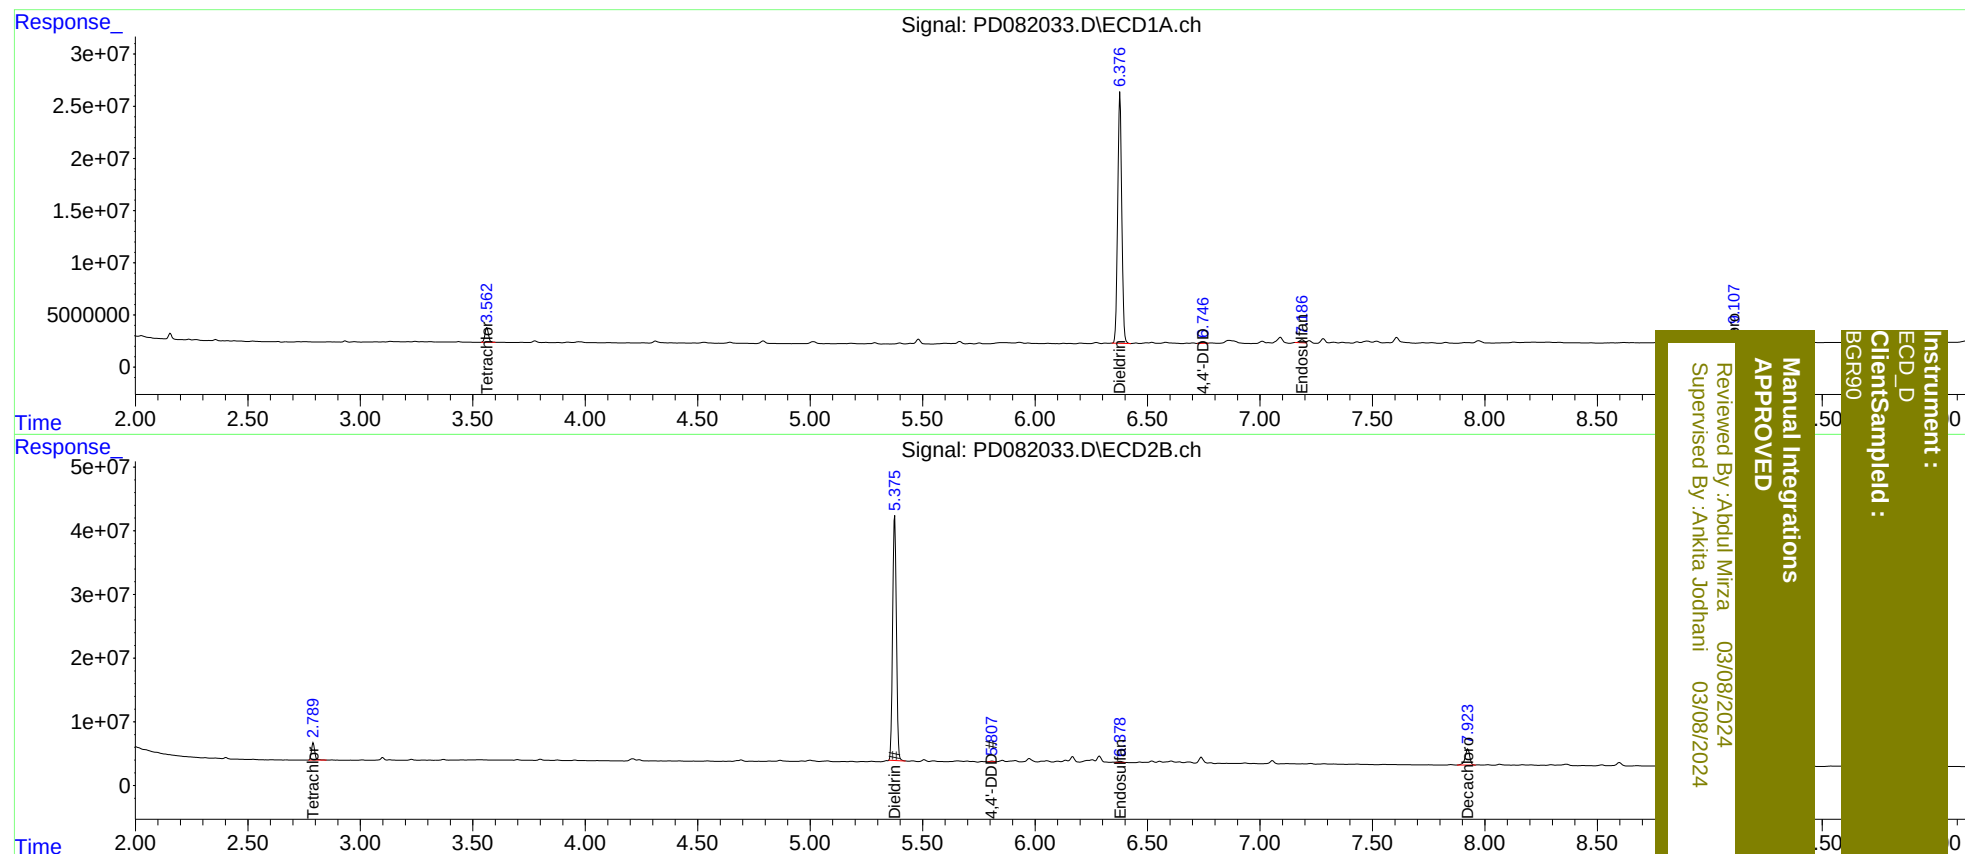

Reviewed By: Abdul Mirza 03/08/2024
Supervised By: Ankita Jodhani 03/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BGR90