

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051651.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 9:46
 Operator : AJ\SJ
 Sample : PIBLK19
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:53:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.223	4.043	29558581	674.5E6	20.569	21.830
2) SA Decachlor...	7.822	9.154	51739018	767.1E6	43.021	40.467
Target Compounds						
6) B beta-BHC	0.000	4.938f	0	47475883	N.D.	2.393

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051651.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 9:46
Operator : AJ\SJ
Sample : PIBLK19
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:53:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

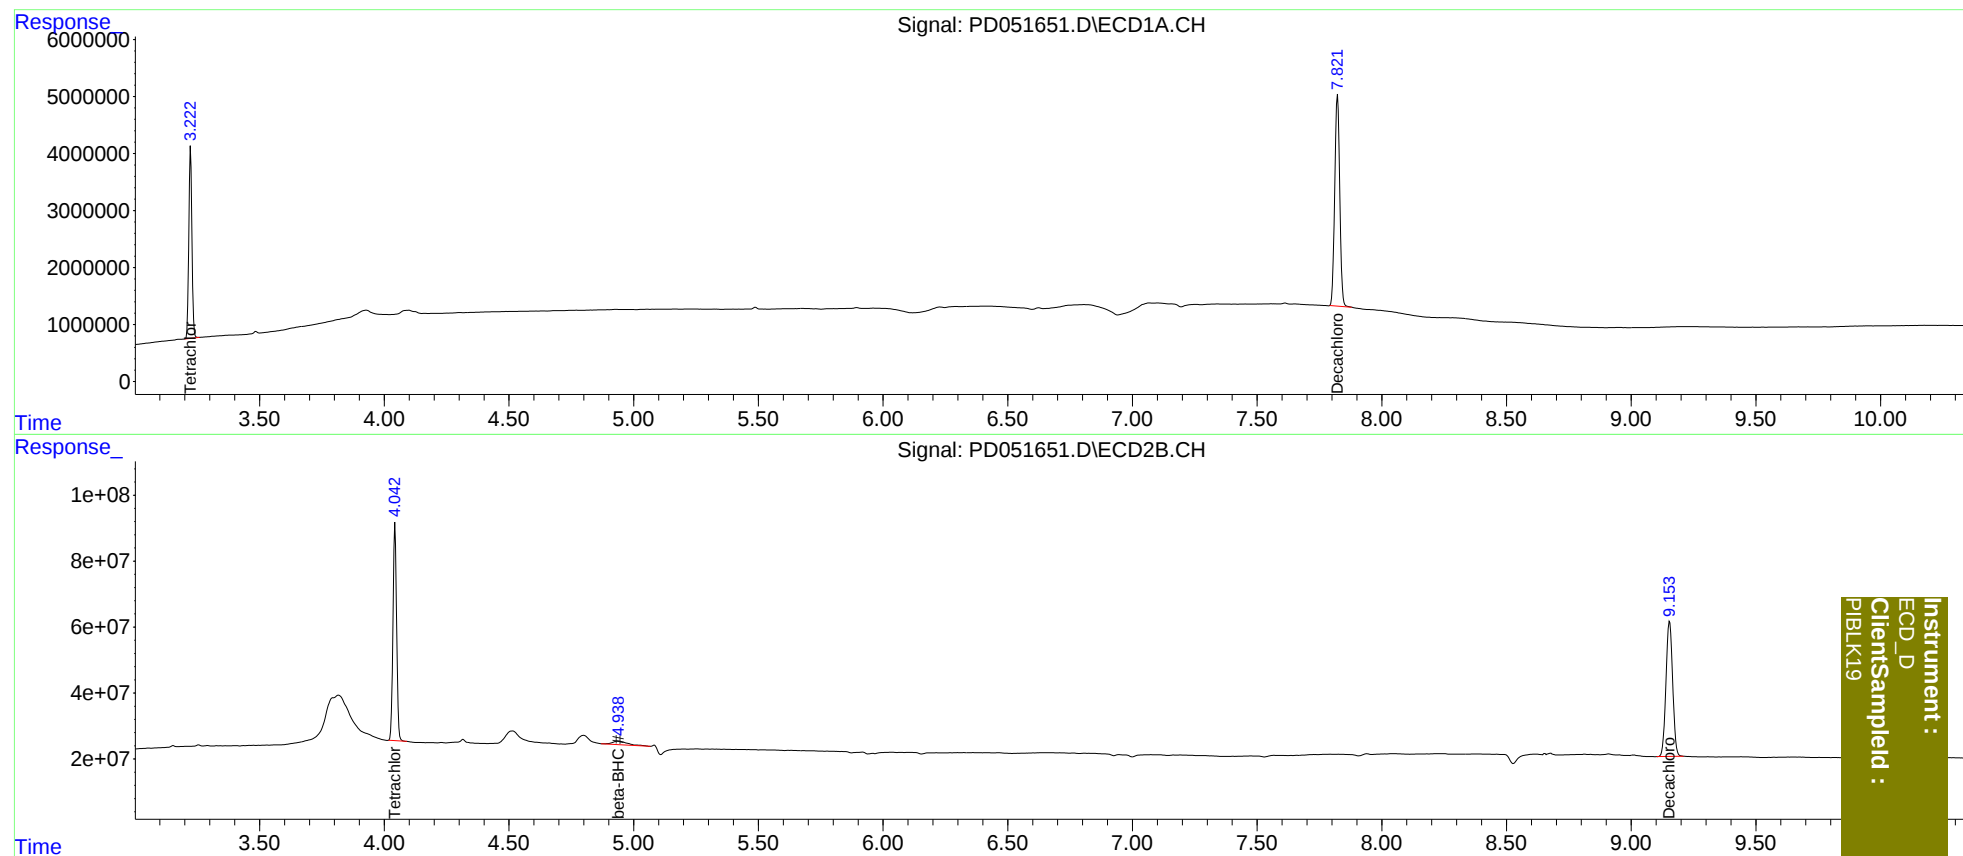


Instrument :
ECD_D
ClientSampleId :
PIBLK19

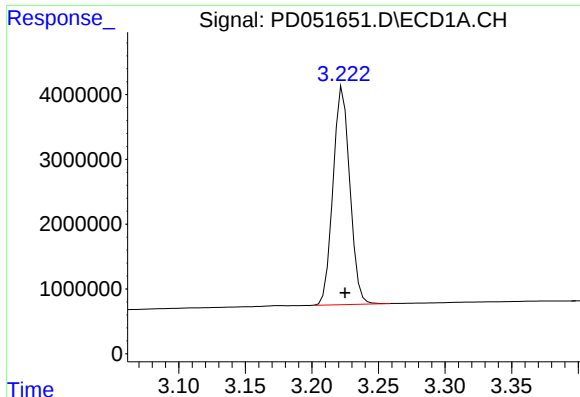

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.002 min
Response: 29558581
Conc: 20.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK19

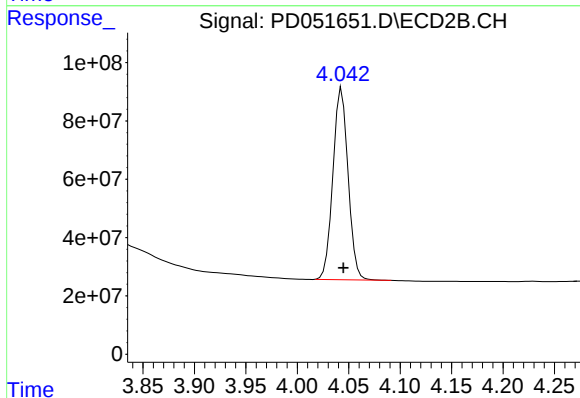


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 674460817
Conc: 21.83 ng/ml

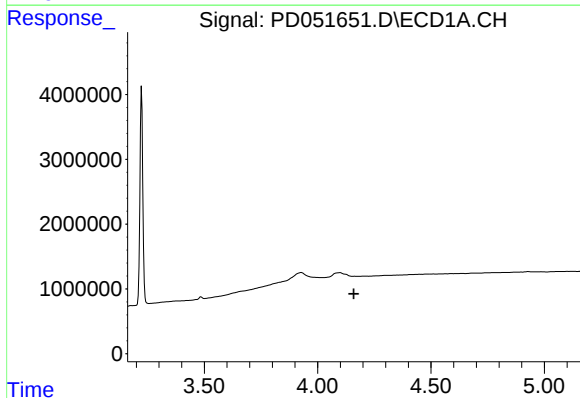


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

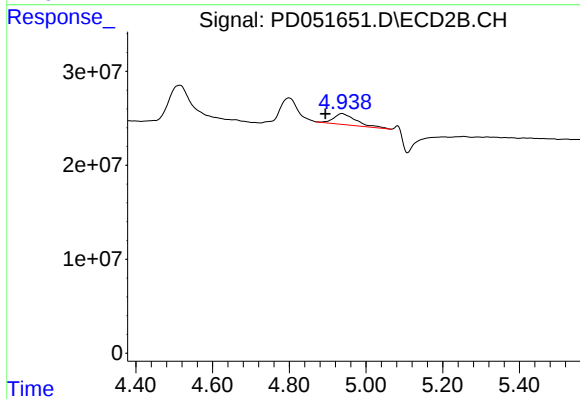

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.044 min
Response: 47475883
Conc: 2.39 ng/ml

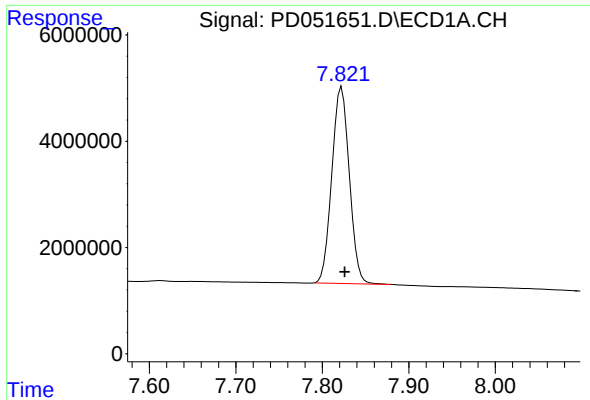

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: -0.003 min
Response: 51739018
Conc: 43.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK19

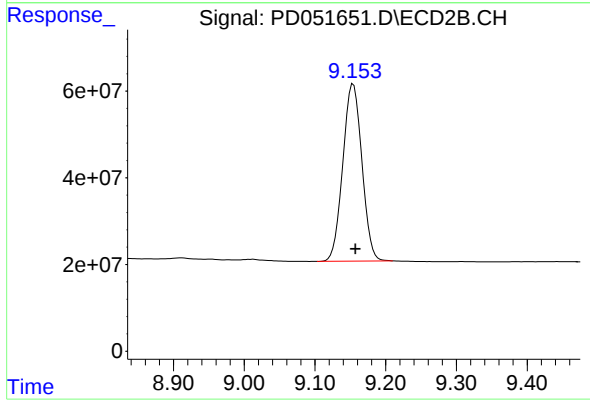

#27 Decachlorobiphenyl

R.T.: 9.154 min
Delta R.T.: -0.003 min
Response: 767149337
Conc: 40.47 ng/ml