

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051654.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 13:18
 Operator : AJ\SJ
 Sample : PB117623BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:53:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.230	4.044	25117747	527.8E6	17.479	17.082
27)	SA Decachlor...	7.833	9.163	44973586	649.3E6	37.396	34.252
Target Compounds							
8)	B Heptachlo...	0.000	5.921	0 39248523	N.D.	1.096	
9)	A Endosulfan I	0.000	6.254f	0 14171128	N.D.	0.427	
11)	B cis-Chlor...	0.000	6.254	0 14171128	N.D.	0.409	
15)	B Endosulfa...	0.000	6.999	0 872814	N.D.	<MDL	
20)	A Methoxychlor	0.000	7.627	0 5193364	N.D.	0.491	
26)	Toxaphene-5	0.000	7.712	0 12728335	N.D.	44.228	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051654.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 13:18
Operator : AJ\SJ
Sample : PB117623BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:53:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

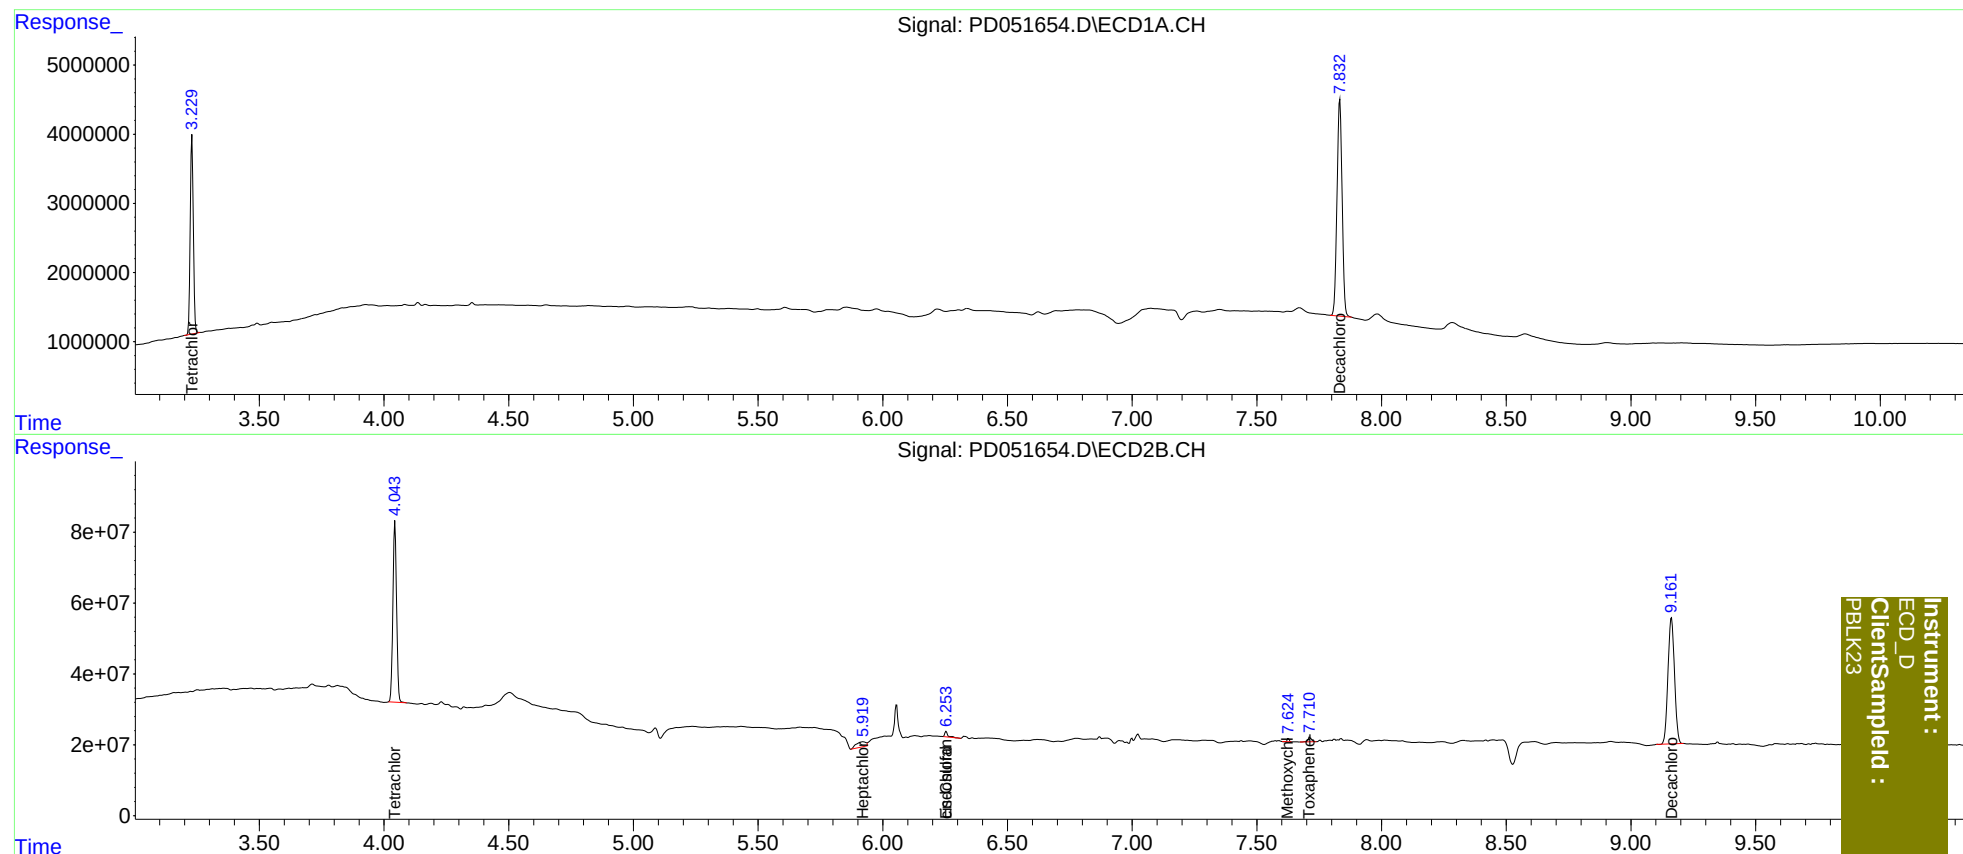


Instrument :
ECD_D
ClientSampleId :
PBLK23

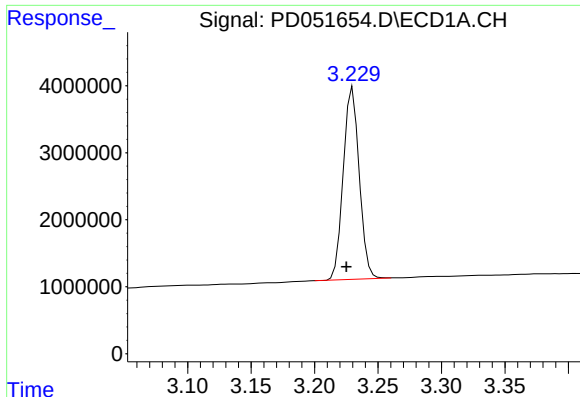

#1 Tetrachloro-m-xylene


R.T.: 3.230 min
Delta R.T.: 0.005 min
Response: 25117747
Conc: 17.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK23

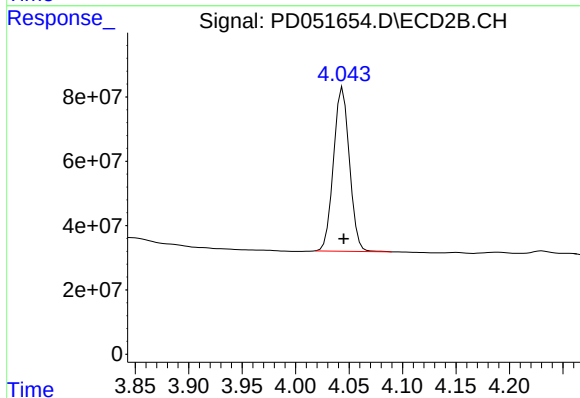


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 527763813
Conc: 17.08 ng/ml

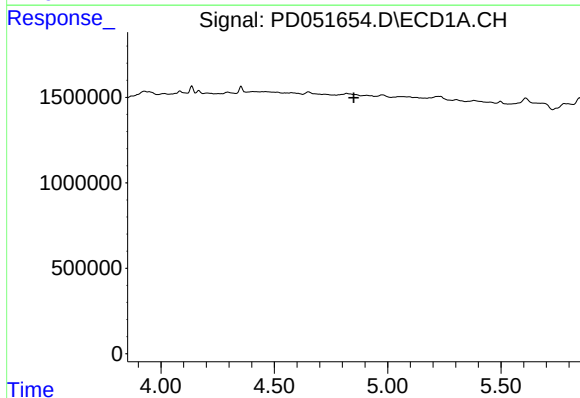


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

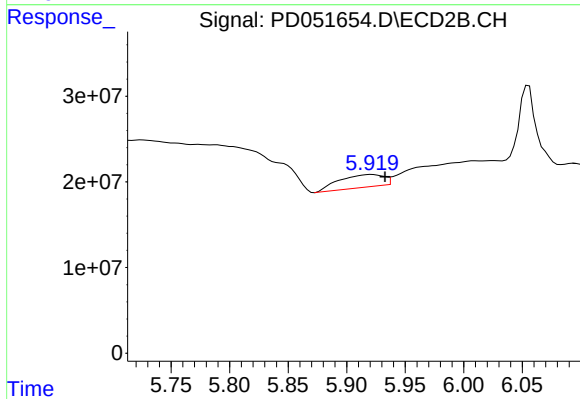

#8 Heptachlor epoxide


R.T.: 5.921 min
Delta R.T.: -0.012 min
Response: 39248523
Conc: 1.10 ng/ml

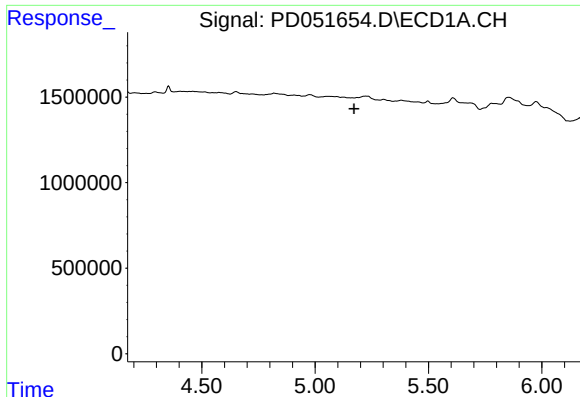

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK23

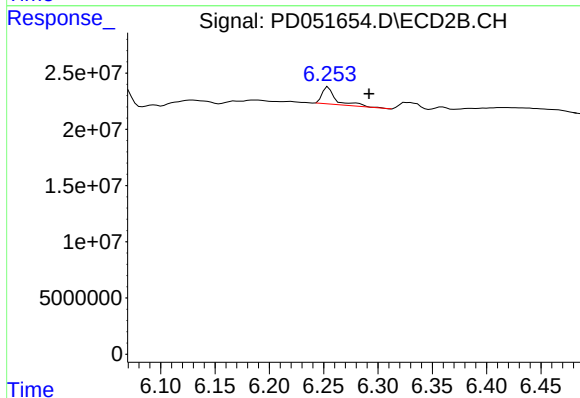


#9 Endosulfan I

R.T.: 6.254 min
Delta R.T.: -0.037 min
Response: 14171128
Conc: 0.43 ng/ml

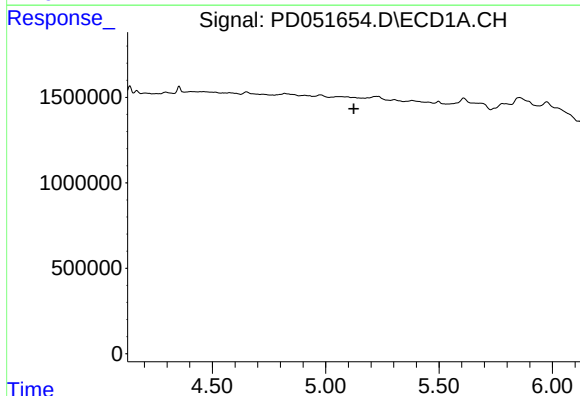


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.125 min
Response: 0
Conc: N.D.

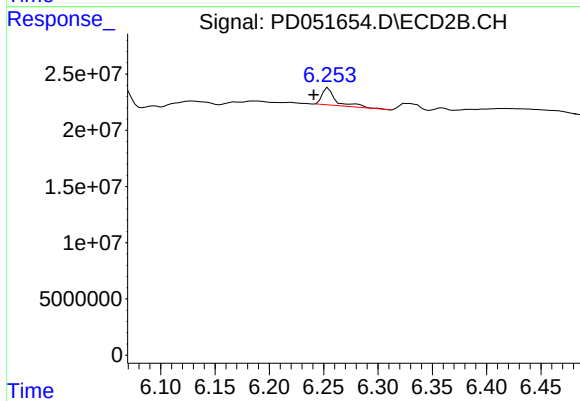

#11 cis-Chlordane


R.T.: 6.254 min
Delta R.T.: 0.014 min
Response: 14171128
Conc: 0.41 ng/ml

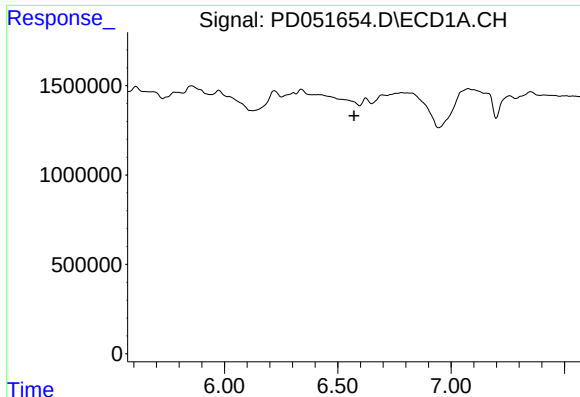

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK23

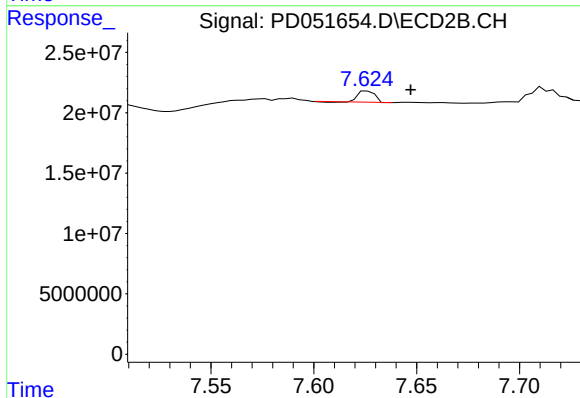


#20 Methoxychlor

R.T.: 7.627 min
Delta R.T.: -0.021 min
Response: 5193364
Conc: 0.49 ng/ml

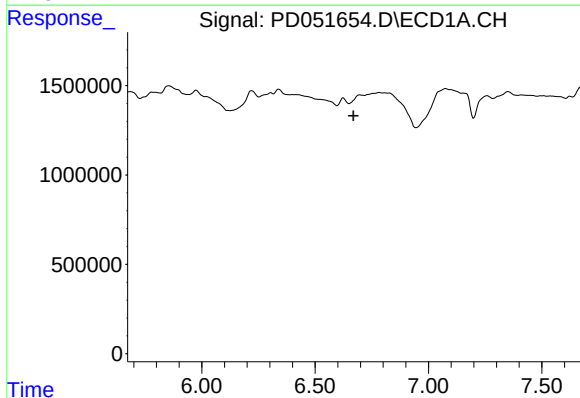


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 6.670 min
Response: 0
Conc: N.D.

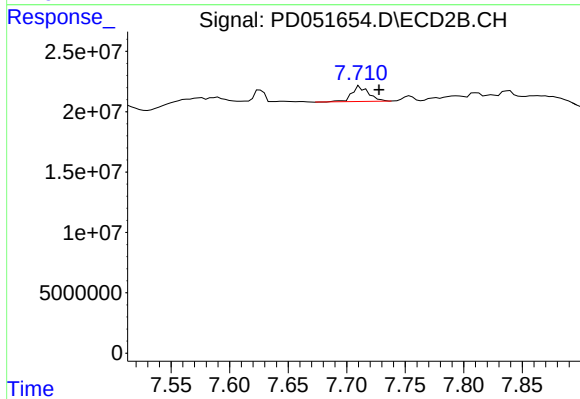

#26 Toxaphene-5


R.T.: 7.712 min
Delta R.T.: -0.016 min
Response: 12728335
Conc: 44.23 ng/ml

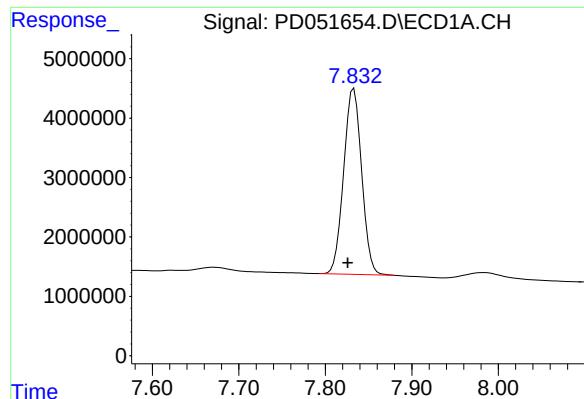

#27 Decachlorobiphenyl

R.T.: 7.833 min
Delta R.T.: 0.007 min
Response: 44973586
Conc: 37.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK23

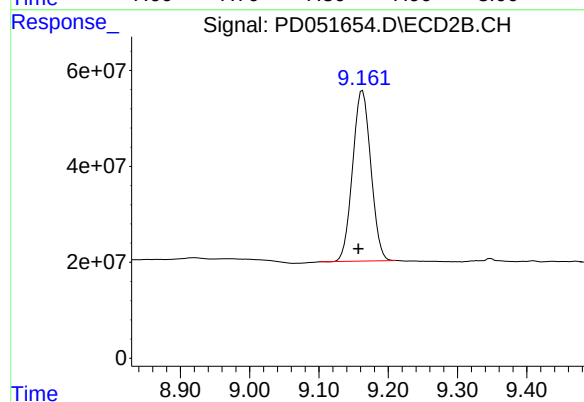

#27 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.006 min
Response: 649331193
Conc: 34.25 ng/ml