

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051662.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 15:52
 Operator : AJ\SJ
 Sample : K1657-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DB653

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:55:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.224	4.044	20831619	471.6E6	14.496	15.263
2) SA Decachlor...	7.823	9.156	28697671	425.3E6	23.862	22.434
Target Compounds						
8) B Heptachlo...	0.000	5.915	0 46131876	N.D.		1.288
10) B trans-Chl...	0.000	6.157	0 40928586	N.D.		1.133

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051662.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 15:52
Operator : AJ\SJ
Sample : K1657-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:55:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

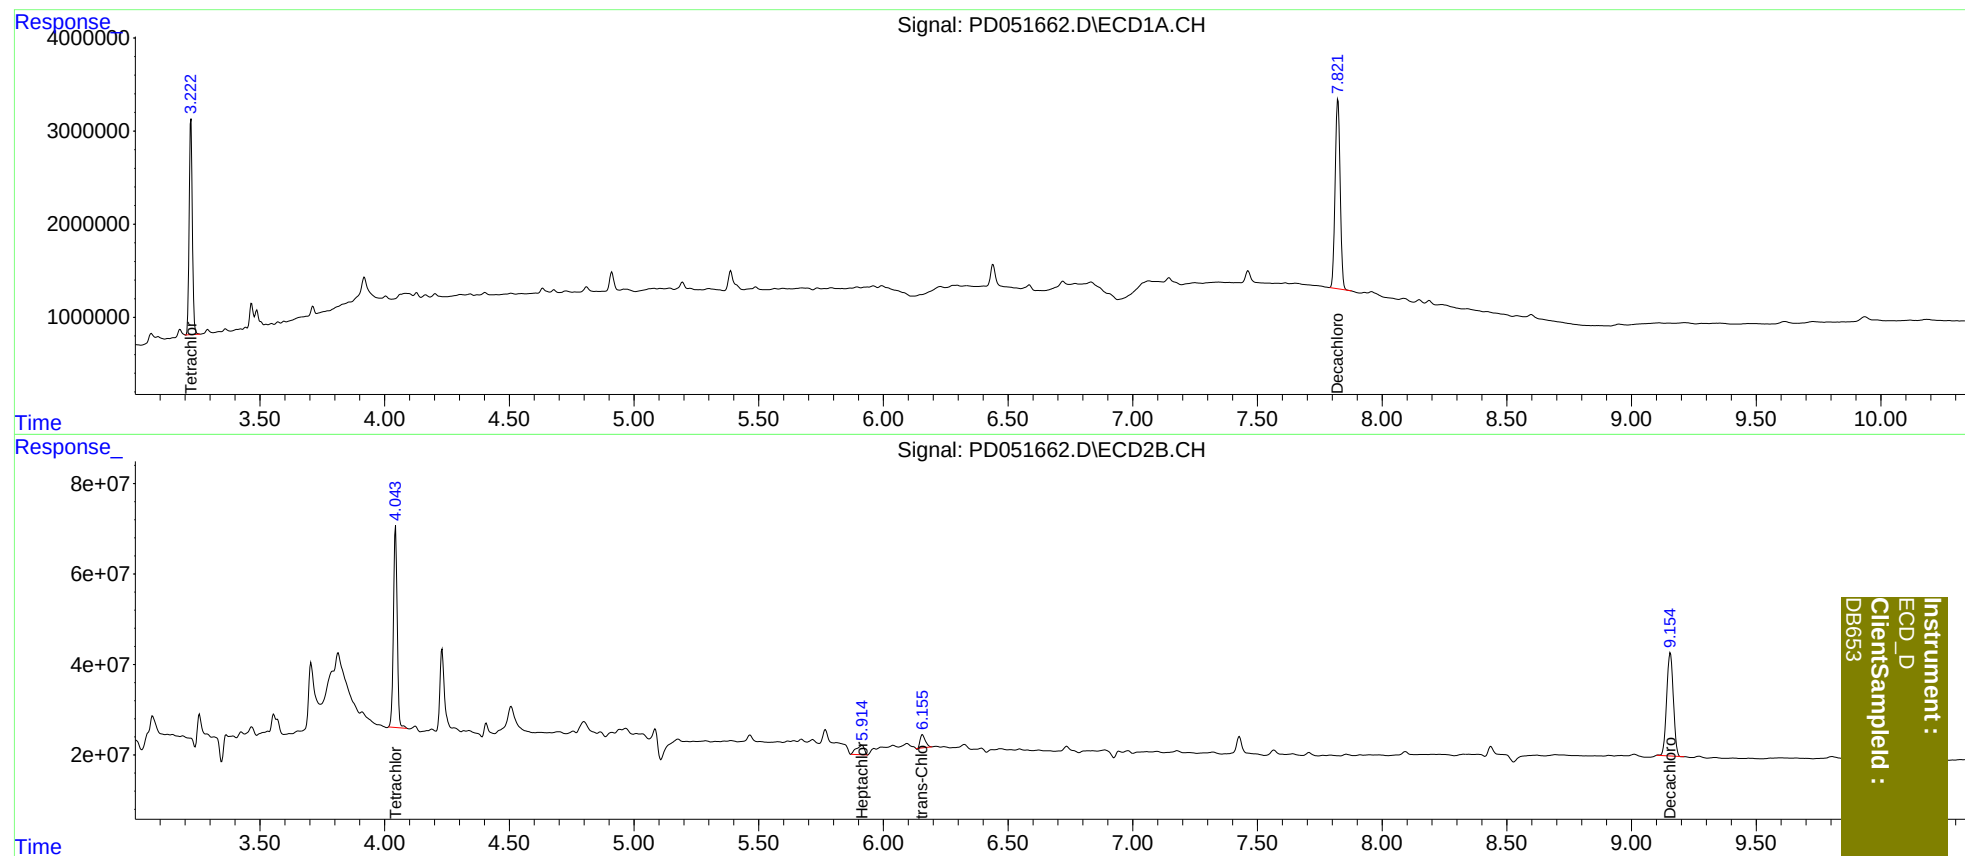


Instrument :
ECD_D
ClientSampleId :
DB653

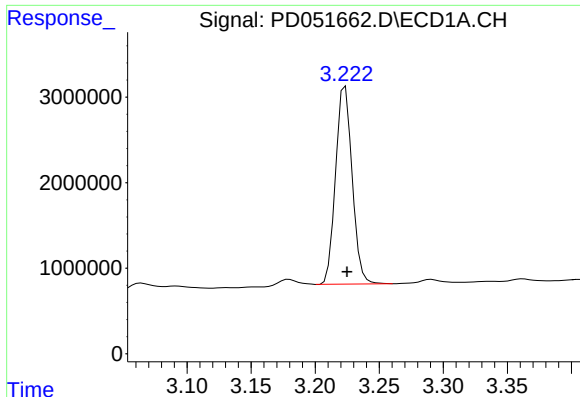

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 20831619
Conc: 14.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
DB653

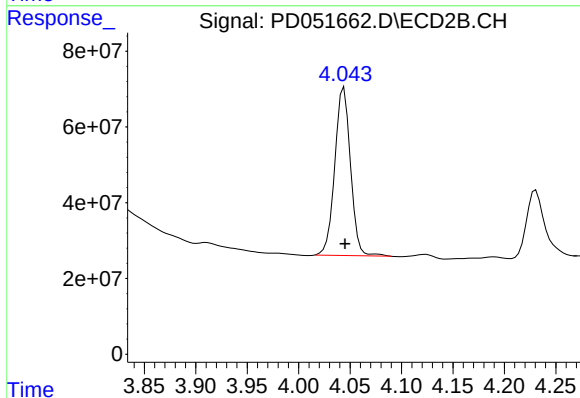


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 471553754
Conc: 15.26 ng/ml

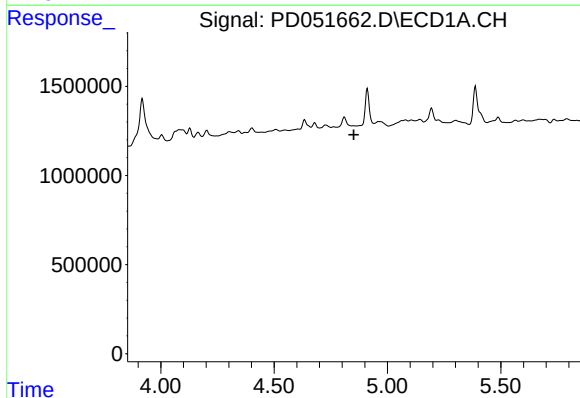


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

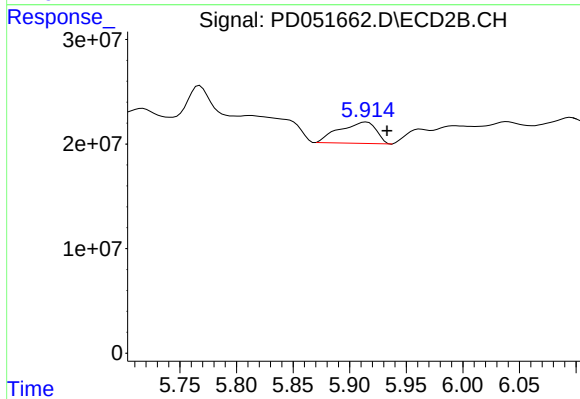

#8 Heptachlor epoxide


R.T.: 5.915 min
Delta R.T.: -0.018 min
Response: 46131876
Conc: 1.29 ng/ml

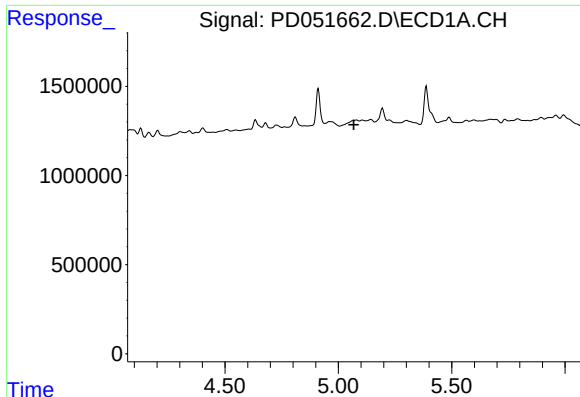

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
DB653

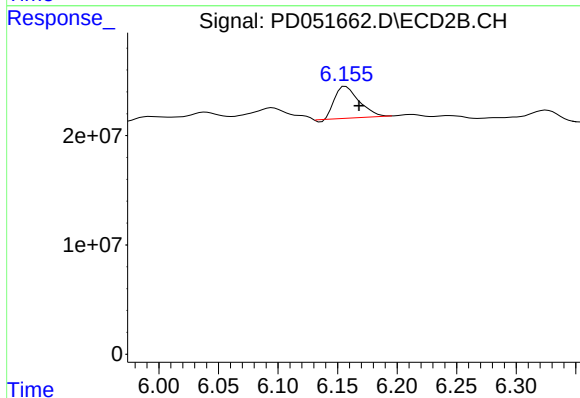


#10 trans-Chlordane

R.T.: 6.157 min
Delta R.T.: -0.011 min
Response: 40928586
Conc: 1.13 ng/ml

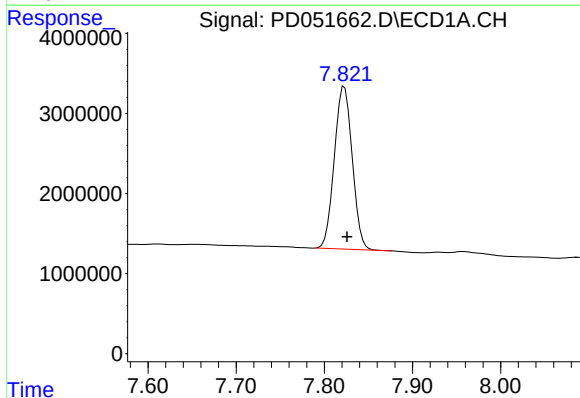

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 28697671
Conc: 23.86 ng/ml

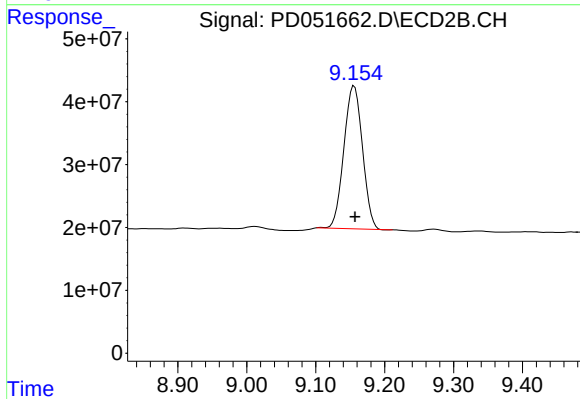

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 425289445
Conc: 22.43 ng/ml