

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051670.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 17:44
 Operator : AJ\SJ
 Sample : K1720-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF8B0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:56:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.223	4.044	12679533	288.5E6	8.823	9.338
2) SA Decachlor...	7.823	9.156	12411183	180.3E6	10.320	9.509
Target Compounds						
6) B beta-BHC	0.000	4.937f	0	28681090	N.D.	1.446
8) B Heptachlo...	0.000	5.916	0	25720332	N.D.	0.718


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051670.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 17:44
Operator : AJ\SJ
Sample : K1720-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:56:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

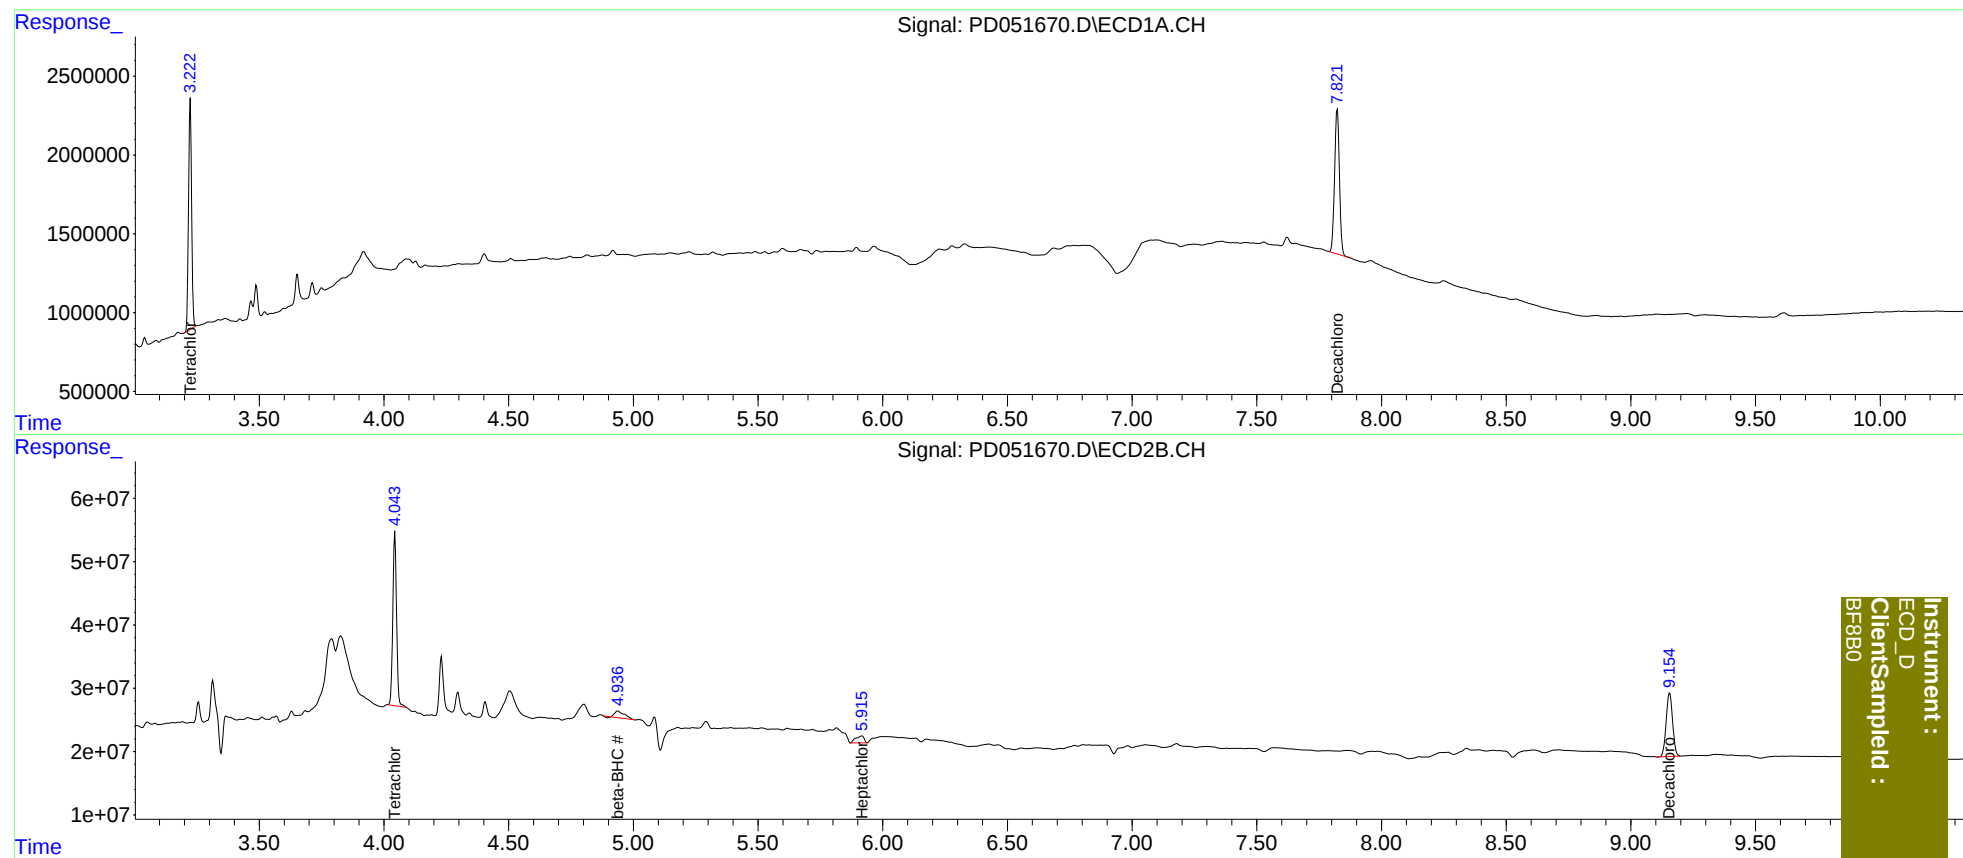


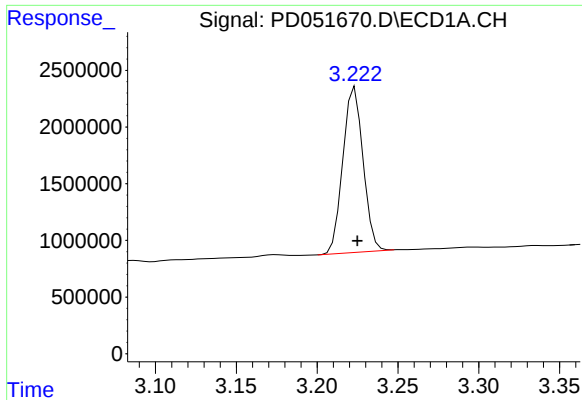

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: -0.002 min
Response: 12679533
Conc: 8.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF8B0

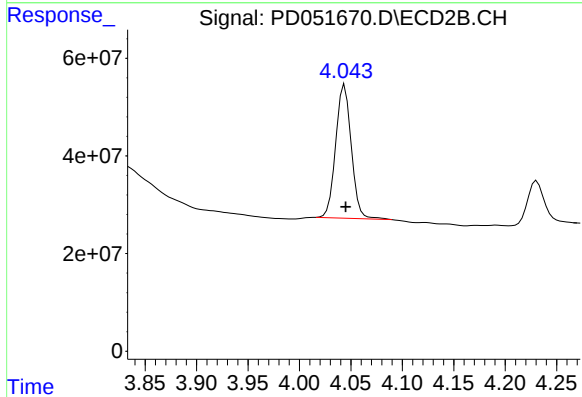


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 288522165
Conc: 9.34 ng/ml

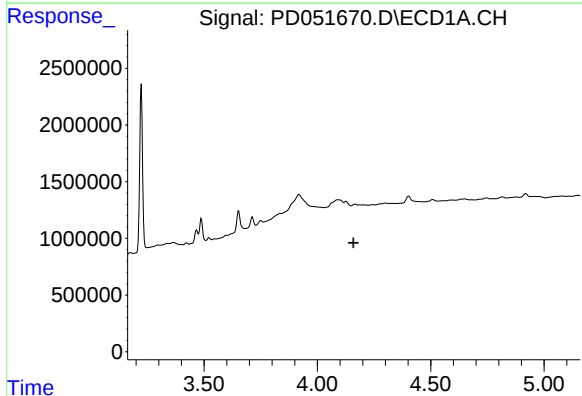


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

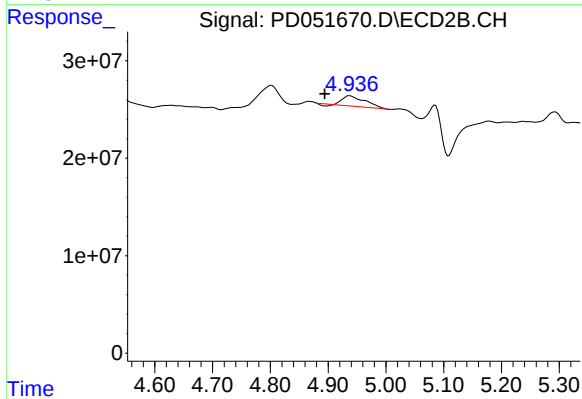

#6 beta-BHC


R.T.: 4.937 min
Delta R.T.: 0.043 min
Response: 28681090
Conc: 1.45 ng/ml

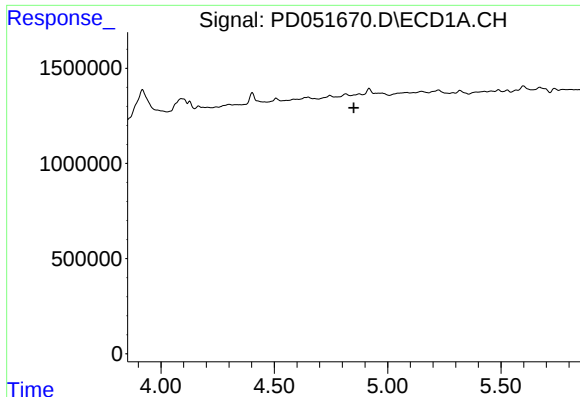

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF8B0

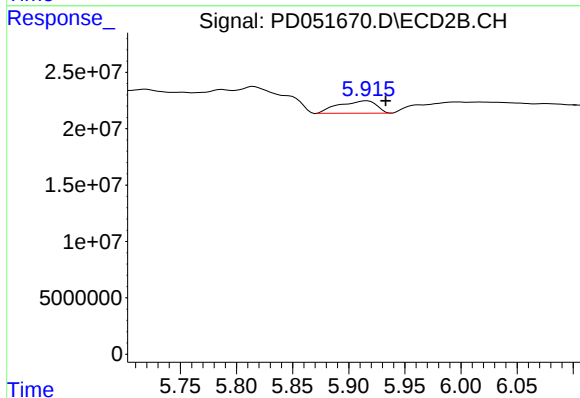


#8 Heptachlor epoxide

R.T.: 5.916 min
Delta R.T.: -0.016 min
Response: 25720332
Conc: 0.72 ng/ml

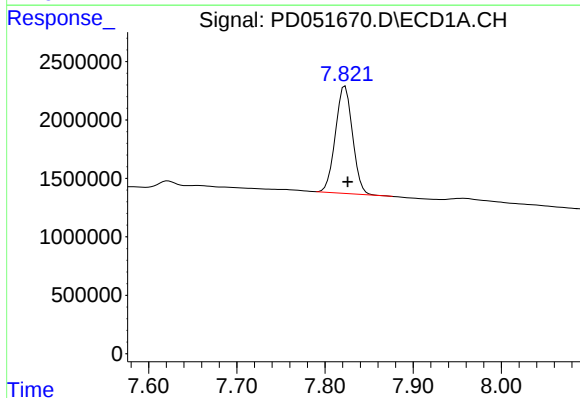

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 12411183
Conc: 10.32 ng/ml

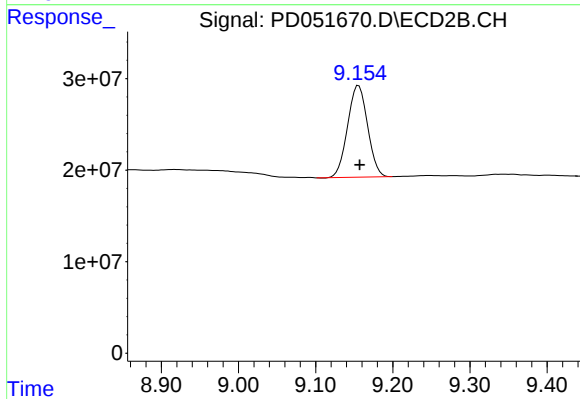

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 180258507
Conc: 9.51 ng/ml