

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051673.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 19:35
 Operator : AJ\SJ
 Sample : PIBLK21
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:57:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.224	4.044	31852773	648.2E6	22.166	20.979
2)	SA Decachlor...	7.823	9.156	48317242	752.5E6	40.176	39.695
Target Compounds							
6)	B beta-BHC	0.000	4.938f	0 48079951	N.D.		2.423
8)	B Heptachlo...	0.000	5.924	0 61994649	N.D.		1.731


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051673.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 19:35
Operator : AJ\SJ
Sample : PIBLK21
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:57:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

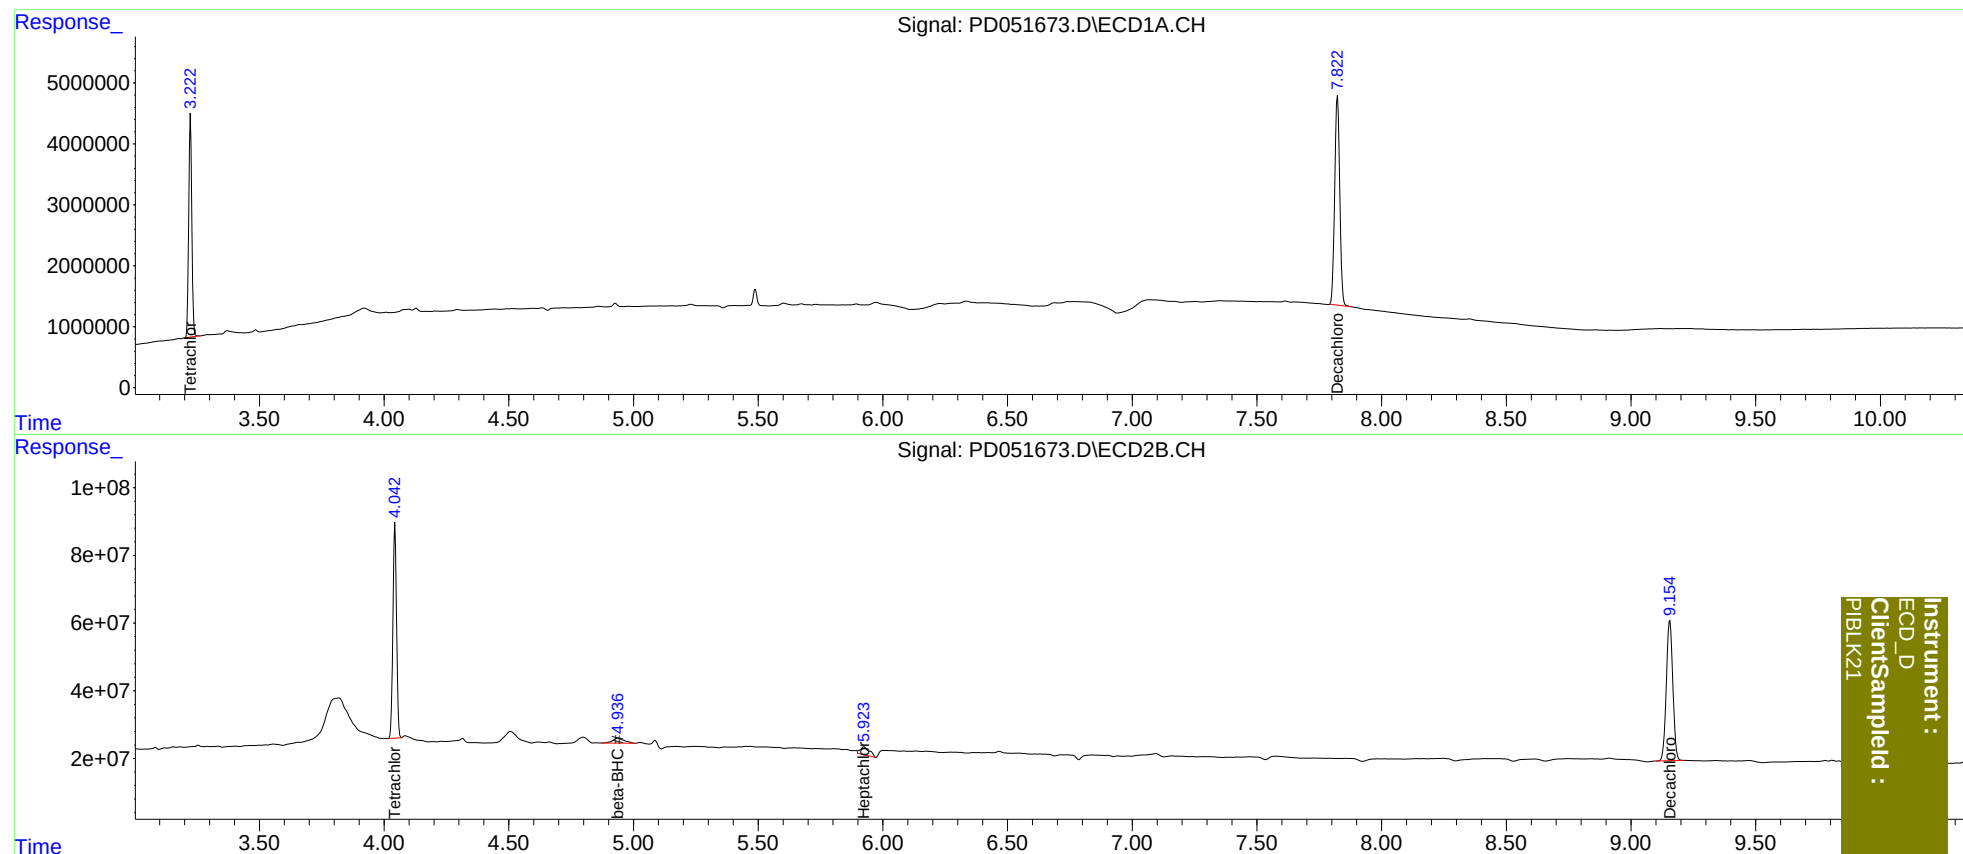


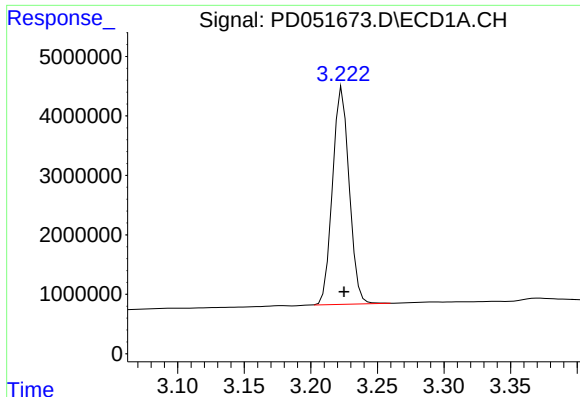

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: -0.001 min
Response: 31852773
Conc: 22.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK21

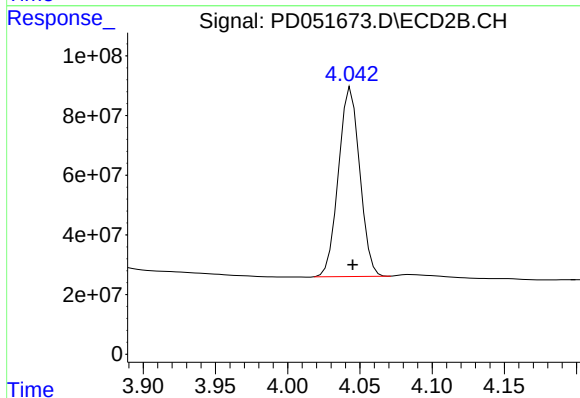


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 648162967
Conc: 20.98 ng/ml

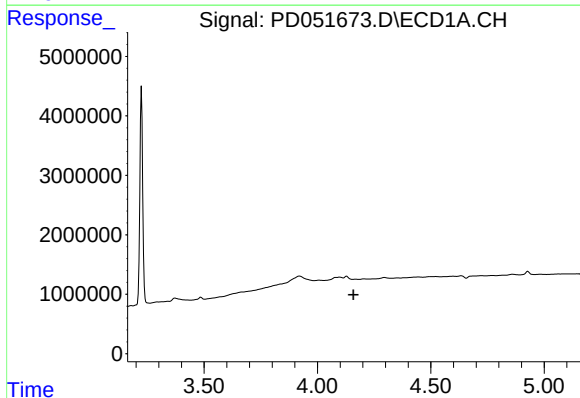


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

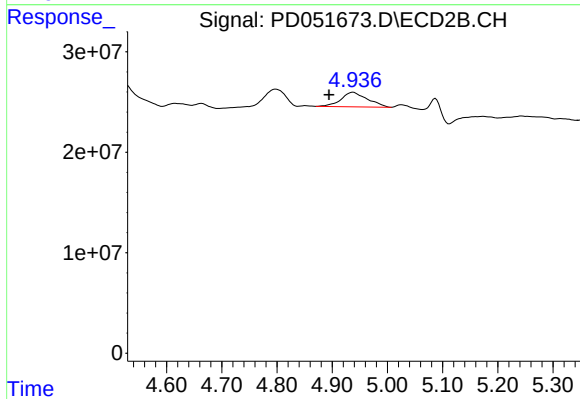

#6 beta-BHC


R.T.: 4.938 min
Delta R.T.: 0.044 min
Response: 48079951
Conc: 2.42 ng/ml

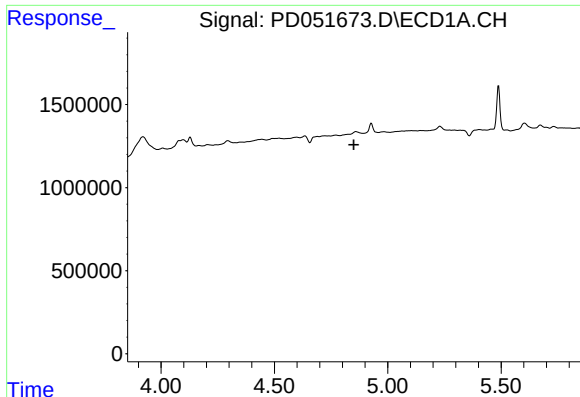

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK21

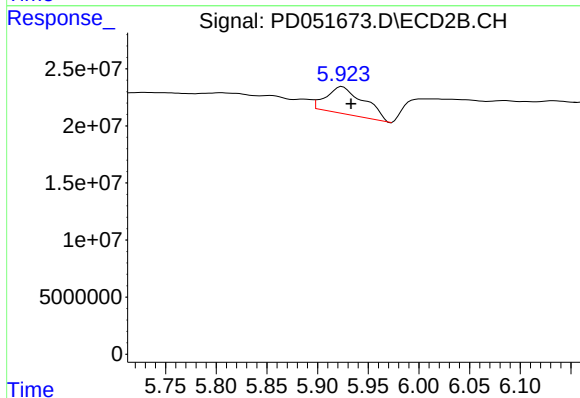


#8 Heptachlor epoxide

R.T.: 5.924 min
Delta R.T.: -0.009 min
Response: 61994649
Conc: 1.73 ng/ml

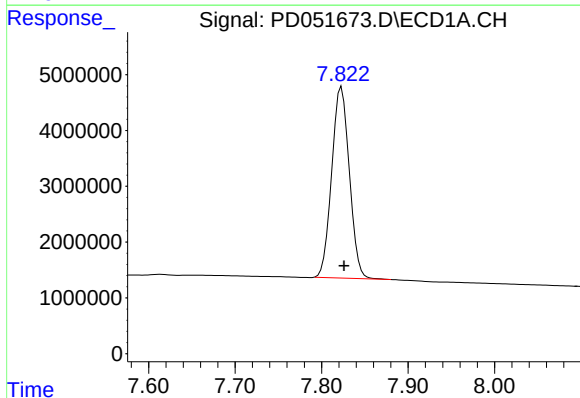

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 48317242
Conc: 40.18 ng/ml

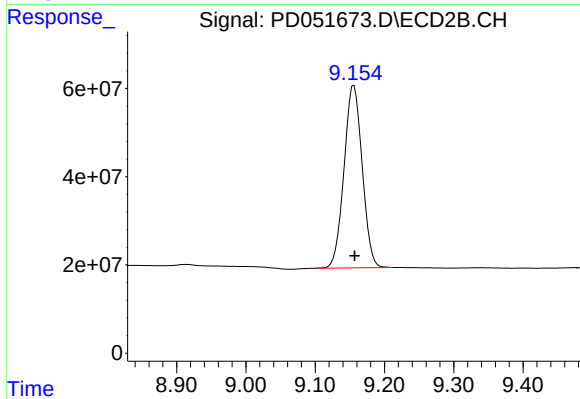

#27 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.001 min
Response: 752514906
Conc: 39.70 ng/ml