

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051689.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Mar 2019 1:31
 Operator : AJ\SJ
 Sample : K1736-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF626

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 03:24:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.224	4.044	16881734	366.9E6	11.748	11.875
27) SA	Decachlor...	7.823	9.157	19726290	286.9E6	16.402	15.134
Target Compounds							
6) B	beta-BHC	0.000	4.939f	0 49679631	N.D.	2.504	
8) B	Heptachlo...	0.000	5.917	0 42308588	N.D.	1.182	
10) B	trans-Chl...	0.000	6.098f	0 7580421	N.D.	0.210	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051689.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Mar 2019 1:31
Operator : AJ\SJ
Sample : K1736-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BF626

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 03:24:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

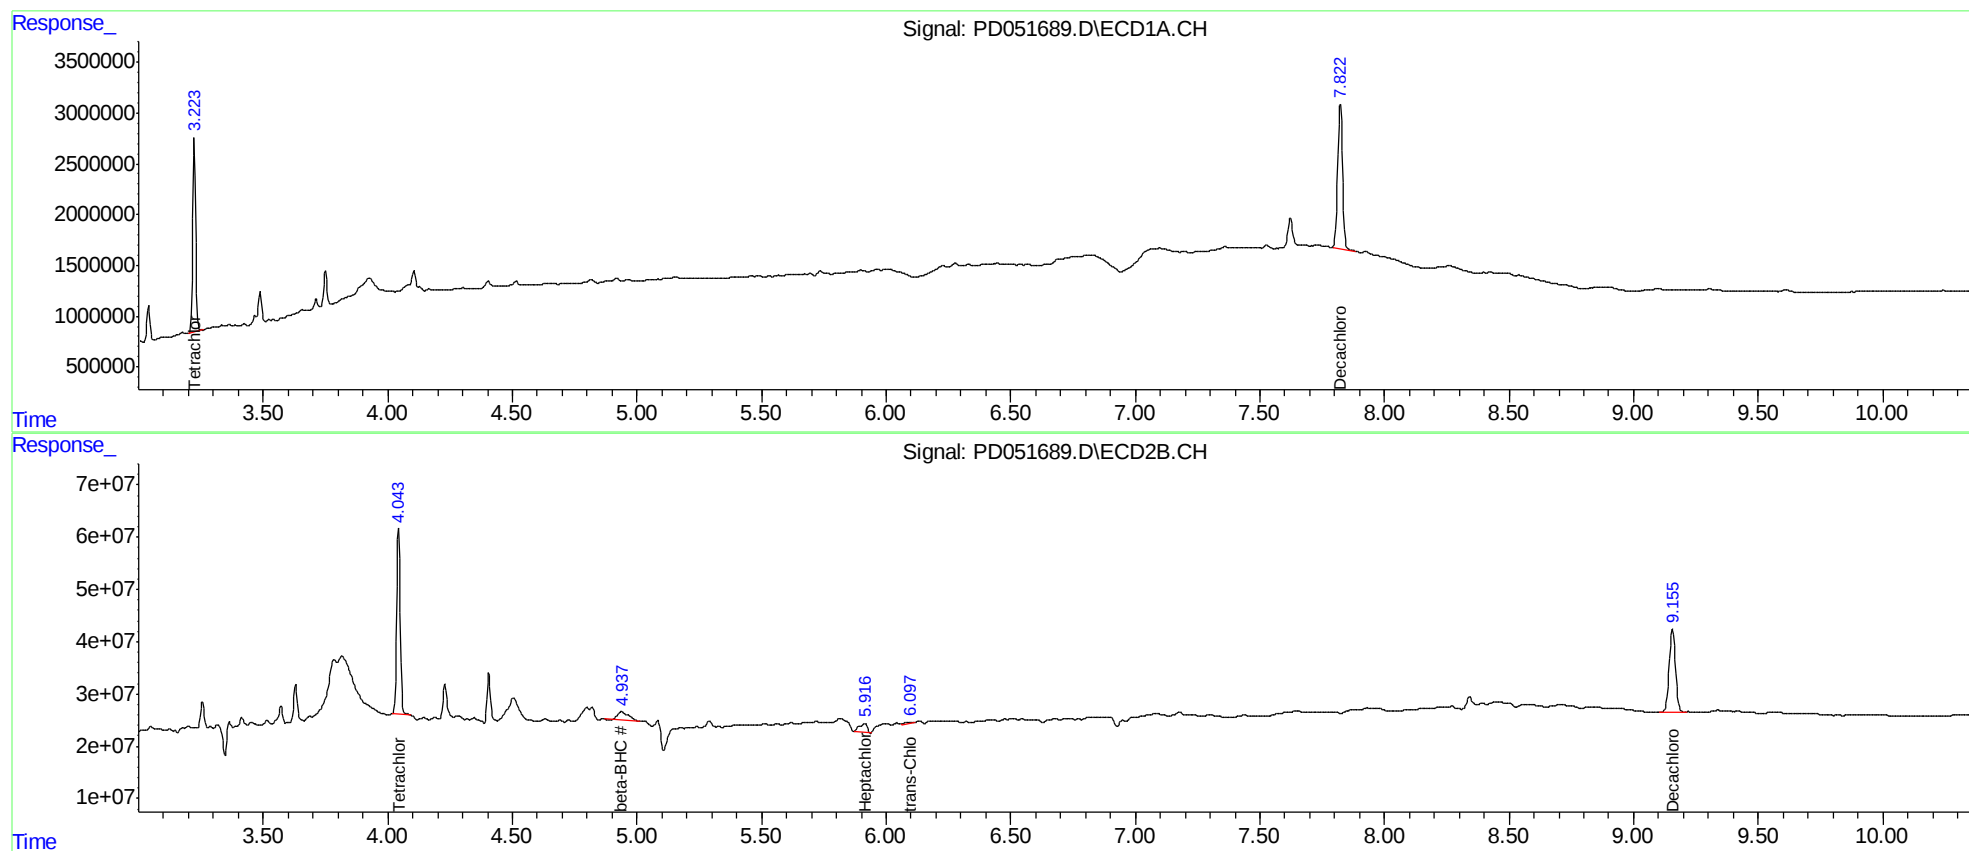


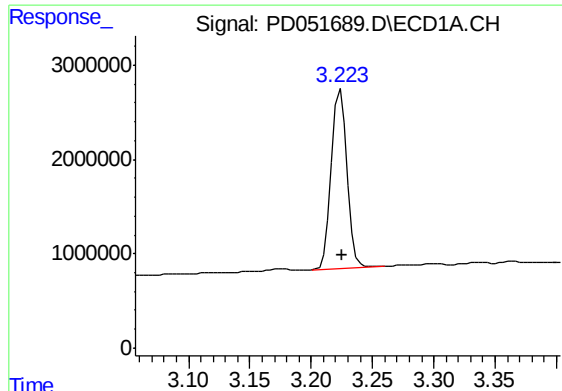

#1 Tetrachloro-m-xylene


R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 16881734
Conc: 11.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF626

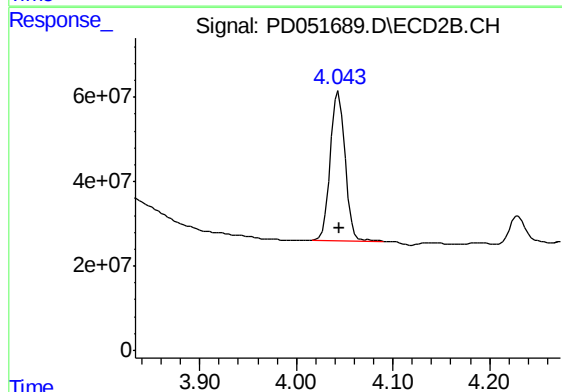


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 366899946
Conc: 11.88 ng/ml

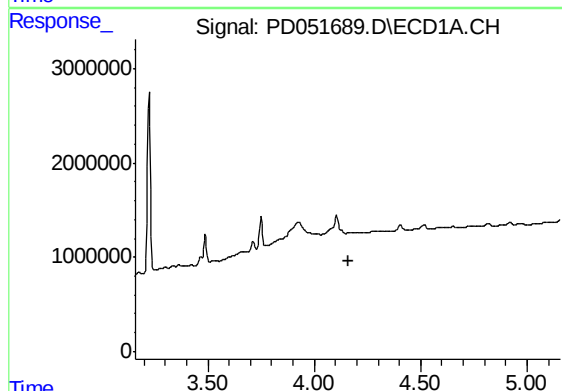


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.159 min
Response: 0
Conc: N.D.

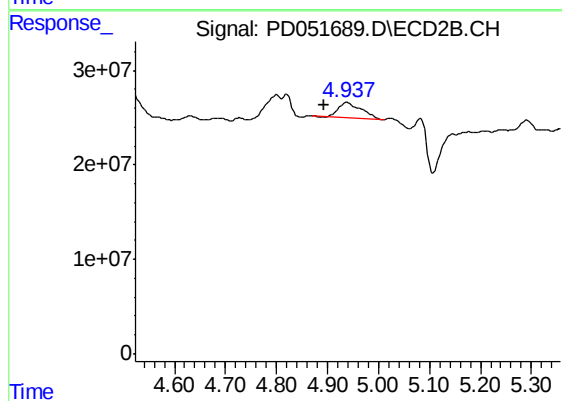

#6 beta-BHC


R.T.: 4.939 min
Delta R.T.: 0.045 min
Response: 49679631
Conc: 2.50 ng/ml

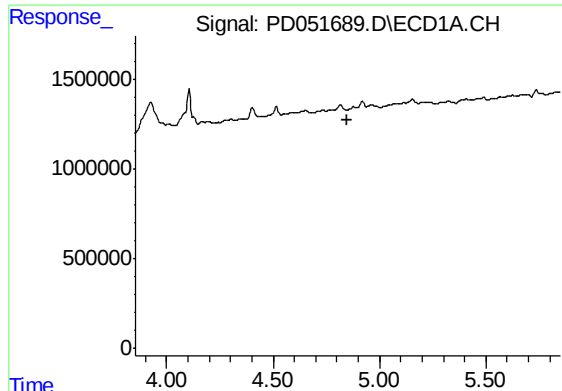

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.851 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF626

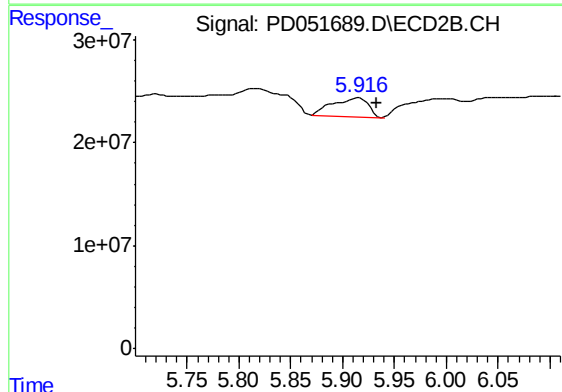


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.016 min
Response: 42308588
Conc: 1.18 ng/ml

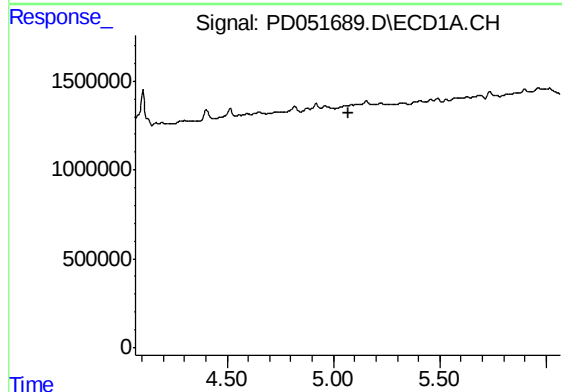


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.068 min
Response: 0
Conc: N.D.

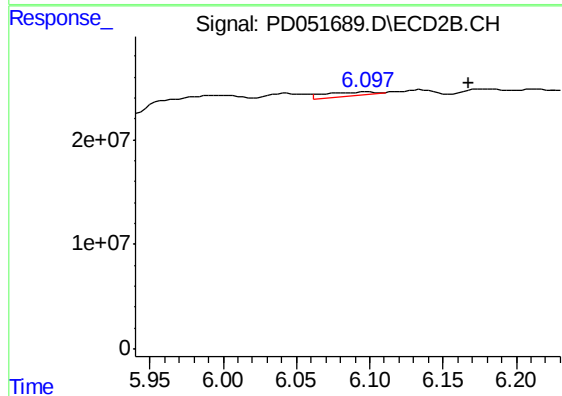

#10 trans-Chlordane


R.T.: 6.098 min
Delta R.T.: -0.070 min
Response: 7580421
Conc: 0.21 ng/ml

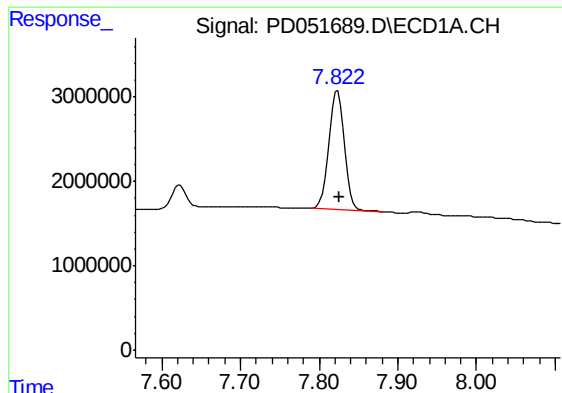

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: -0.003 min
Response: 19726290
Conc: 16.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF626

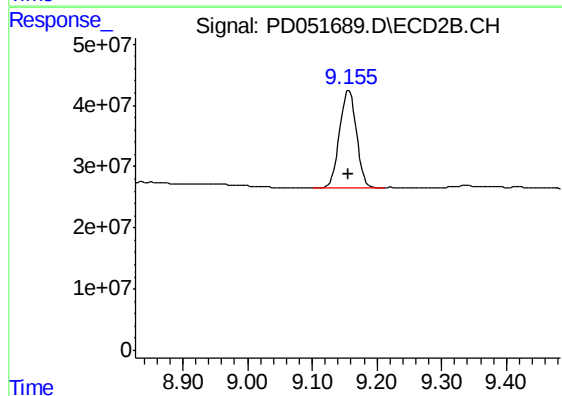

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 286897791
Conc: 15.13 ng/ml