

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051653.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 12:07
 Operator : AJ\SJ
 Sample : K1657-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DB638

Manual Integrations
 APPROVED

Sohil
 3/12/2019 5:59:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:53:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.226	4.042	27192764	887.3E6	18.923	28.719 #
2)	SA Decachlor...	7.827	9.158	50010033	718.1E6	41.583	37.880
Target Compounds							
2)	A alpha-BHC	3.647	4.436	160.9E6	2779.8E6	72.613	59.497
3)	MA gamma-BHC...	3.915	4.724	124.2E6	2162.0E6	58.990	50.609
4)	MA Heptachlor	4.193	5.237	111.5E6	1792.4E6	51.282	41.899
5)	MB Aldrin	4.425	5.544	62683283	1062.5E6	29.199	26.844
6)	B beta-BHC	4.160	4.893	46072333	854.1E6	48.187m	43.047
7)	B delta-BHC	4.349	5.112	92274243	1101.0E6	41.057	27.048m#
8)	B Heptachlo...	4.853	5.932	81550921	1134.6E6	38.685	31.687
9)	A Endosulfan I	5.174	6.291	134.1E6	1792.8E6	65.646	54.052
10)	B trans-Chl...	5.070	6.167	101.7E6	1443.8E6	46.661	39.965
11)	B cis-Chlor...	5.126	6.240	142.1E6	1901.5E6	66.497	54.926
12)	B 4,4'-DDE	5.295	6.396	184.3E6	2475.7E6	85.647	75.771
13)	MA Dieldrin	5.408	6.547	138.3E6	1732.2E6	59.742m	52.038m
14)	MA Endrin	5.661	6.766	318.2E6	1708.4E6	156.185m	64.637m#
16)	A 4,4'-DDD	5.797	6.887	105.2E6	1456.3E6	59.815	55.636
17)	MA 4,4'-DDT	6.028	7.188	231.8E6	2563.8E6	127.301	111.163
19)	B Endosulfa...	6.301	7.325	57971436	800.9E6	31.391	31.545

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
Data File : PD051653.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2019 12:07
Operator : AJ\SJ
Sample : K1657-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:53:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
Quant Title : GC Extractables
QLast Update : Fri Feb 22 04:35:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

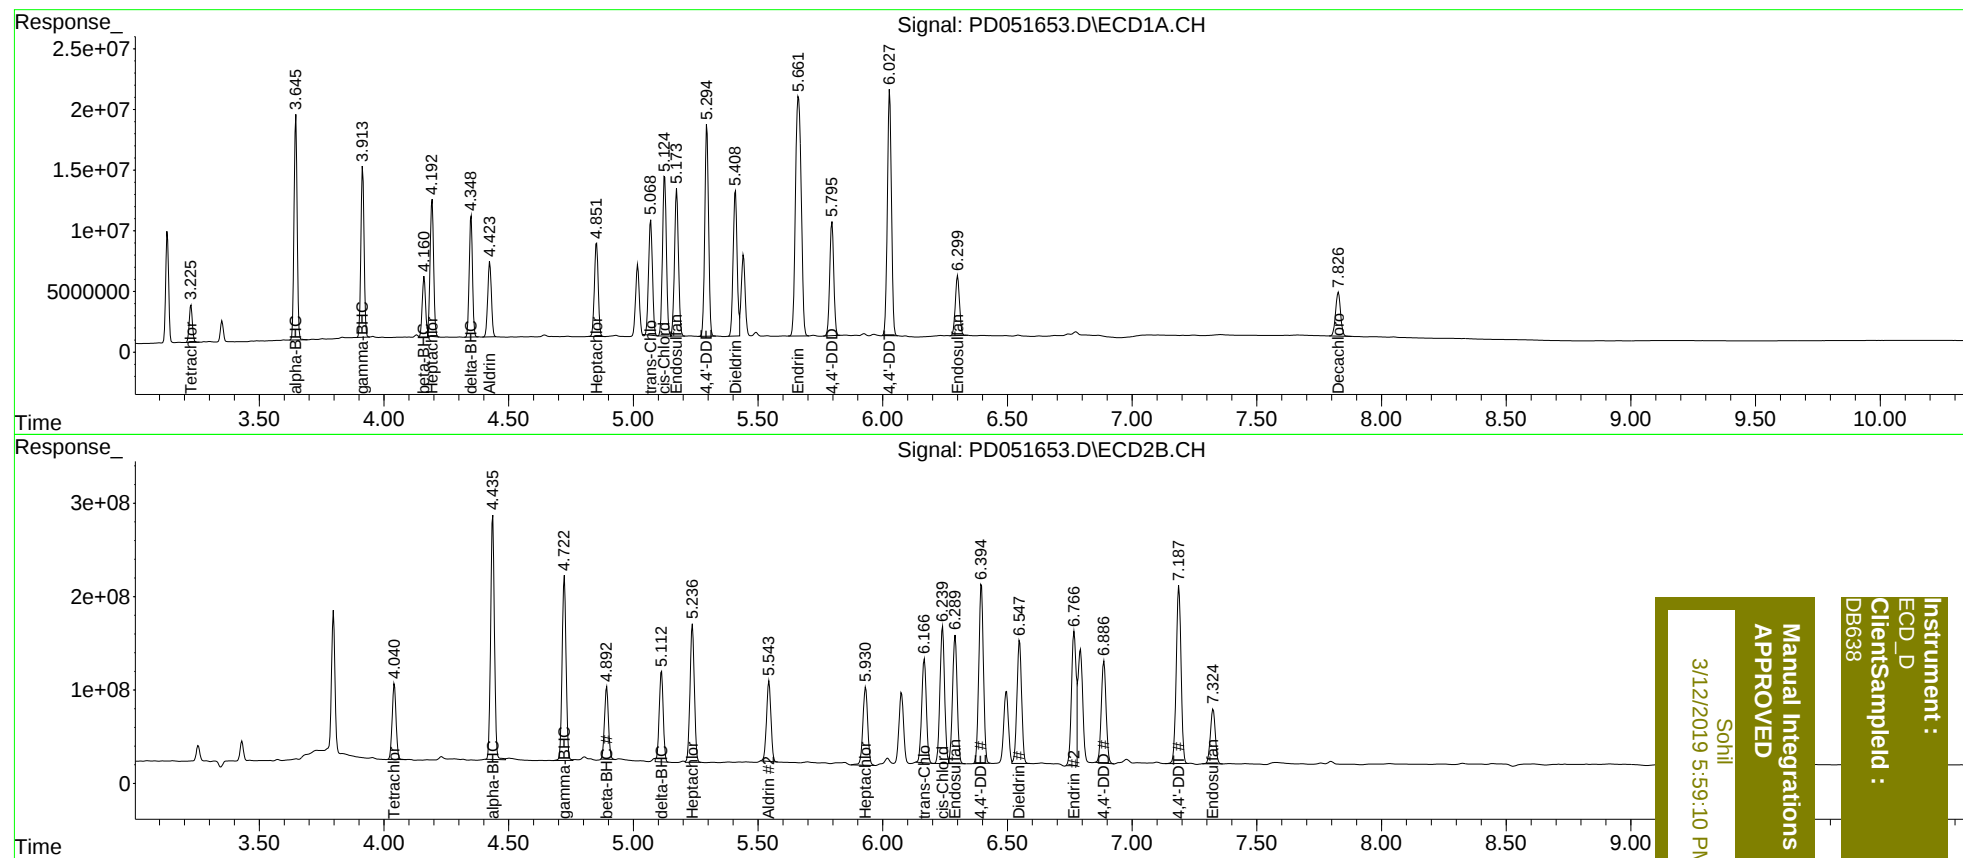

3/12/2019 5:59:10 PM
Sohil

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DB638

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030819\
 Data File : PD051653.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2019 12:07
 Operator : AJ\SJ
 Sample : K1657-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DB638

Manual Integrations
 APPROVED

Sohil
 3/12/2019 5:59:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:53:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022219CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 22 04:35:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.226	4.042	27192764	887.3E6	18.923	28.719 #
27) SA Decachlor...	7.827	9.158	50010033	718.1E6	41.583	37.880
Target Compounds						
2) A alpha-BHC	3.647	4.436	160.9E6	2779.8E6	72.613	59.497
3) MA gamma-BHC...	3.915	4.724	124.2E6	2162.0E6	58.990	50.609
4) MA Heptachlor	4.193	5.237	111.5E6	1792.4E6	51.282	41.899
5) MB Aldrin	4.425	5.544	62683283	1062.5E6	29.199	26.844
6) B beta-BHC	4.160	4.893	46072333	854.1E6	48.187m	43.047
7) B delta-BHC	4.349	5.112	92274243	1101.0E6	41.057	27.048m#
8) B Heptachlo...	4.853	5.932	81550921	1134.6E6	38.685	31.687
9) A Endosulfan I	5.174	6.291	134.1E6	1792.8E6	65.646	54.052
10) B trans-Chl...	5.070	6.167	101.7E6	1443.8E6	46.661	39.965
11) B cis-Chlor...	5.126	6.240	142.1E6	1901.5E6	66.497	54.926
12) B 4,4'-DDE	5.295	6.396	184.3E6	2475.7E6	85.647	75.771
13) MA Dieldrin	5.408	6.547	138.3E6	1732.2E6	59.742m	52.038m
14) MA Endrin	5.661	6.766	318.2E6	1708.4E6	156.185m	64.637m#
16) A 4,4'-DDD	5.797	6.887	105.2E6	1456.3E6	59.815	55.636
17) MA 4,4'-DDT	6.028	7.188	231.8E6	2563.8E6	127.301	111.163
19) B Endosulfa...	6.301	7.325	57971436	800.9E6	31.391	31.545

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

53
 03/11/19

53
 03/11/19