

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030821\
 Data File : PD061476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 14:24
 Operator : AR\AJ
 Sample : M1558-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AE2

Manual Integrations
 APPROVED

Ankita
 3/10/2021 1:58:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:45:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:53:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.980	23601157	180.5E6	25.978m	19.329m#
27)	SA Decachlor...	8.257	9.038	25972216	187.9E6	19.392	20.088
Target Compounds							
10)	B trans-Chl...	5.436	6.085	721568	11981843	0.537m	0.928m#
11)	B cis-Chlor...	5.485	6.162	1459659	11354587	1.119	0.934
13)	MA Dieldrin	5.791	6.466	2469548	22171131	1.869m	1.823
15)	B Endosulfa...	6.331	6.890	630222	11954206	0.552m	1.220m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030821\
Data File : PD061476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 14:24
Operator : AR\AJ
Sample : M1558-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:45:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:53:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

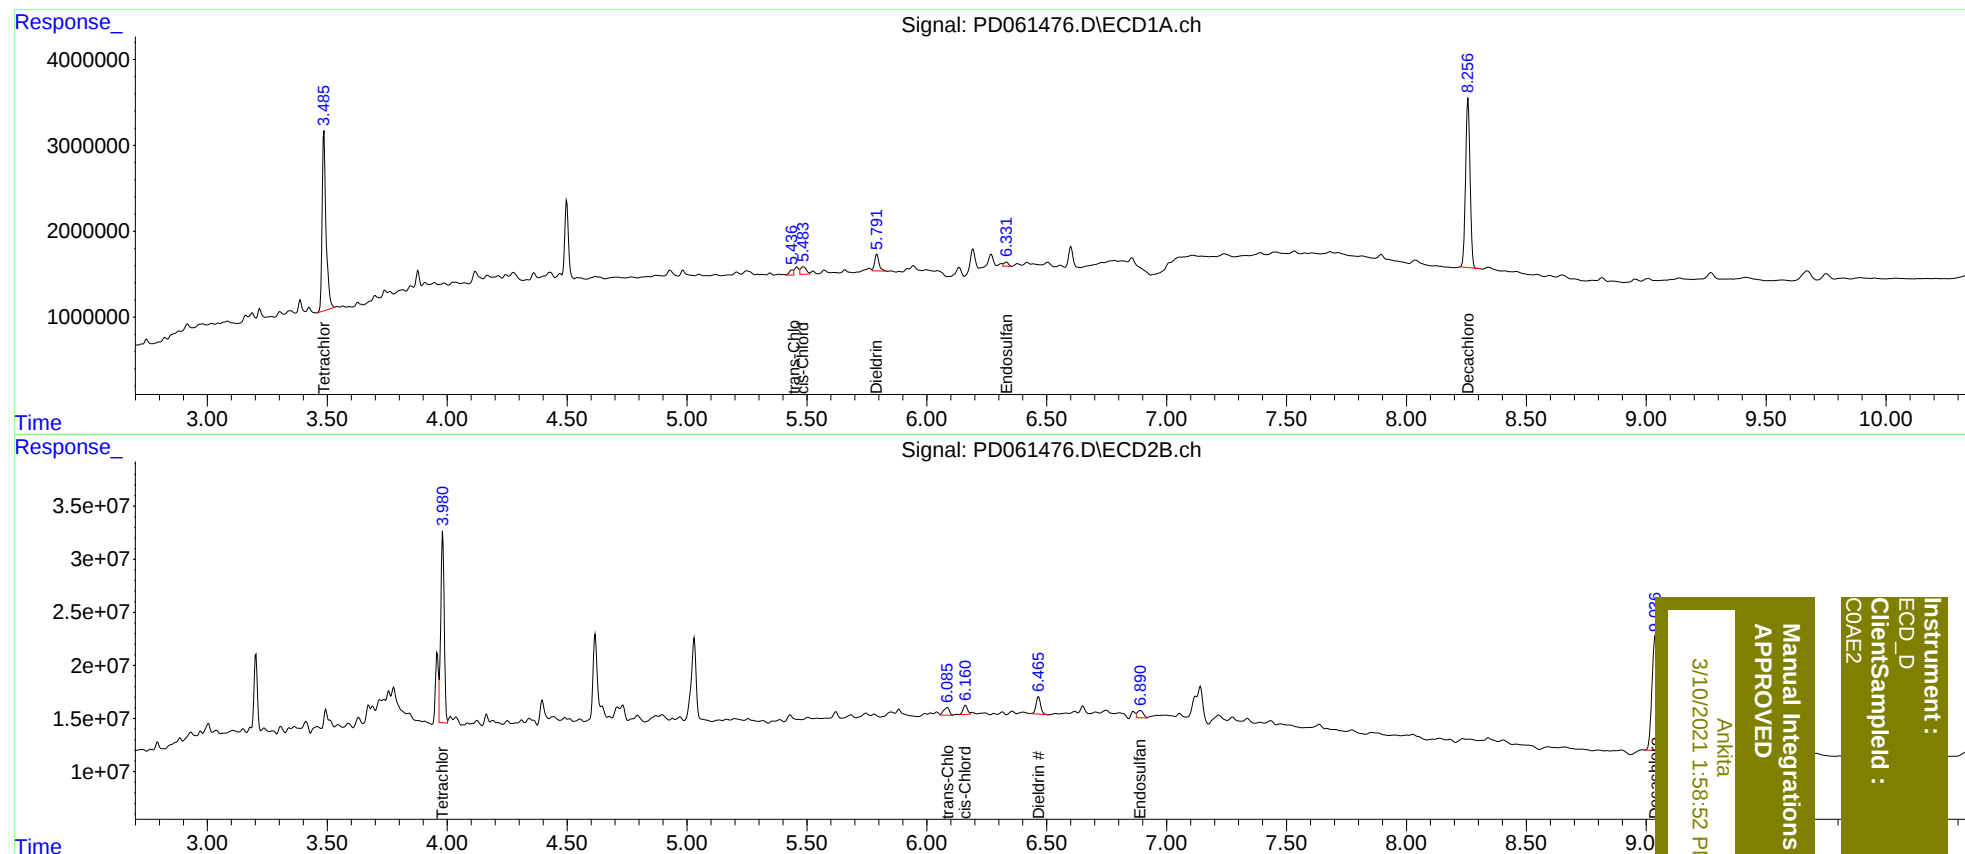

Manual Integrations
APPROVED

Ankita
3/10/2021 1:58:52 PM

Instrument :
ECD_D
ClientSampled :
COAE2