

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030821\
 Data File : PD061459.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 09:57
 Operator : AR\AJ
 Sample : M1344-01
 Misc : TOX MDL 100 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Manual Integrations
 APPROVED

Ankita
 3/9/2021 4:15:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 03:44:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:53:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.981	17688058	172.5E6	19.470	18.465
27)	SA Decachlor...	8.258	9.036	48615489	347.9E6	36.298	37.203
Target Compounds							
22)	Toxaphene-1	5.753	6.363	719130	5590504	79.527	95.248m
23)	Toxaphene-2	5.916	6.655	619390	6351411	66.421	87.254 #
24)	Toxaphene-3	6.238	7.062	946029	10402959	87.379	101.259
25)	Toxaphene-4	6.358	7.137	2017791	23260405	86.413	82.441
26)	Toxaphene-5	7.092	7.636	3010459	8840312	113.998	72.634m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030821\
Data File : PD061459.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 09:57
Operator : AR\AJ
Sample : M1344-01
Misc : TOX MDL 100 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 03:44:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:53:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

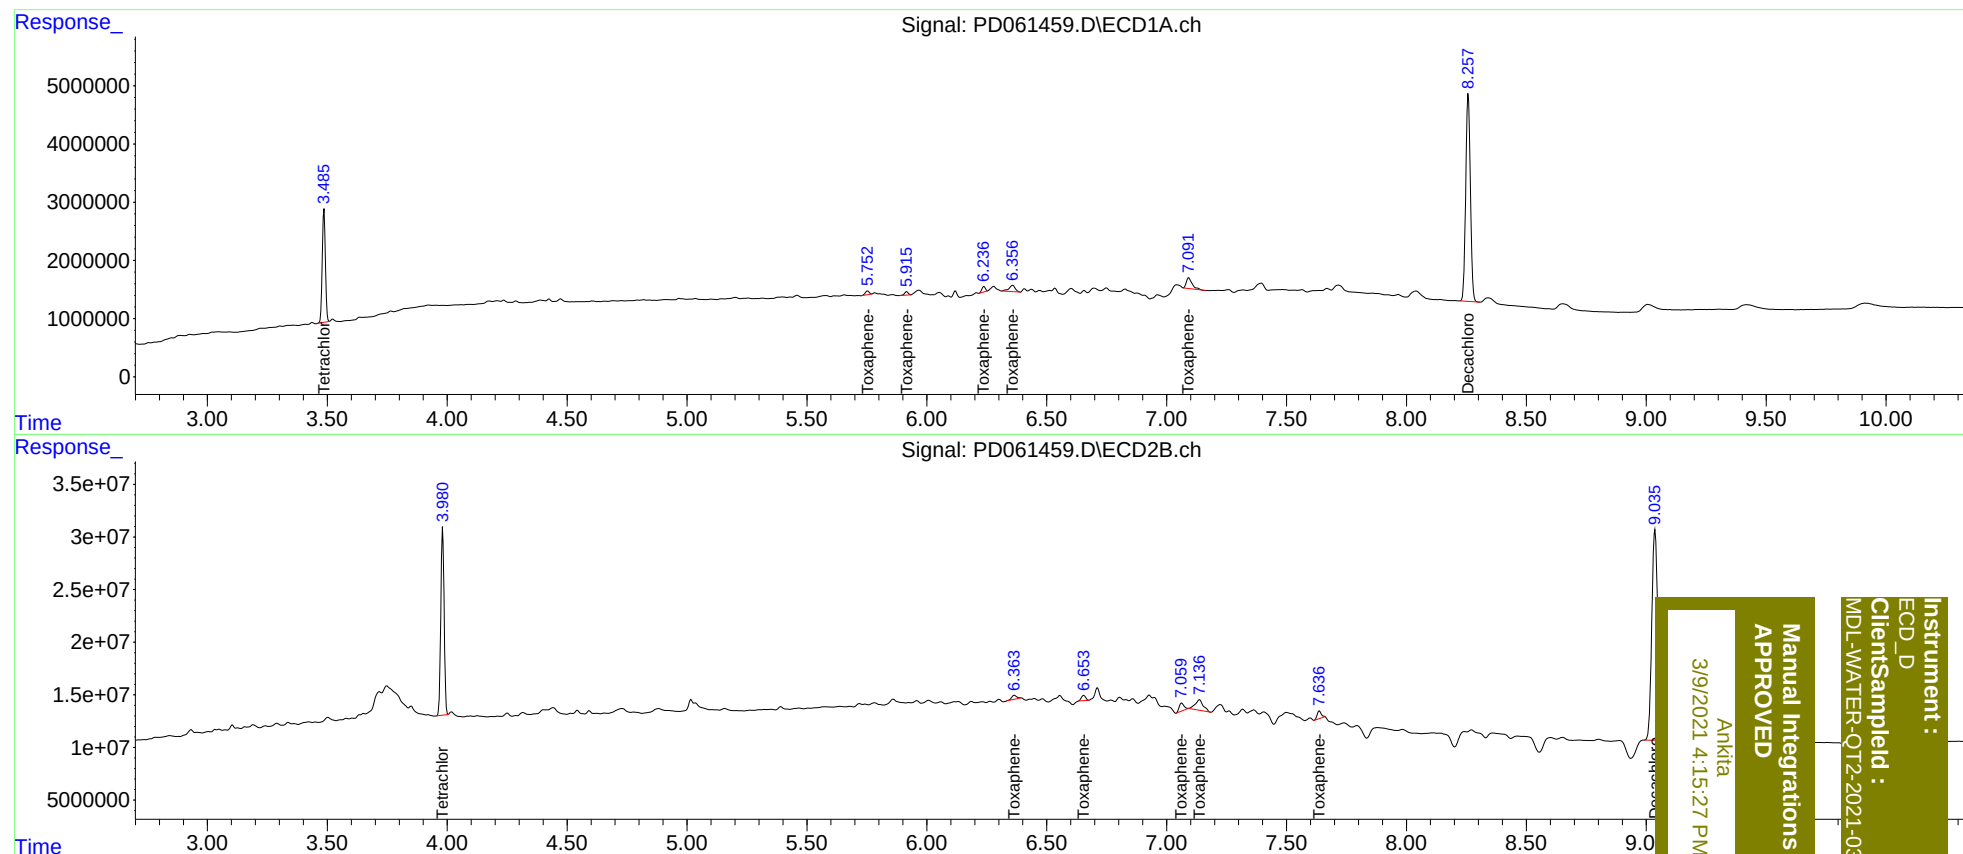

Manual Integrations
APPROVED

Ankita
3/9/2021 4:15:27 PM

Instrument :
ECD_D
ClientSample :
MDL-WATER-QT2-2021-03