

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
 Data File : PD068385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 10:58
 Operator : AR\AJ
 Sample : N1808-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CL-01-030422

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/09/2022
 Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 23:51:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.450	4.174	1963640	16999174	1.675	1.771m
28) SA Decachlor...	8.212	9.371	1846178	12397138	1.586	2.091 #
Target Compounds						
10) B gamma-Chl...	5.390	6.325	377928	5030284	0.254m	0.476m#
11) B alpha-Chl...	5.448	6.401	372658	6711874	0.254m	0.651m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
Data File : PD068385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 10:58
Operator : AR\AJ
Sample : N1808-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CL-01-030422


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/09/2022
Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 23:51:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

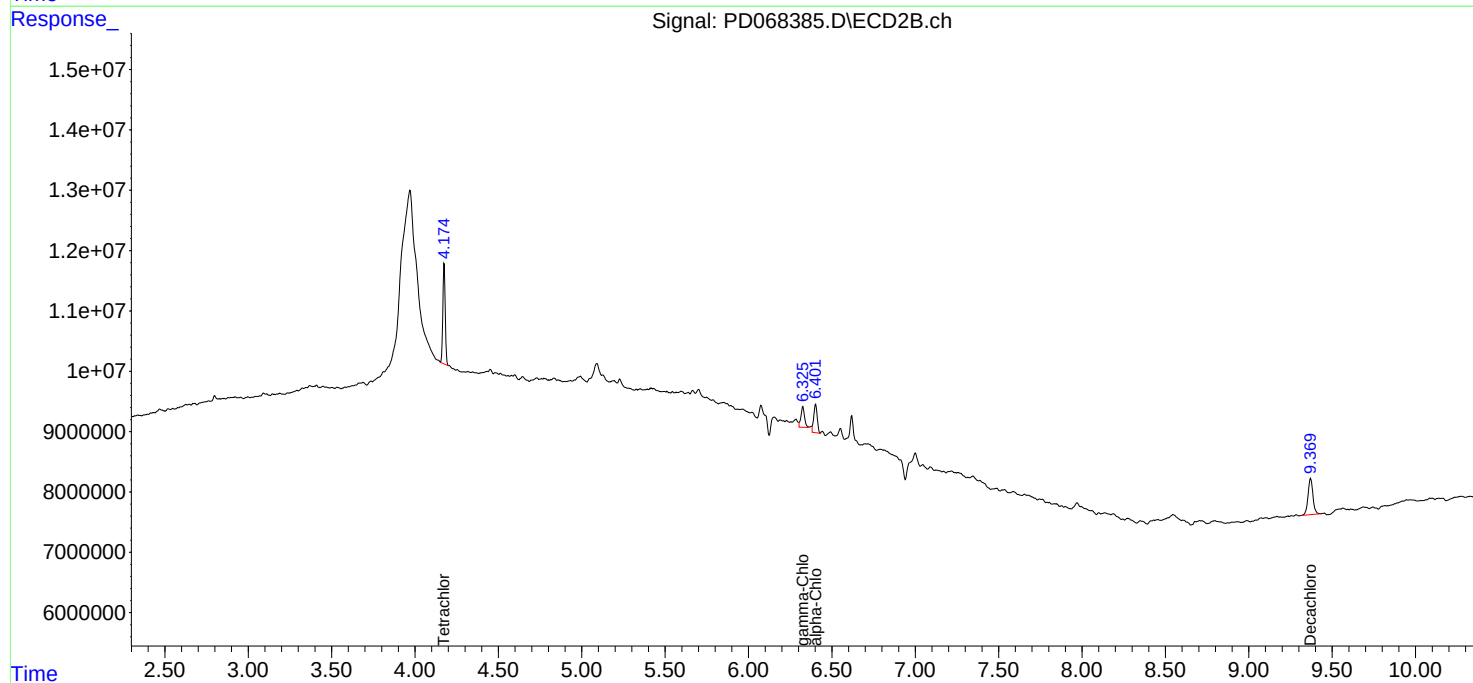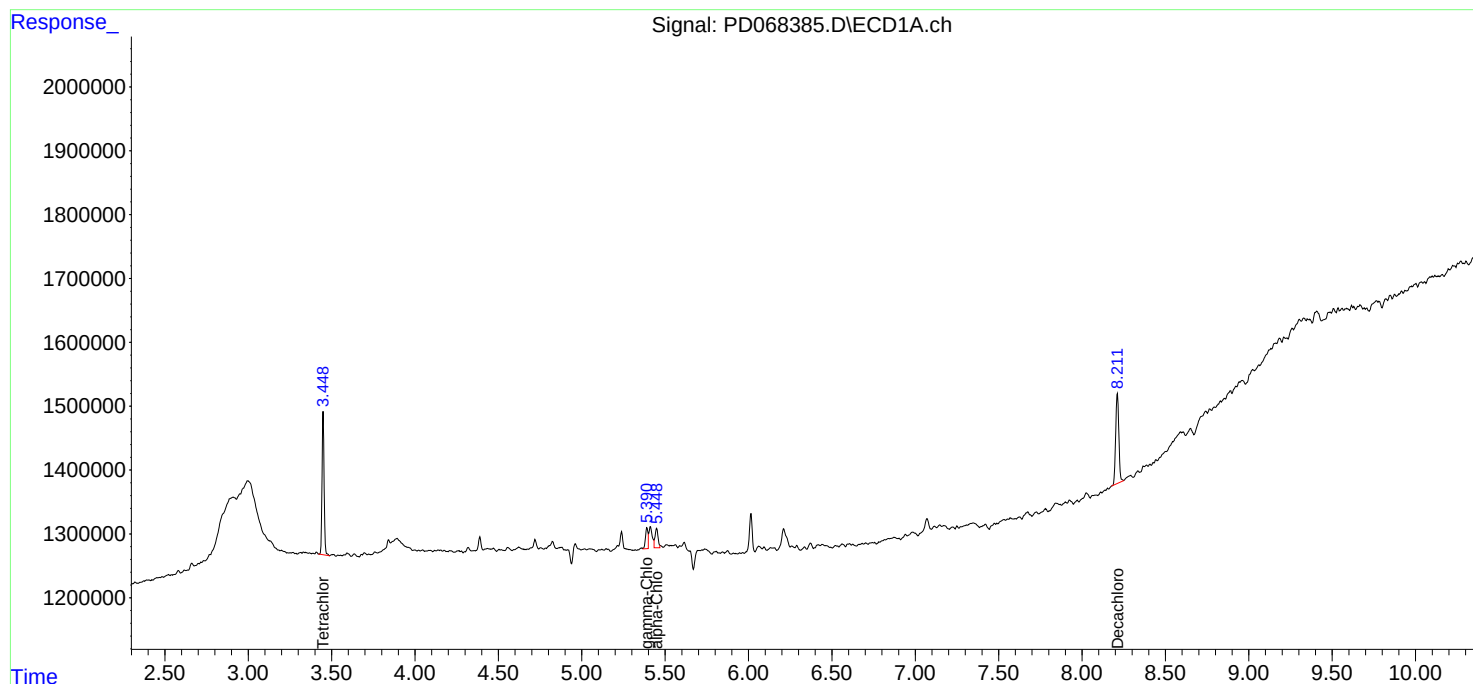

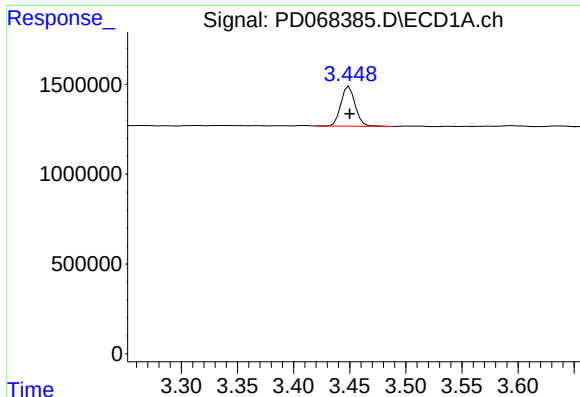


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 1963640
Conc: 1.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
CL-01-030422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

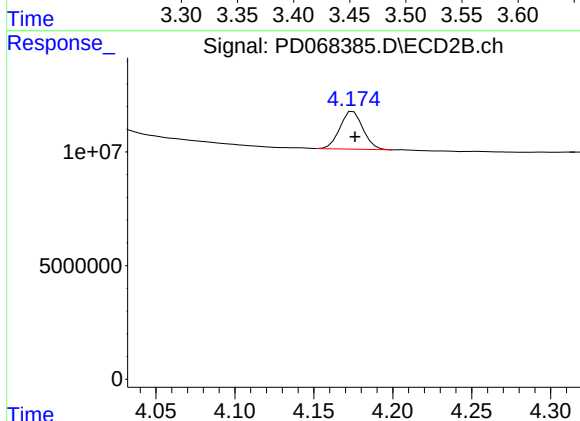


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.003 min
Response: 16999174
Conc: 1.77 ng/ml m

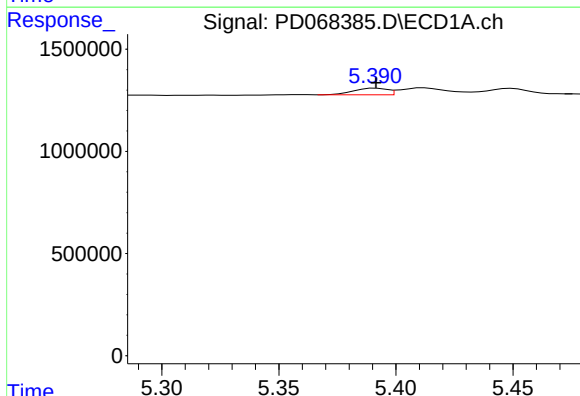


#10 gamma-Chlordane

R.T.: 5.390 min
Delta R.T.: -0.002 min
Response: 377928
Conc: 0.25 ng/ml m

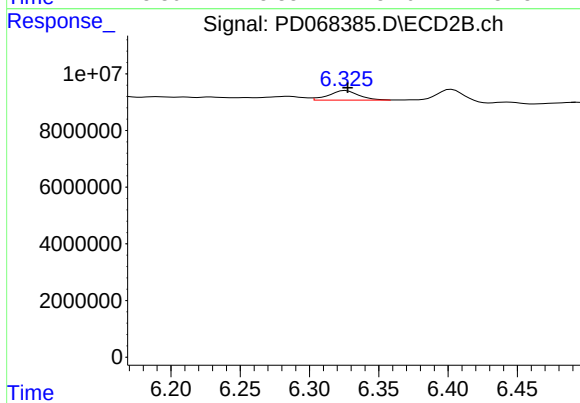

#10 gamma-Chlordane

R.T.: 6.325 min
Delta R.T.: -0.003 min
Response: 5030284
Conc: 0.48 ng/ml m

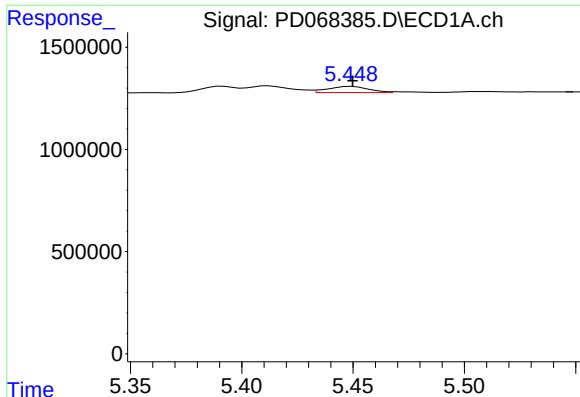


#11 alpha-Chlordane

R.T.: 5.448 min
Delta R.T.: -0.002 min
Response: 372658
Conc: 0.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
CL-01-030422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

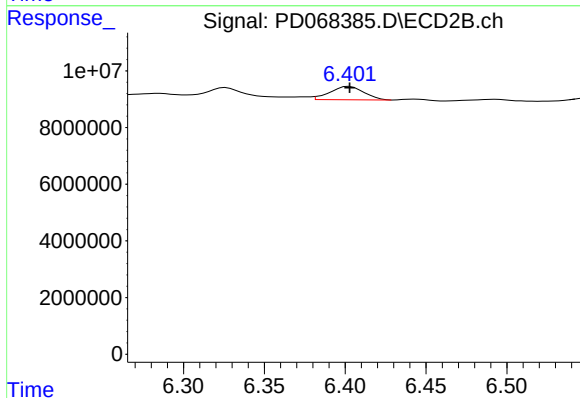


#11 alpha-Chlordane

R.T.: 6.401 min
Delta R.T.: -0.002 min
Response: 6711874
Conc: 0.65 ng/ml m

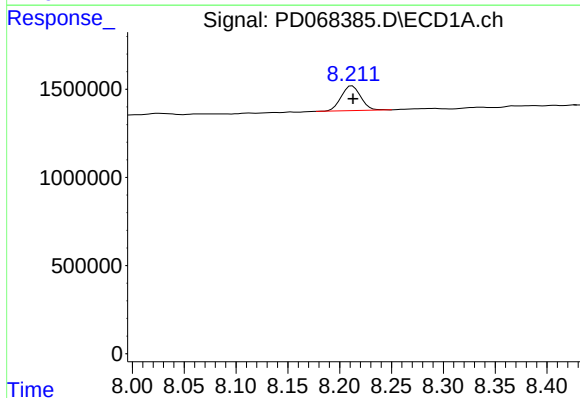

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 1846178
Conc: 1.59 ng/ml

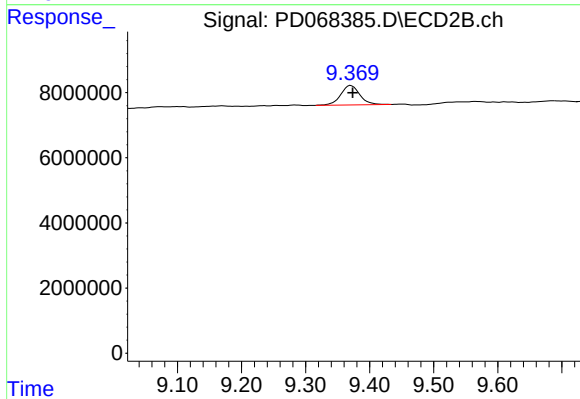

#28 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.003 min
Response: 12397138
Conc: 2.09 ng/ml