

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
 Data File : PD068405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 18:15
 Operator : AR\AJ
 Sample : N1831-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 AU-06-03072022

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/09/2022
 Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:11:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.176	13299498	93040190	11.345m	9.694
2)	SA Decachlor...	8.211	9.372	14115932	66727376	12.130	11.255
Target Compounds							
12)	B 4,4'-DDE	5.614	6.551	6993297	50330226	5.127m	5.148

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
Data File : PD068405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 18:15
Operator : AR\AJ
Sample : N1831-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
AU-06-03072022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/09/2022
Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:11:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

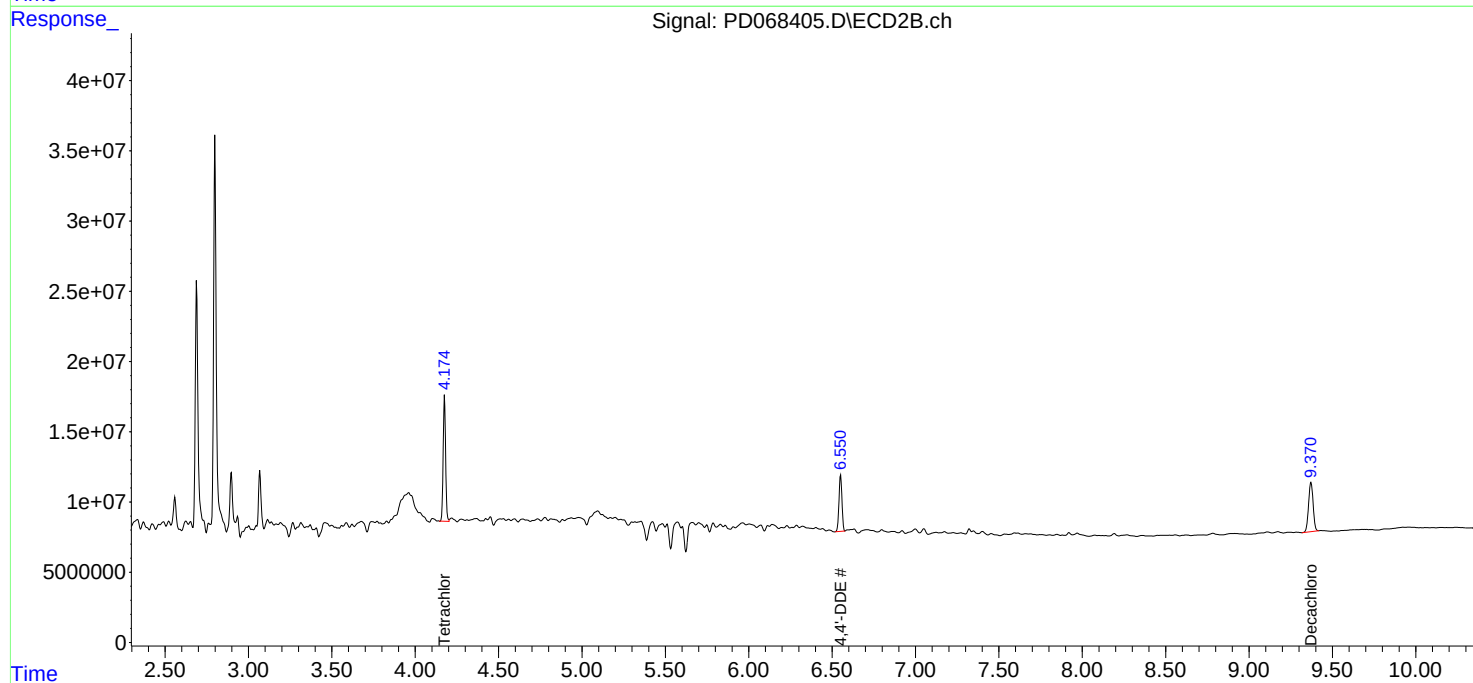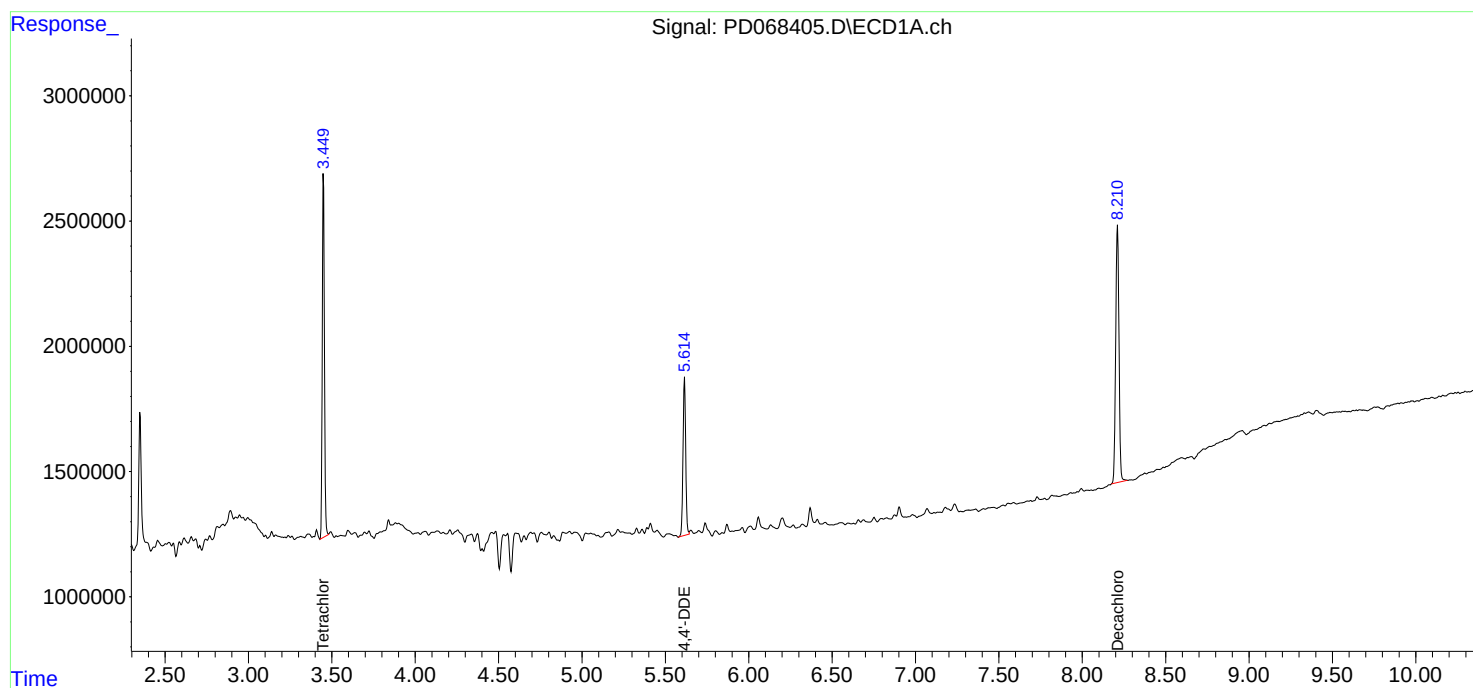

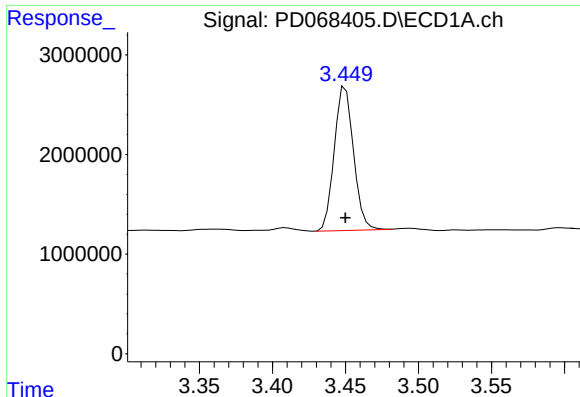


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: -0.001 min
Response: 13299498
Conc: 11.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-06-03072022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

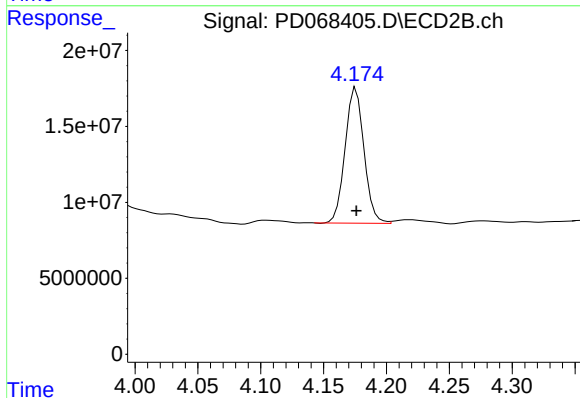


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 93040190
Conc: 9.69 ng/ml

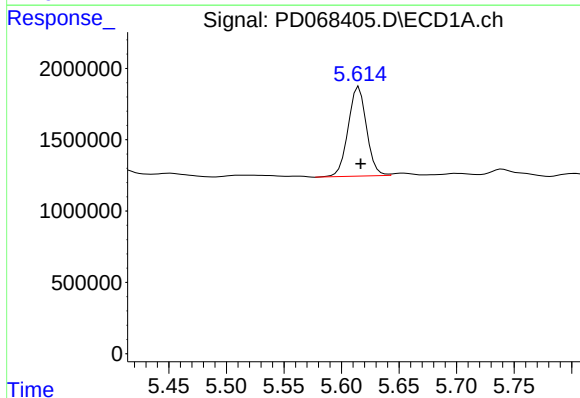


#12 4,4'-DDE

R.T.: 5.614 min
Delta R.T.: -0.003 min
Response: 6993297
Conc: 5.13 ng/ml m

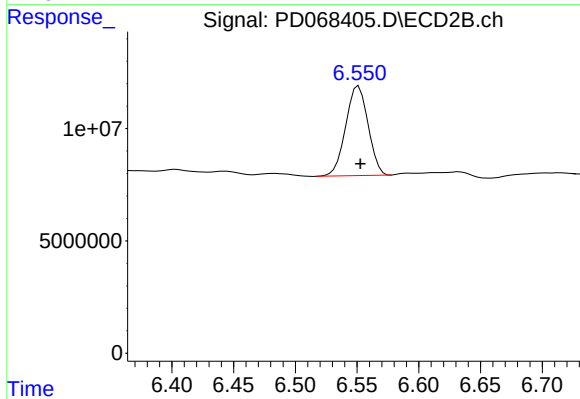

#12 4,4'-DDE

R.T.: 6.551 min
Delta R.T.: -0.002 min
Response: 50330226
Conc: 5.15 ng/ml

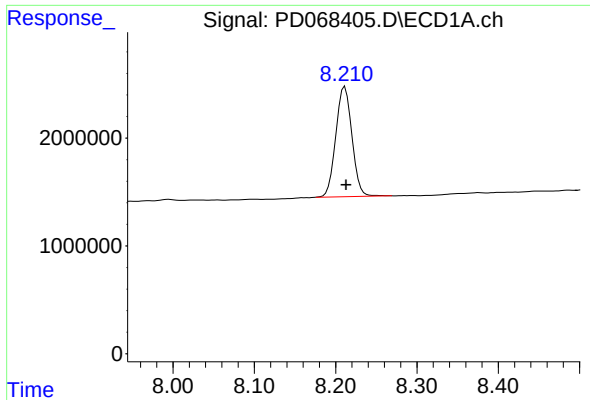


#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.001 min
Response: 14115932
Conc: 12.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
AU-06-03072022

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

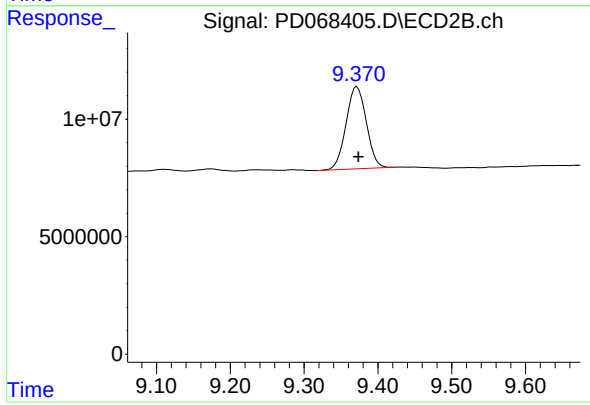

#28 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.002 min
Response: 66727376
Conc: 11.25 ng/ml