

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
 Data File : PD068411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 20:50
 Operator : AR\AJ
 Sample : N1833-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TR-05-03072022

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/09/2022
 Supervised By : Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 00:16:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.448	4.174	1937571	15711745	1.653m	1.637m
28) SA Decachlor...	8.210	9.369	2299188	10177528	1.976	1.717m
Target Compounds						
12) B 4,4'-DDE	5.612	6.552	1667065	21983365	1.222m	2.249 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030822\
Data File : PD068411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 20:50
Operator : AR\AJ
Sample : N1833-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TR-05-03072022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 00:16:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

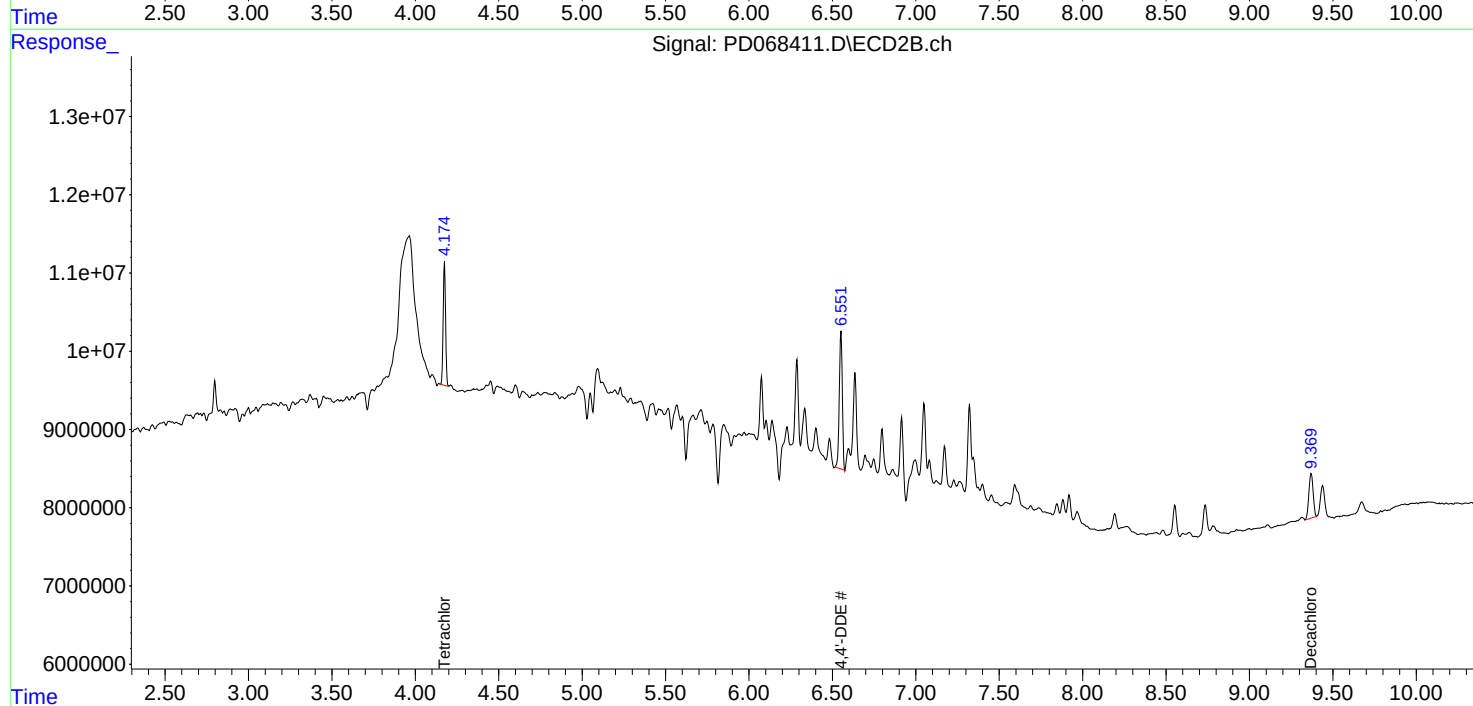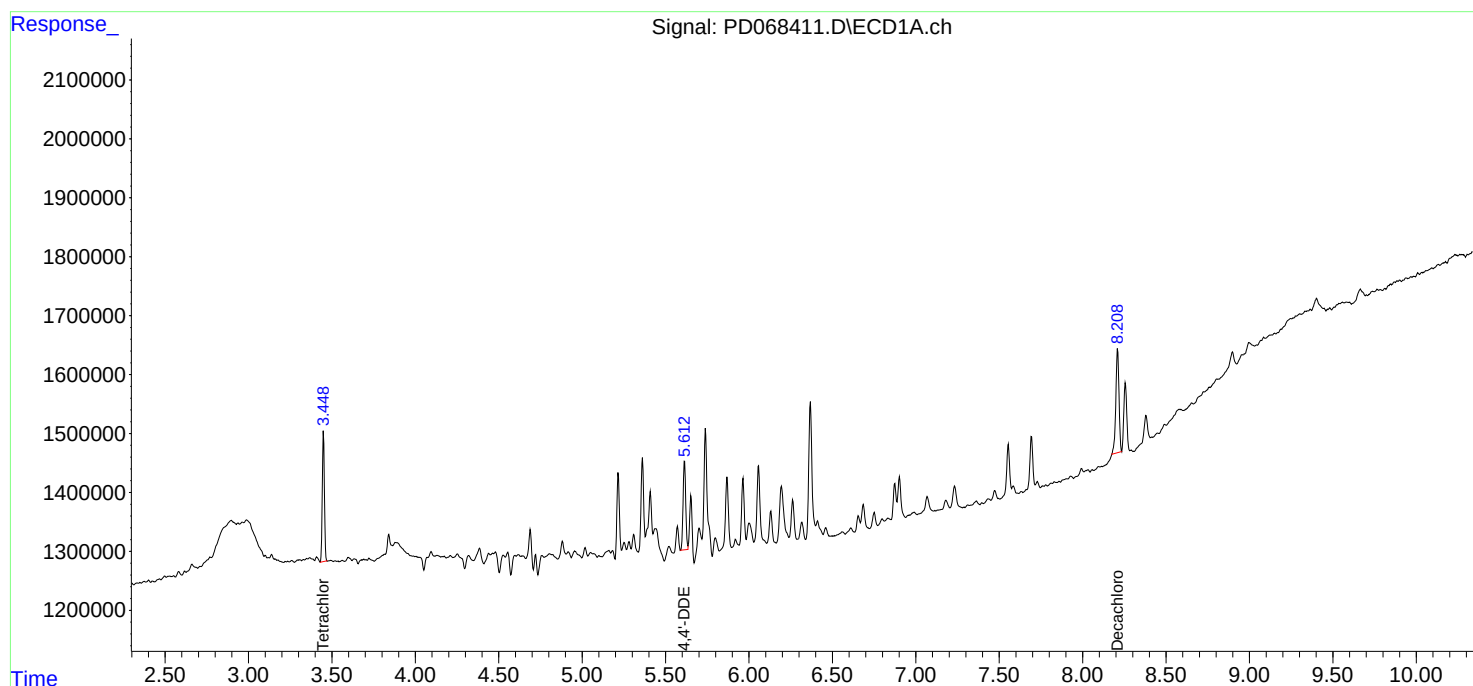

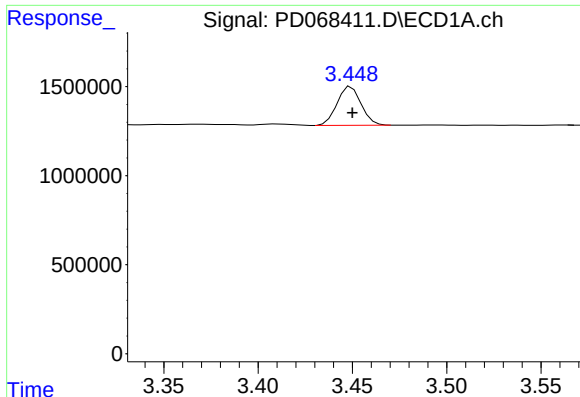


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: -0.002 min
Response: 1937571
Conc: 1.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-05-03072022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

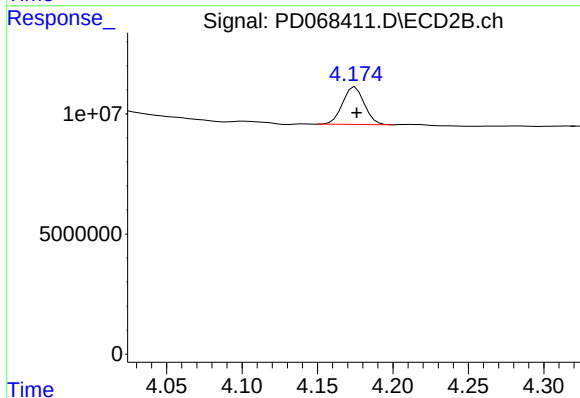


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.002 min
Response: 15711745
Conc: 1.64 ng/ml m

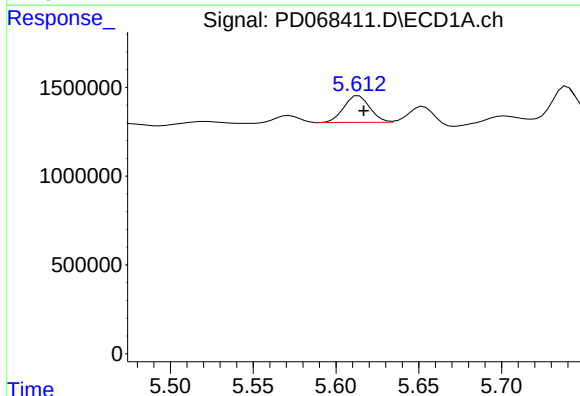


#12 4,4'-DDE

R.T.: 5.612 min
Delta R.T.: -0.004 min
Response: 1667065
Conc: 1.22 ng/ml m

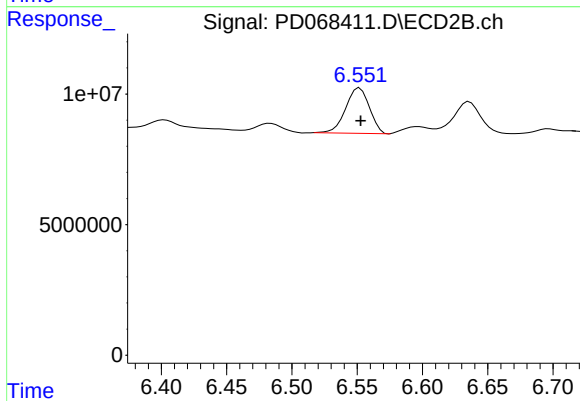

#12 4,4'-DDE

R.T.: 6.552 min
Delta R.T.: 0.000 min
Response: 21983365
Conc: 2.25 ng/ml

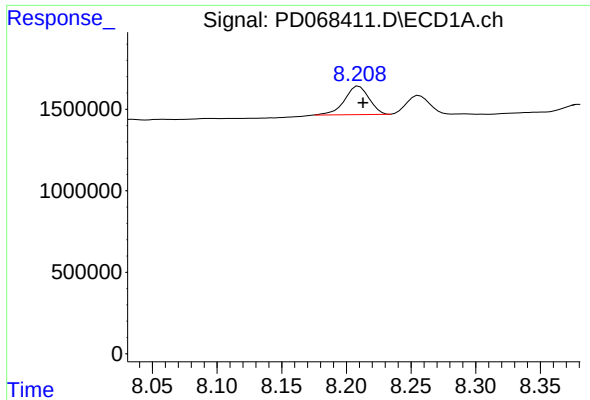


#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.003 min
Response: 2299188
Conc: 1.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-05-03072022

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

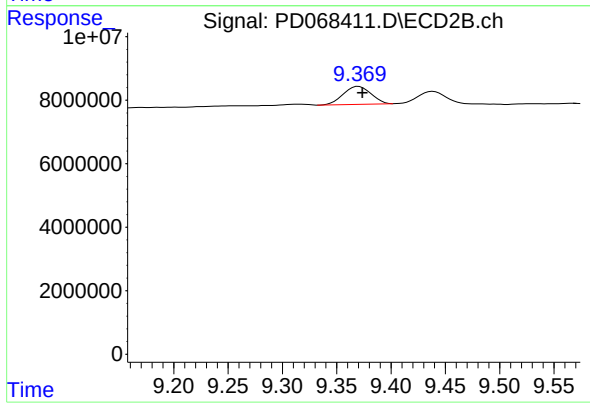

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.005 min
Response: 10177528
Conc: 1.72 ng/ml m