

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030823\
 Data File : PD074158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 16:57
 Operator : AR\AJ
 Sample : 01804-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/13/2023
 Supervised By : Ankita Jodhani 03/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 08:18:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 13 06:07:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.774	46126219	22768000	19.031	18.306
2)	SA Decachlor...	9.096	7.928	96186798	42732585	36.587	34.834
Target Compounds							
2)	A alpha-BHC	4.009	3.278	216.0E6	98366131	58.060	55.372
3)	MA gamma-BHC...	4.342	3.608	201.4E6	90340042	56.352	53.288
4)	MA Heptachlor	4.935	3.949	195.8E6	85623102	56.646	51.116m
5)	MB Aldrin	5.278	4.231	197.1E6	88481796	56.666	52.248
6)	B beta-BHC	4.536	3.902	82286480	38436465	49.534	45.961m
7)	B delta-BHC	4.785	4.135	167.9E6	81421419	57.337	45.925
8)	B Heptachlo...	5.705	4.734	172.6E6	80275086	56.901	50.547
9)	A Endosulfan I	6.090	5.103	162.9E6	73184424	54.958m	50.737m
10)	B trans-Chl...	5.961	4.984	174.6E6	81056520	55.669	52.244
11)	B cis-Chlor...	6.041	5.049	167.9E6	79039135	51.401	49.678
12)	B 4,4'-DDE	6.213	5.239	352.1E6	160.5E6	115.172	107.510
13)	MA Dieldrin	6.367	5.370	381.0E6	172.1E6	116.471	109.162
14)	MA Endrin	6.598	5.645	317.8E6	151.2E6	115.263	114.253
15)	B Endosulfa...	6.816	5.939	310.3E6	143.1E6	106.333	104.225
16)	A 4,4'-DDD	6.730	5.794	279.2E6	132.3E6	113.459	108.582
17)	MA 4,4'-DDT	7.045	6.045	319.6E6	143.7E6	118.301	111.614
18)	B Endrin al...	6.946	6.119	225.3E6	104.7E6	94.709	93.308
19)	B Endosulfa...	7.181	6.342	272.8E6	128.1E6	98.062	98.041
20)	A Methoxychlor	7.521	6.622	826.1E6	335.4E6	550.338	512.298
21)	B Endrin ke...	7.668	6.848	343.0E6	162.7E6	107.029	103.138

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030823\
Data File : PD074158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 16:57
Operator : AR\AJ
Sample : 01804-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 08:18:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD022223CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 13 06:07:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

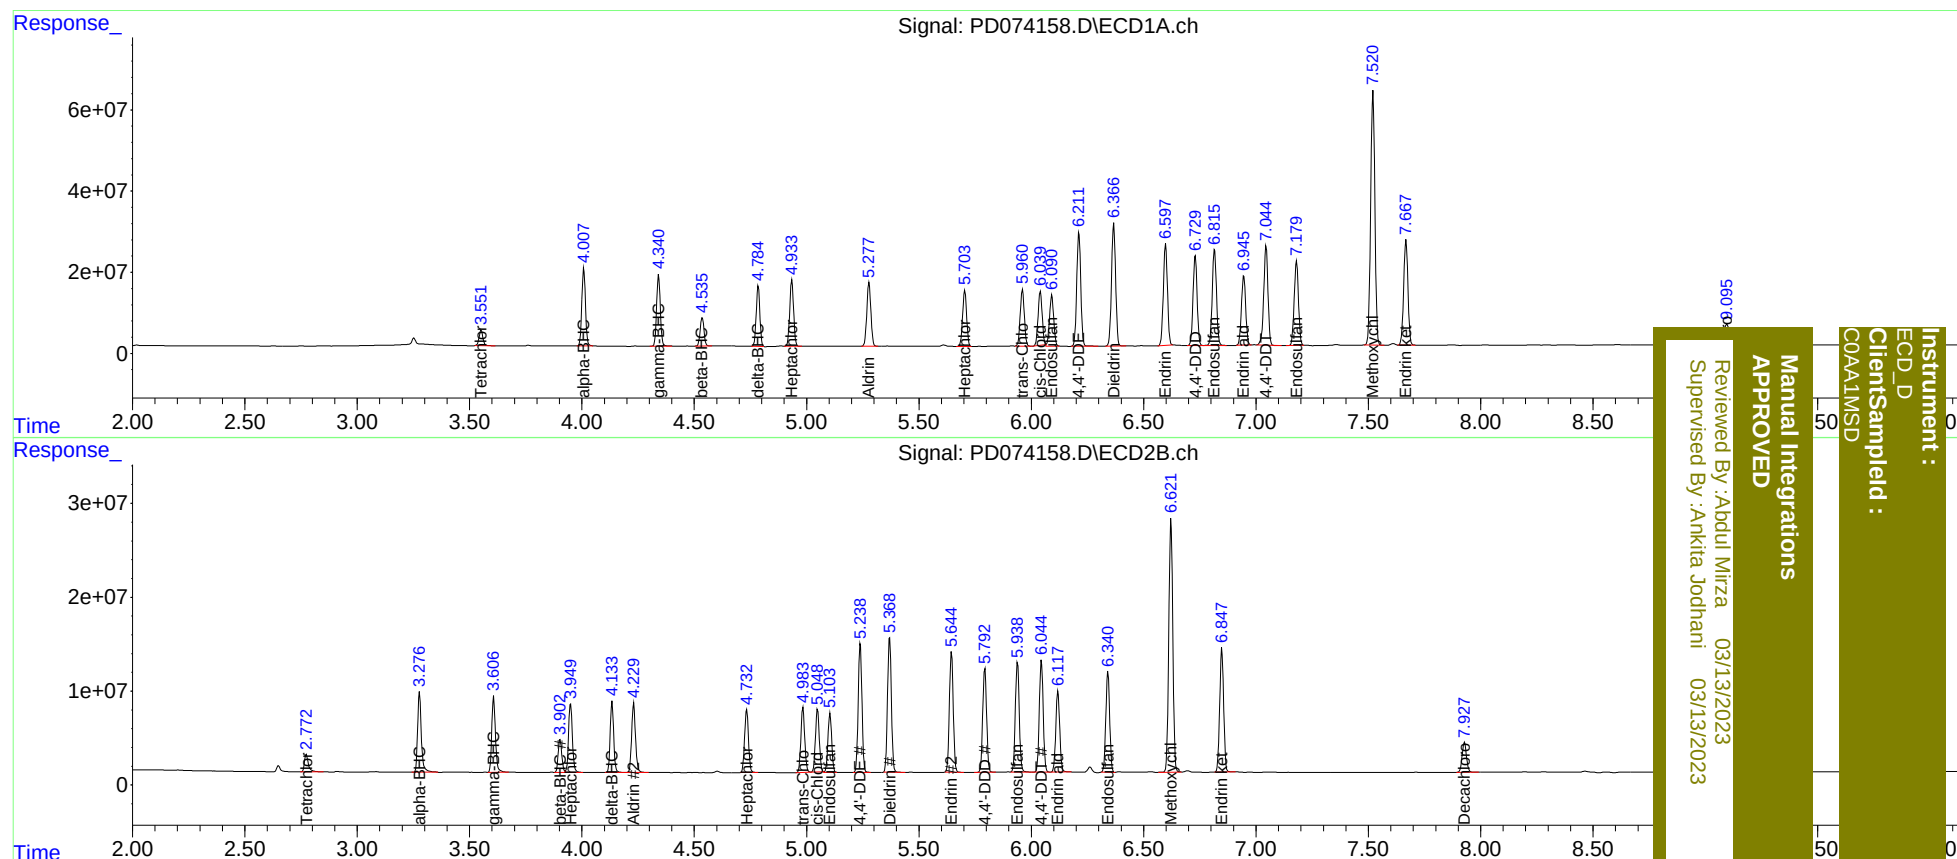

Instrument :
ECD_D
Client Sampled :
COA01MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/13/2023
Supervised By : Ankita Jodhani 03/13/2023