

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030920\
 Data File : PD057550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 12:06
 Operator : AJ\MA
 Sample : L1733-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:08:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 09 05:47:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.850f	0	561933	N.D.	0.233
Target Compounds							
2)	A alpha-BHC	0.000	4.232f	0	64242	N.D.	<MDL
3)	MA gamma-BHC...	3.933	0.000	941504	0	0.605	N.D. #
6)	B beta-BHC	0.000	4.779f	0	219707	N.D.	0.132
7)	B delta-BHC	0.000	4.921	0	593501	N.D.	0.198
8)	B Heptachlo...	4.837	0.000	34538	0	<MDL	N.D. #
9)	A Endosulfan I	0.000	6.103	0	228694	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.103f	0	228694	N.D.	<MDL
13)	MA Dieldrin	0.000	6.349	0	26203	N.D.	<MDL
15)	B Endosulfa...	0.000	6.798	0	284529	N.D.	<MDL
19)	B Endosulfa...	6.290f	0.000	1148207	0	0.920	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030920\
Data File : PD057550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 12:06
Operator : AJ\MA
Sample : L1733-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
PEST-GPC-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:08:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 09 05:47:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

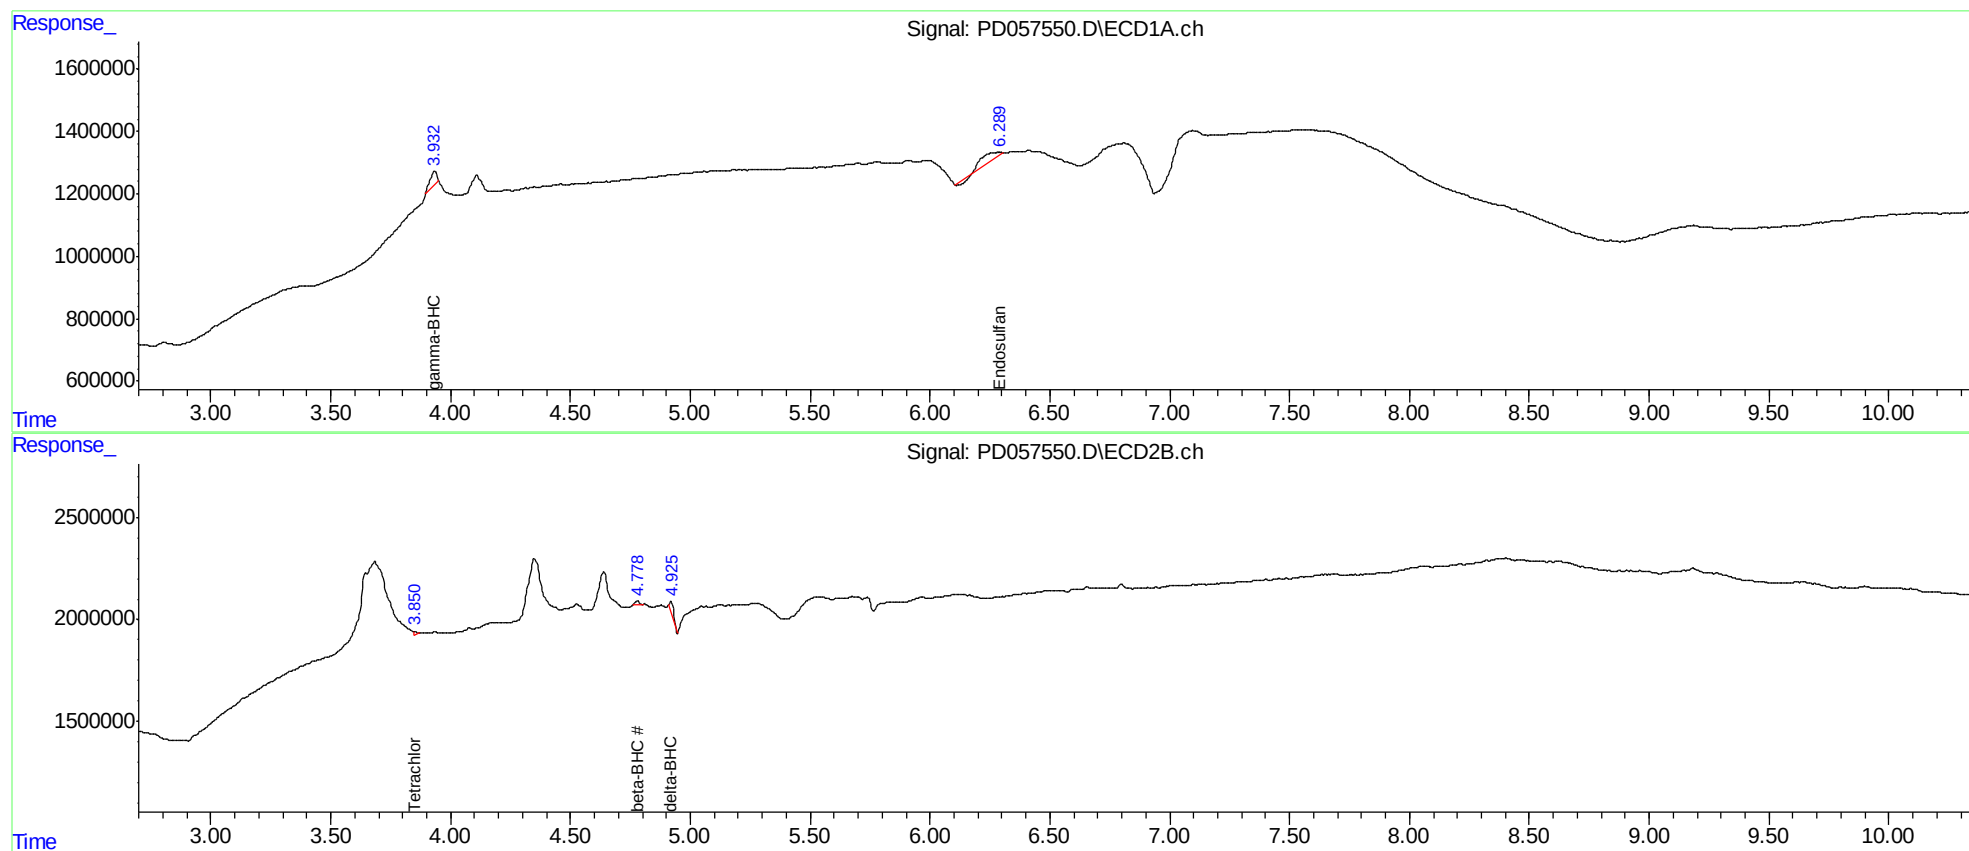


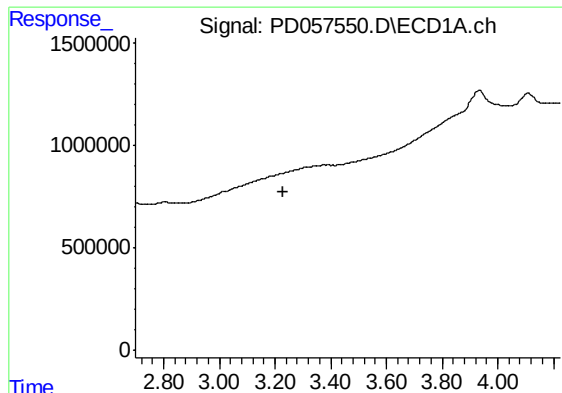

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK

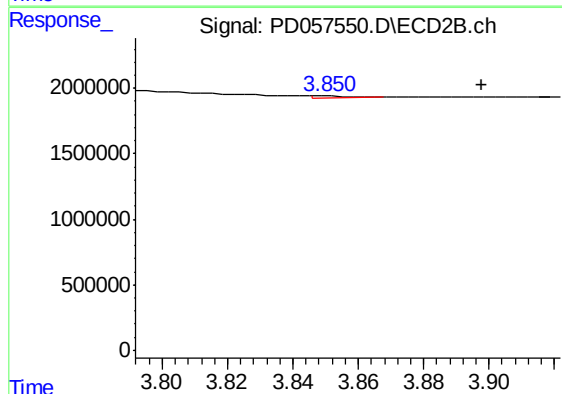


#1 Tetrachloro-m-xylene

R.T.: 3.850 min
Delta R.T.: -0.047 min
Response: 561933
Conc: 0.23 ng/ml

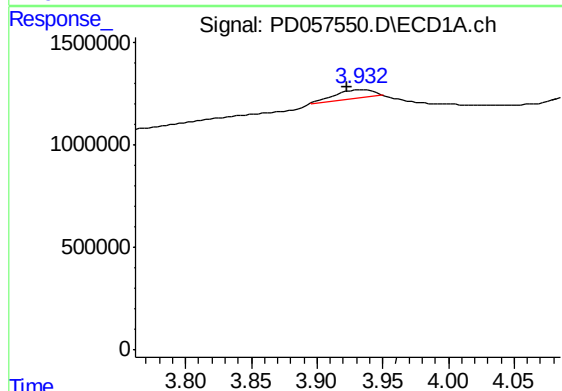


#3 gamma-BHC (Lindane)

R.T.: 3.933 min
Delta R.T.: 0.011 min
Response: 941504
Conc: 0.61 ng/ml

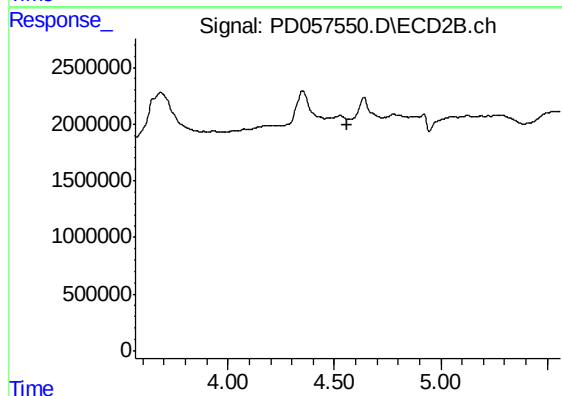

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.562 min
Response: 0
Conc: N.D.

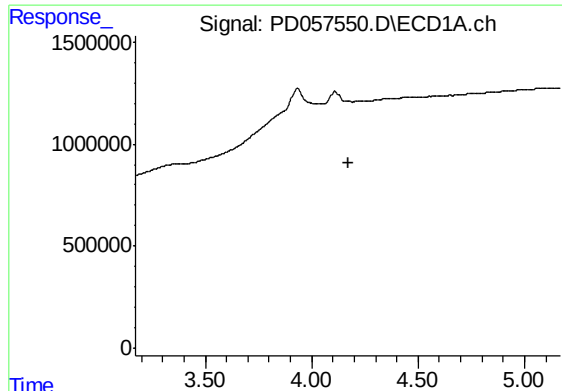

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK

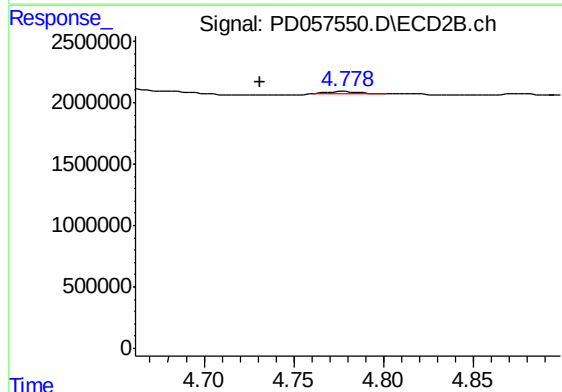


#6 beta-BHC

R.T.: 4.779 min
Delta R.T.: 0.048 min
Response: 219707
Conc: 0.13 ng/ml

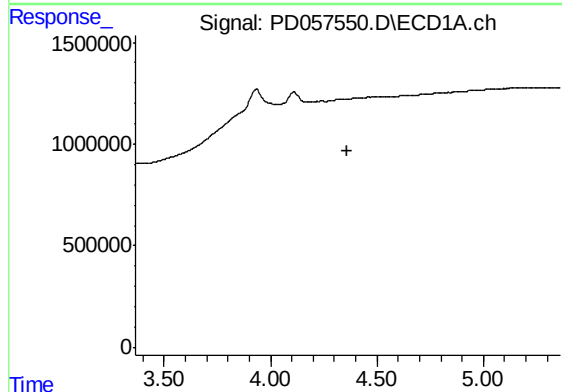


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.362 min
Response: 0
Conc: N.D.

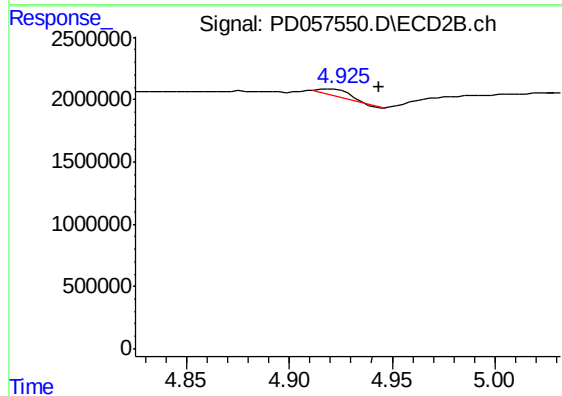

#7 delta-BHC


R.T.: 4.921 min
Delta R.T.: -0.023 min
Response: 593501
Conc: 0.20 ng/ml

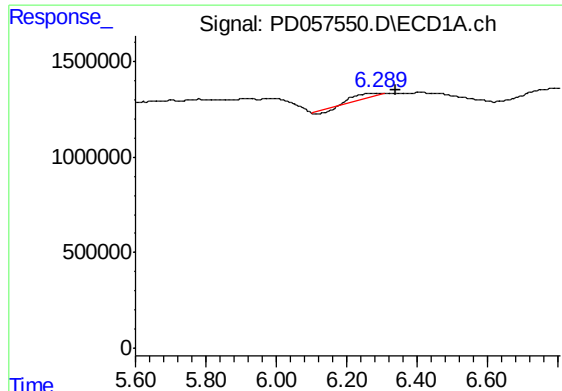

#19 Endosulfan Sulfate


R.T.: 6.290 min
Delta R.T.: -0.049 min
Response: 1148207
Conc: 0.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK

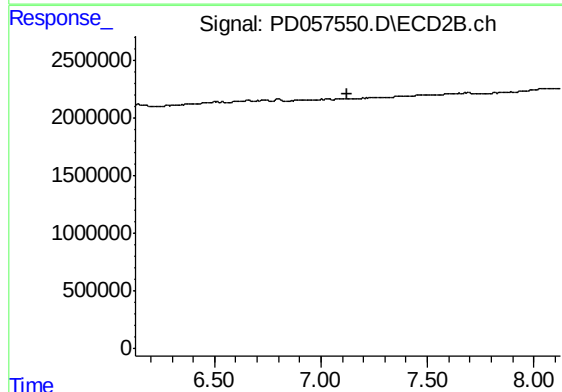


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.126 min
Response: 0
Conc: N.D.

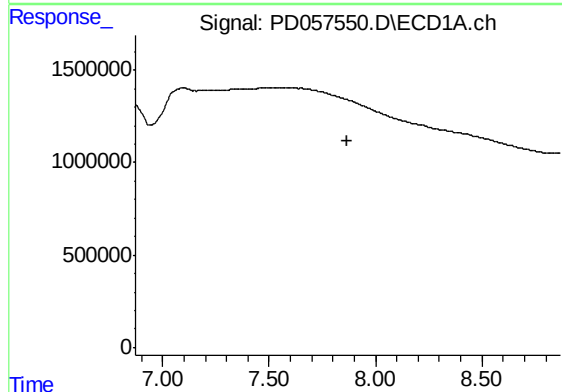

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.870 min
Response: 0
Conc: N.D.

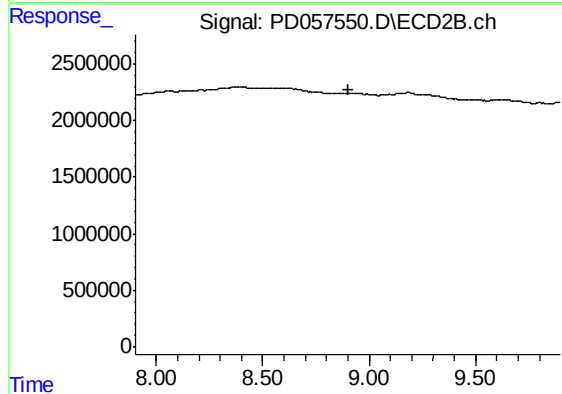

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.900 min
Response: 0
Conc: N.D.