

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030920\
 Data File : PD057563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 16:04
 Operator : AJ\MA
 Sample : L1707-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CB706

Manual Integrations
 APPROVED

mohammad
 3/10/2020 12:53:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:14:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 09 05:47:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	3.896	21933632	49061972	20.729	20.379
27)	SA Decachlor...	7.866	8.896	46051049	91431406	37.414	35.305
Target Compounds							
4)	MA Heptachlor	4.200	5.059	1239425	3868319	0.877m	1.056m
10)	B trans-Chl...	5.088	5.976	2733660	8865450	2.015m	2.480m
11)	B cis-Chlor...	5.145	6.051	2890535	12500924	2.115	3.488 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030920\
Data File : PD057563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 16:04
Operator : AJ\MA
Sample : L1707-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:14:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030620CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 09 05:47:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

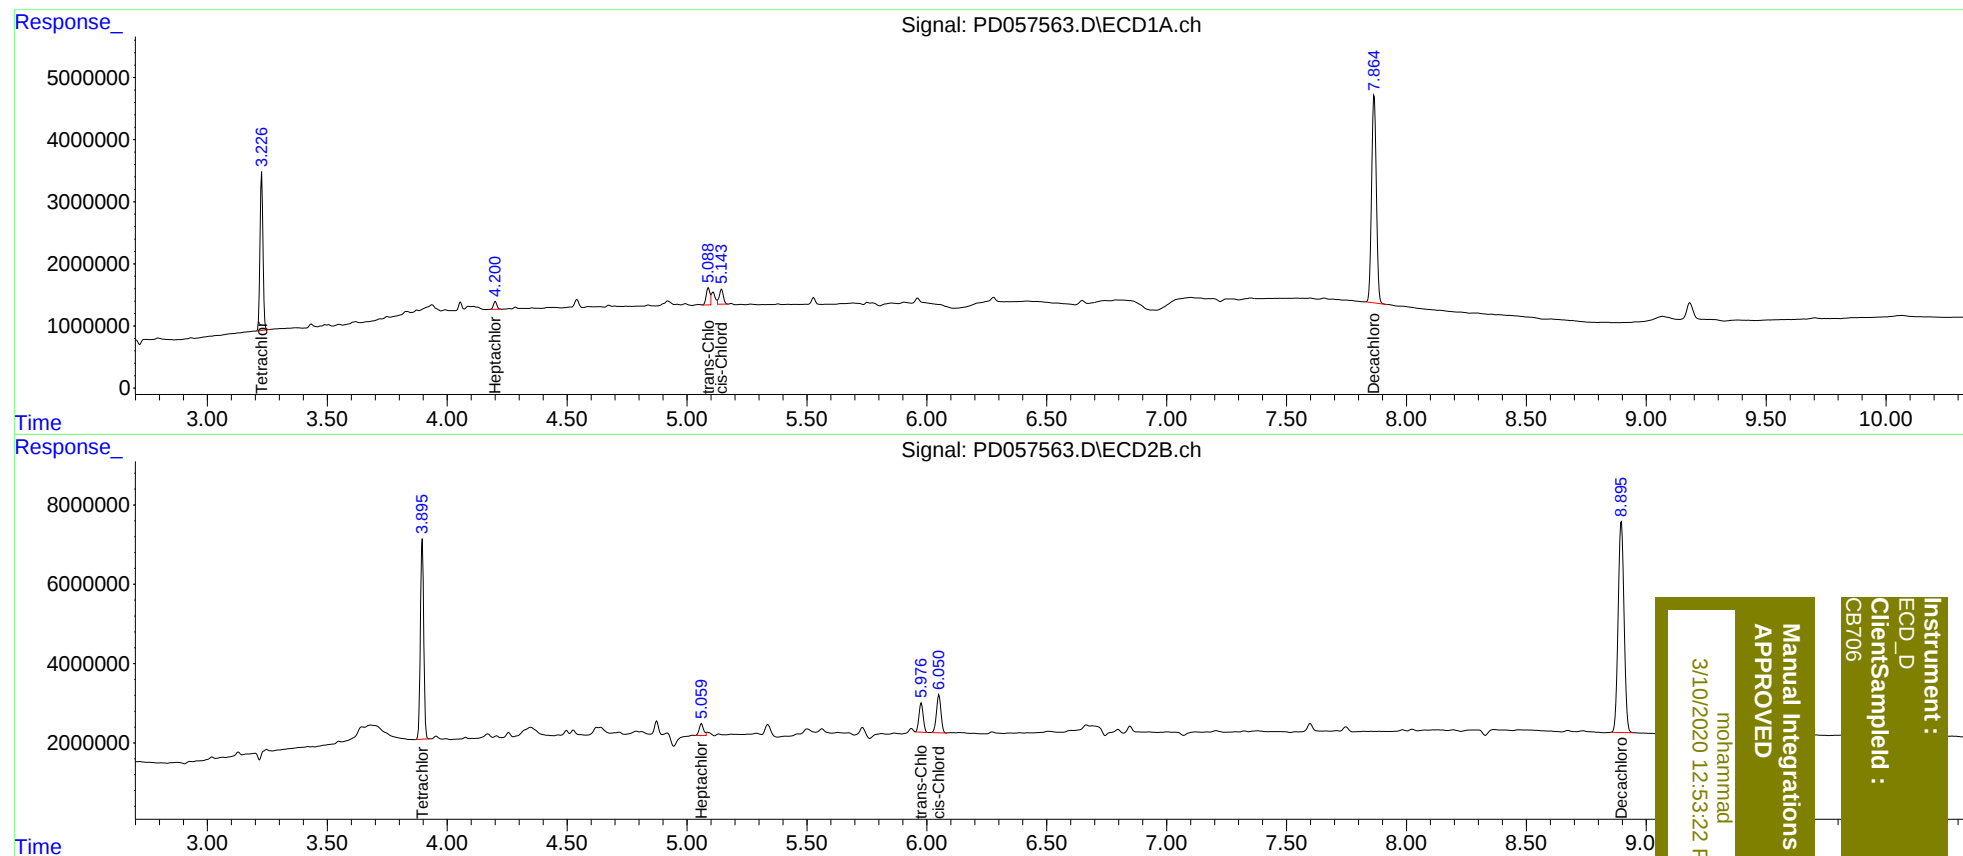

Manual Integrations
APPROVED

mohammad
3/10/2020 12:53:22 PM

Instrument :
ECD_D
ClientSampled :
CB706