

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030921\
 Data File : PD061486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 10:40
 Operator : AR\AJ
 Sample : M1344-02
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2021-04

Manual Integrations
 APPROVED

Ankita
 3/10/2021 2:01:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 00:28:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 05:53:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.980	19982623	206.7E6	21.995	22.133m
27)	SA Decachlor...	8.258	9.038	53791904	384.0E6	40.163	41.053
Target Compounds							
2)	A alpha-BHC	3.925	4.370	1224069	15668108	0.931	1.084
3)	MA gamma-BHC...	4.210	4.652	1339394	14818639	1.032	1.119m
4)	MA Heptachlor	4.514	5.161	1169611	13743580	0.868	1.009m
5)	MB Aldrin	4.764	5.467	1104064	12800895	0.856	0.965
6)	B beta-BHC	4.459	4.823	751002	4763773	1.136m	0.846 #
7)	B delta-BHC	4.667	5.039	1063711	16814830	0.802	1.197 #
8)	B Heptachlo...	5.208	5.854	1189330	14688190	0.931	1.208 #
9)	A Endosulfan I	5.549	6.209	1181762	11515190	0.982	1.011
10)	B trans-Chl...	5.436	6.087	1210133	13238537	0.900	1.026
11)	B cis-Chlor...	5.495	6.159	1208873	12358609	0.927	1.017
12)	B 4,4'-DDE	5.658	6.315	1056350	11480669	0.841	0.942m
13)	MA Dieldrin	5.793	6.466	1164940	12464169	0.882	1.025
14)	MA Endrin	6.049	6.683	1131033	9999401	0.978m	0.984m
15)	B Endosulfa...	6.325	6.892	1083561	11870858	0.949	1.212m#
16)	A 4,4'-DDD	6.175	6.804	814510	10562880	0.783m	1.096m#
17)	MA 4,4'-DDT	6.417	7.104	829191	11204771	0.747	1.151 #
18)	B Endrin al...	6.493	7.016	975491	11325664	1.003	1.339 #
19)	B Endosulfa...	6.707	7.239	1106297	11565794	0.959	1.183
20)	A Methoxychlor	6.966	7.560	288068	5045349	0.472	1.107 #
21)	B Endrin ke...	7.200	7.709	1296723	10167323	0.982	1.060

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030921\
Data File : PD061486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 10:40
Operator : AR\AJ
Sample : M1344-02
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 00:28:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030421CLP.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 05:53:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

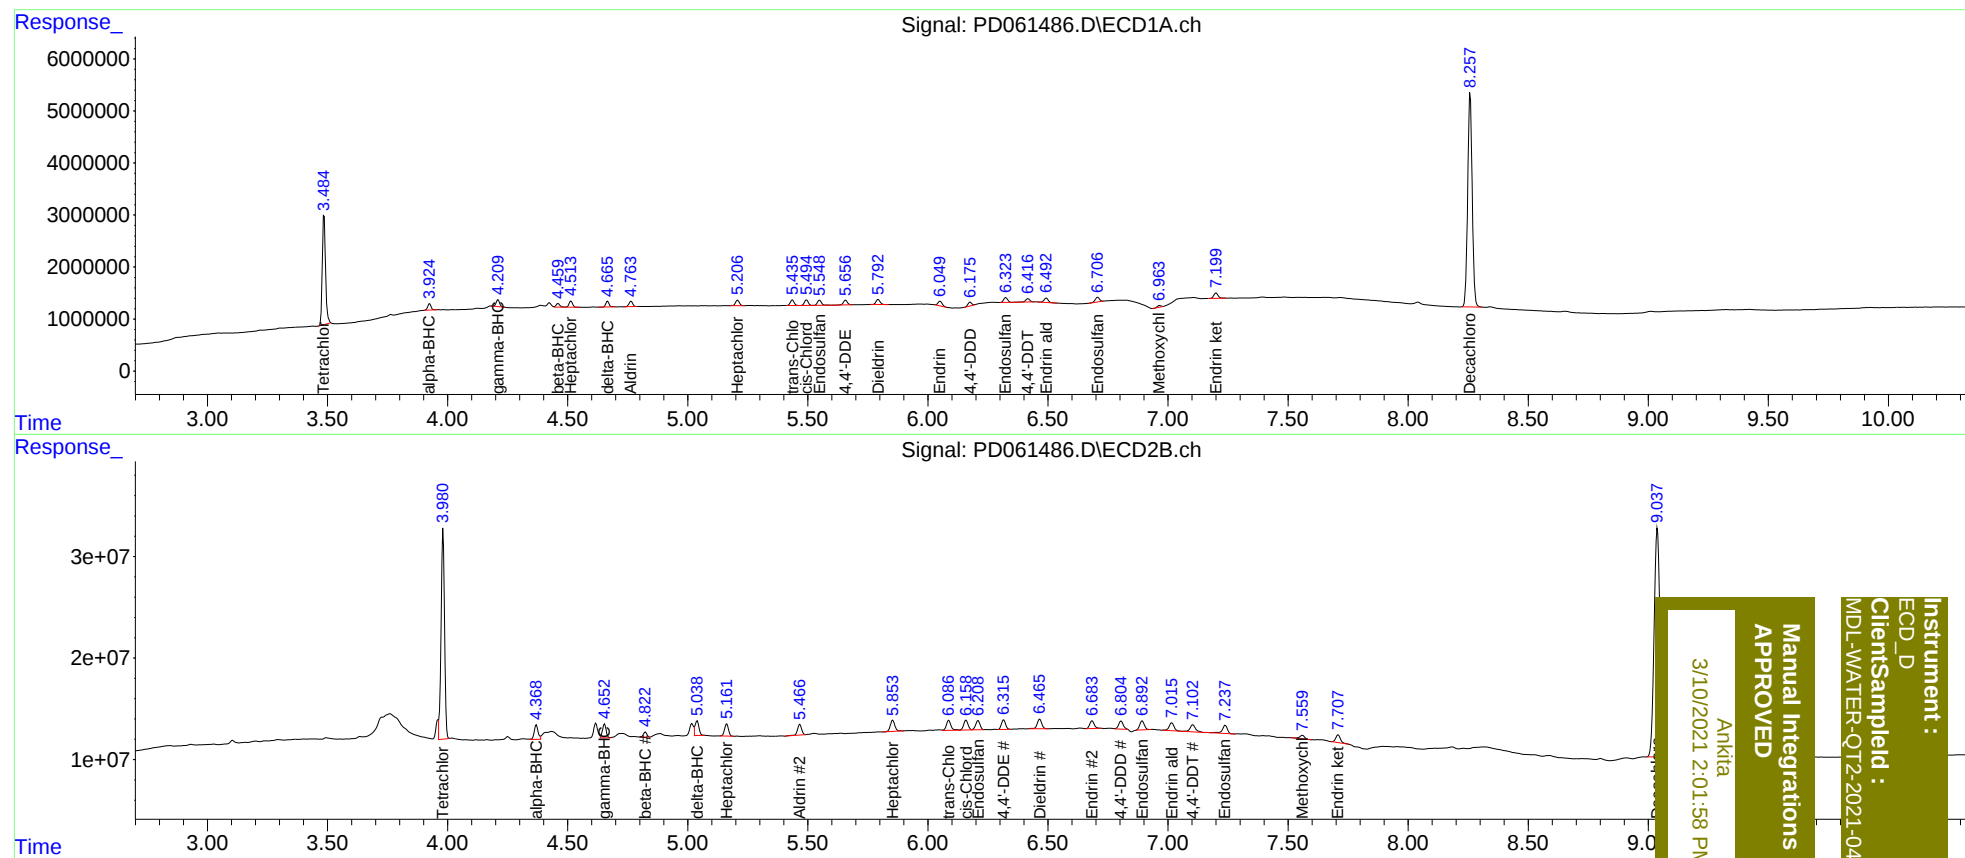

Manual Integrations
APPROVED

Ankita
3/10/2021 2:01:58 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT2-2021-04