

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030922\
 Data File : PD068422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 15:49
 Operator : AR\AJ
 Sample : N1851-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:24:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) MA	gamma-BHC...	0.000	4.851	0	51045	N.D. 0.004 #
5) MB	Aldrin	0.000	5.724f	0	304682	N.D. 0.026 #
7) B	delta-BHC	4.651f	5.268f	148185	92998	0.092 0.007 #
8) B	Heptachlo...	0.000	6.081	0	806356	N.D. 0.075 #
15) B	Endosulfa...	0.000	7.128	0	155695	N.D. 0.019 #
17) MA	4,4'-DDT	0.000	7.332	0	97719	N.D. 0.014 #
20) A	Methoxychlor	0.000	7.776f	0	687434	N.D. 0.198 #
21) B	Endrin ke...	0.000	7.969	0	4022065	N.D. 0.479 #
22)	Mirex	0.000	8.442	0	899652	N.D. 0.141 #
23)	Chlordane-1	0.000	5.180f	0	890380	N.D. 2.199 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030922\
Data File : PD068422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 15:49
Operator : AR\AJ
Sample : N1851-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:24:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

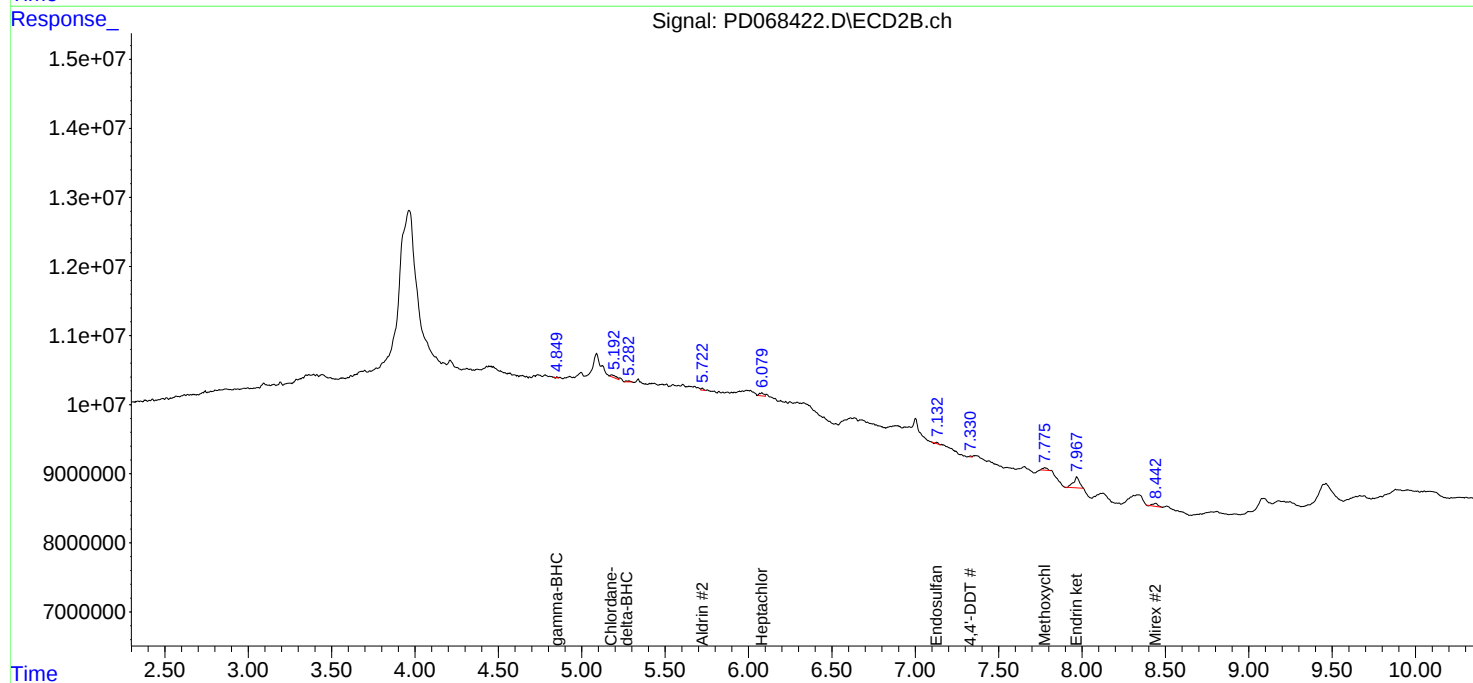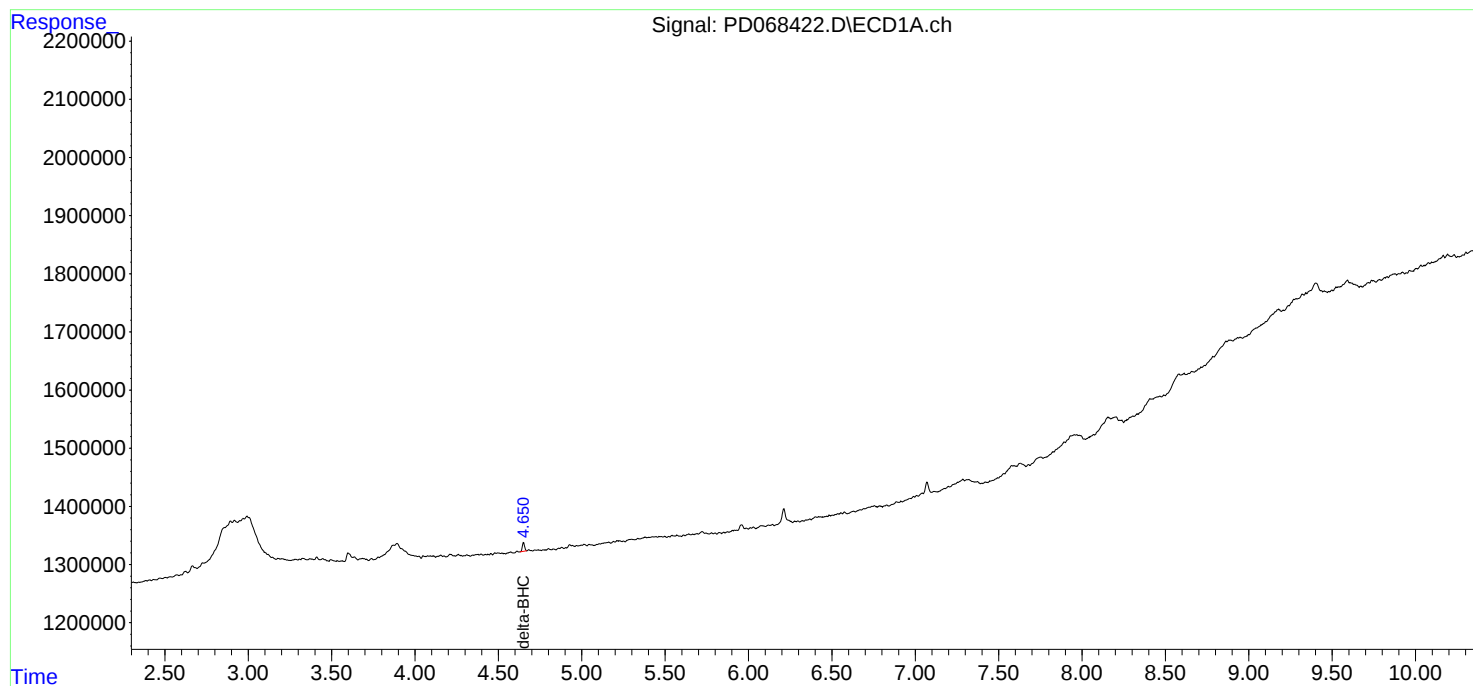


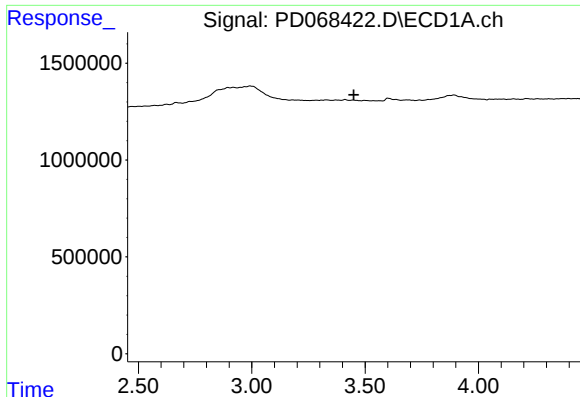

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

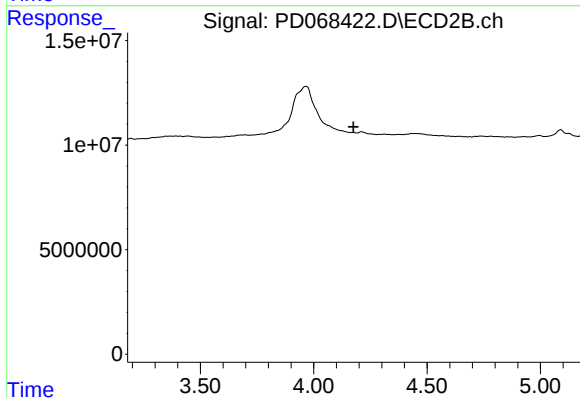


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.176 min
Response: 0
Conc: N.D.

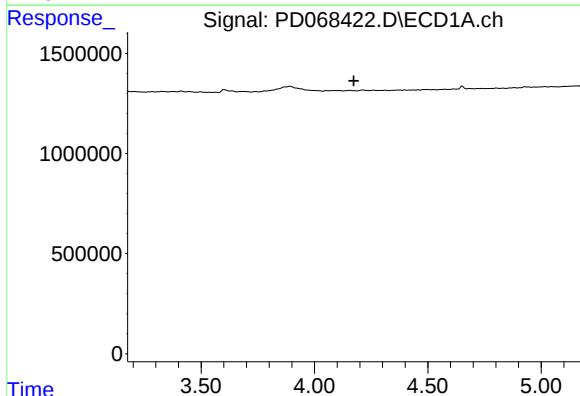


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.173 min
Response: 0
Conc: N.D.

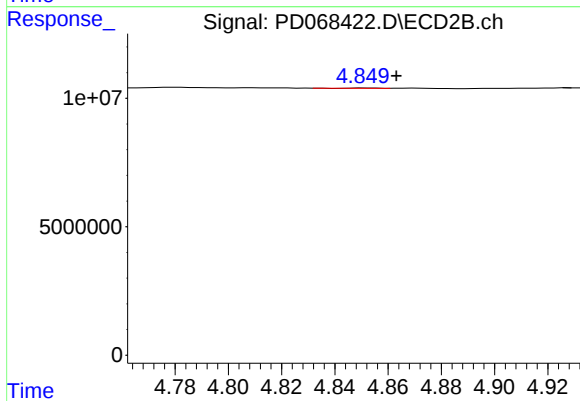

#3 gamma-BHC (Lindane)


R.T.: 4.851 min
Delta R.T.: -0.012 min
Response: 51045
Conc: 0.00 ng/ml

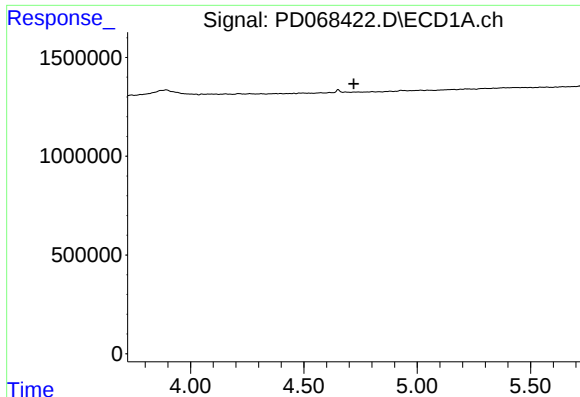

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.720 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

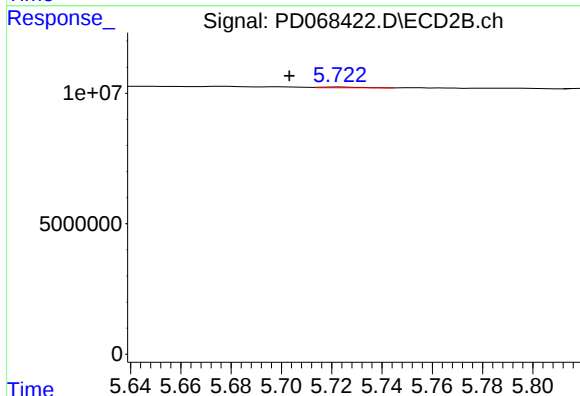


#5 Aldrin

R.T.: 5.724 min
Delta R.T.: 0.020 min
Response: 304682
Conc: 0.03 ng/ml

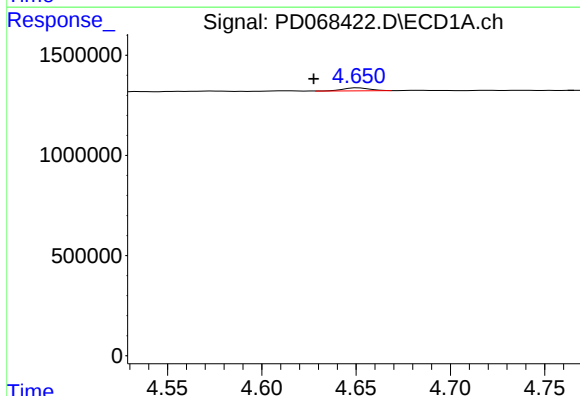


#7 delta-BHC

R.T.: 4.651 min
Delta R.T.: 0.024 min
Response: 148185
Conc: 0.09 ng/ml

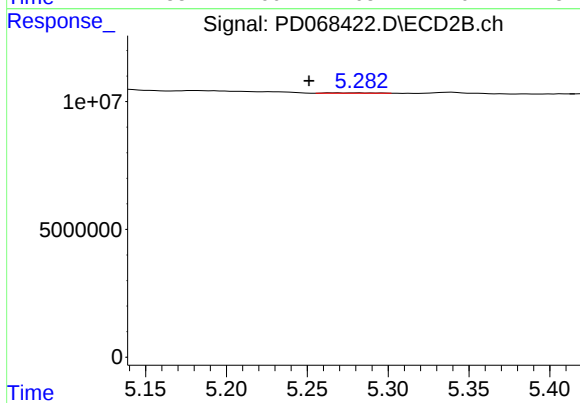

#7 delta-BHC


R.T.: 5.268 min
Delta R.T.: 0.017 min
Response: 92998
Conc: 0.01 ng/ml

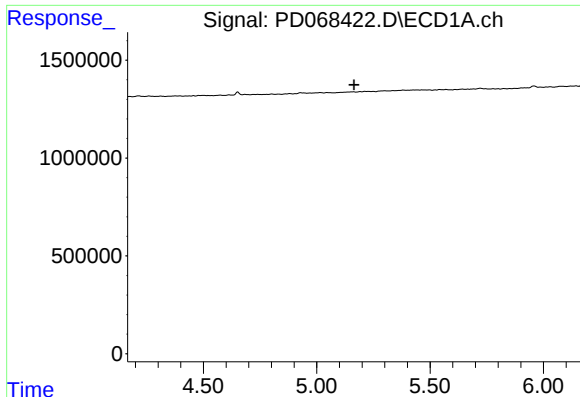

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

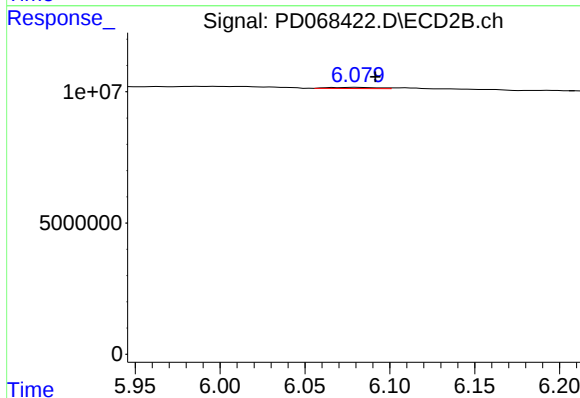


#8 Heptachlor epoxide

R.T.: 6.081 min
Delta R.T.: -0.010 min
Response: 806356
Conc: 0.08 ng/ml

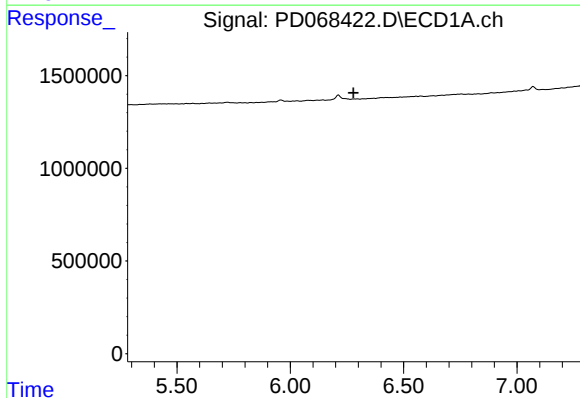


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

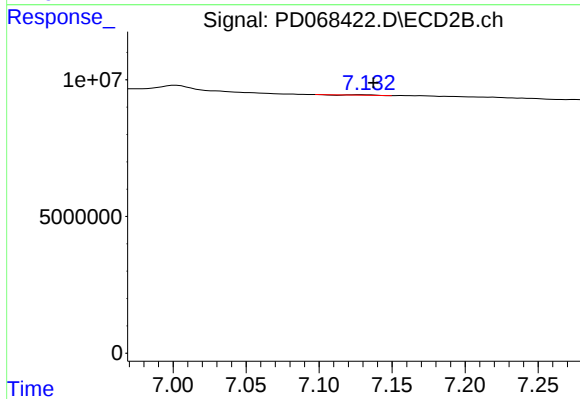

#15 Endosulfan II


R.T.: 7.128 min
Delta R.T.: -0.010 min
Response: 155695
Conc: 0.02 ng/ml

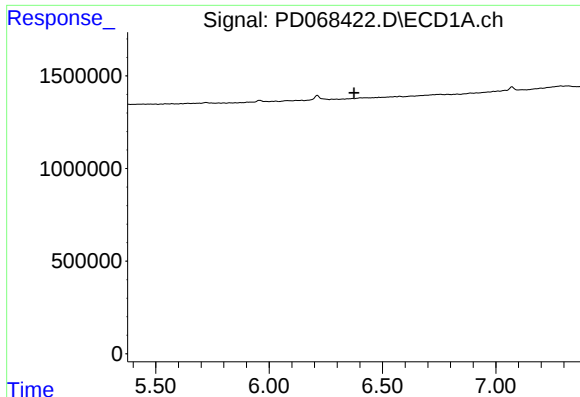

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.374 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

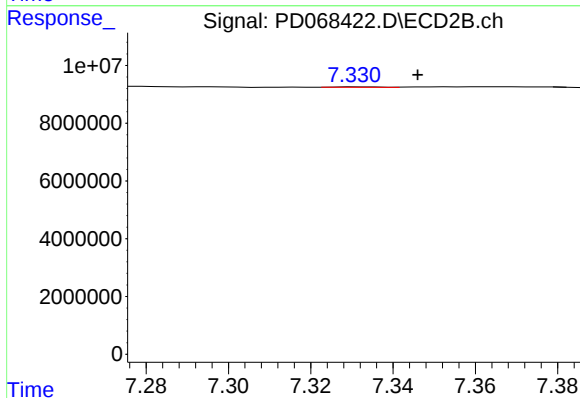


#17 4,4'-DDT

R.T.: 7.332 min
Delta R.T.: -0.014 min
Response: 97719
Conc: 0.01 ng/ml

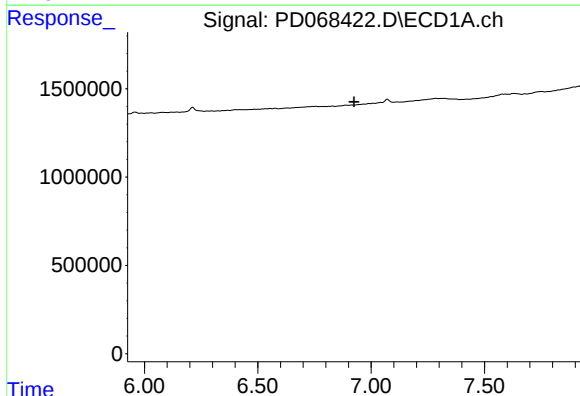


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.925 min
Response: 0
Conc: N.D.

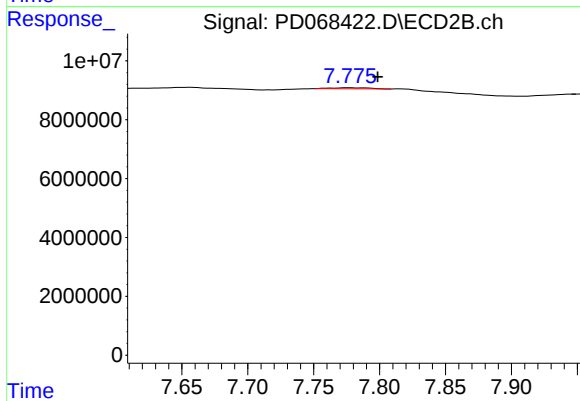

#20 Methoxychlor


R.T.: 7.776 min
Delta R.T.: -0.022 min
Response: 687434
Conc: 0.20 ng/ml

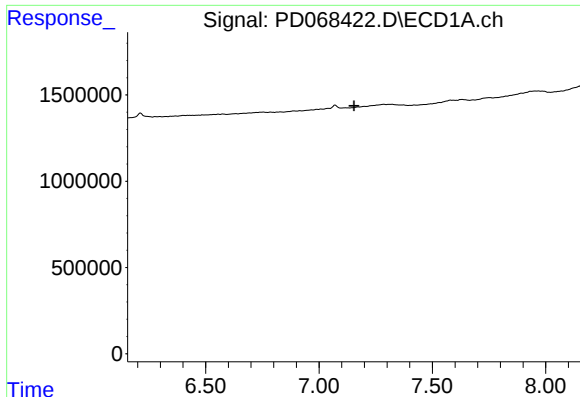

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

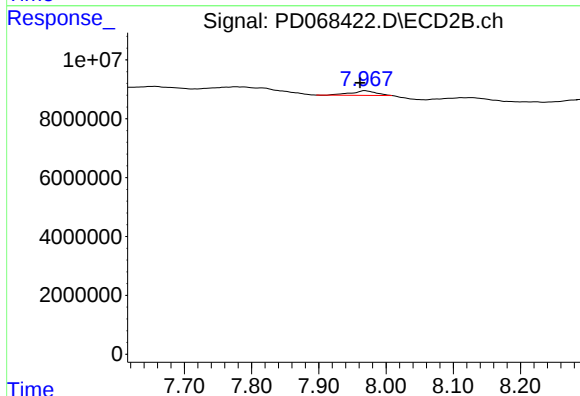


#21 Endrin ketone

R.T.: 7.969 min
Delta R.T.: 0.008 min
Response: 4022065
Conc: 0.48 ng/ml

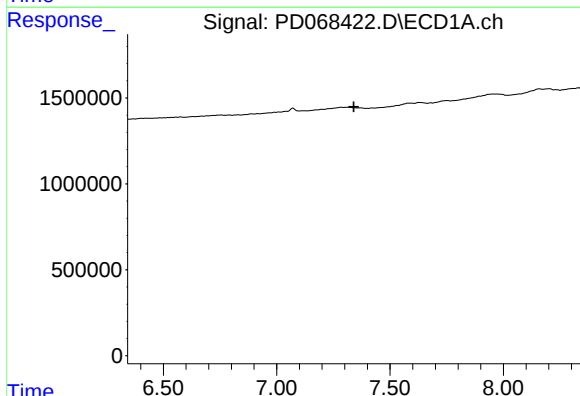


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.340 min
Response: 0
Conc: N.D.

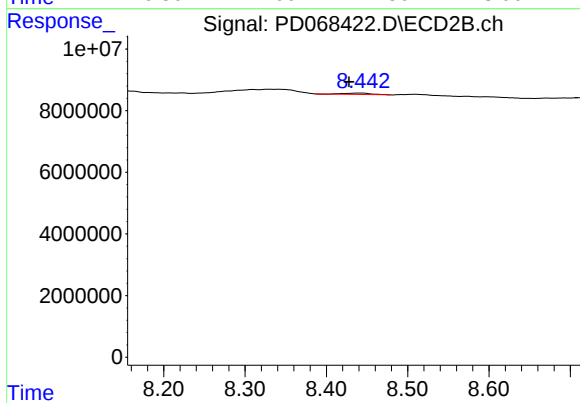

#22 Mirex


R.T.: 8.442 min
Delta R.T.: 0.014 min
Response: 899652
Conc: 0.14 ng/ml

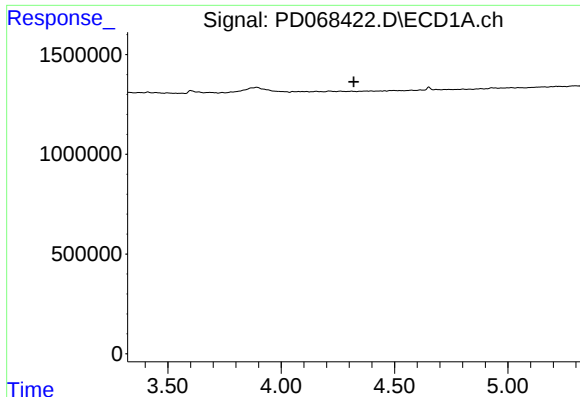

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

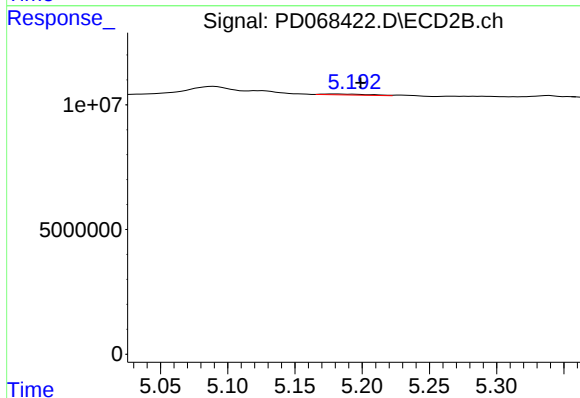


#23 Chlordane-1

R.T.: 5.180 min
Delta R.T.: -0.019 min
Response: 890380
Conc: 2.20 ng/ml

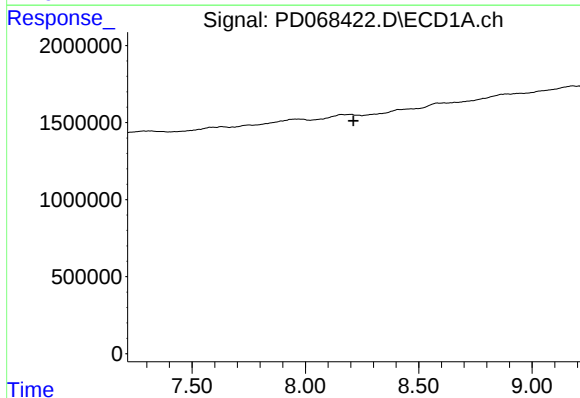

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.213 min
Response: 0
Conc: N.D.

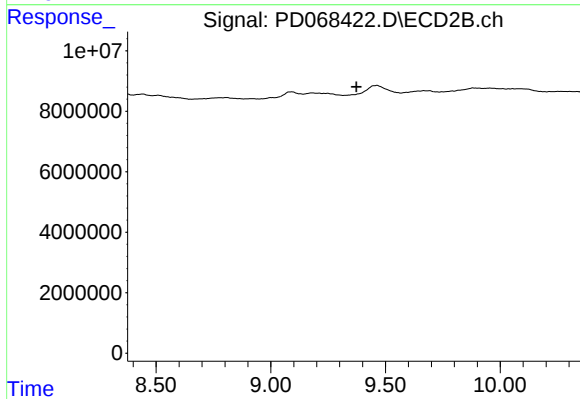

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.374 min
Response: 0
Conc: N.D.