

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030922\
 Data File : PD068421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 15:35
 Operator : AR\AJ
 Sample : N1843-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FS-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:23:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.176	12797365	108.0E6	10.917	11.249
28)	SA Decachlor...	8.213	9.373	16964198	87673009	14.578	14.788
Target Compounds							
12)	B 4,4'-DDE	5.616	6.552	7358552	85713598	5.395	8.767m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030922\
Data File : PD068421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 15:35
Operator : AR\AJ
Sample : N1843-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
FS-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:23:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

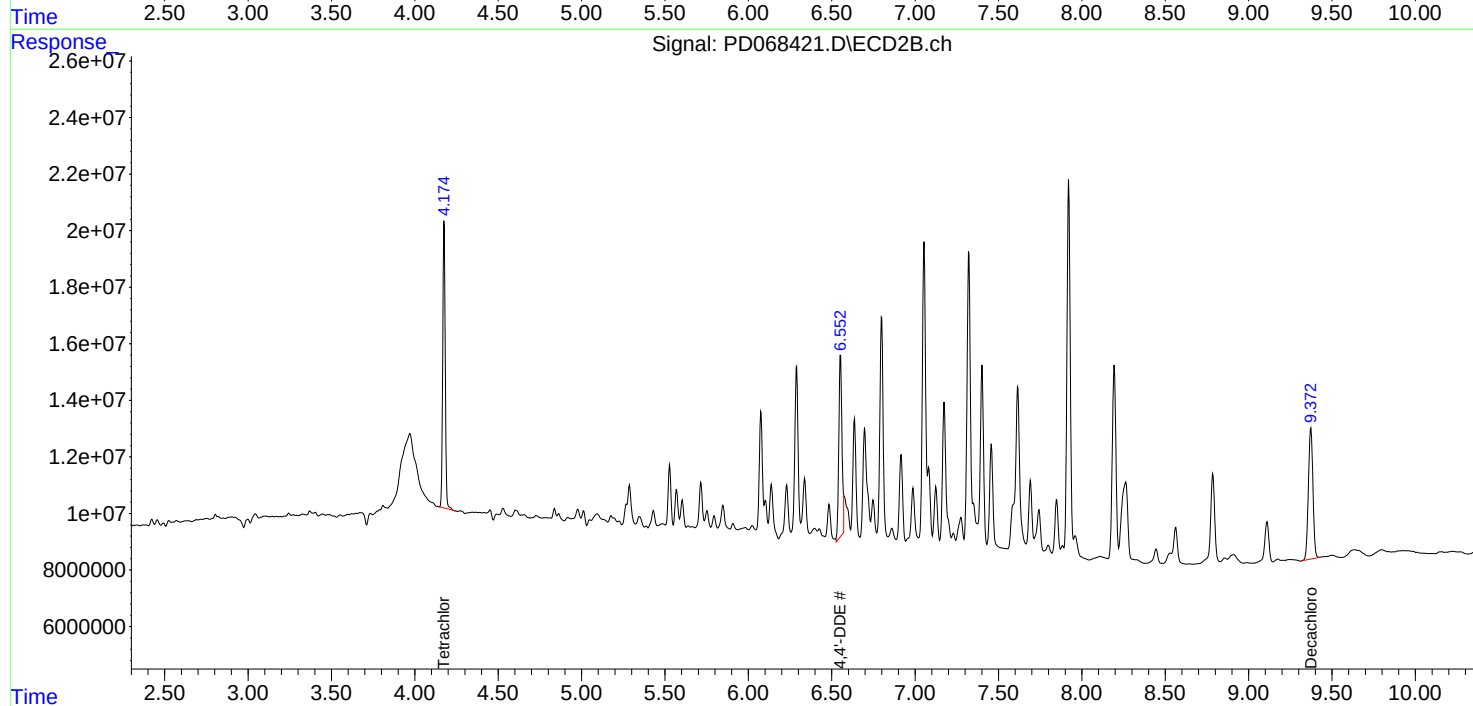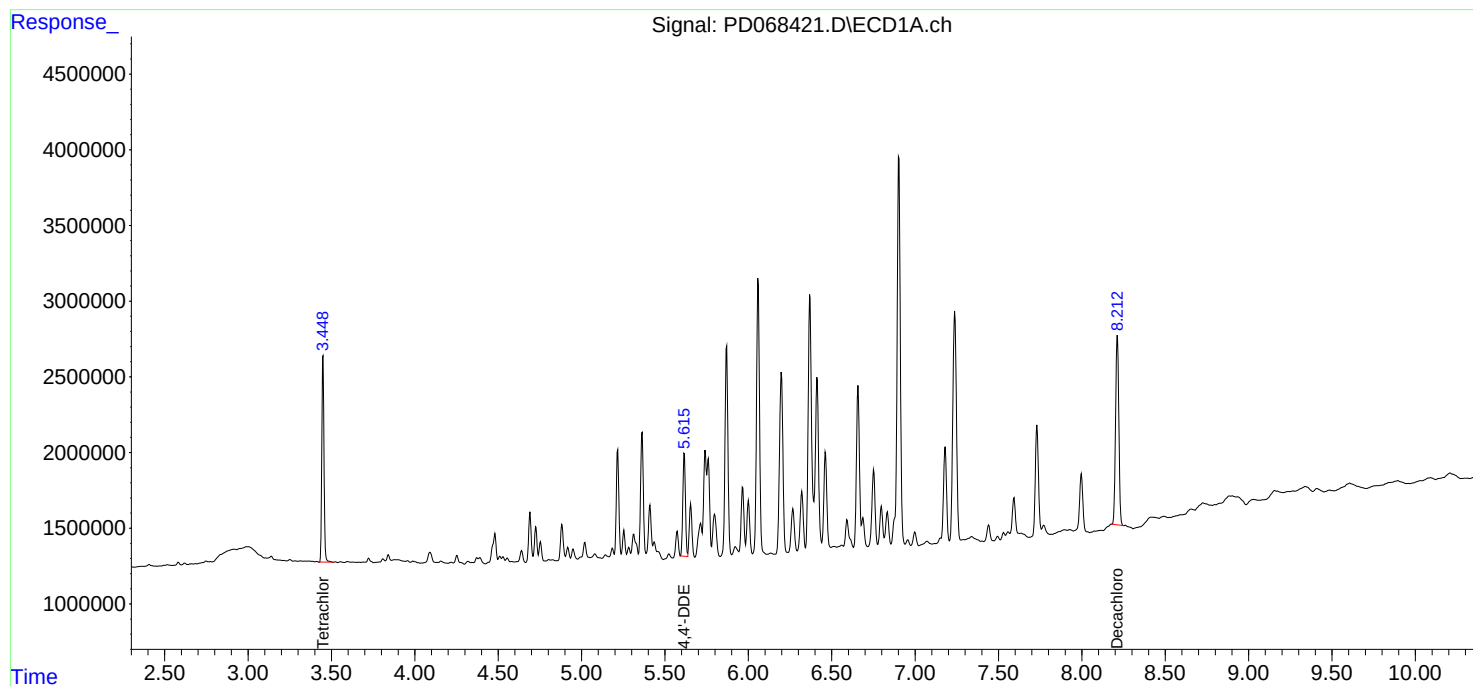


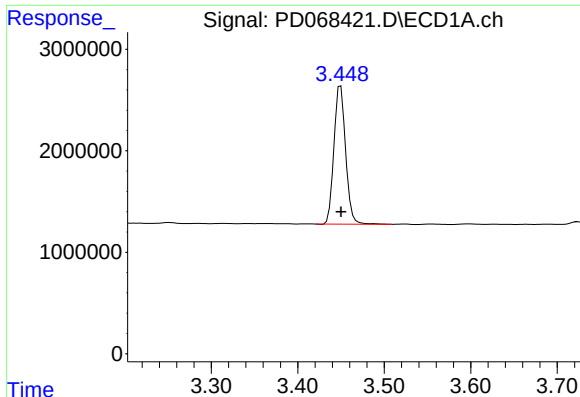

#1 Tetrachloro-m-xylene


R.T.: 3.450 min
Delta R.T.: 0.000 min
Response: 12797365
Conc: 10.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
FS-2

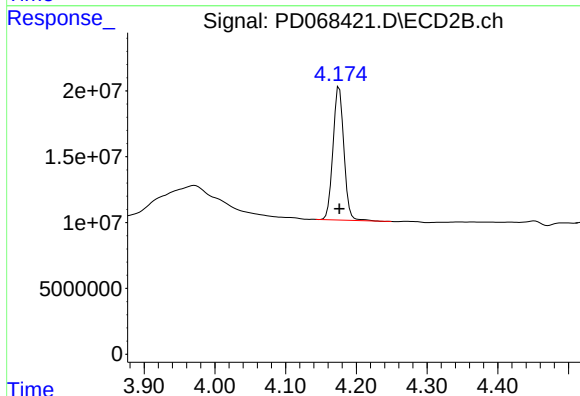


#1 Tetrachloro-m-xylene

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 107969535
Conc: 11.25 ng/ml

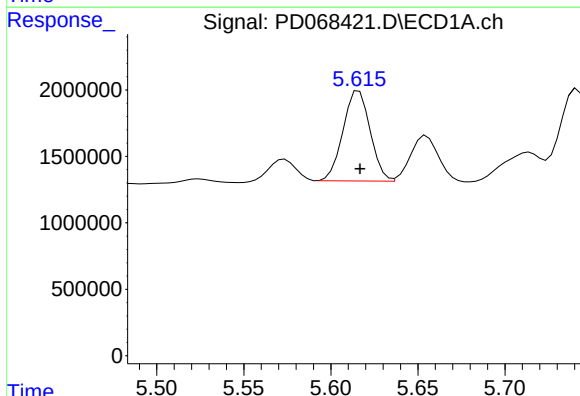


#12 4,4'-DDE

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 7358552
Conc: 5.39 ng/ml

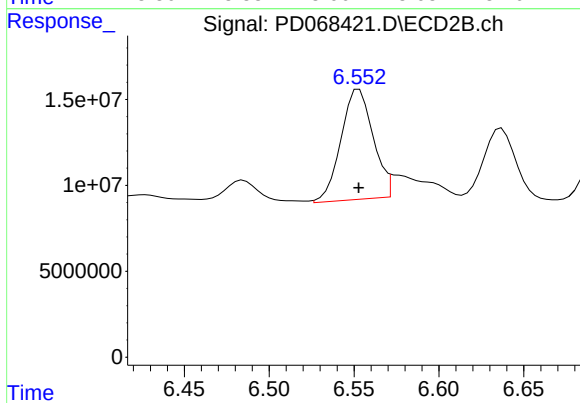

#12 4,4'-DDE


R.T.: 6.552 min
Delta R.T.: -0.001 min
Response: 85713598
Conc: 8.77 ng/ml m

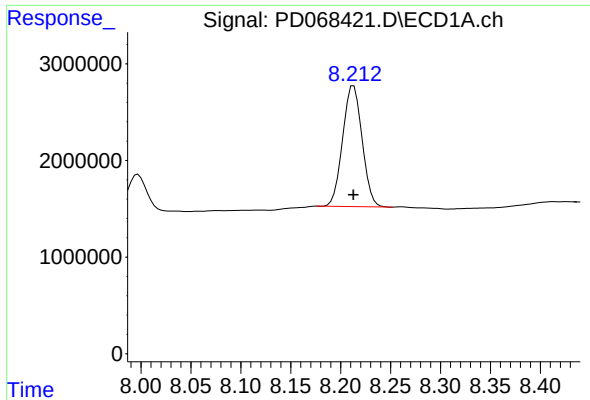

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 16964198
Conc: 14.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
FS-2

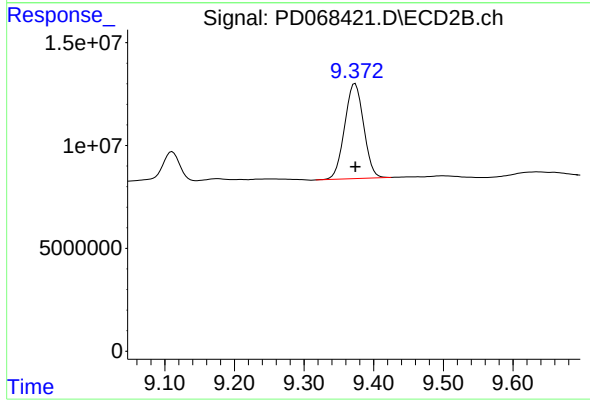

#28 Decachlorobiphenyl

R.T.: 9.373 min
Delta R.T.: 0.000 min
Response: 87673009
Conc: 14.79 ng/ml