

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
 Data File : PD082065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2024 17:09
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:03:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 09 04:00:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.790	28218926	53329141	20.000	20.000
27)	SA Decachlor...	9.108	7.924	76312974	102.8E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.019	3.291	46471787	80712716	20.000	20.000
3)	MA gamma-BHC...	4.353	3.620	46388563	75008461	20.000	20.000
4)	MA Heptachlor	4.945	3.961	48411414	70464231	20.000	20.000
9)	A Endosulfan I	6.102	5.112	41669376	59280396	20.000	20.000
13)	MA Dieldrin	6.377	5.376	86941182	131.5E6	40.000	40.000
14)	MA Endrin	6.608	5.651	72061293	112.5E6	40.000	40.000
16)	A 4,4'-DDD	6.739	5.797	63299274	99431497	40.000	40.000
17)	MA 4,4'-DDT	7.054	6.048	66829550	100.8E6	40.000	40.000
20)	A Methoxychlor	7.529	6.622	185.3E6	268.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
Data File : PD082065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2024 17:09
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:03:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:00:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

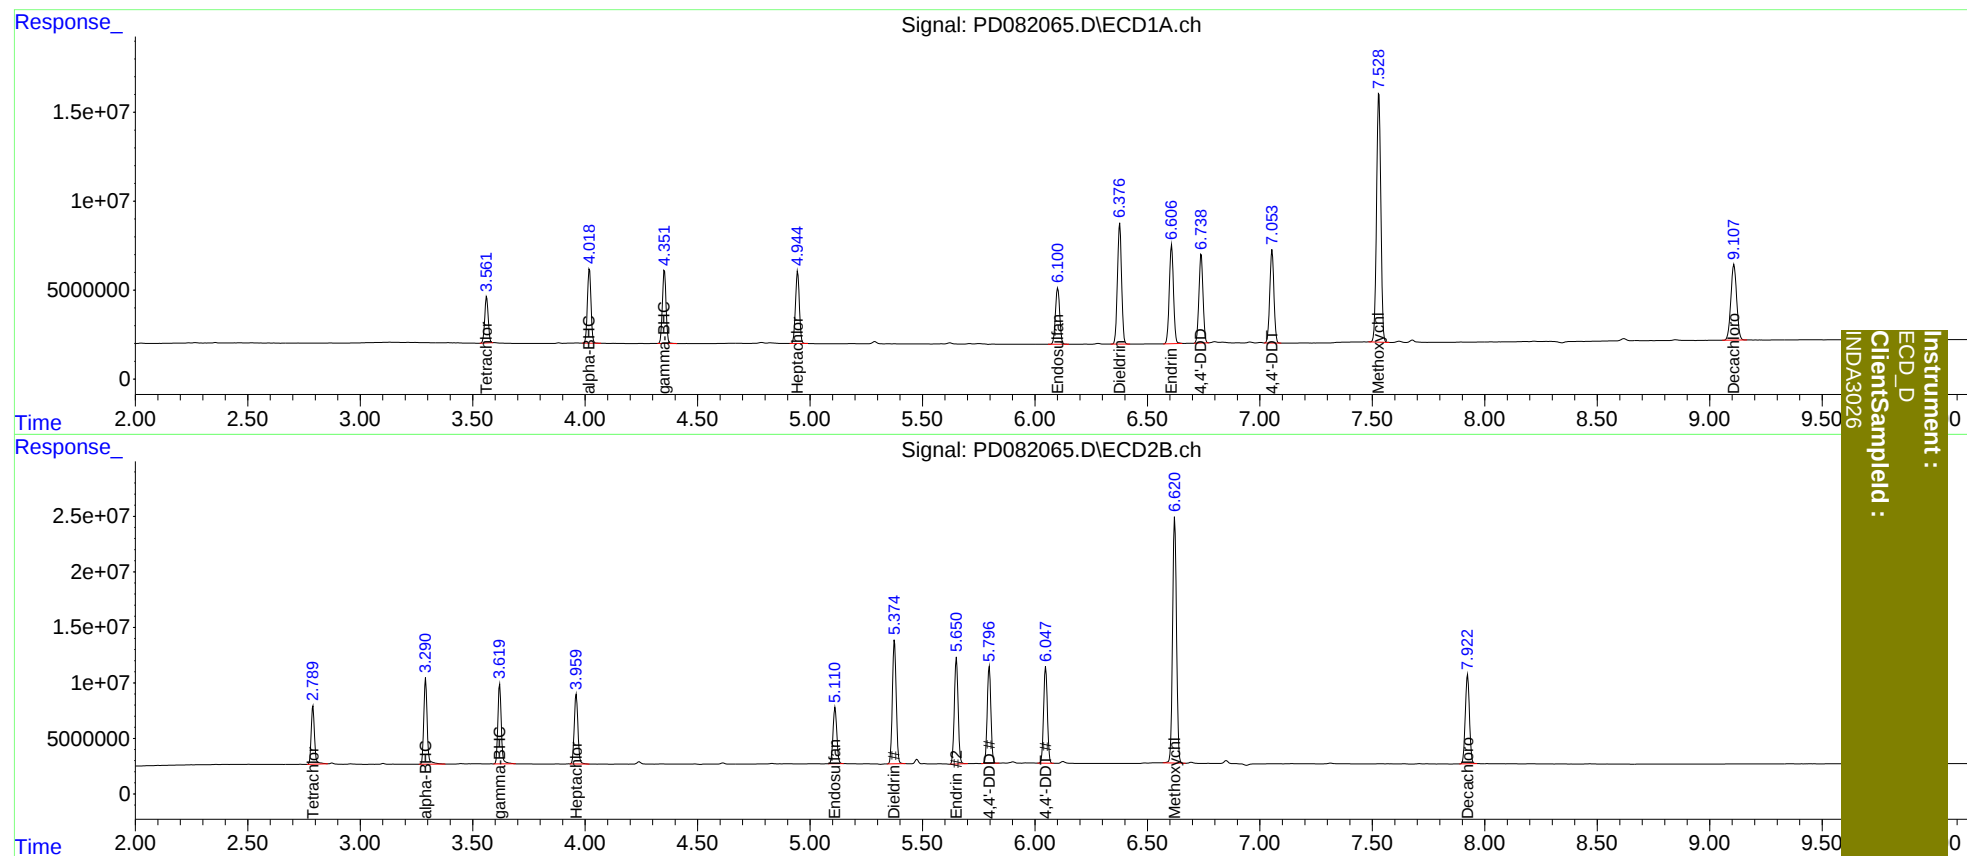


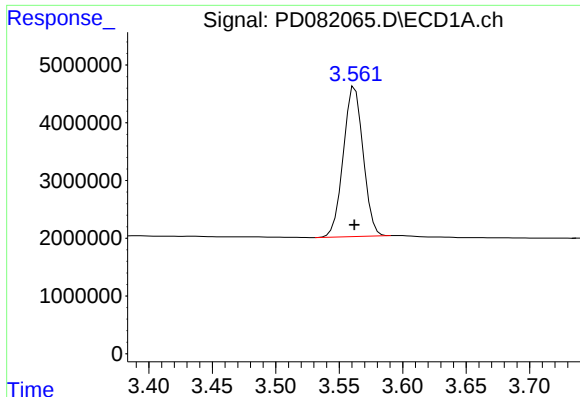

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 28218926
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

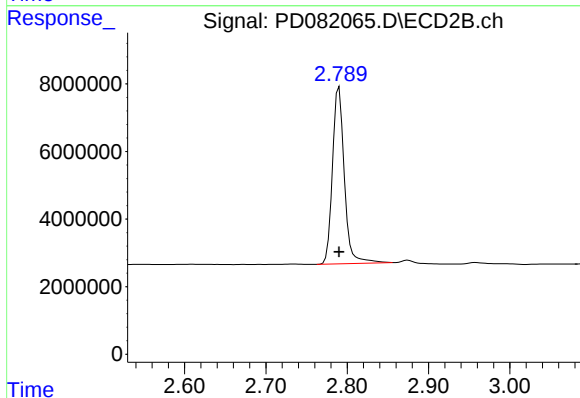


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 53329141
Conc: 20.00 ng/ml

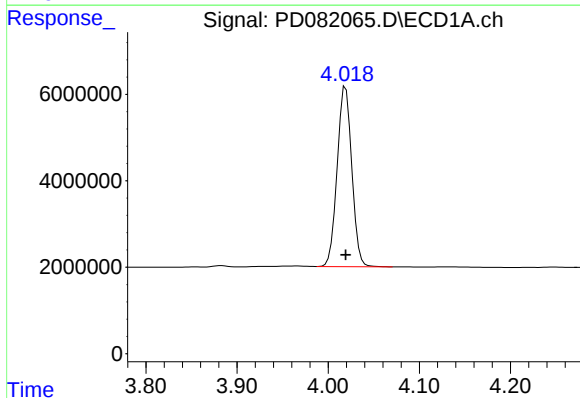


#2 alpha-BHC

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 46471787
Conc: 20.00 ng/ml

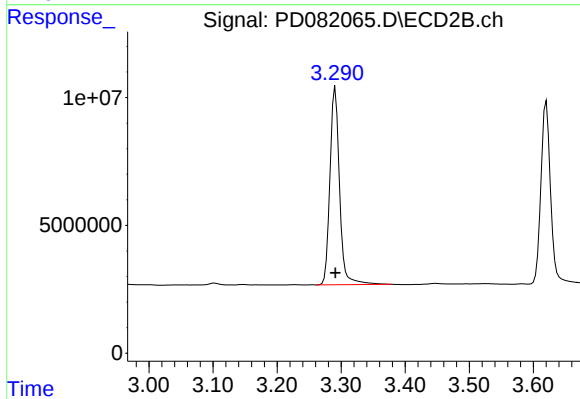

#2 alpha-BHC


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 80712716
Conc: 20.00 ng/ml

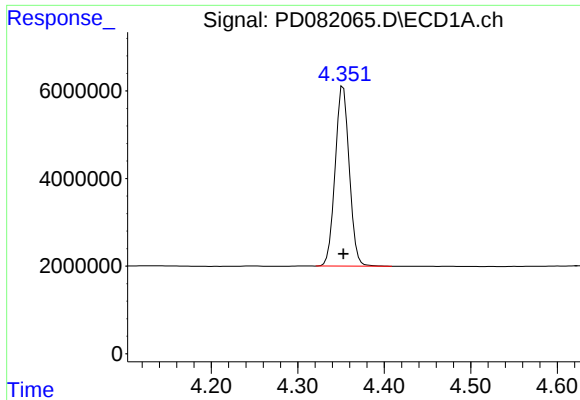

#3 gamma-BHC (Lindane)


R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 46388563
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

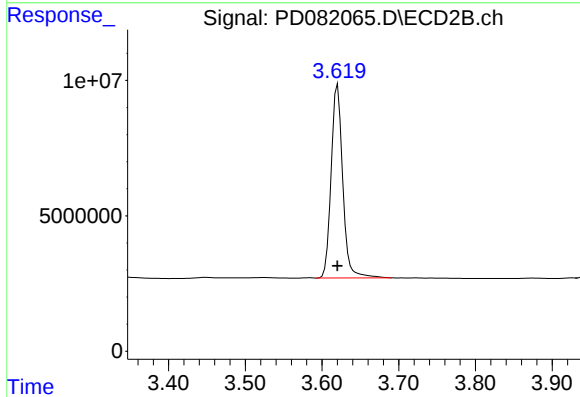


#3 gamma-BHC (Lindane)

R.T.: 3.620 min
Delta R.T.: 0.000 min
Response: 75008461
Conc: 20.00 ng/ml

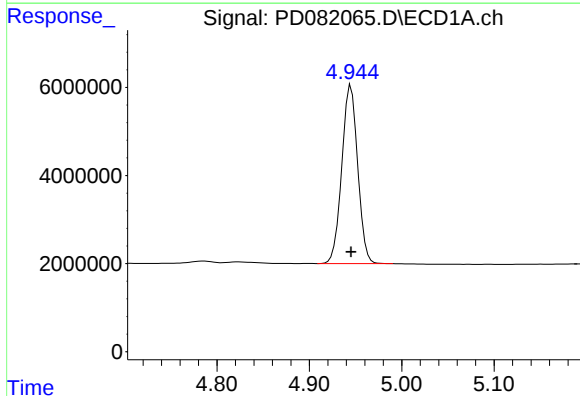


#4 Heptachlor

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 48411414
Conc: 20.00 ng/ml

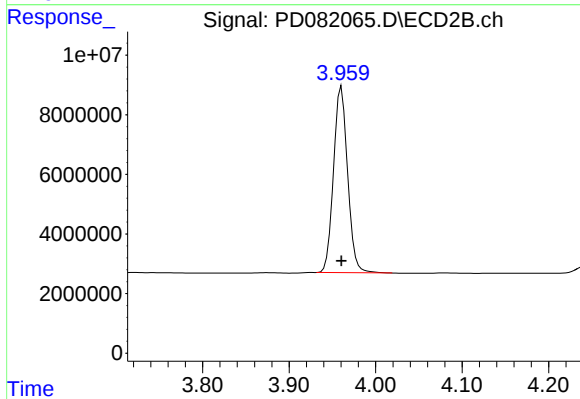

#4 Heptachlor


R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 70464231
Conc: 20.00 ng/ml

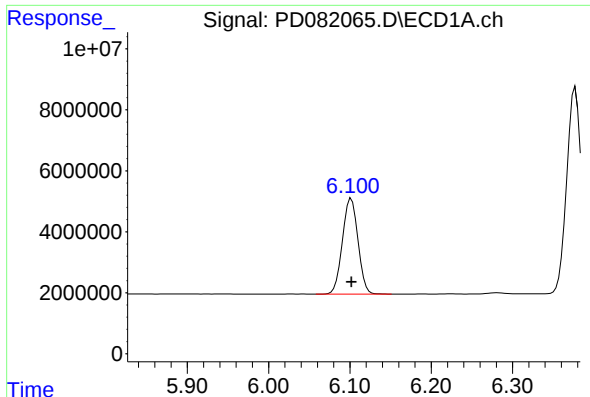

#9 Endosulfan I


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 41669376
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

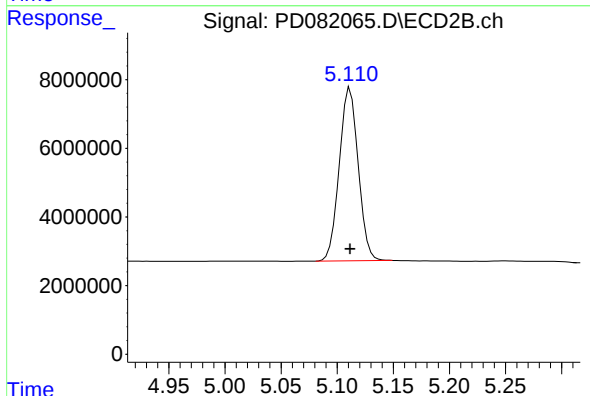


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 59280396
Conc: 20.00 ng/ml

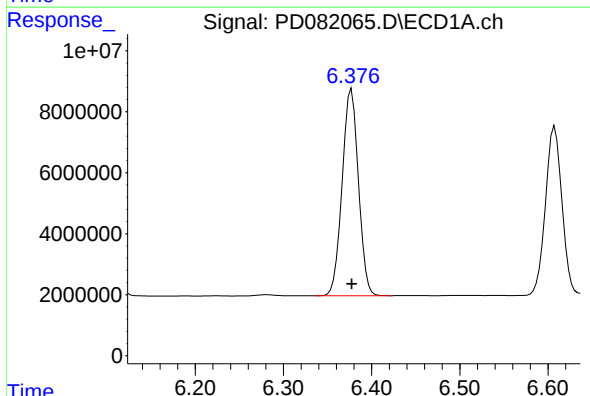


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 86941182
Conc: 40.00 ng/ml

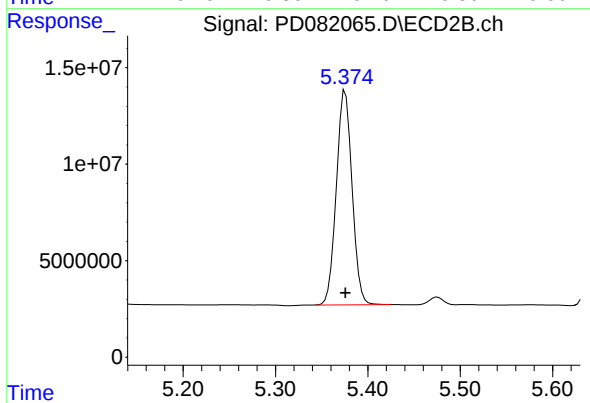

#13 Dieldrin


R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 131500291
Conc: 40.00 ng/ml

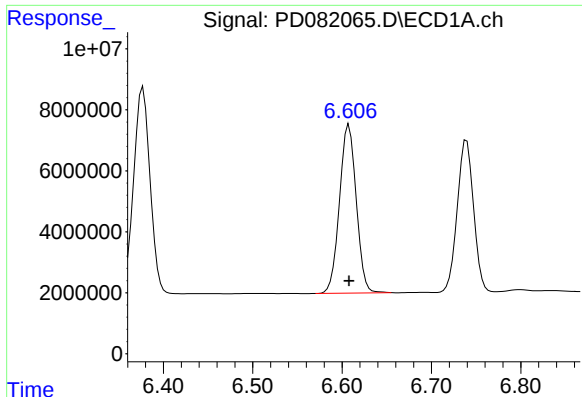

#14 Endrin


R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 72061293
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

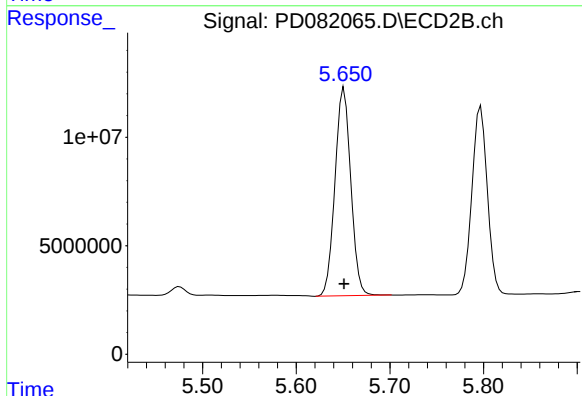


#14 Endrin

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 112486530
Conc: 40.00 ng/ml

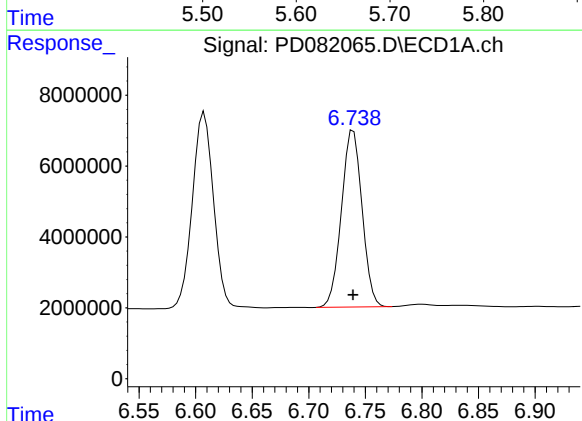


#16 4,4'-DDD

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 63299274
Conc: 40.00 ng/ml

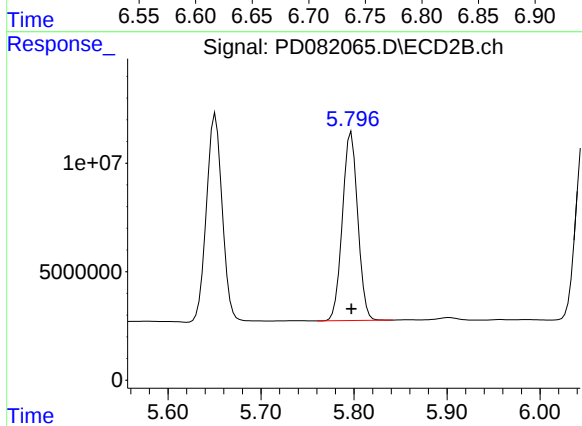

#16 4,4'-DDD


R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 99431497
Conc: 40.00 ng/ml

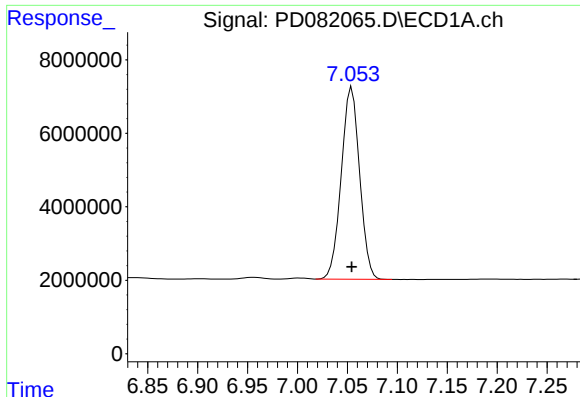

#17 4,4'-DDT


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 66829550
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

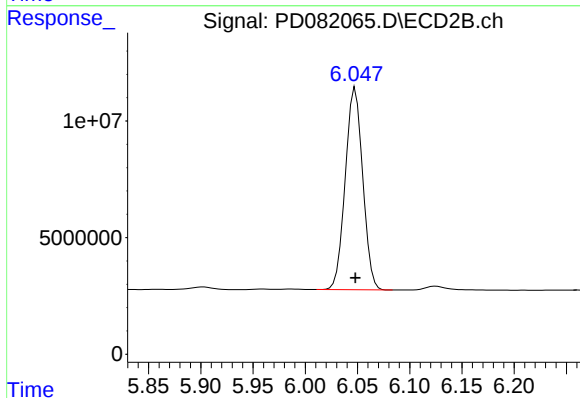


#17 4,4'-DDT

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 100769641
Conc: 40.00 ng/ml

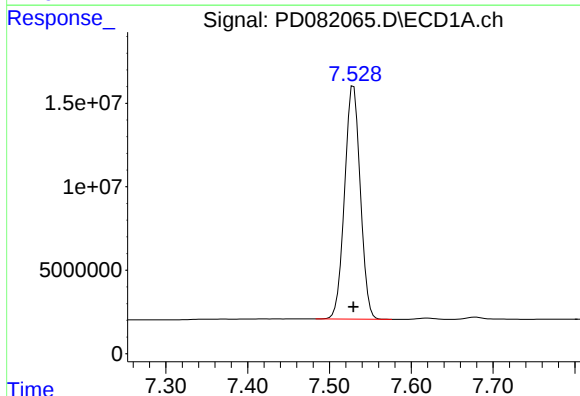


#20 Methoxychlor

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 185335649
Conc: 200.00 ng/ml

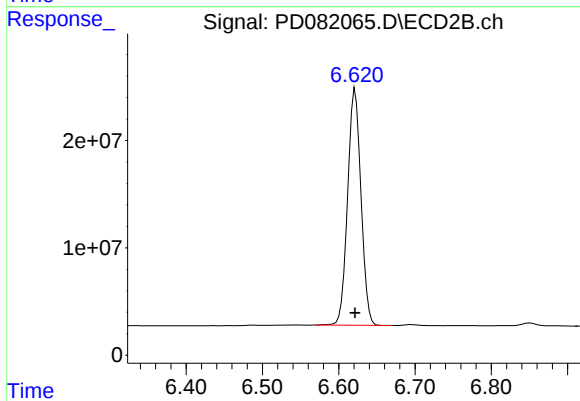

#20 Methoxychlor

R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 268912532
Conc: 200.00 ng/ml

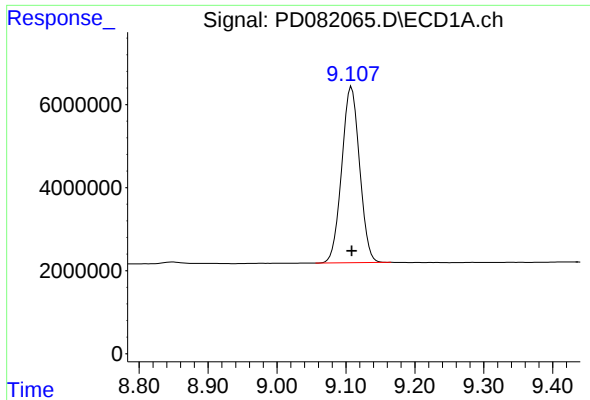

#27 Decachlorobiphenyl


R.T.: 9.108 min

Delta R.T.: 0.000 min

Response: 76312974

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3026

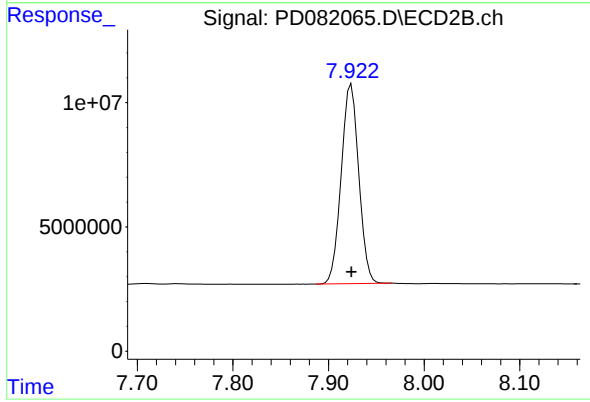

#27 Decachlorobiphenyl

R.T.: 7.924 min

Delta R.T.: 0.000 min

Response: 102797189

Conc: 40.00 ng/ml