

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
 Data File : PD082067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2024 17:35
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:03:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 09 04:00:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.790	55424639	104.4E6	39.282	39.169
27)	SA Decachlor...	9.108	7.924	151.1E6	198.3E6	79.190	77.159
Target Compounds							
2)	A alpha-BHC	4.020	3.292	97505930	164.5E6	41.963	40.767
3)	MA gamma-BHC...	4.353	3.621	95382965	150.5E6	41.123	40.117
4)	MA Heptachlor	4.945	3.961	97315266	140.3E6	40.203	39.831
9)	A Endosulfan I	6.102	5.112	81707689	116.9E6	39.217	39.451
13)	MA Dieldrin	6.377	5.376	175.7E6	263.5E6	80.814	80.148
14)	MA Endrin	6.607	5.651	144.5E6	222.9E6	80.221	79.258
16)	A 4,4'-DDD	6.739	5.798	128.4E6	199.5E6	81.115	80.276
17)	MA 4,4'-DDT	7.054	6.048	135.9E6	205.3E6	81.344	81.473
20)	A Methoxychlor	7.529	6.623	362.0E6	510.3E6	390.610	379.559

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
Data File : PD082067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2024 17:35
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:03:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:00:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

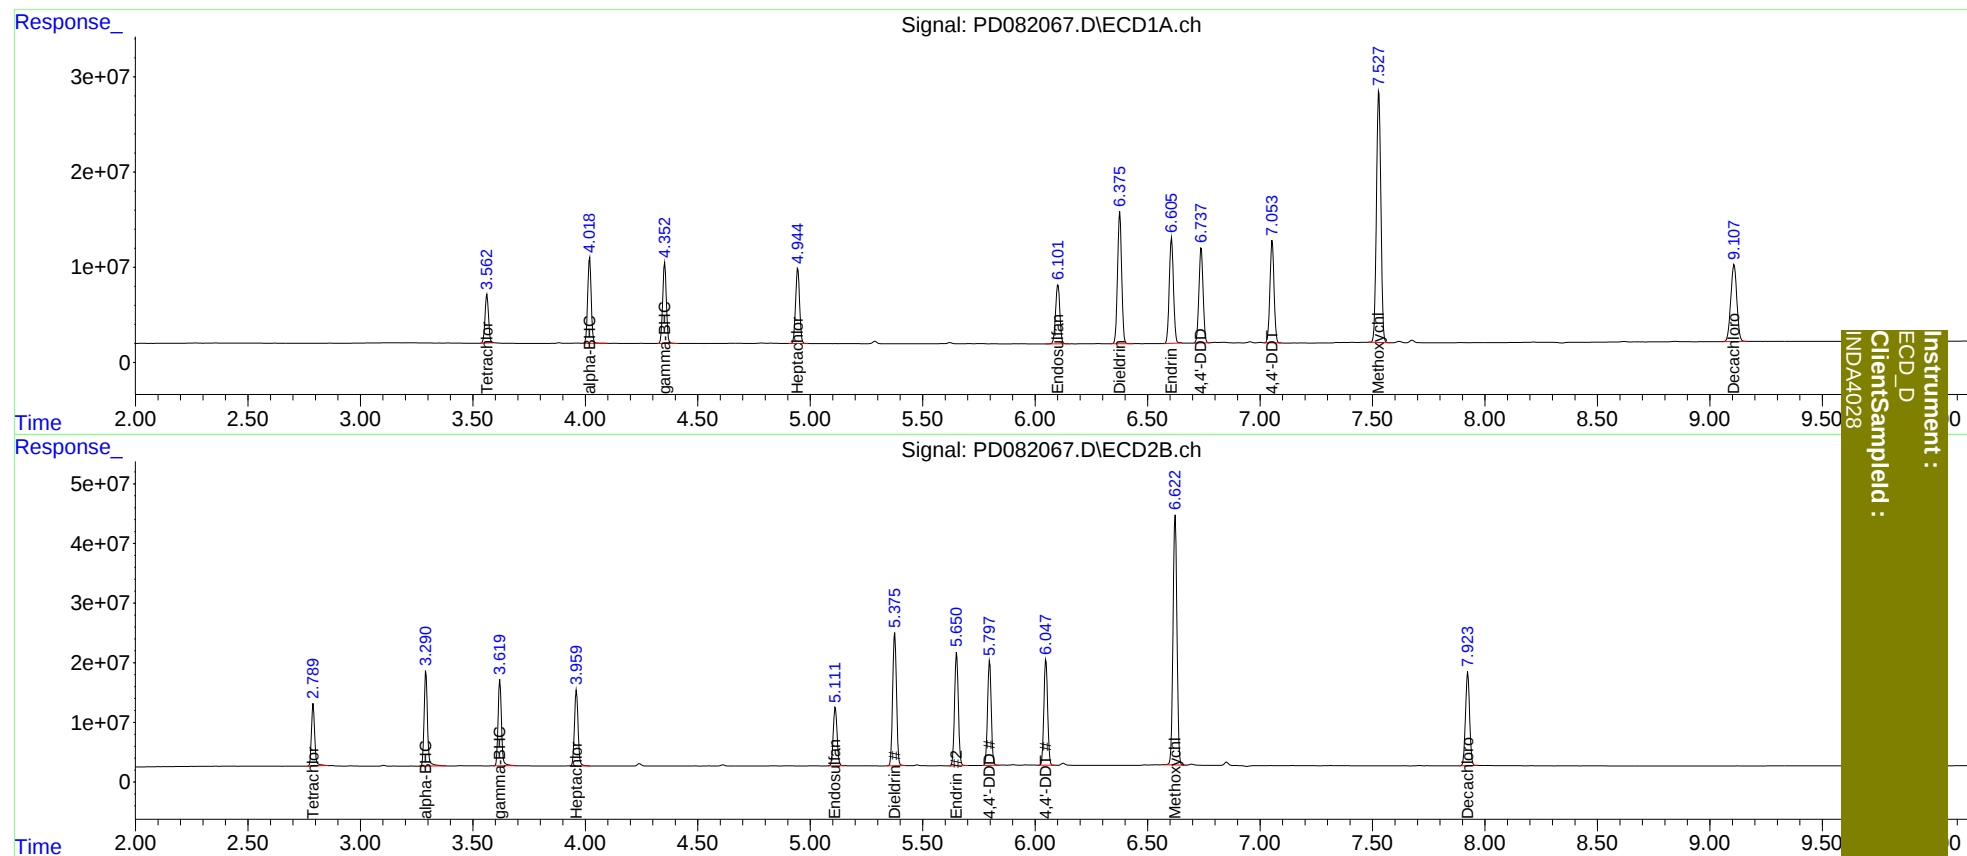


Instrument :
ECD_D
ClientSampled :
INDA4028

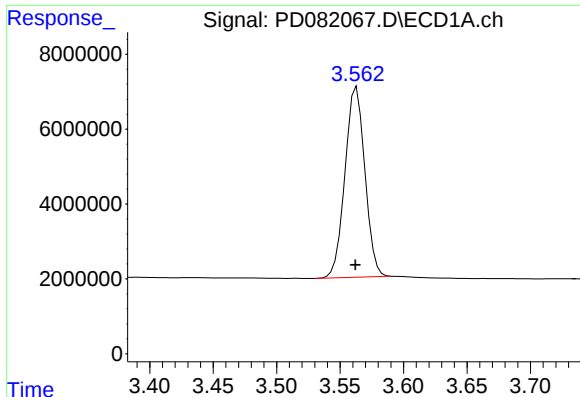

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.001 min
Response: 55424639
Conc: 39.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

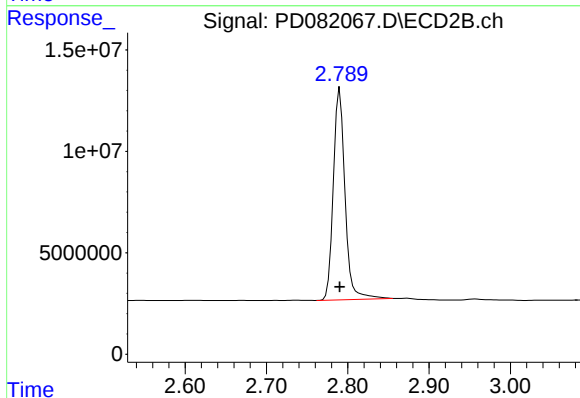


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 104441914
Conc: 39.17 ng/ml

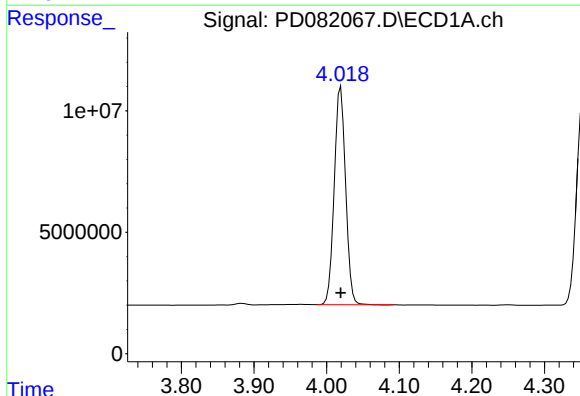


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 97505930
Conc: 41.96 ng/ml

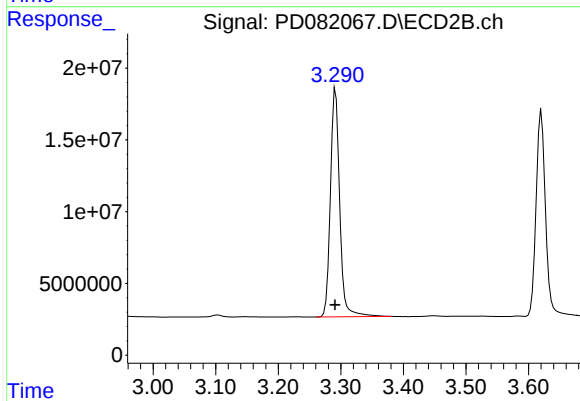

#2 alpha-BHC


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 164520956
Conc: 40.77 ng/ml

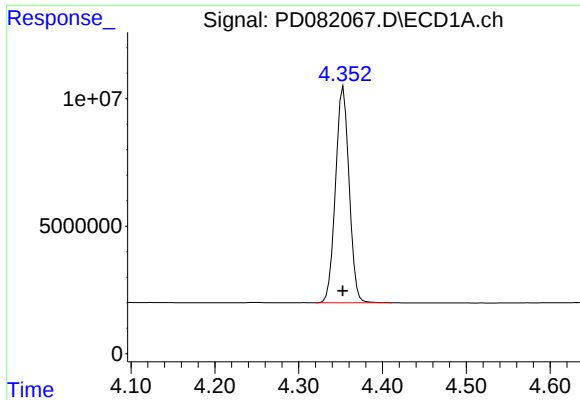

#3 gamma-BHC (Lindane)


R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 95382965
Conc: 41.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

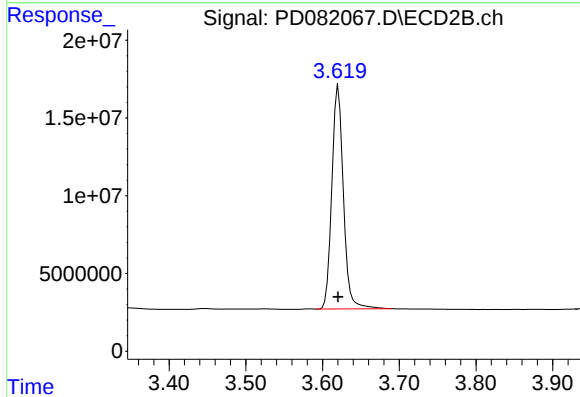


#3 gamma-BHC (Lindane)

R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 150454226
Conc: 40.12 ng/ml

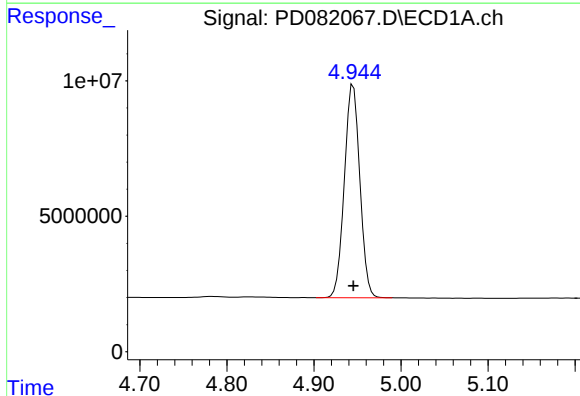


#4 Heptachlor

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 97315266
Conc: 40.20 ng/ml

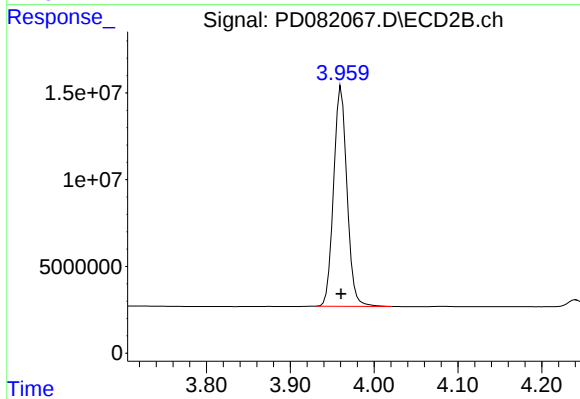

#4 Heptachlor


R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 140331383
Conc: 39.83 ng/ml

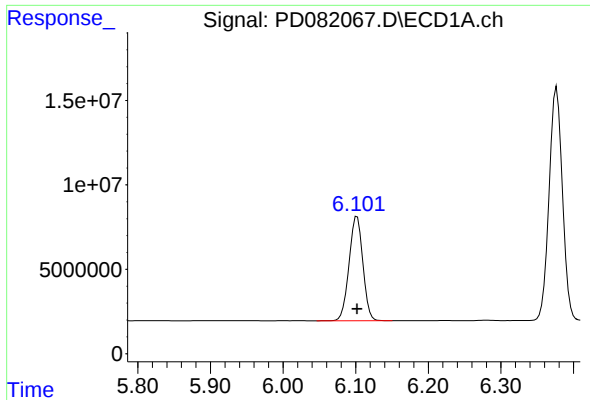

#9 Endosulfan I


R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 81707689
Conc: 39.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

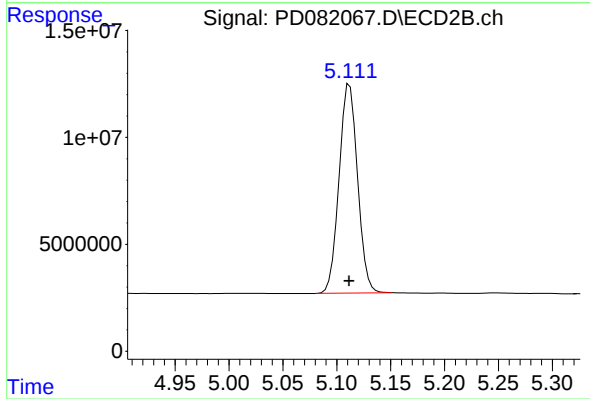


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 116934141
Conc: 39.45 ng/ml

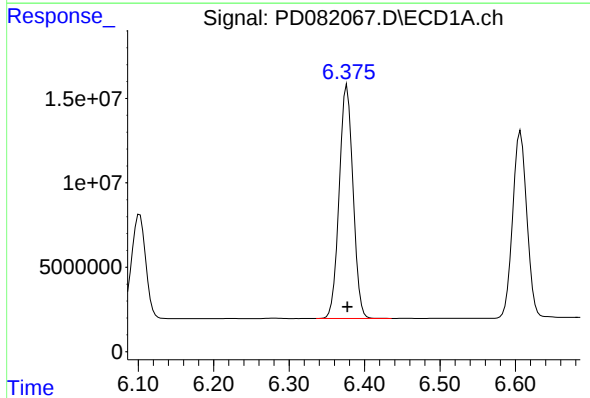


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 175652333
Conc: 80.81 ng/ml

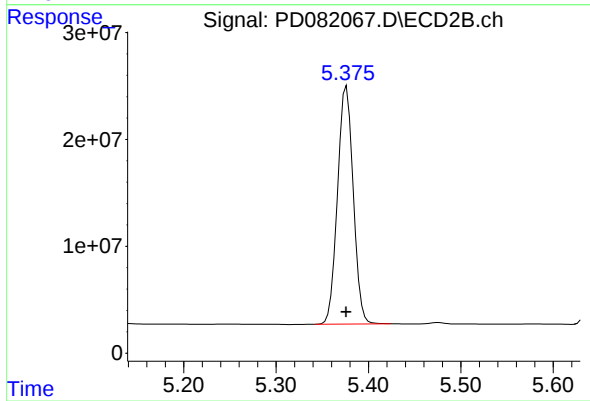

#13 Dieldrin


R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 263485817
Conc: 80.15 ng/ml

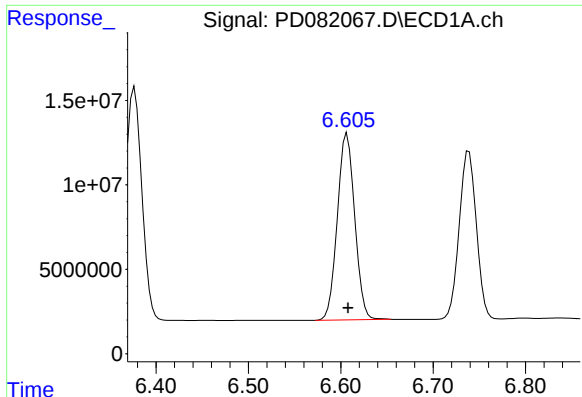

#14 Endrin


R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 144521363
Conc: 80.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

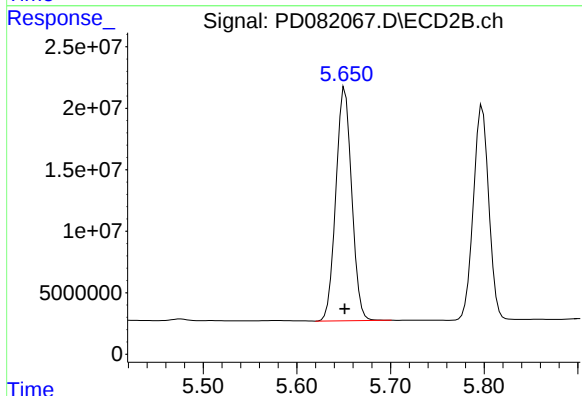


#14 Endrin

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 222886515
Conc: 79.26 ng/ml

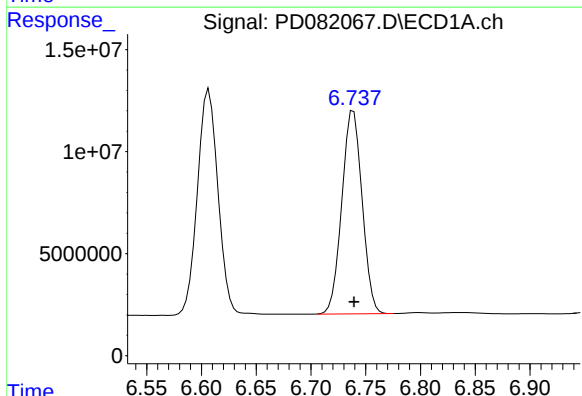


#16 4,4'-DDD

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 128362483
Conc: 81.11 ng/ml

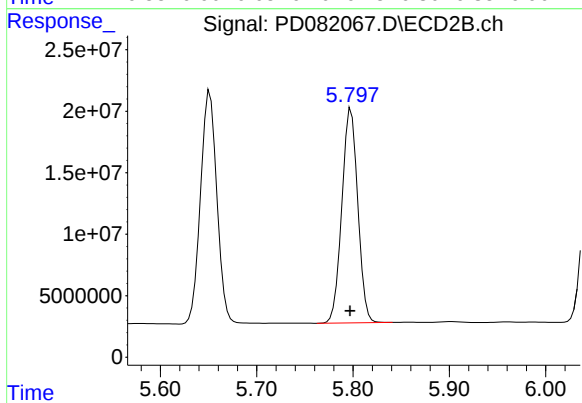

#16 4,4'-DDD


R.T.: 5.798 min
Delta R.T.: 0.001 min
Response: 199549525
Conc: 80.28 ng/ml

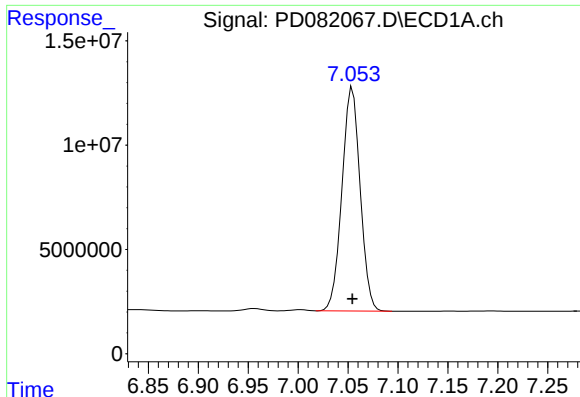

#17 4,4'-DDT


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 135903761
Conc: 81.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

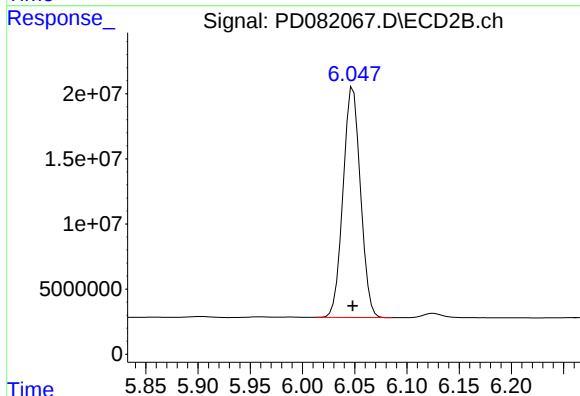


#17 4,4'-DDT

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 205250192
Conc: 81.47 ng/ml

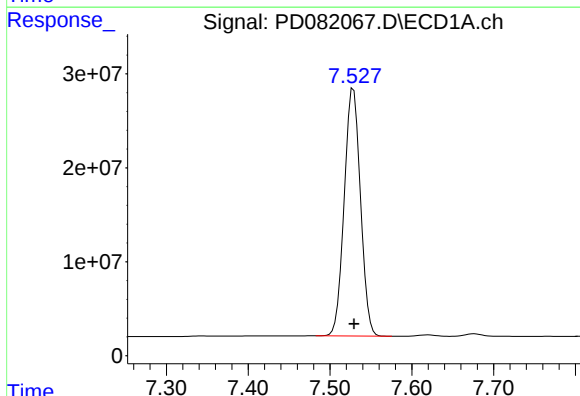


#20 Methoxychlor

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 361969333
Conc: 390.61 ng/ml

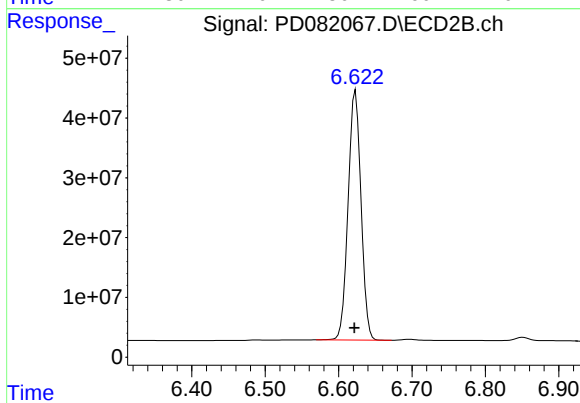

#20 Methoxychlor

R.T.: 6.623 min
Delta R.T.: 0.002 min
Response: 510340811
Conc: 379.56 ng/ml

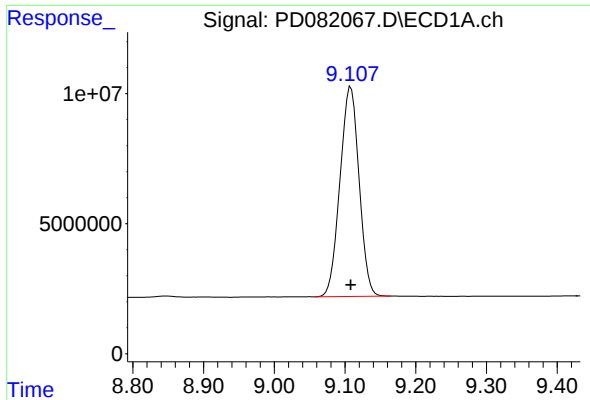

#27 Decachlorobiphenyl


R.T.: 9.108 min

Delta R.T.: 0.000 min

Response: 151079969

Conc: 79.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4028

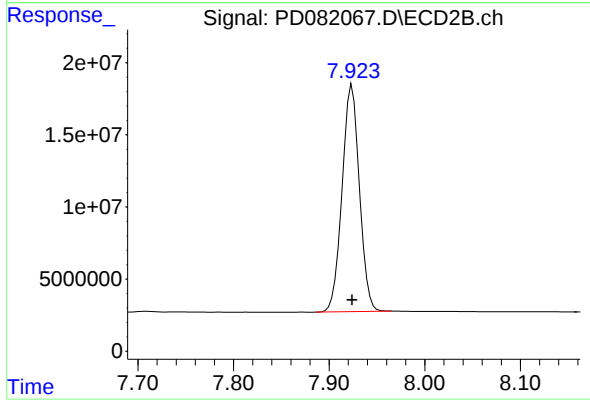

#27 Decachlorobiphenyl

R.T.: 7.924 min

Delta R.T.: 0.000 min

Response: 198292747

Conc: 77.16 ng/ml