

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
 Data File : PD082069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2024 18:02
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5030

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:03:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 09 04:00:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.790	102.7E6	211.6E6	72.795	79.363
27)	SA Decachlor...	9.107	7.924	288.4E6	395.4E6	151.157	153.854
Target Compounds							
2)	A alpha-BHC	4.020	3.291	192.1E6	345.5E6	82.683	85.624
3)	MA gamma-BHC...	4.353	3.621	186.8E6	313.7E6	80.546	83.652
4)	MA Heptachlor	4.945	3.961	194.1E6	289.7E6	80.187	82.240
9)	A Endosulfan I	6.101	5.112	165.0E6	239.2E6	79.183	80.695
13)	MA Dieldrin	6.377	5.376	353.3E6	544.1E6	162.546	165.505
14)	MA Endrin	6.607	5.651	289.6E6	458.6E6	160.729	163.087
16)	A 4,4'-DDD	6.739	5.797	257.7E6	411.5E6	162.870	165.552
17)	MA 4,4'-DDT	7.054	6.048	284.0E6	429.7E6	170.004	170.565
20)	A Methoxychlor	7.529	6.622	723.9E6	980.9E6	781.189	729.541


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD030924\
Data File : PD082069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2024 18:02
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:03:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030924CLP.M
Quant Title : GC Extractables
QLast Update : Sat Mar 09 04:00:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

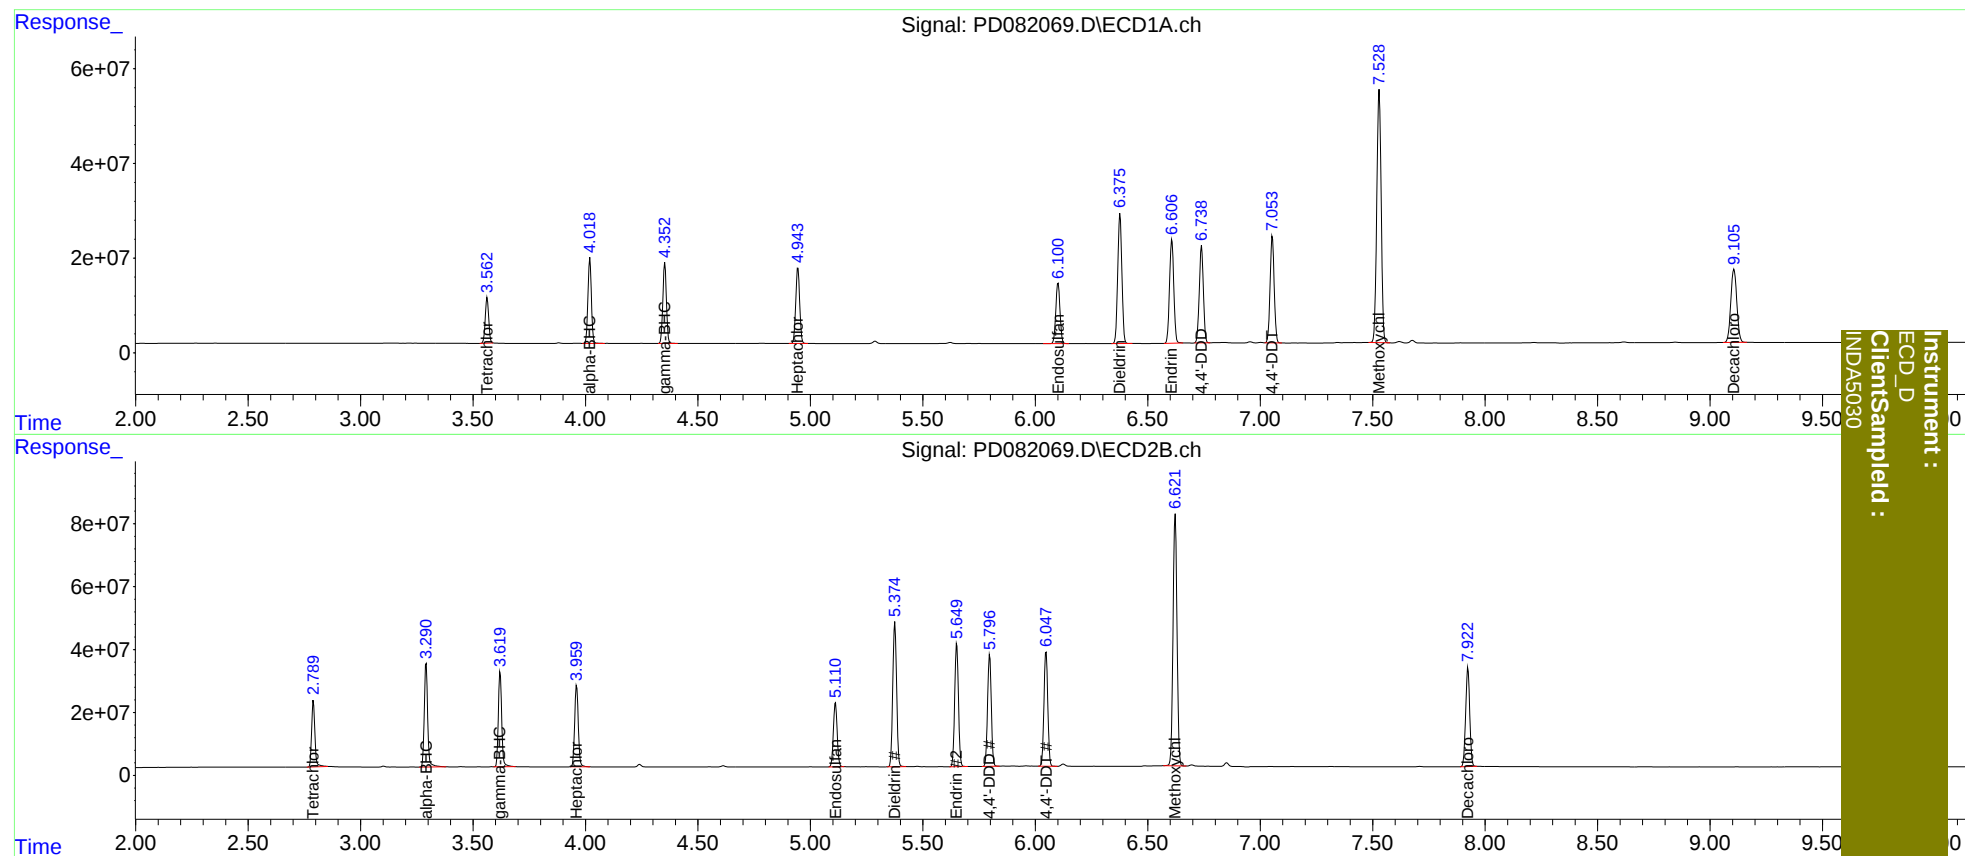


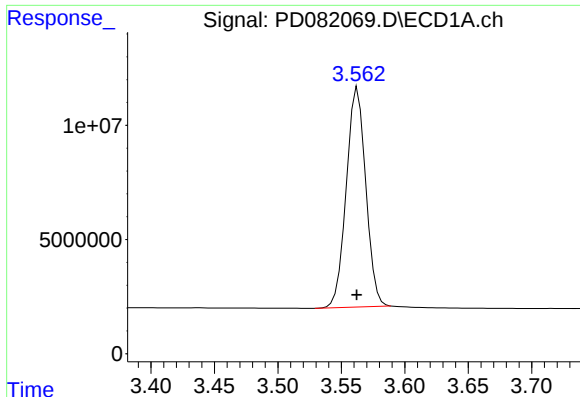

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 102709949
Conc: 72.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

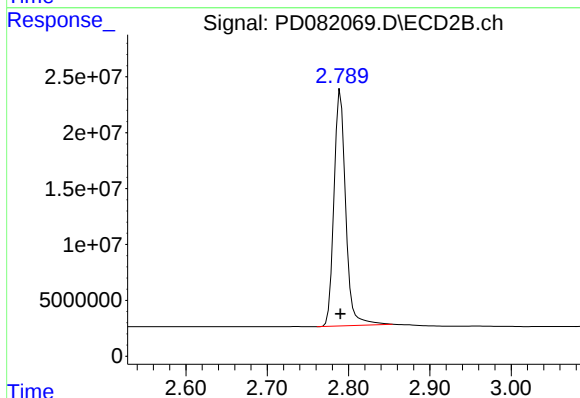


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 211616938
Conc: 79.36 ng/ml

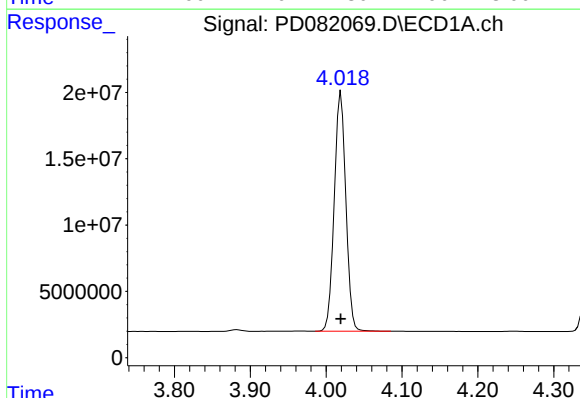


#2 alpha-BHC

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 192120510
Conc: 82.68 ng/ml

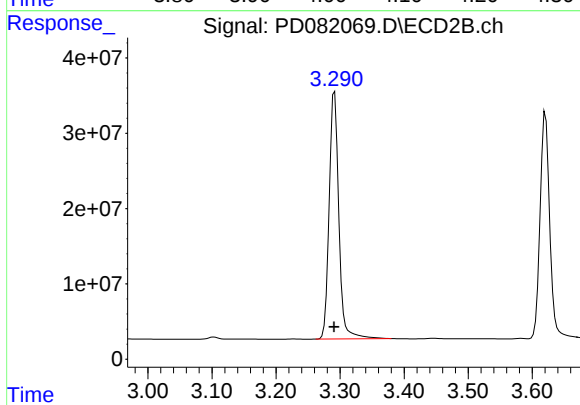

#2 alpha-BHC


R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 345547932
Conc: 85.62 ng/ml

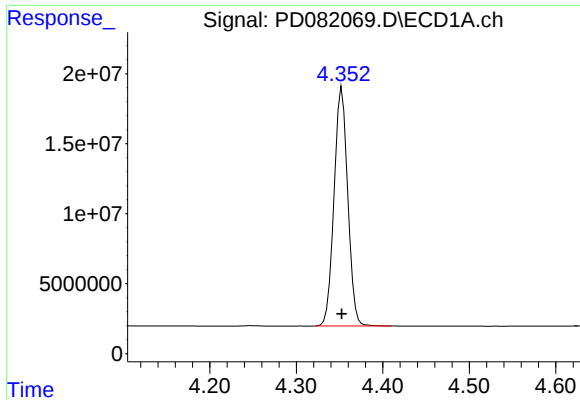

#3 gamma-BHC (Lindane)


R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 186819958
Conc: 80.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

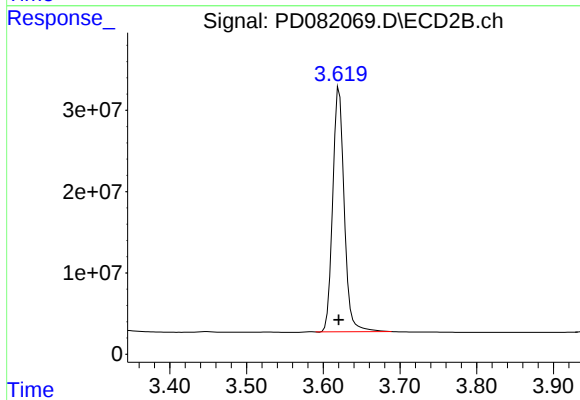


#3 gamma-BHC (Lindane)

R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 313730089
Conc: 83.65 ng/ml

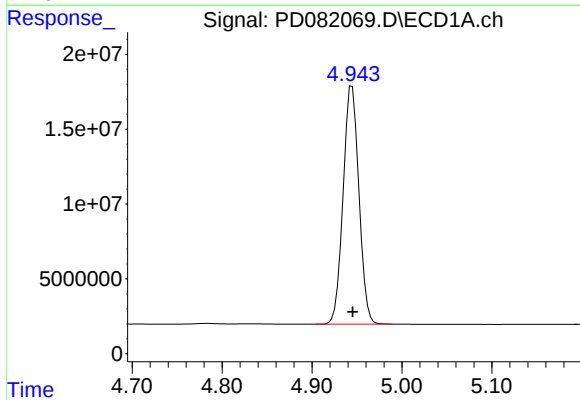


#4 Heptachlor

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 194097105
Conc: 80.19 ng/ml

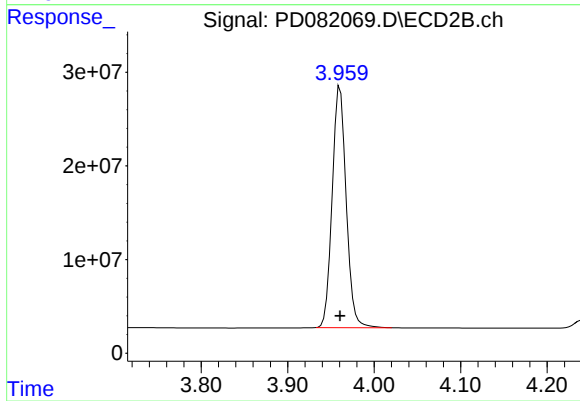

#4 Heptachlor


R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 289748251
Conc: 82.24 ng/ml

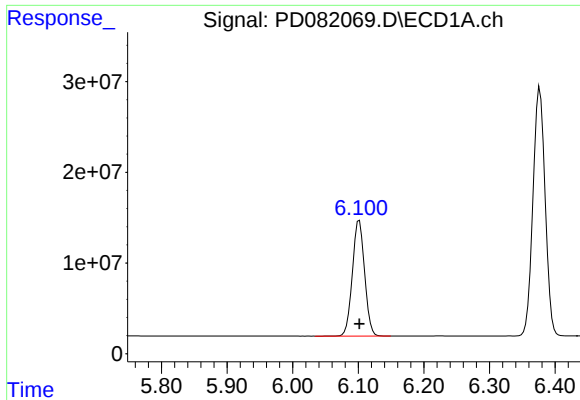

#9 Endosulfan I


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 164975620
Conc: 79.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

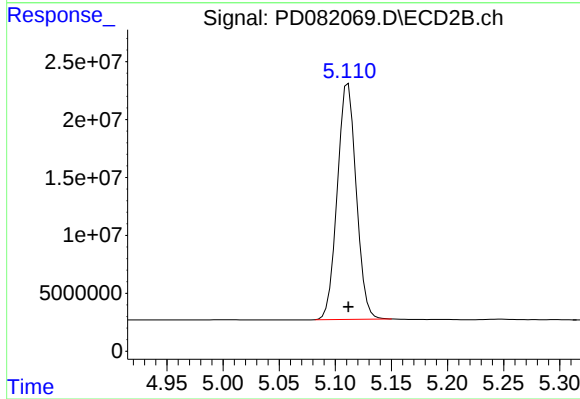


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 239180631
Conc: 80.69 ng/ml

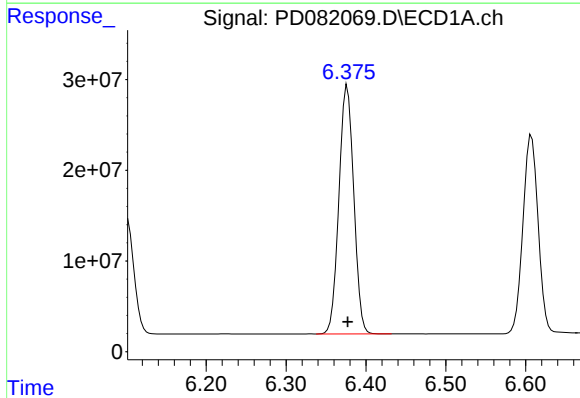


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 353298488
Conc: 162.55 ng/ml

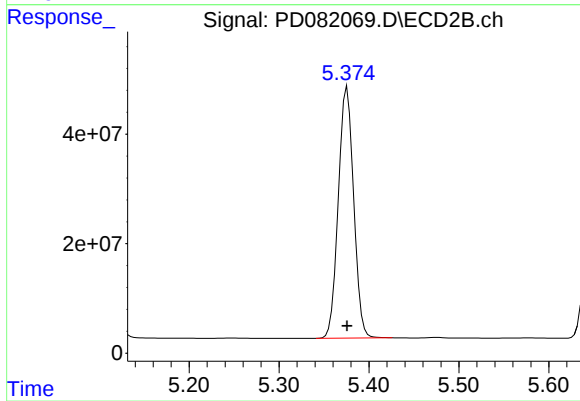

#13 Dieldrin


R.T.: 5.376 min
Delta R.T.: 0.000 min
Response: 544099265
Conc: 165.51 ng/ml

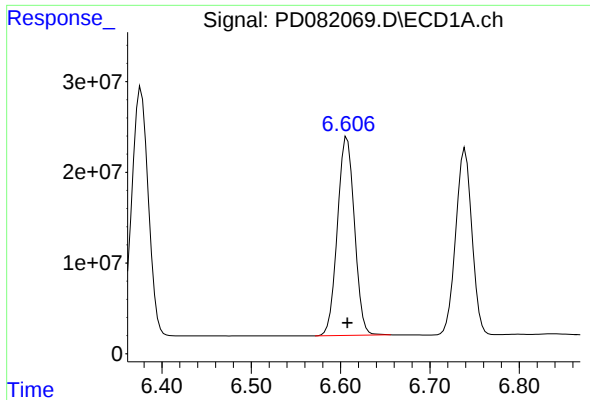

#14 Endrin


R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 289559300
Conc: 160.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

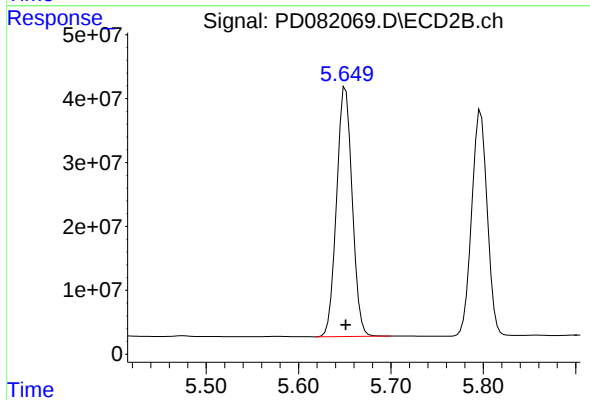


#14 Endrin

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 458628315
Conc: 163.09 ng/ml

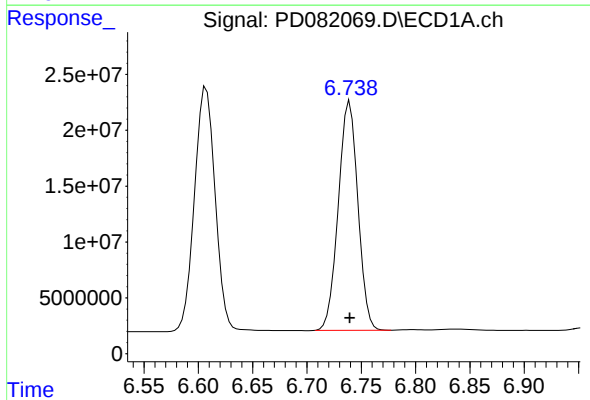


#16 4,4'-DDD

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 257738983
Conc: 162.87 ng/ml

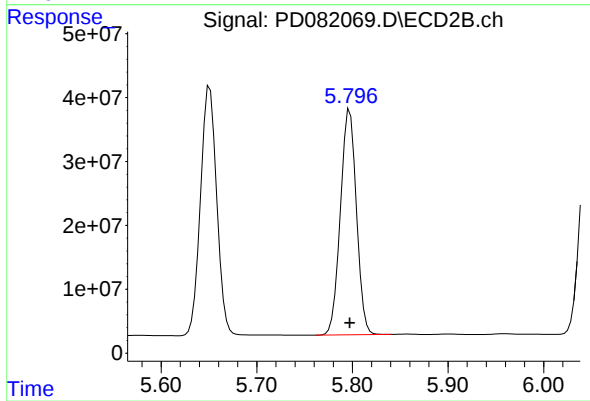

#16 4,4'-DDD


R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 411527007
Conc: 165.55 ng/ml

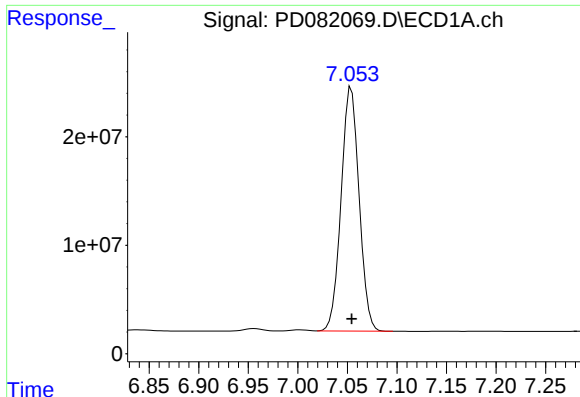

#17 4,4'-DDT


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 284031779
Conc: 170.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

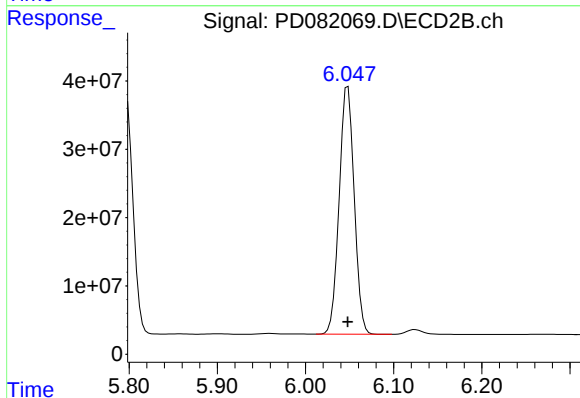


#17 4,4'-DDT

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 429693424
Conc: 170.56 ng/ml

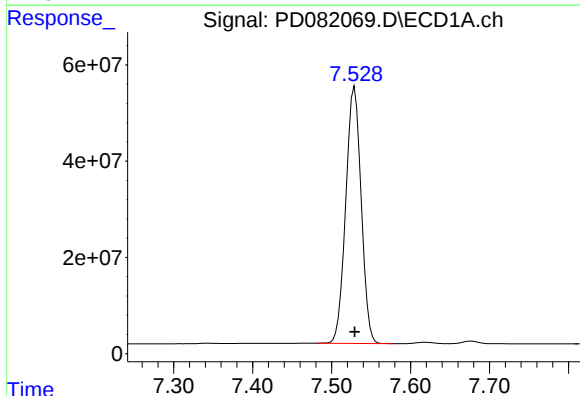


#20 Methoxychlor

R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 723910993
Conc: 781.19 ng/ml

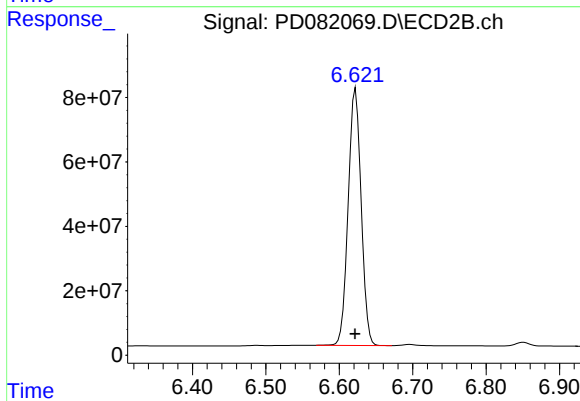

#20 Methoxychlor


R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 980913379
Conc: 729.54 ng/ml

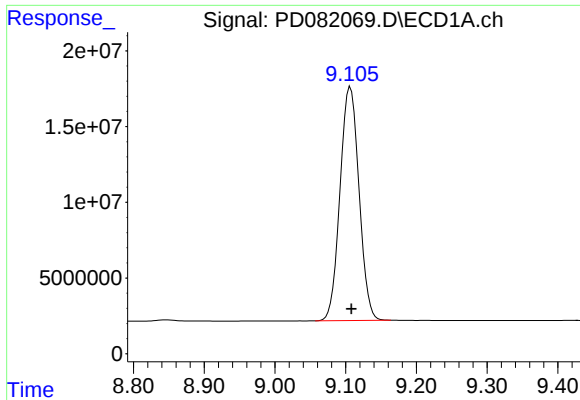

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: -0.002 min
Response: 288381902
Conc: 151.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5030

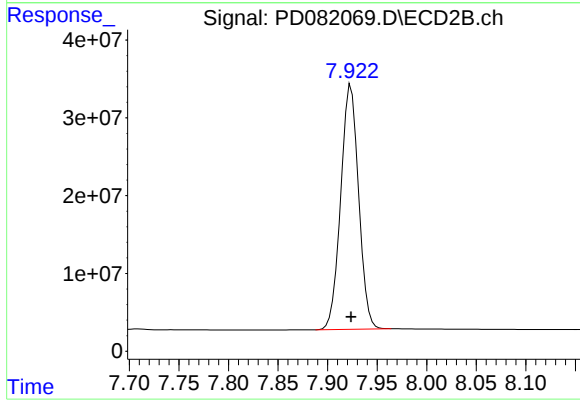

#27 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.000 min
Response: 395392971
Conc: 153.85 ng/ml