

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 13:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:01:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 14:00:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	73189069	626.3E6	73.315	71.526
28)	SA Decachlor...	8.256	9.035	88039705	623.6E6	71.502	71.157
Target Compounds							
23)	Chlordane-1	4.361	4.975	25421462	299.6E6	722.776	728.005
24)	Chlordane-2	4.864	5.441	29309144	283.8E6	715.767	713.887
25)	Chlordane-3	5.435	6.086	91754689	1237.1E6	743.354	724.159
26)	Chlordane-4	5.493	6.161	75910409	1420.2E6	737.329	721.734
27)	Chlordane-5	6.333	6.964	34883282	267.5E6	730.799	727.732



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 13:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:01:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 14:00:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

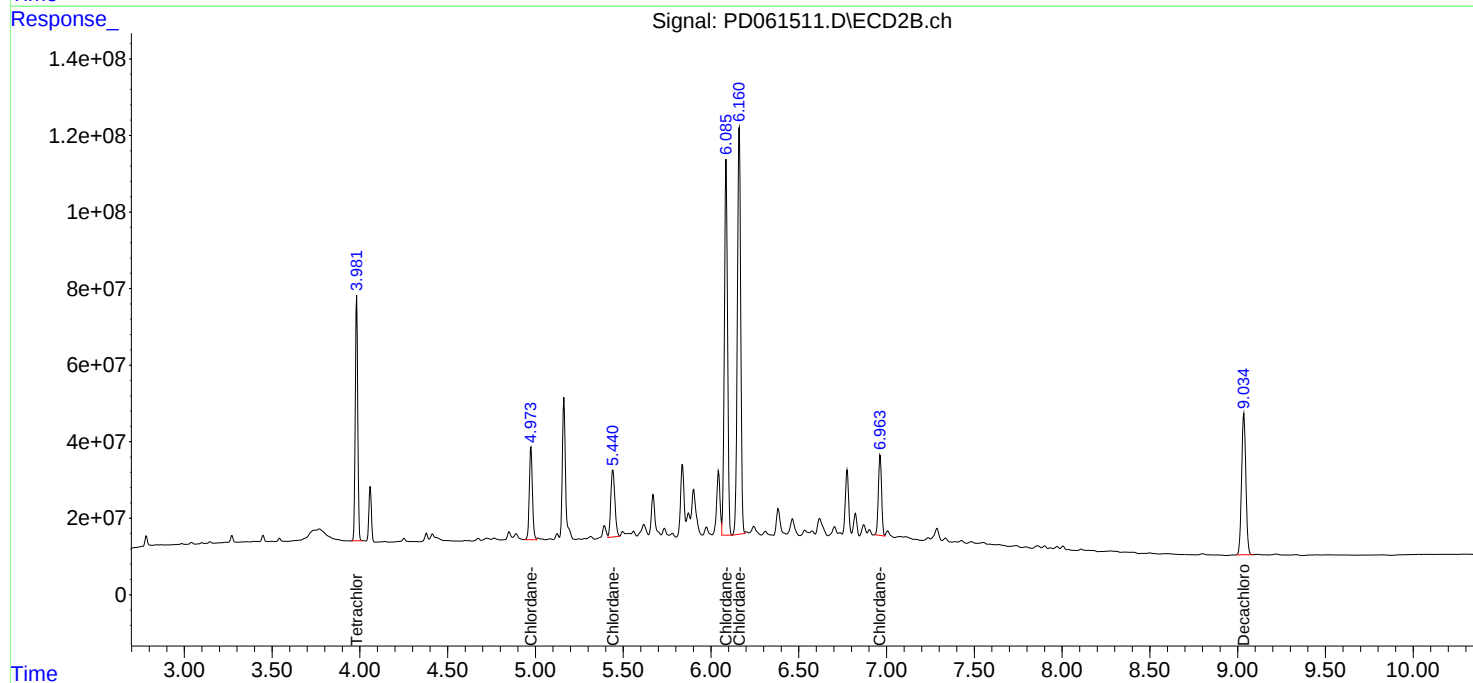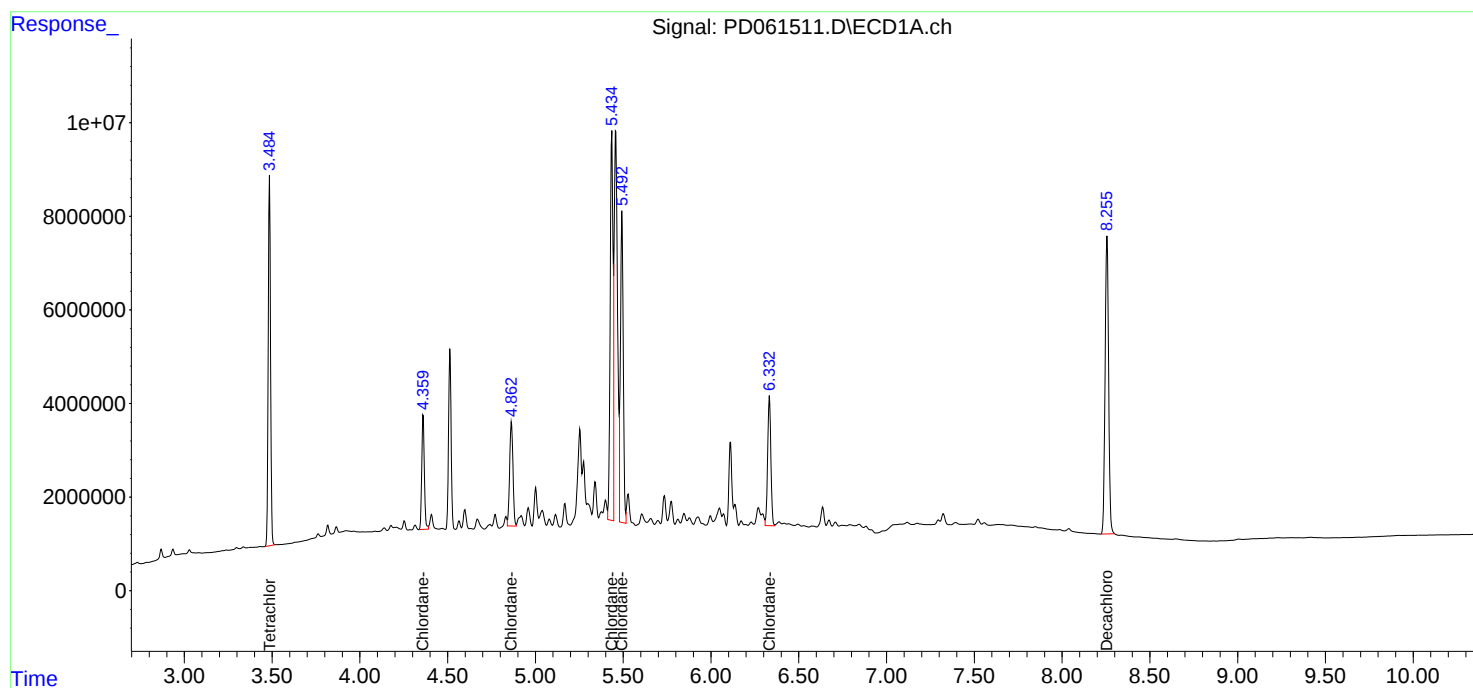


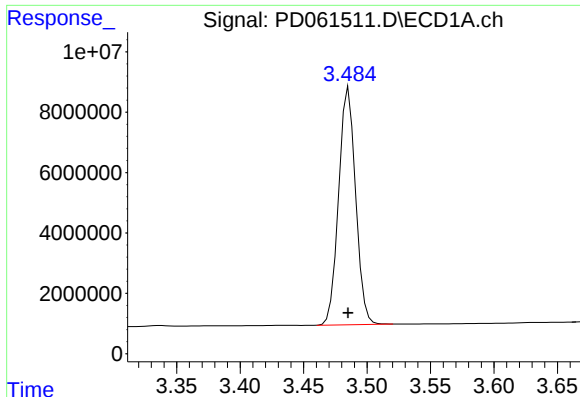

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 73189069
Conc: 73.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

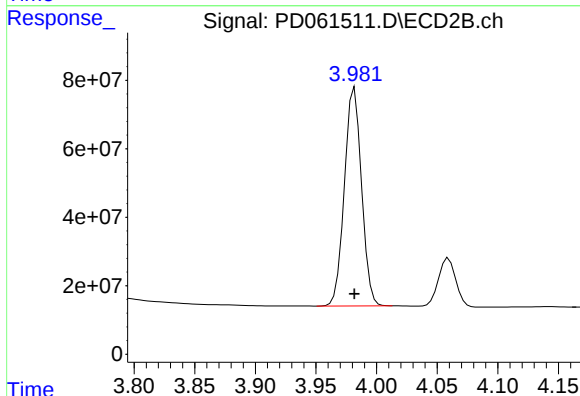


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 626311101
Conc: 71.53 ng/ml

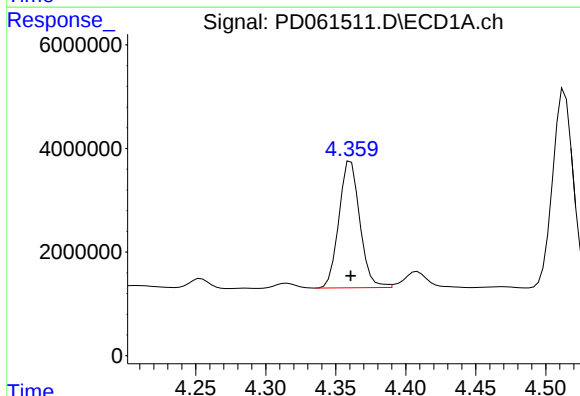


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 25421462
Conc: 722.78 ng/ml

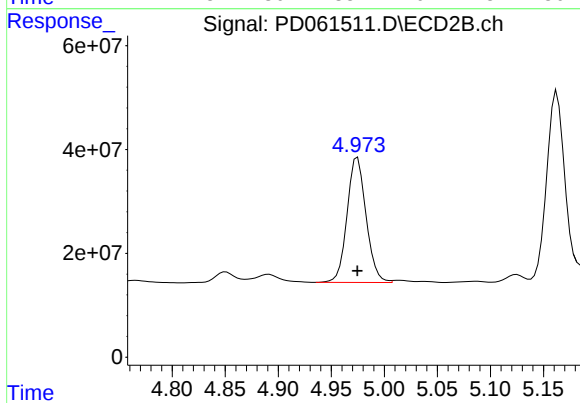

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 299552975
Conc: 728.01 ng/ml

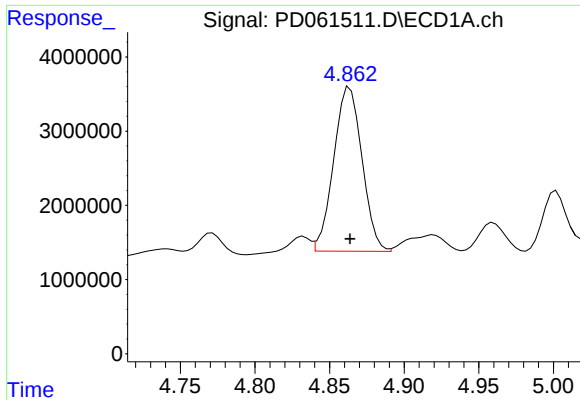

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 29309144
Conc: 715.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

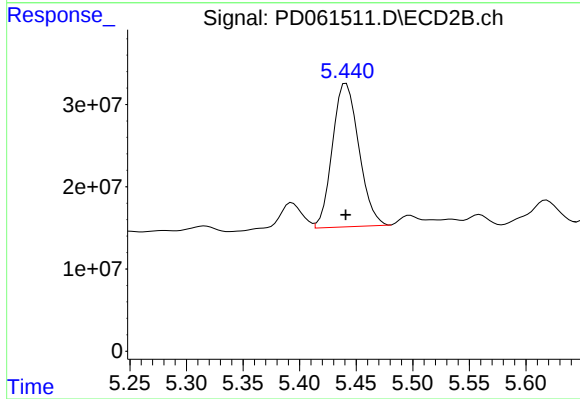


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 283758507
Conc: 713.89 ng/ml

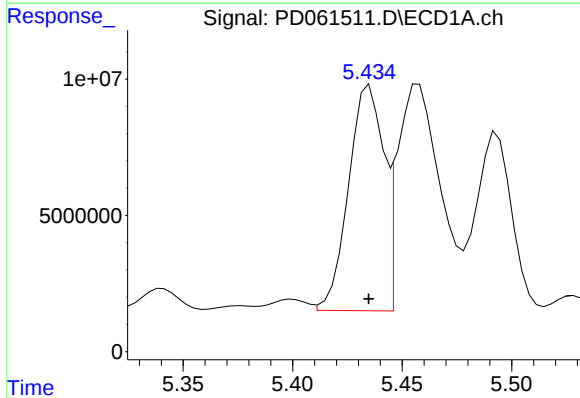


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 91754689
Conc: 743.35 ng/ml

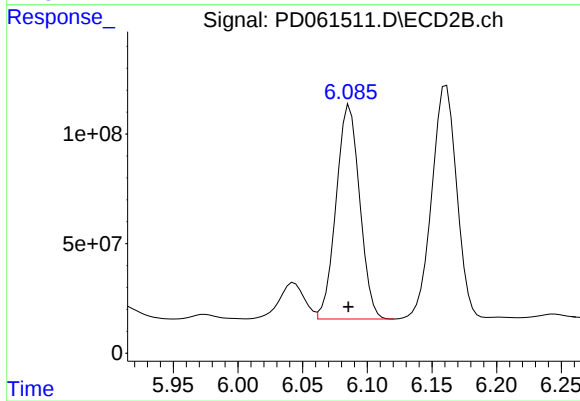

#25 Chlordane-3


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 1237090641
Conc: 724.16 ng/ml

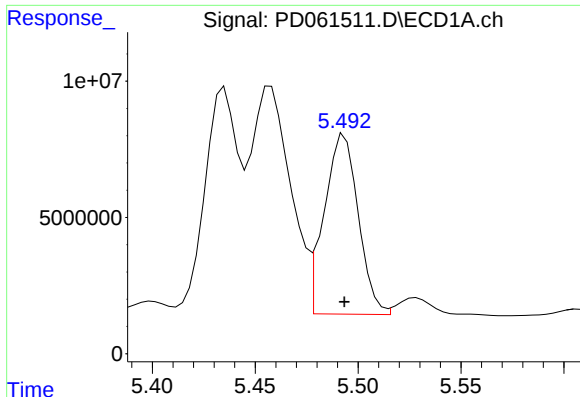

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 75910409
Conc: 737.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

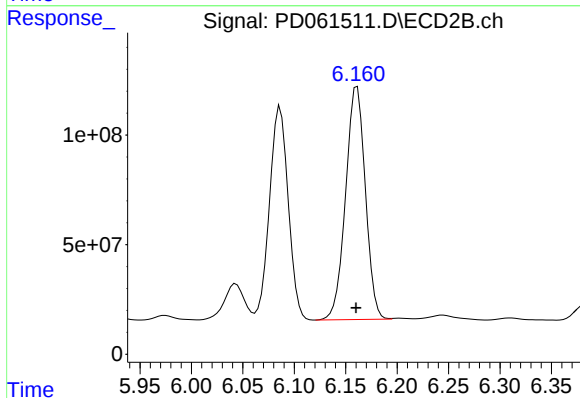


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.001 min
Response: 1420203402
Conc: 721.73 ng/ml

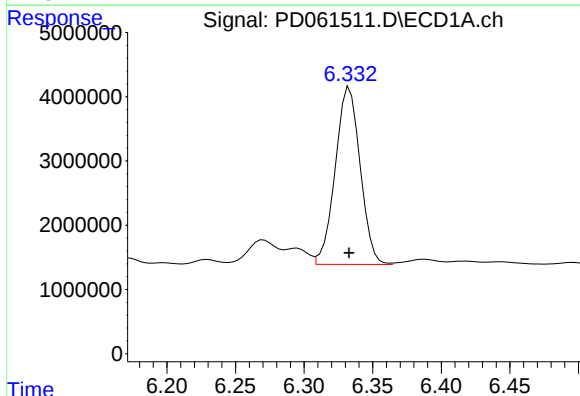


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 34883282
Conc: 730.80 ng/ml

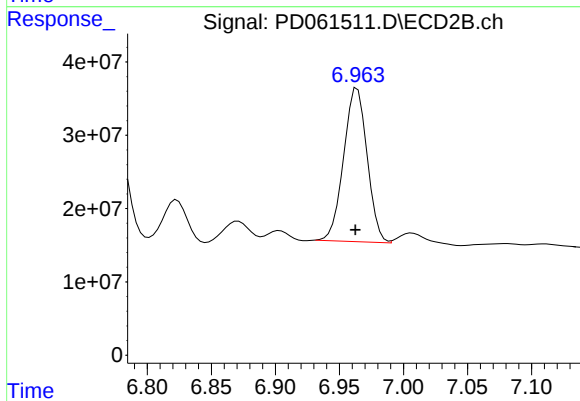

#27 Chlordane-5


R.T.: 6.964 min
Delta R.T.: 0.001 min
Response: 267486585
Conc: 727.73 ng/ml

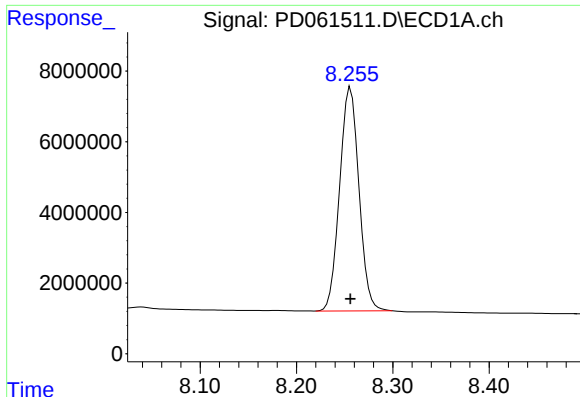

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 88039705
Conc: 71.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

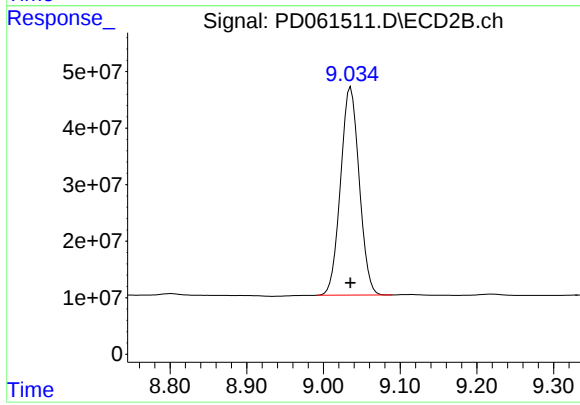

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.000 min
Response: 623617606
Conc: 71.16 ng/ml