

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 13:34
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:01:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 14:00:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	49914274	437.8E6	50.000	50.000
28)	SA Decachlor...	8.256	9.035	61564221	438.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.361	4.974	17585988	205.7E6	500.000	500.000
24)	Chlordane-2	4.864	5.441	20473950	198.7E6	500.000	500.000
25)	Chlordane-3	5.435	6.085	61716701	854.2E6	500.000	500.000
26)	Chlordane-4	5.493	6.160	51476626	983.9E6	500.000	500.000
27)	Chlordane-5	6.333	6.963	23866522	183.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 13:34
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:01:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 14:00:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

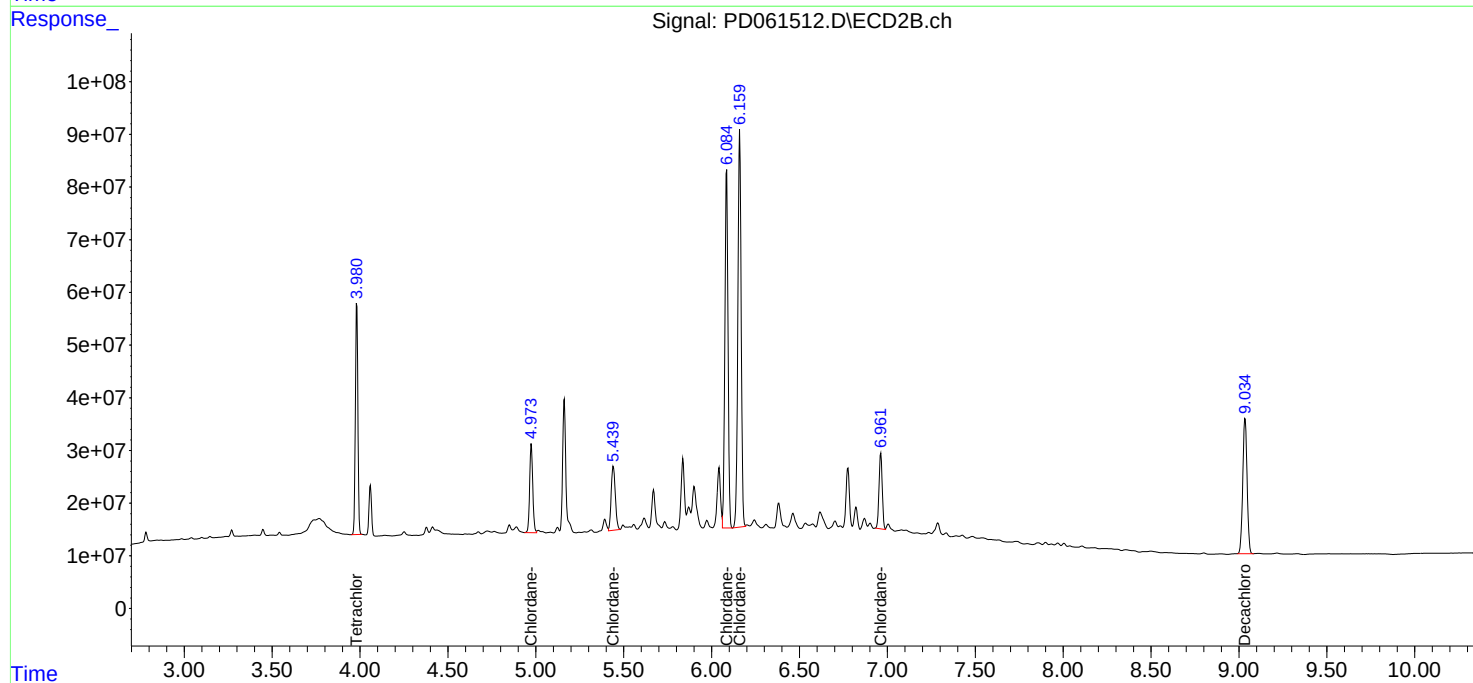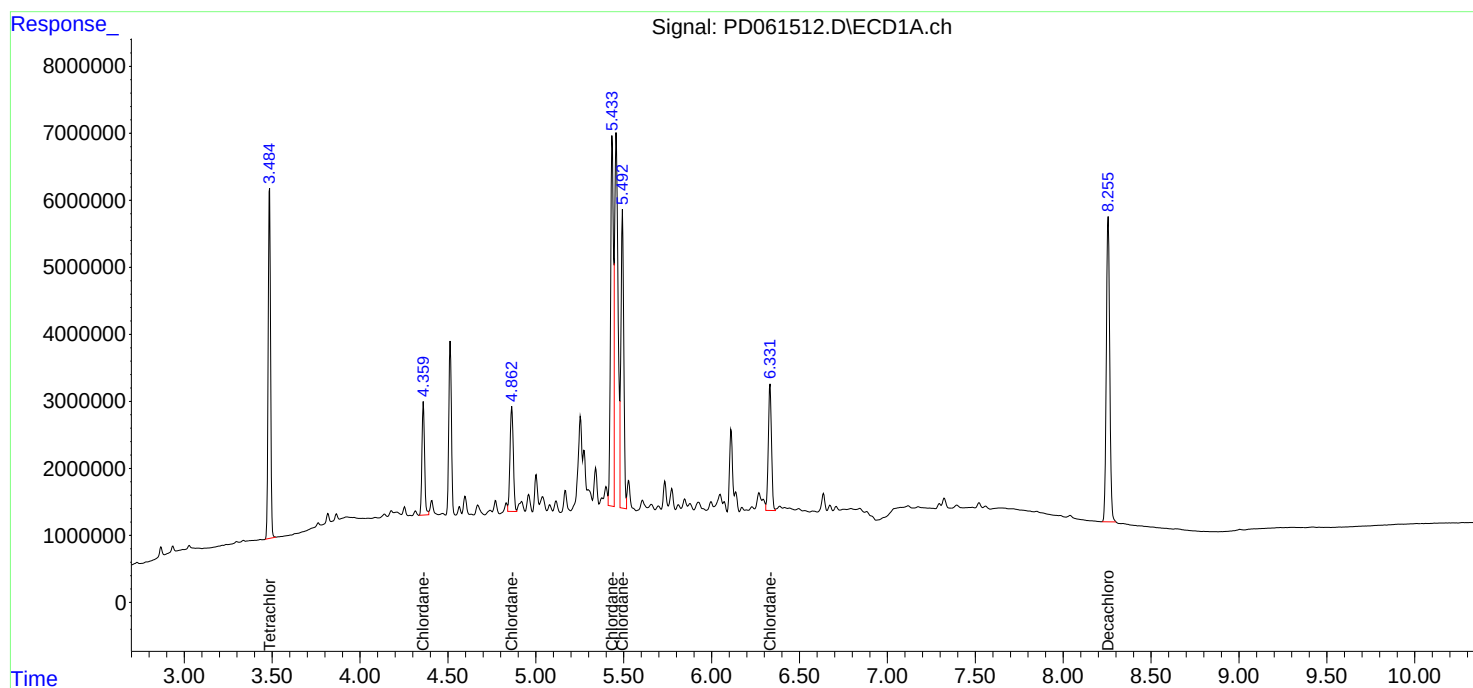


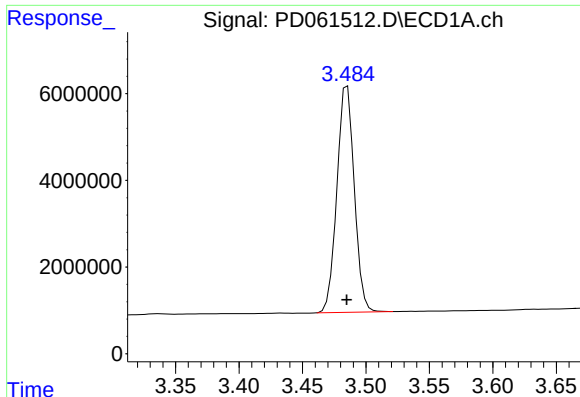

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 49914274
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

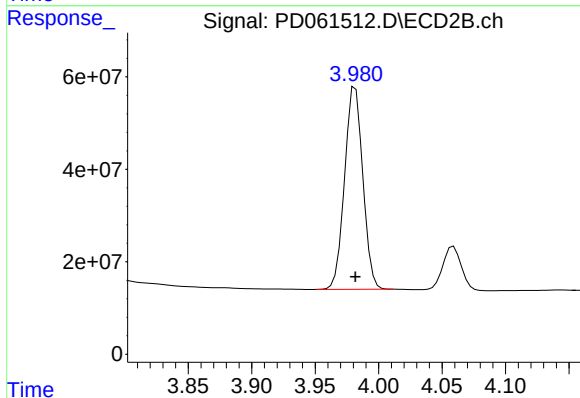


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 437821570
Conc: 50.00 ng/ml

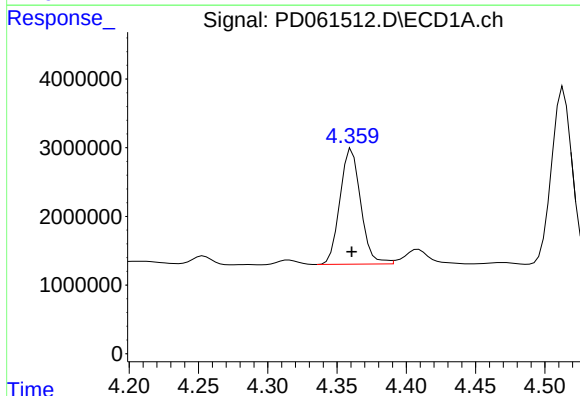


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 17585988
Conc: 500.00 ng/ml

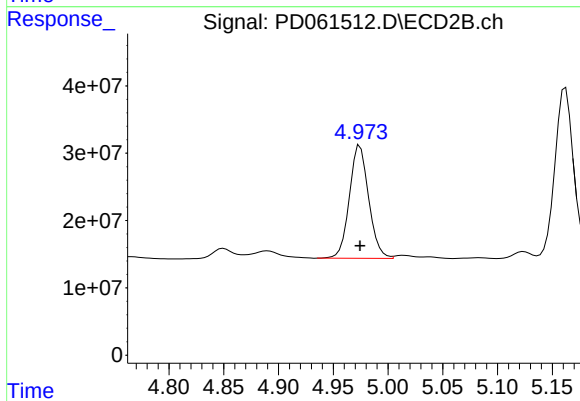

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 205735413
Conc: 500.00 ng/ml

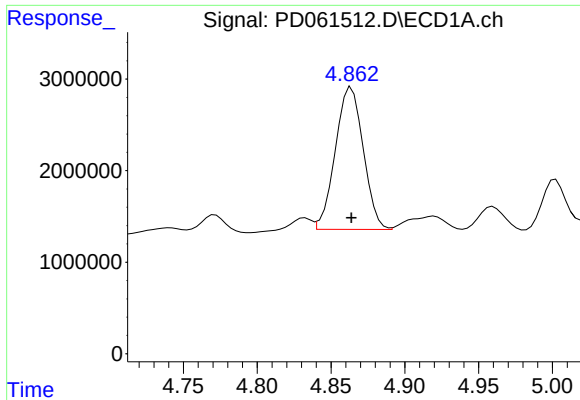

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 20473950
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

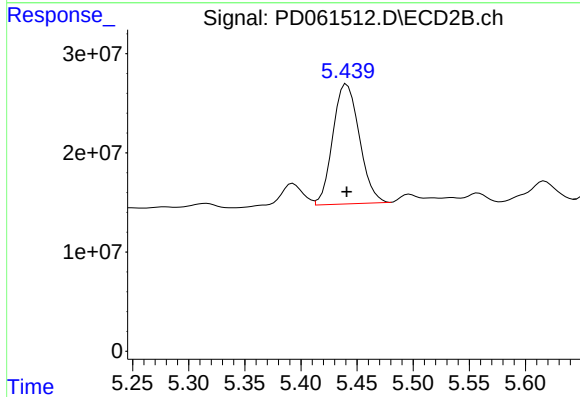


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 198741910
Conc: 500.00 ng/ml

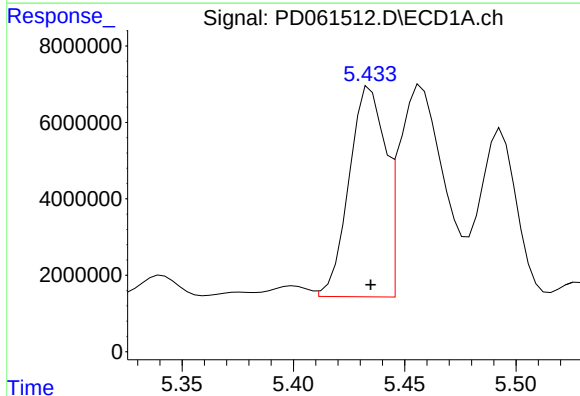


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 61716701
Conc: 500.00 ng/ml

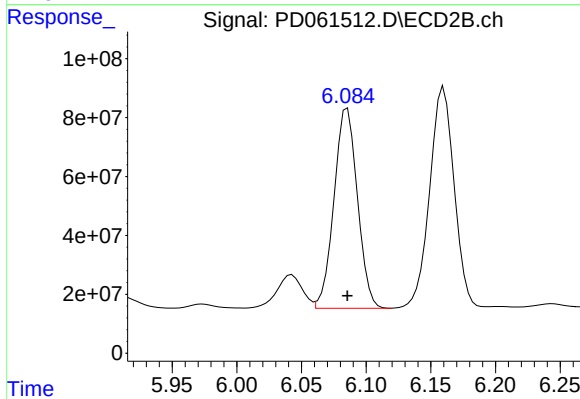

#25 Chlordane-3


R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 854156752
Conc: 500.00 ng/ml

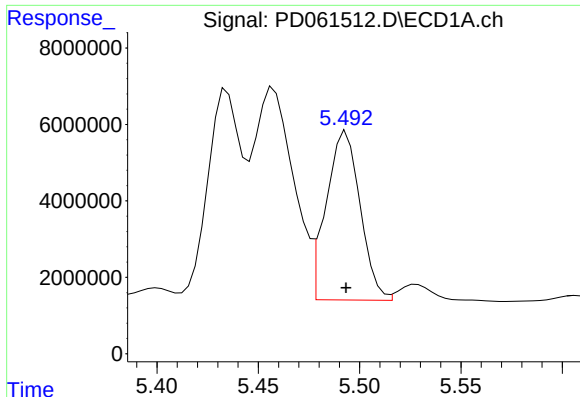

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 51476626
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

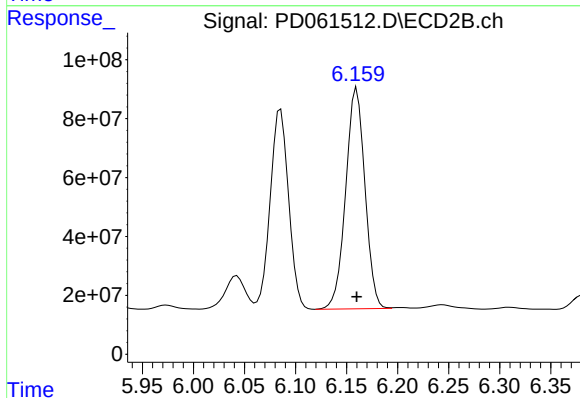


#26 Chlordane-4

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 983883522
Conc: 500.00 ng/ml

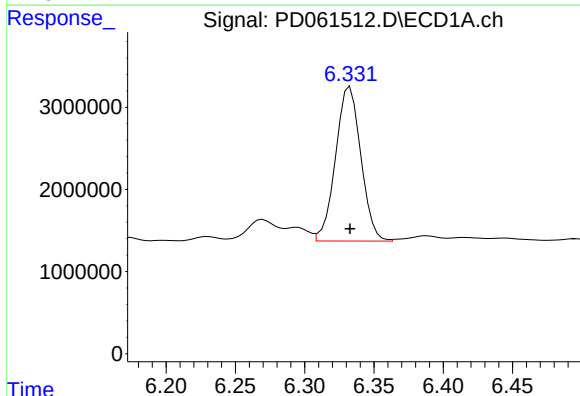


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 23866522
Conc: 500.00 ng/ml

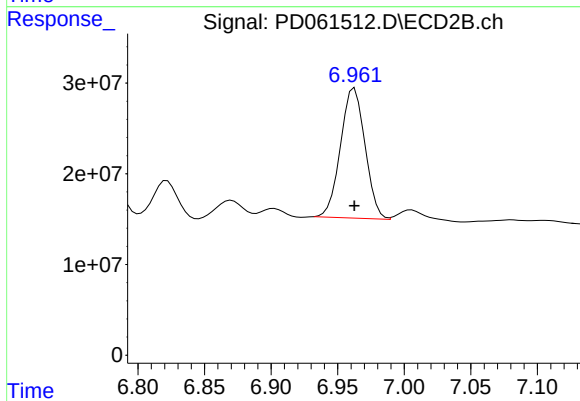

#27 Chlordane-5


R.T.: 6.963 min
Delta R.T.: 0.000 min
Response: 183781091
Conc: 500.00 ng/ml

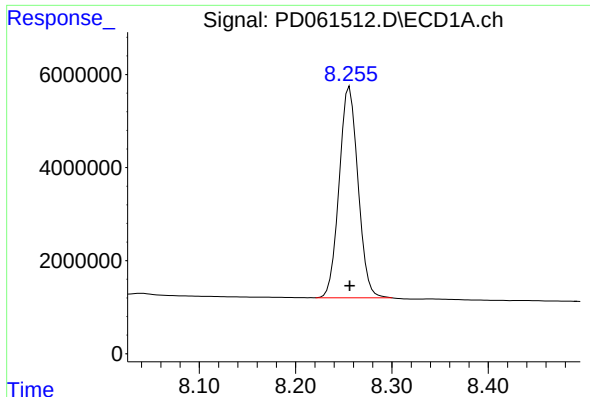

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 61564221
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

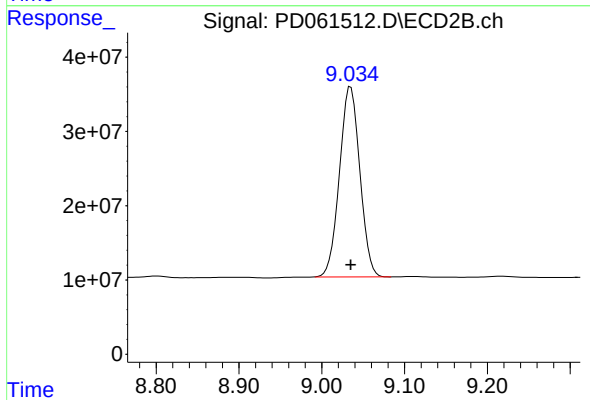

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.000 min
Response: 438197386
Conc: 50.00 ng/ml