

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 13:48
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:01:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 14:00:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	24422113	220.8E6	24.464	25.211
28)	SA Decachlor...	8.257	9.036	32559649	230.7E6	26.444	26.319
Target Compounds							
23)	Chlordane-1	4.361	4.975	8994754	102.2E6	255.736	248.351
24)	Chlordane-2	4.864	5.441	10872285	100.3E6	265.515	252.422
25)	Chlordane-3	5.436	6.086	30283365	431.8E6	245.342	252.760
26)	Chlordane-4	5.494	6.161	25598900	502.1E6	248.646	255.144
27)	Chlordane-5	6.333	6.964	11724642	93115096	245.629	253.332



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 13:48
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:01:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 14:00:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

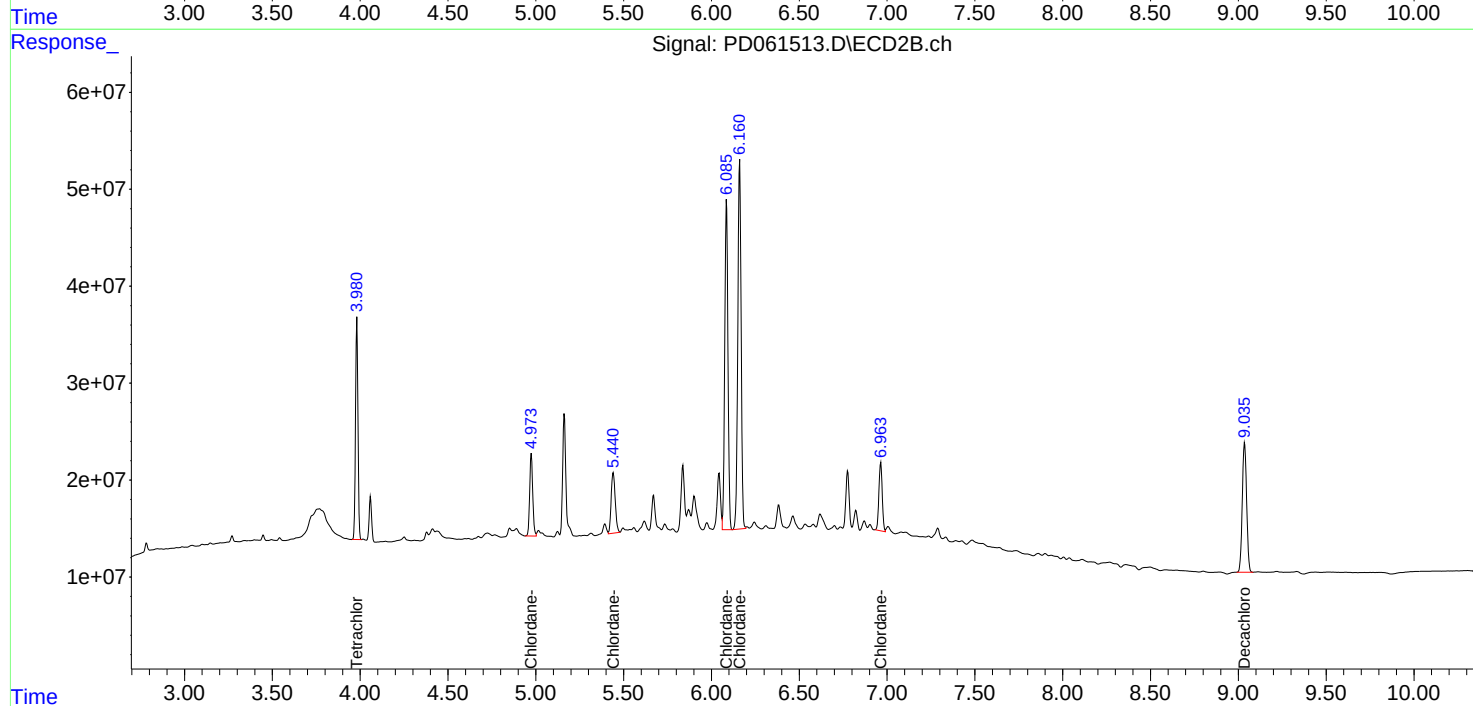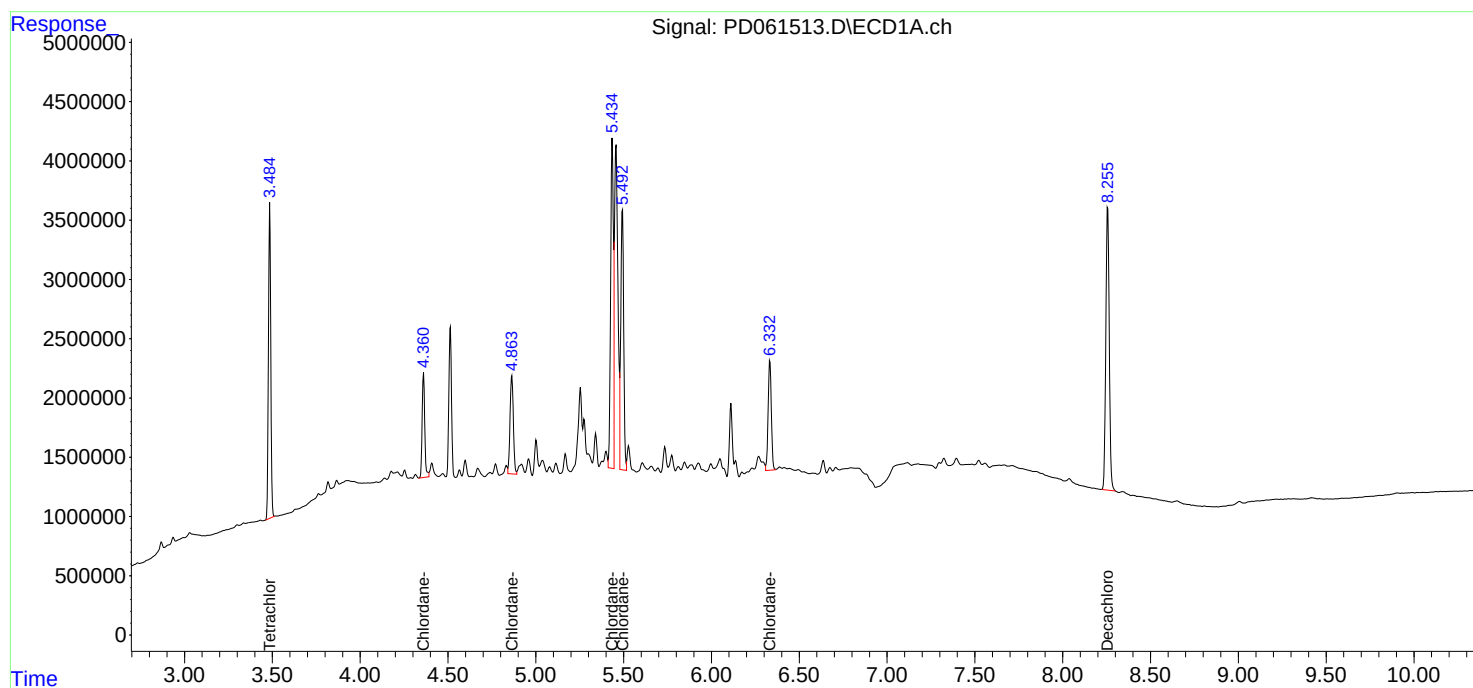


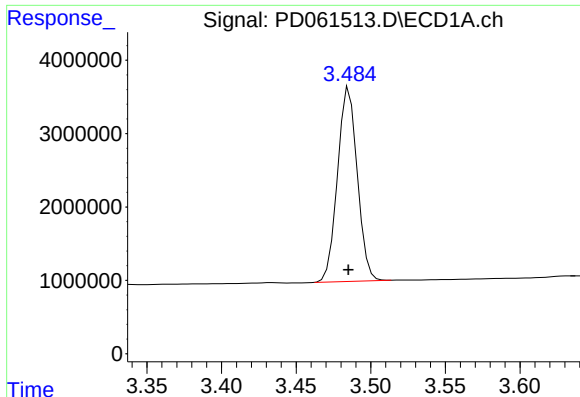

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 24422113
Conc: 24.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

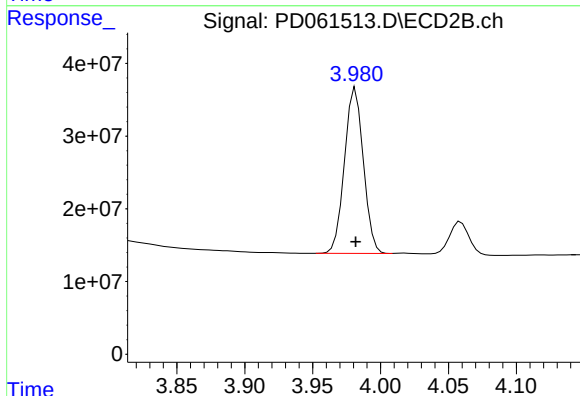


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 220761569
Conc: 25.21 ng/ml

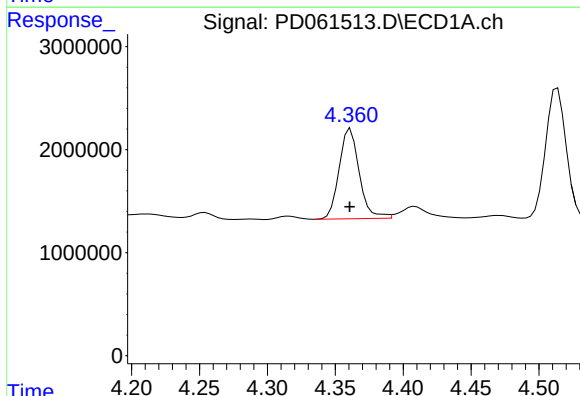


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 8994754
Conc: 255.74 ng/ml

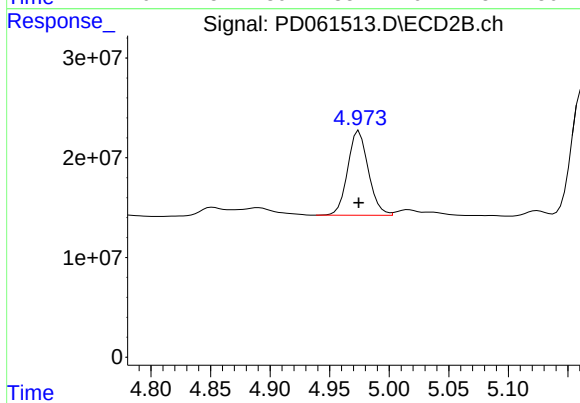

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 102189376
Conc: 248.35 ng/ml

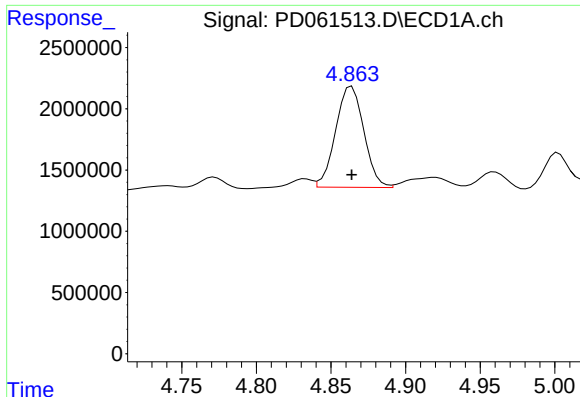

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 10872285
Conc: 265.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

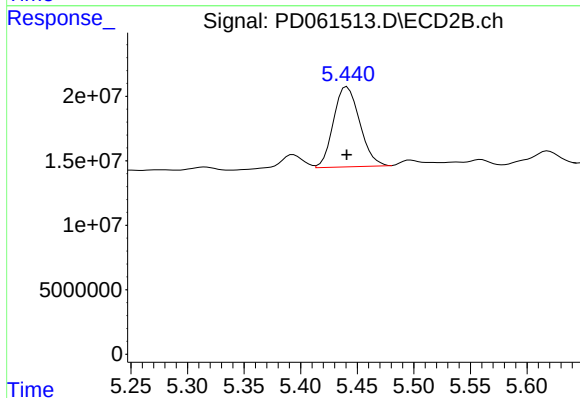


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 100333697
Conc: 252.42 ng/ml

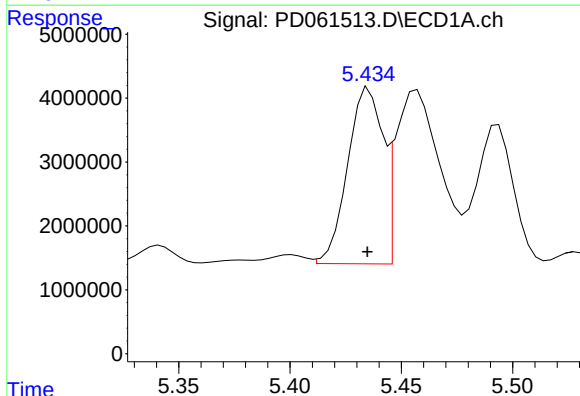


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 30283365
Conc: 245.34 ng/ml

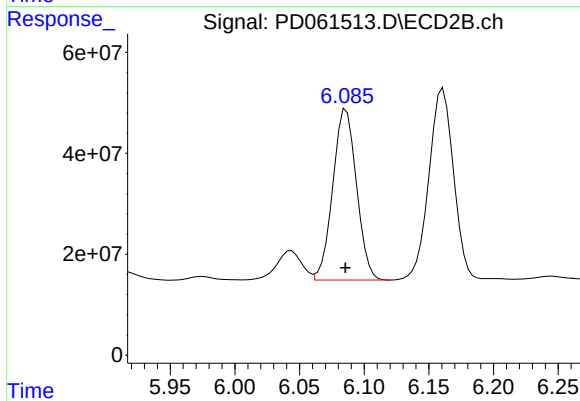

#25 Chlordane-3


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 431793478
Conc: 252.76 ng/ml

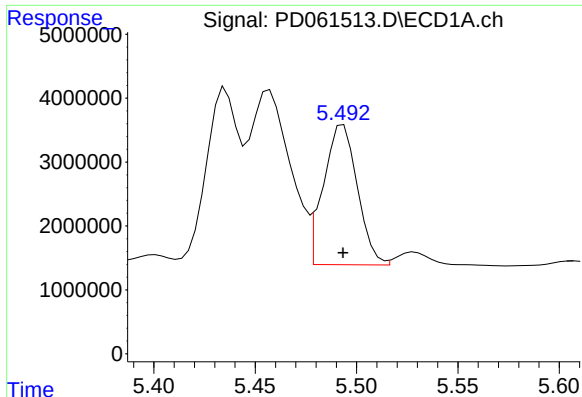

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 25598900
Conc: 248.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

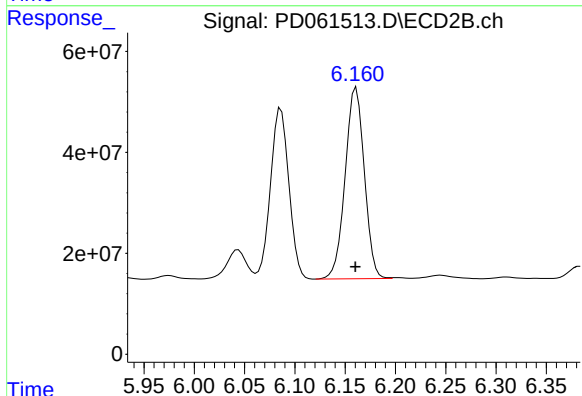


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.000 min
Response: 502064230
Conc: 255.14 ng/ml

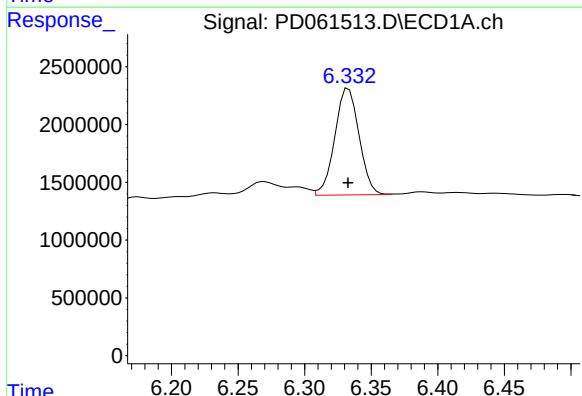


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 11724642
Conc: 245.63 ng/ml

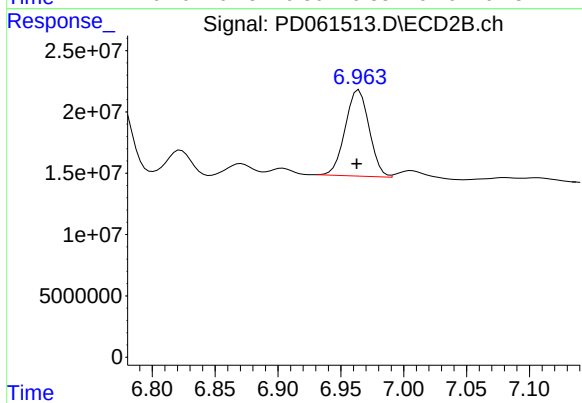

#27 Chlordane-5


R.T.: 6.964 min
Delta R.T.: 0.002 min
Response: 93115096
Conc: 253.33 ng/ml

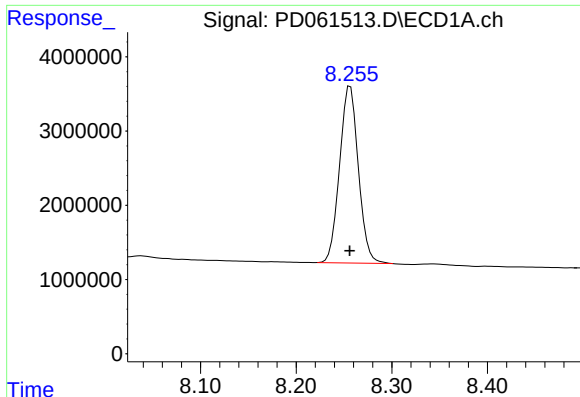

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 32559649
Conc: 26.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

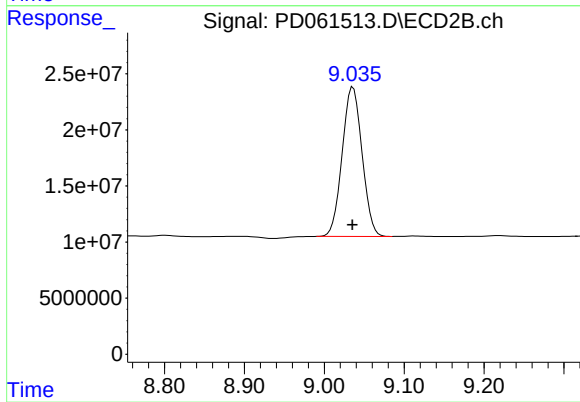

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 230656106
Conc: 26.32 ng/ml