

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 14:02
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:13:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 14:00:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	5443219	50048266	5.453	5.716
28)	SA Decachlor...	8.257	9.036	8347068	57568817	6.779	6.569
Target Compounds							
23)	Chlordane-1	4.361	4.974	2109805	23180774	59.985	56.336
24)	Chlordane-2	4.864	5.441	2411649	23230982	58.896	58.445
25)	Chlordane-3	5.435	6.085	6884250	100.7E6	55.773	58.931
26)	Chlordane-4	5.494	6.160	5772528	118.8E6	56.069	60.378
27)	Chlordane-5	6.332	6.963	2782103	22983881	58.285	62.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 14:02
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:13:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 14:00:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

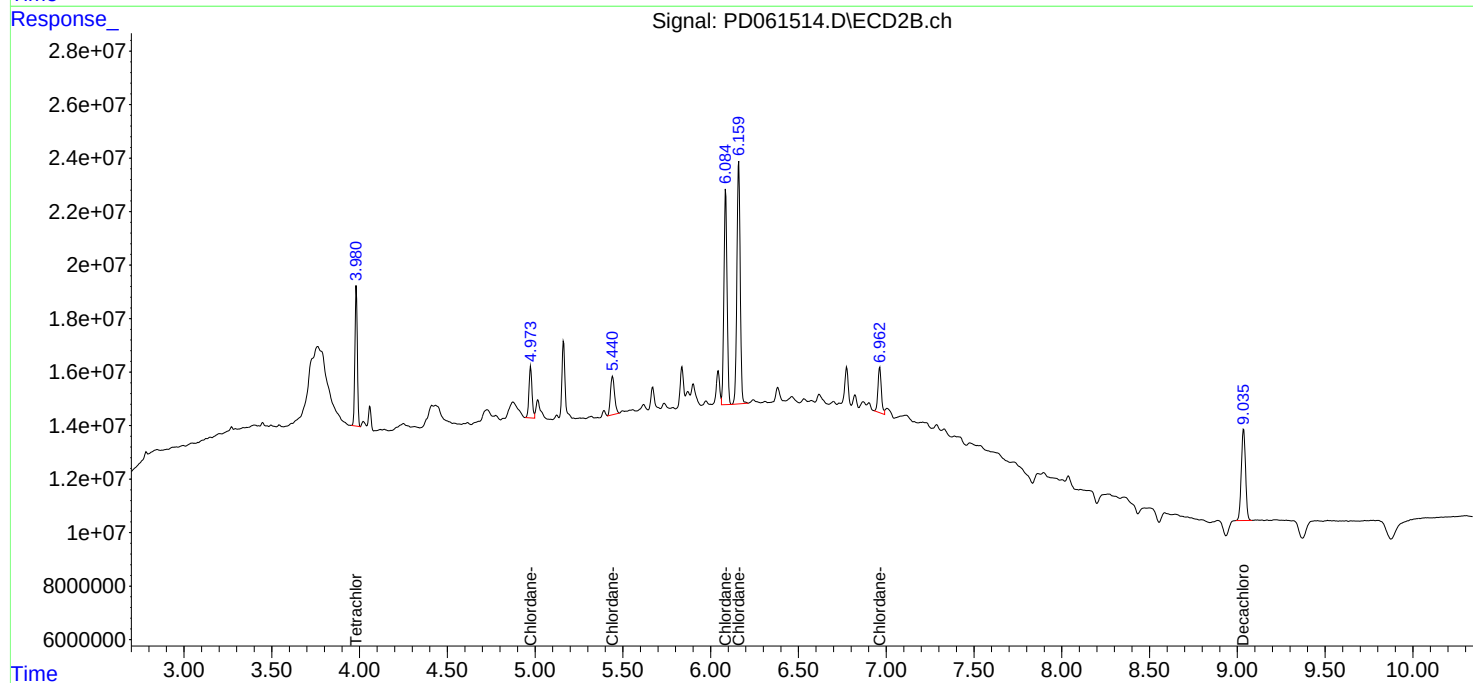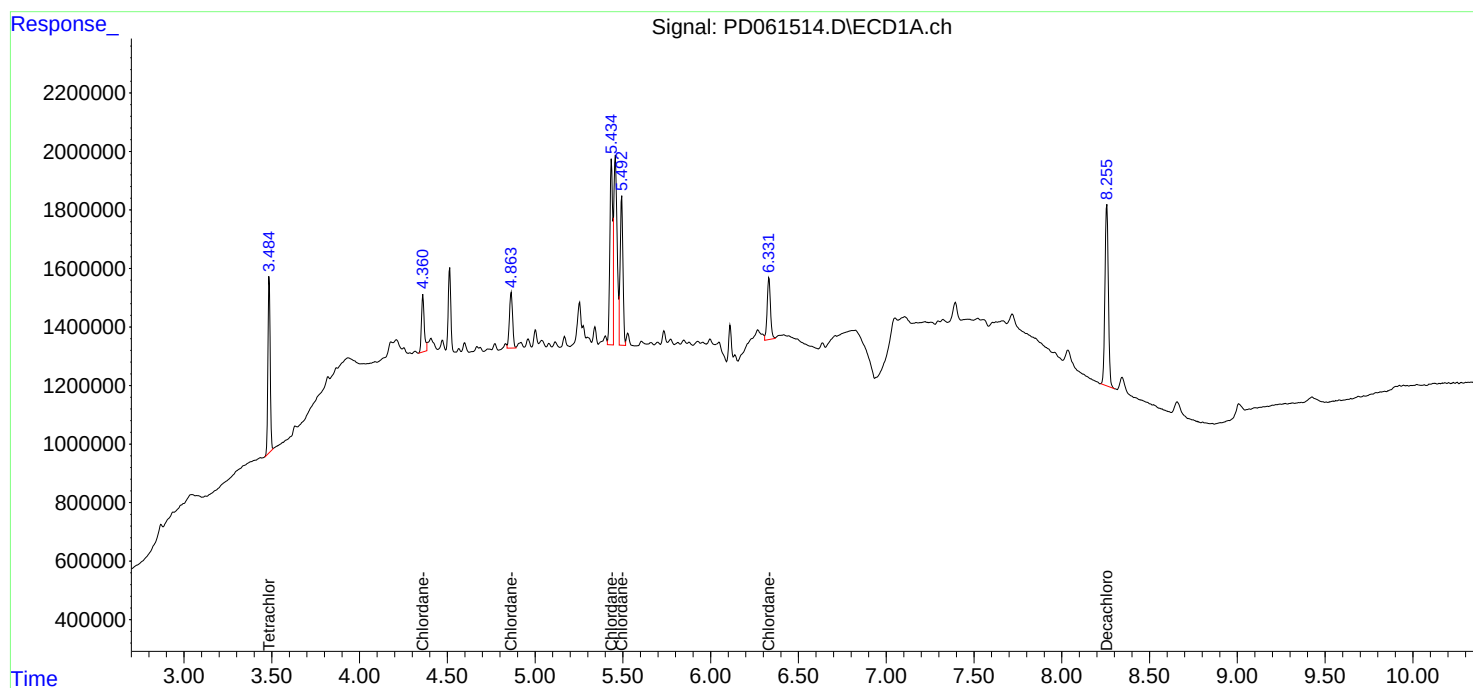


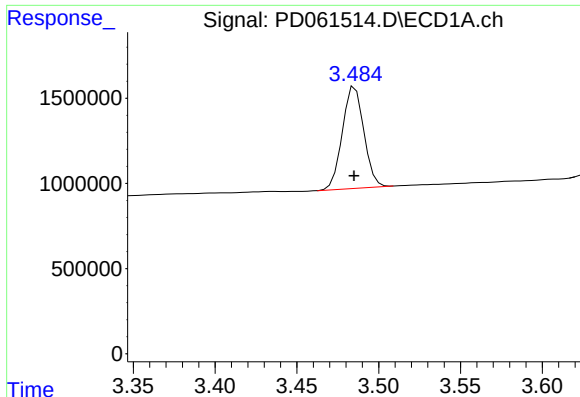

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 5443219
Conc: 5.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

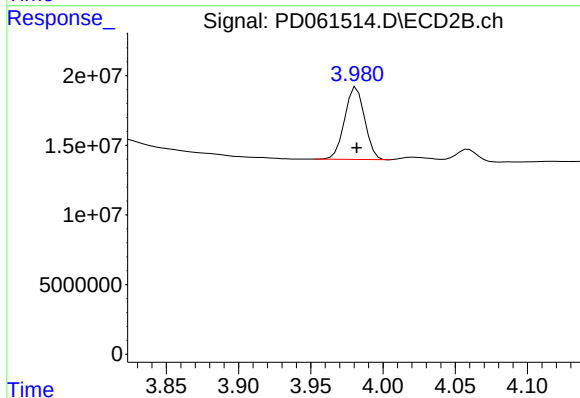


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 50048266
Conc: 5.72 ng/ml

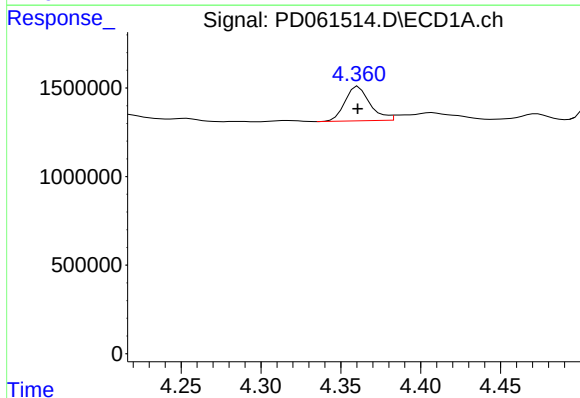


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 2109805
Conc: 59.99 ng/ml

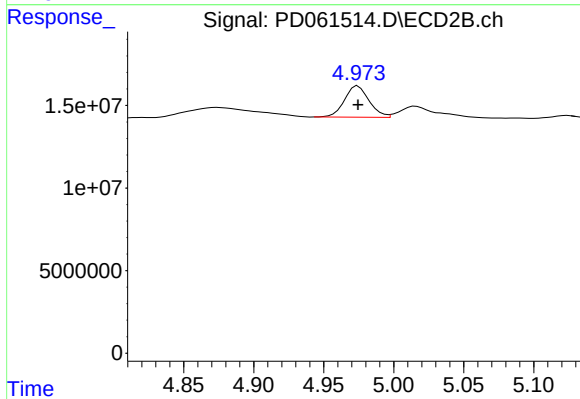

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 23180774
Conc: 56.34 ng/ml

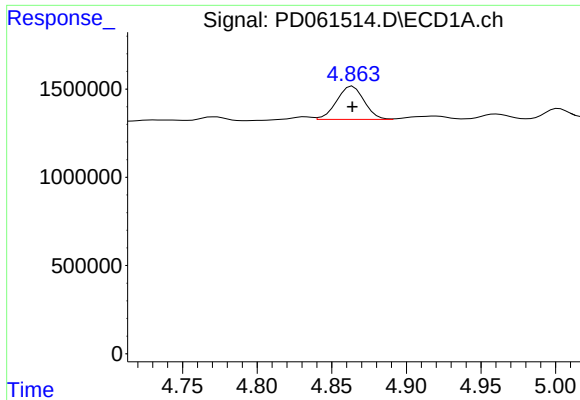

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 2411649
Conc: 58.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

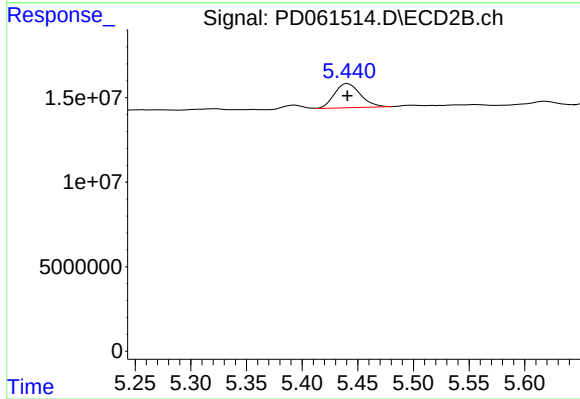


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 23230982
Conc: 58.45 ng/ml

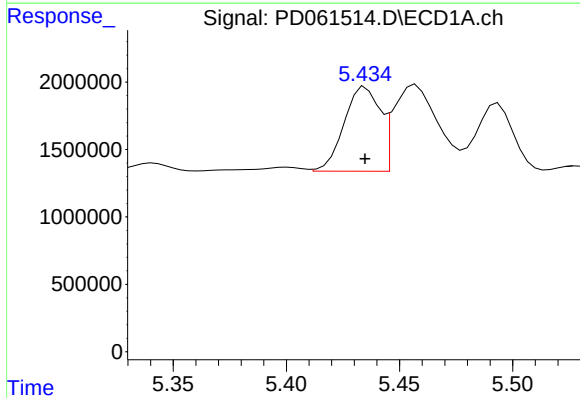


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 6884250
Conc: 55.77 ng/ml

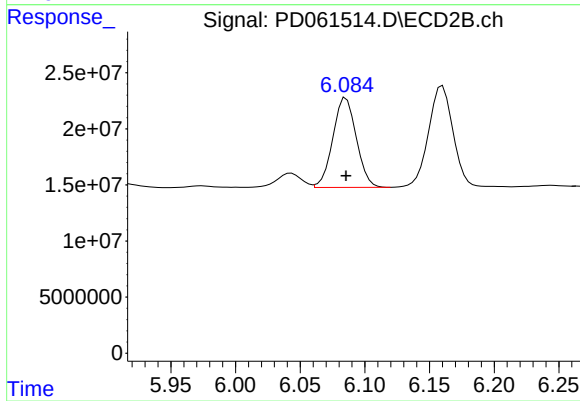

#25 Chlordane-3


R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 100672136
Conc: 58.93 ng/ml

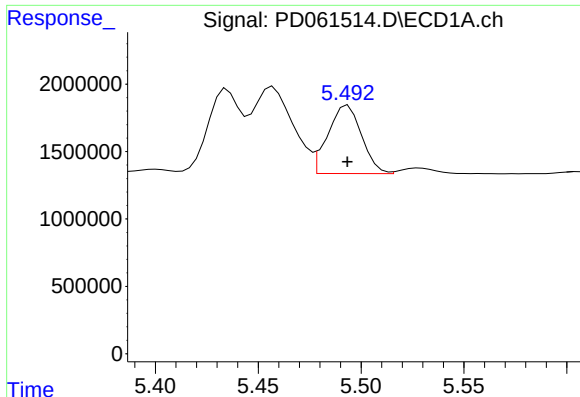

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 5772528
Conc: 56.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

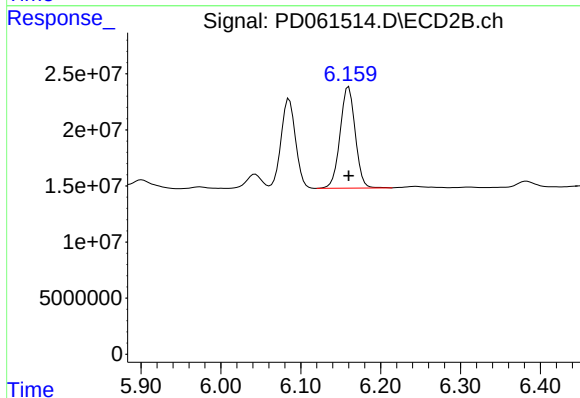


#26 Chlordane-4

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 118809815
Conc: 60.38 ng/ml

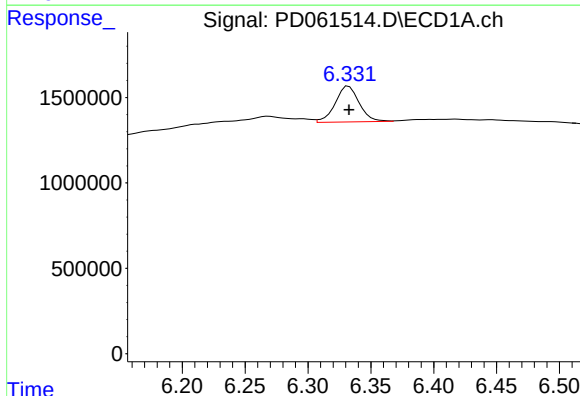


#27 Chlordane-5

R.T.: 6.332 min
Delta R.T.: 0.000 min
Response: 2782103
Conc: 58.28 ng/ml

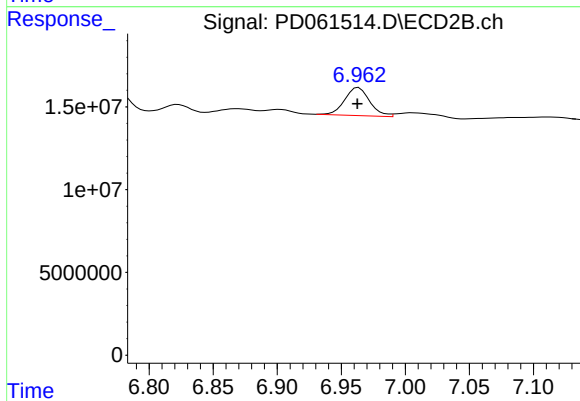

#27 Chlordane-5


R.T.: 6.963 min
Delta R.T.: 0.000 min
Response: 22983881
Conc: 62.53 ng/ml

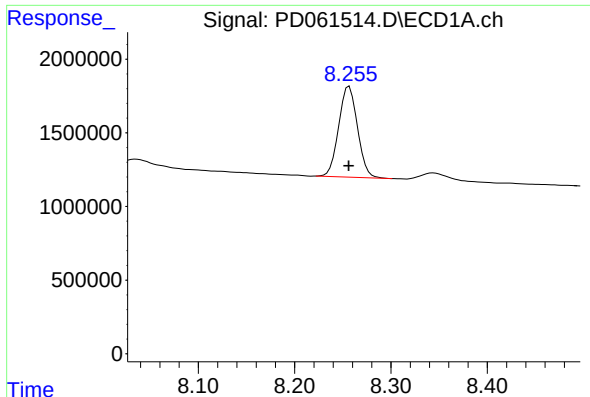

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 8347068
Conc: 6.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC050

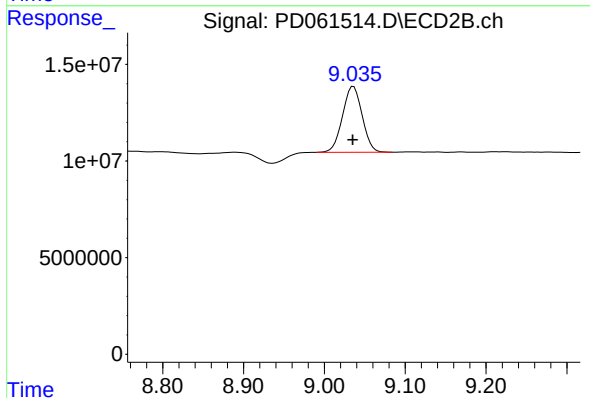

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 57568817
Conc: 6.57 ng/ml