

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 15:40
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:32:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 04:32:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	3.982	47308781	413.4E6	47.182	46.955
28)	SA Decachlor...	8.257	9.037	57735599	410.6E6	44.393	44.805
Target Compounds							
23)	Chlordane-1	4.361	4.975	16656855	196.9E6	461.239	475.167
24)	Chlordane-2	4.864	5.441	19655939	188.1E6	468.220	467.828
25)	Chlordane-3	5.435	6.087	58341186	805.3E6	465.318	462.780
26)	Chlordane-4	5.493	6.161	48760808	925.8E6	467.207	459.048
27)	Chlordane-5	6.333	6.964	22620718	172.5E6	467.057	452.703



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 15:40
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD031021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:32:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 04:32:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

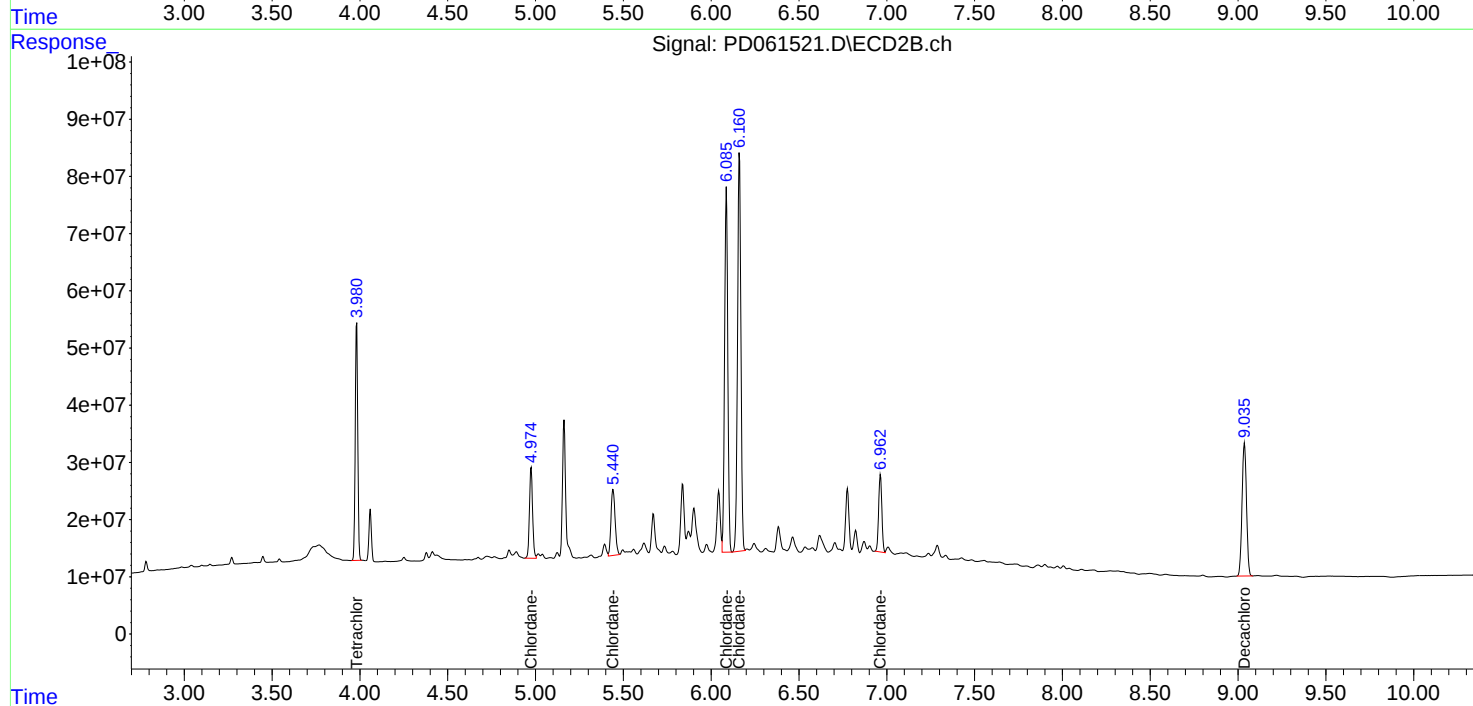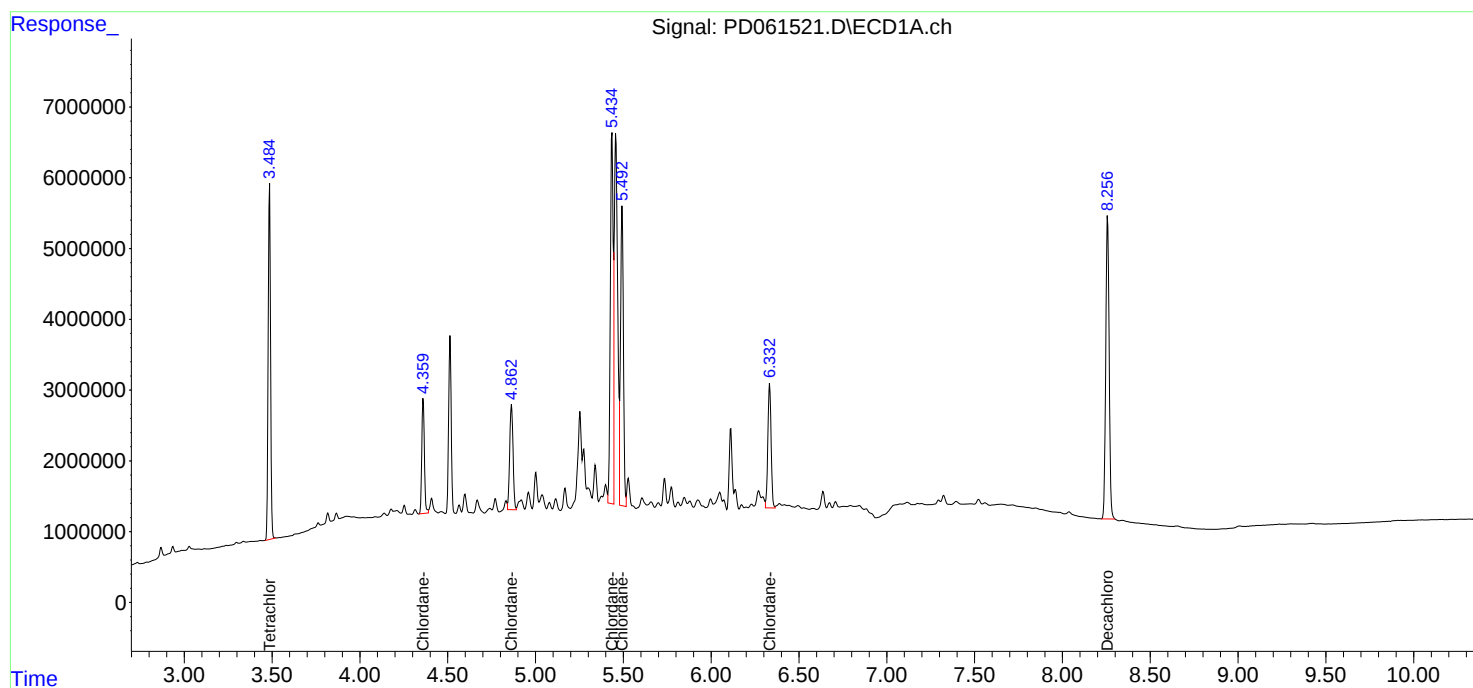


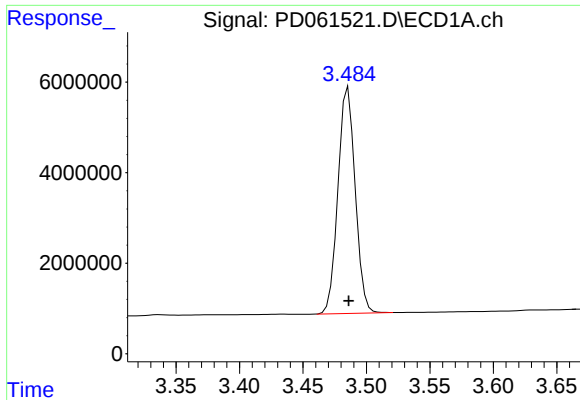

#1 Tetrachloro-m-xylene


R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 47308781
Conc: 47.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031021

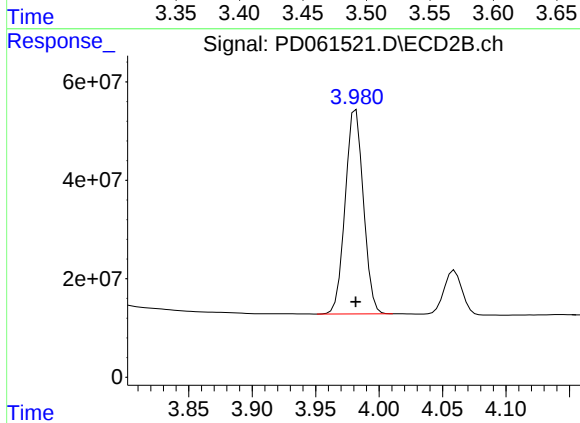


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 413420582
Conc: 46.95 ng/ml

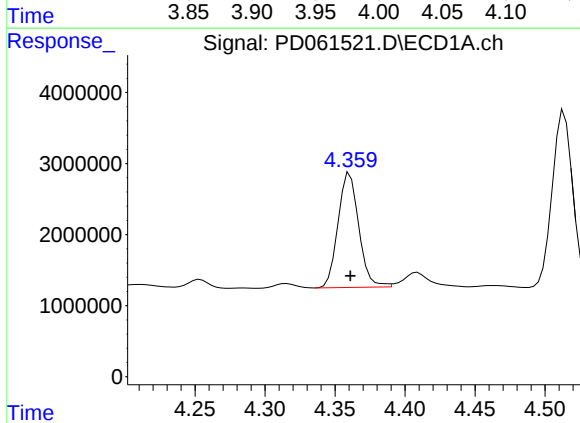


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 16656855
Conc: 461.24 ng/ml

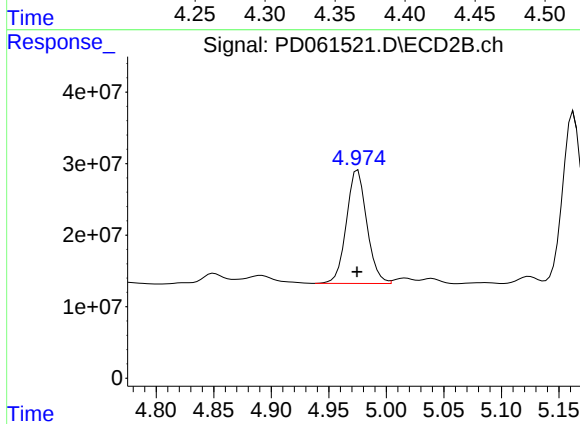

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 196891922
Conc: 475.17 ng/ml

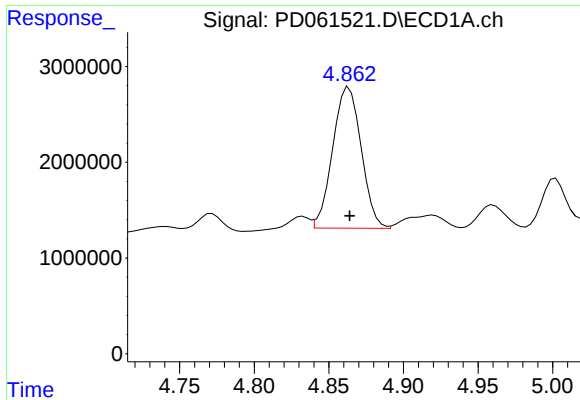

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 19655939
Conc: 468.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031021

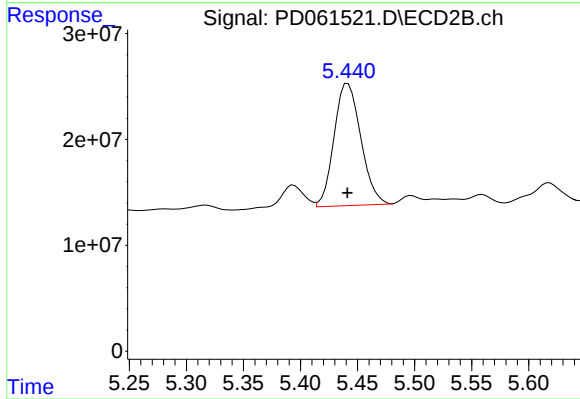


#24 Chlordane-2

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 188119338
Conc: 467.83 ng/ml

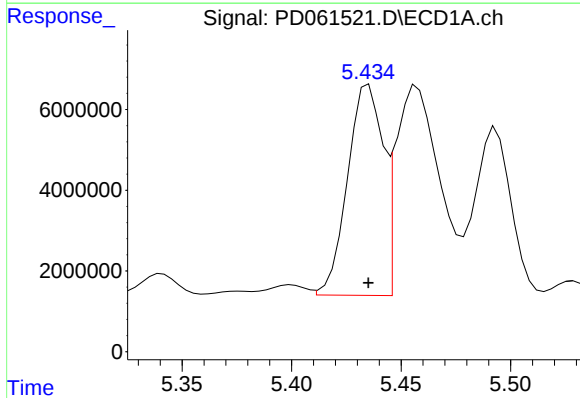


#25 Chlordane-3

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 58341186
Conc: 465.32 ng/ml

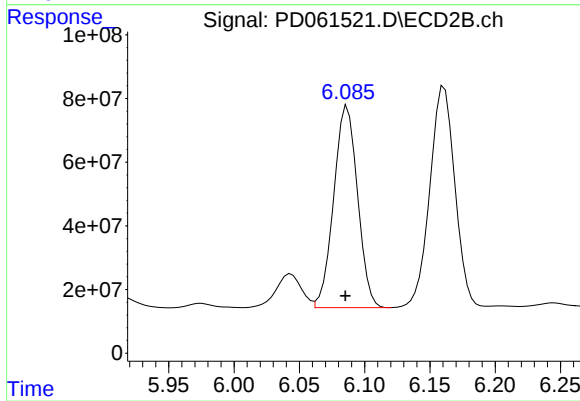

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.001 min
Response: 805330715
Conc: 462.78 ng/ml

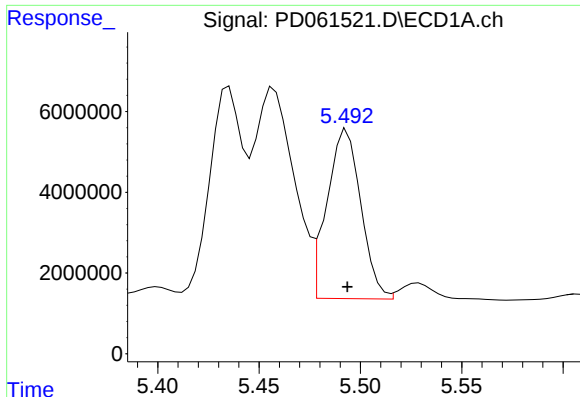

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 48760808
Conc: 467.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031021

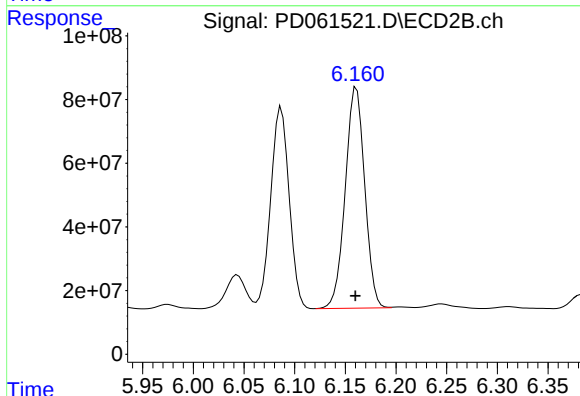


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.001 min
Response: 925755917
Conc: 459.05 ng/ml

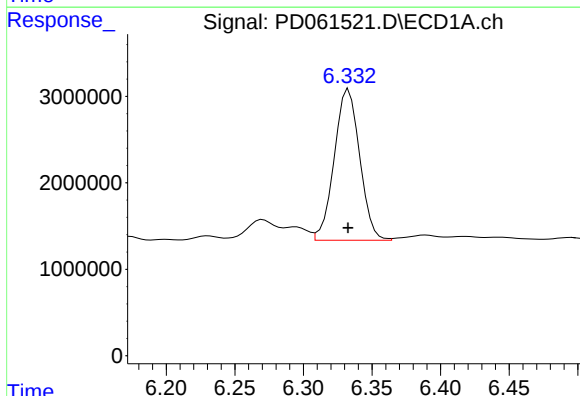


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 22620718
Conc: 467.06 ng/ml

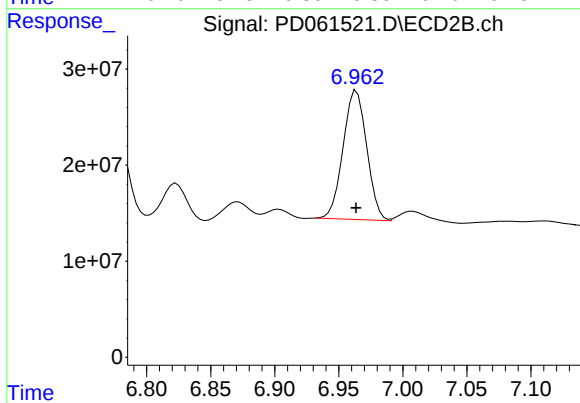

#27 Chlordane-5


R.T.: 6.964 min
Delta R.T.: 0.000 min
Response: 172485803
Conc: 452.70 ng/ml

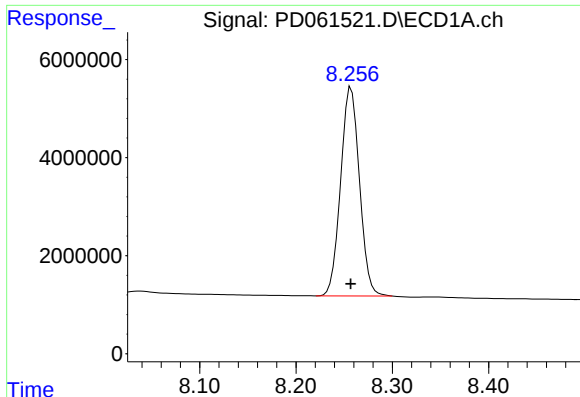

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 57735599
Conc: 44.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD031021

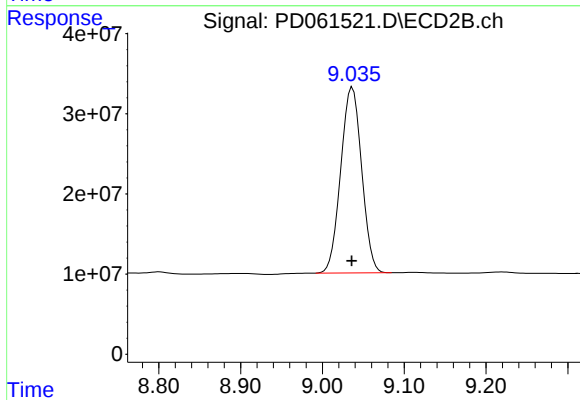

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 410573993
Conc: 44.81 ng/ml