

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 14:16
 Operator : AR\AJ
 Sample : PTOXICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC1000

Manual Integrations
 APPROVED

Ankita
 3/11/2021 3:48:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 15:23:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 15:22:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.982	81702370	821.4E6	98.418	94.667
7) SA Decachlor...	8.257	9.035	114.2E6	812.0E6	95.002	93.312
Target Compounds						
2) Toxaphene-1	5.969	6.555	11752664	107.3E6	950.577	995.822
3) Toxaphene-2	6.237	7.060	9324337	92403056	912.210	969.313m
4) Toxaphene-3	6.604	7.138	20982611	254.0E6	967.338	960.726
5) Toxaphene-4	6.747	7.224	7736278	159.9E6	951.815	973.738
6) Toxaphene-5	7.028	7.636	8420381	109.7E6	926.138	961.683

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 14:16
Operator : AR\AJ
Sample : PTOXICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 15:23:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 15:22:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

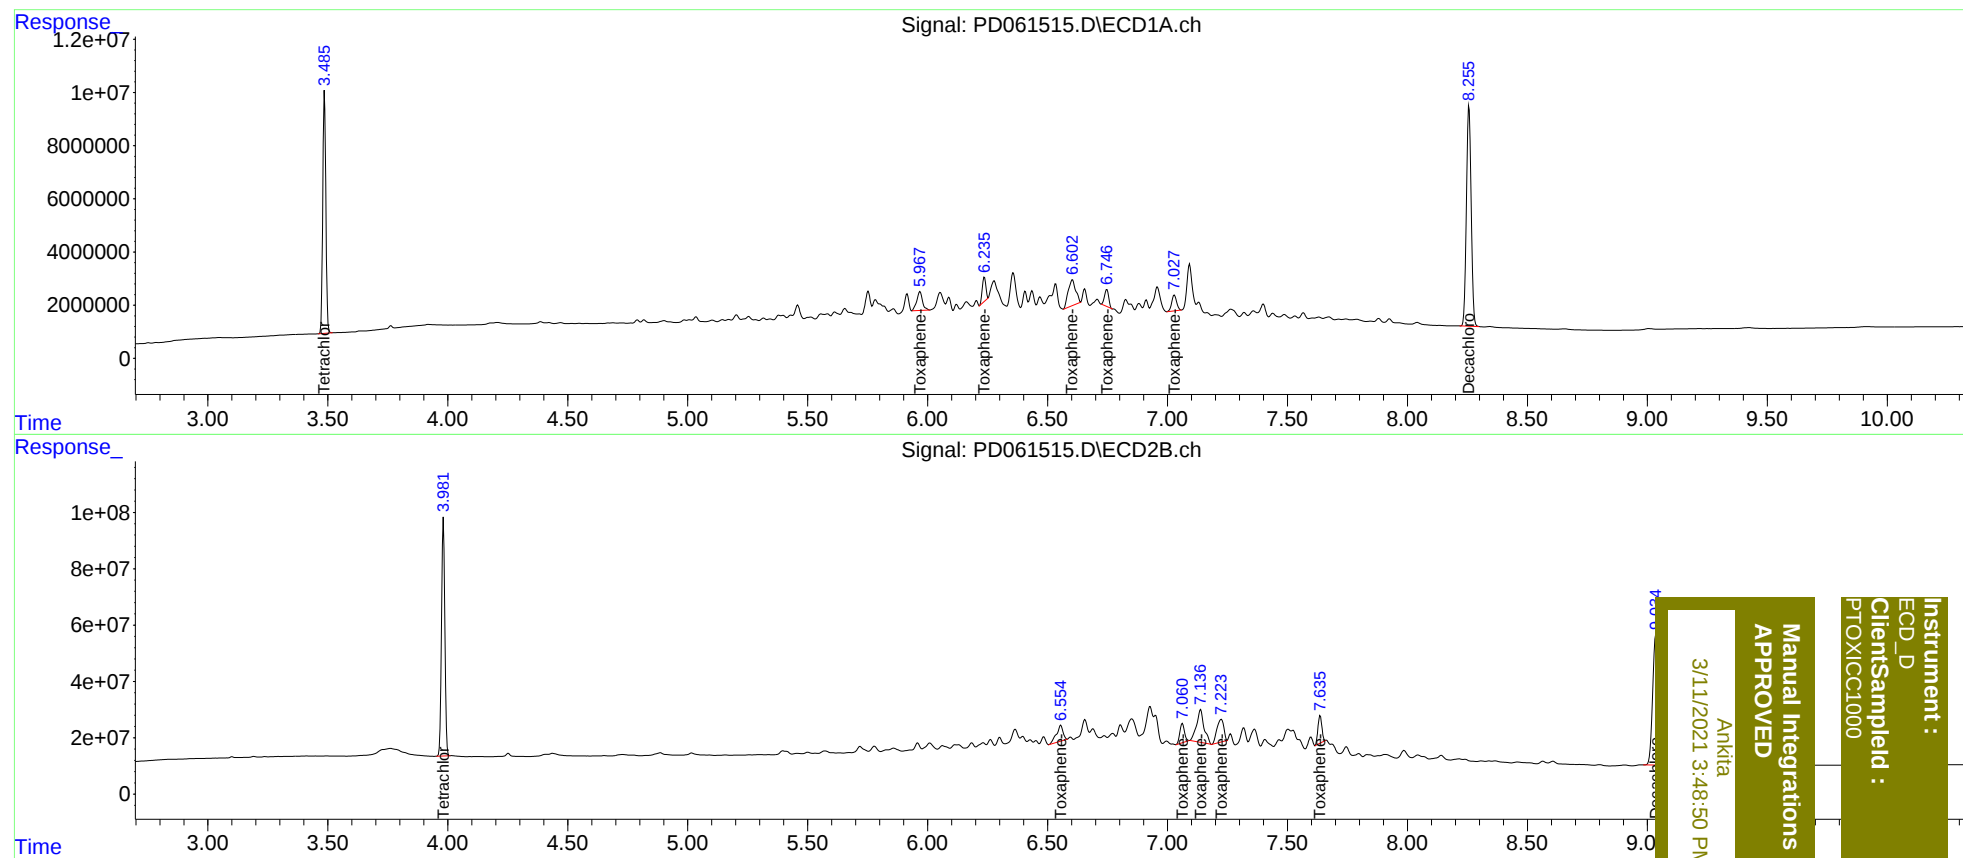

Manual Integrations
APPROVED

Ankita
3/11/2021 3:48:50 PM

Instrument :
ECD_D
ClientSampled :
PTOXICC1000