

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 15:54
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD031021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:05:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031021.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 03:56:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.486	3.982	39516511	413.0E6	46.893	47.183
7) SA Decachlor...	8.257	9.036	58226391	417.5E6	46.134	46.486
Target Compounds						
2) Toxaphene-1	5.969	6.555	6248757	54667832	503.985	506.273
3) Toxaphene-2	6.237	7.062	4950070	43886298	492.387	480.387
4) Toxaphene-3	6.605	7.138	10447399	125.8E6	489.684	472.867
5) Toxaphene-4	6.747	7.225	3888744	79243786	488.166	459.438
6) Toxaphene-5	7.028	7.637	4487305	53280629	474.056	462.948

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 15:54
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX031021.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 03:56:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

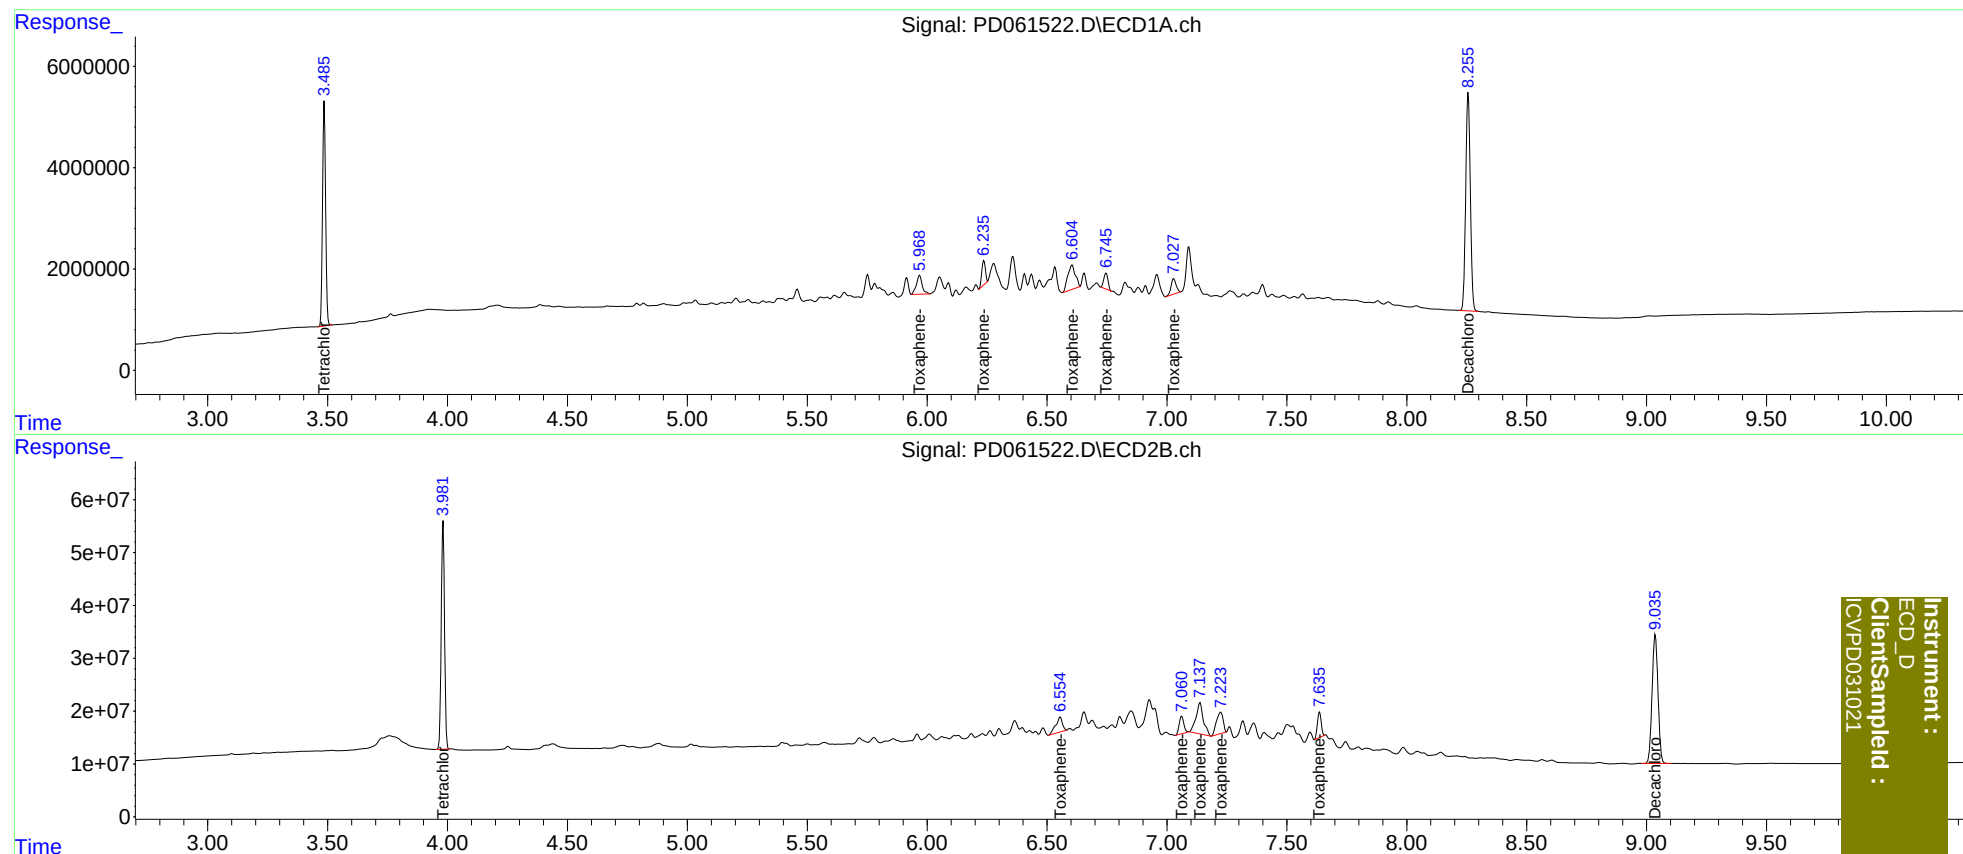

Instrument :
ECD_D
ClientSampled :
ICV/PD031021