

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
 Data File : PD061510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 13:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:00:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 10 14:00:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.982	97380828	807.6E6	97.548	92.230
28)	SA Decachlor...	8.257	9.036	112.6E6	799.9E6	91.438	91.272
Target Compounds							
23)	Chlordane-1	4.361	4.975	33324063	388.6E6	947.461	944.342
24)	Chlordane-2	4.864	5.442	38151635	368.8E6	931.712	927.781
25)	Chlordane-3	5.436	6.087	122.3E6	1602.6E6	990.853	938.129
26)	Chlordane-4	5.494	6.161	99819274	1837.6E6	969.559	933.851
27)	Chlordane-5	6.334	6.964	45377556	348.7E6	950.653	948.732



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031021\
Data File : PD061510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 13:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:00:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031021.M
Quant Title : GC Extractables
QLast Update : Wed Mar 10 14:00:05 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

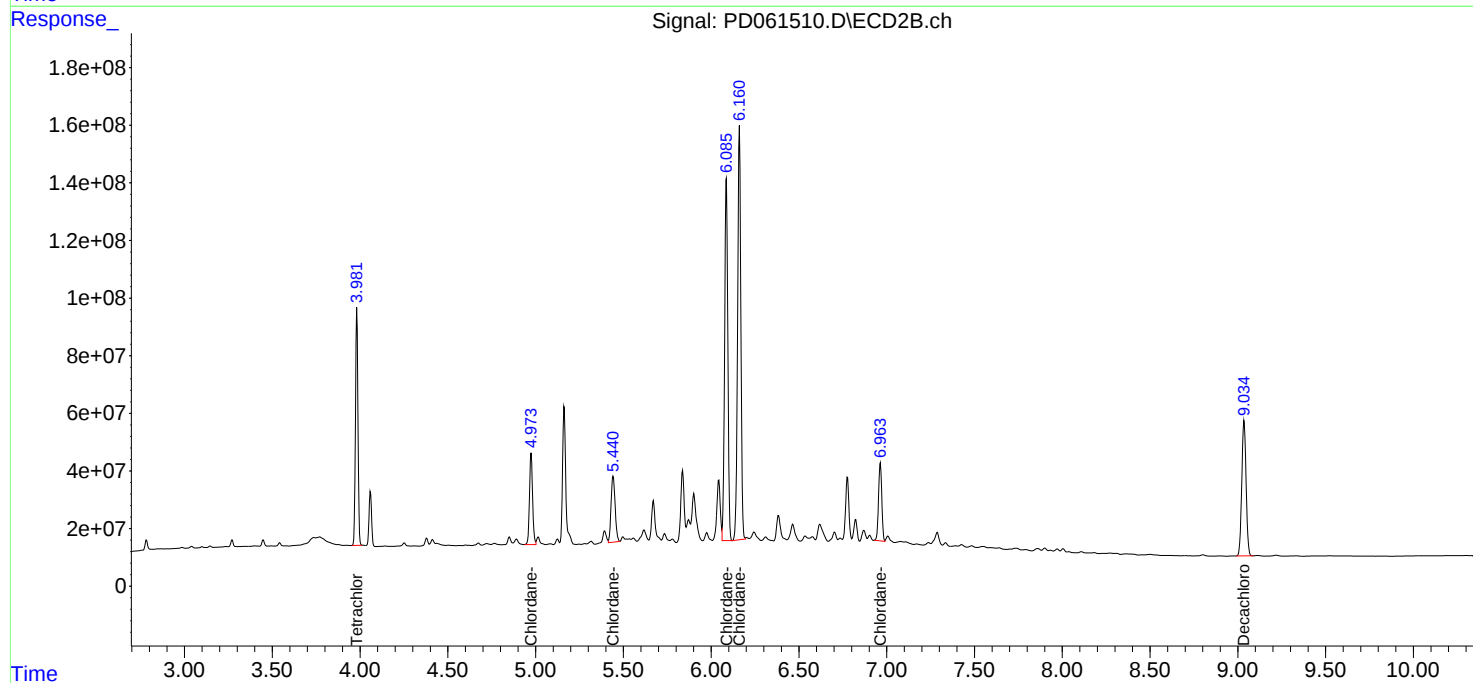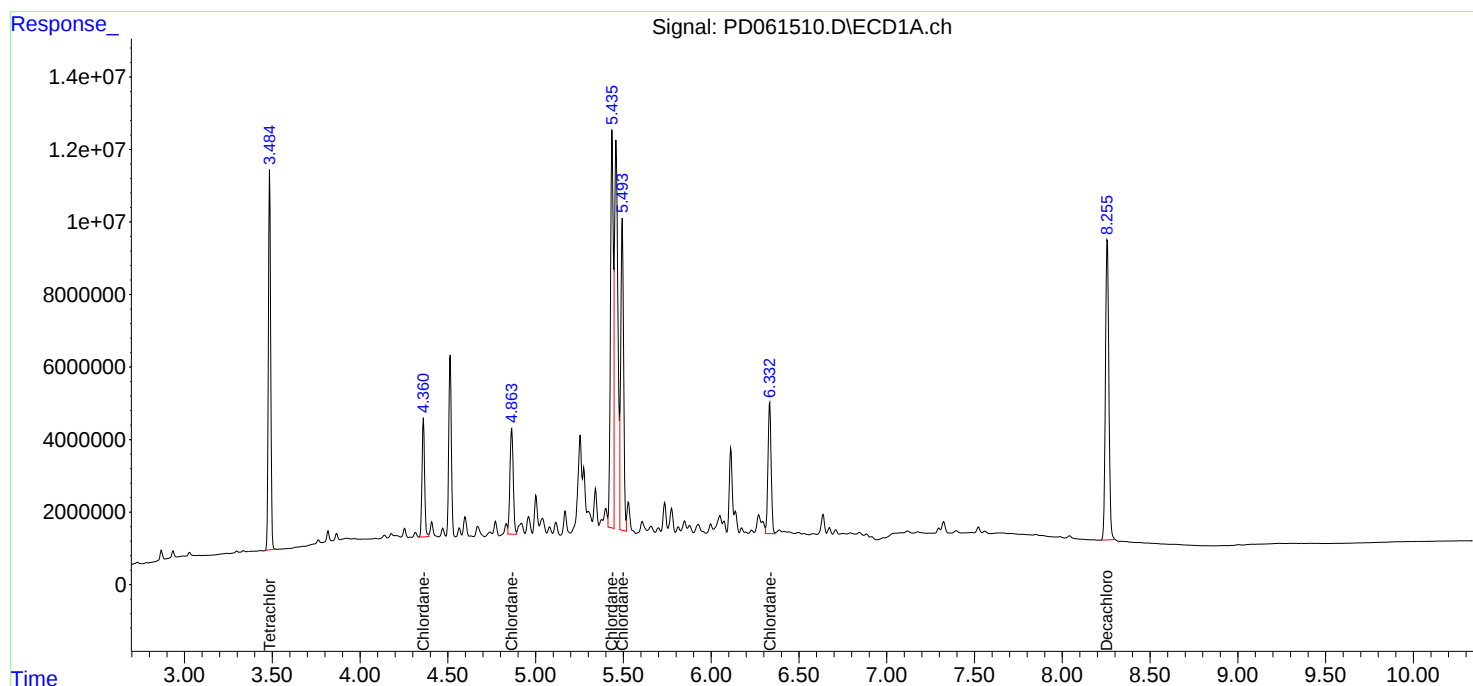


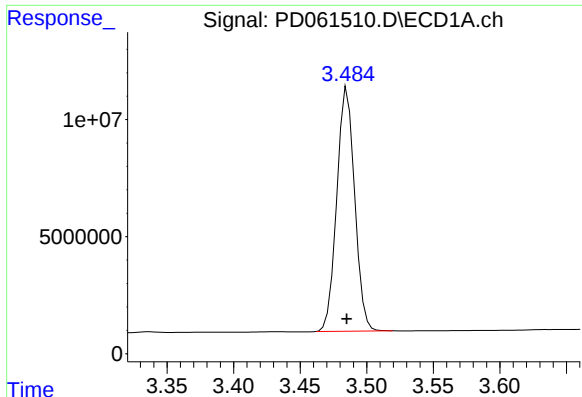

#1 Tetrachloro-m-xylene


R.T.: 3.485 min
Delta R.T.: 0.000 min
Response: 97380828
Conc: 97.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

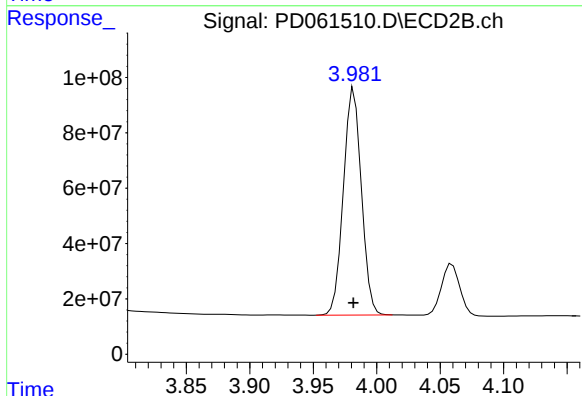


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 807601770
Conc: 92.23 ng/ml

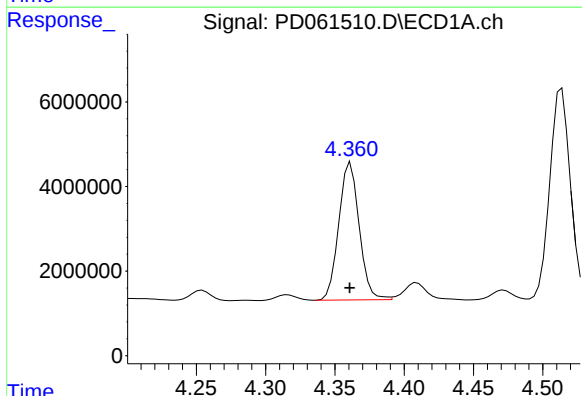


#23 Chlordane-1

R.T.: 4.361 min
Delta R.T.: 0.000 min
Response: 33324063
Conc: 947.46 ng/ml

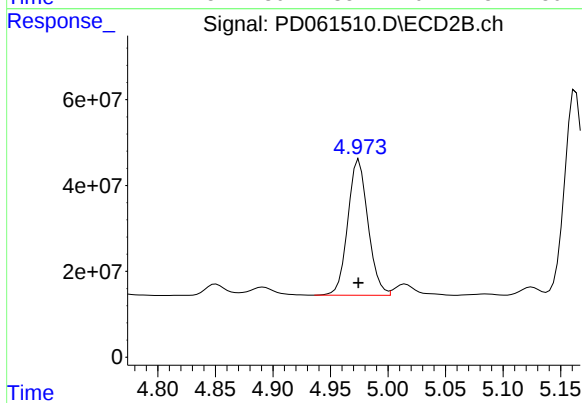

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 388569246
Conc: 944.34 ng/ml

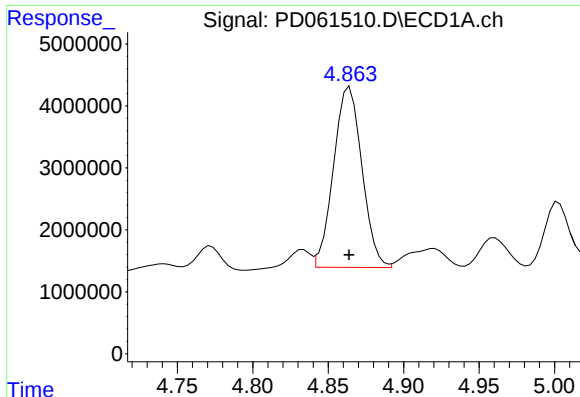

#24 Chlordane-2


R.T.: 4.864 min
Delta R.T.: 0.000 min
Response: 38151635
Conc: 931.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

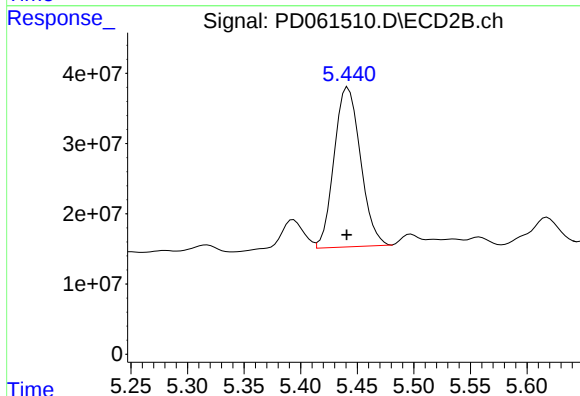


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.001 min
Response: 368778078
Conc: 927.78 ng/ml

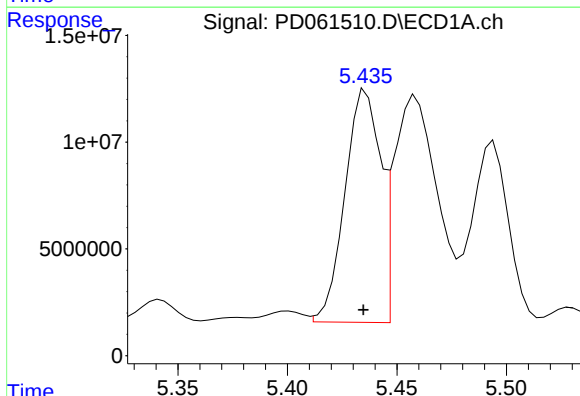


#25 Chlordane-3

R.T.: 5.436 min
Delta R.T.: 0.001 min
Response: 122304295
Conc: 990.85 ng/ml

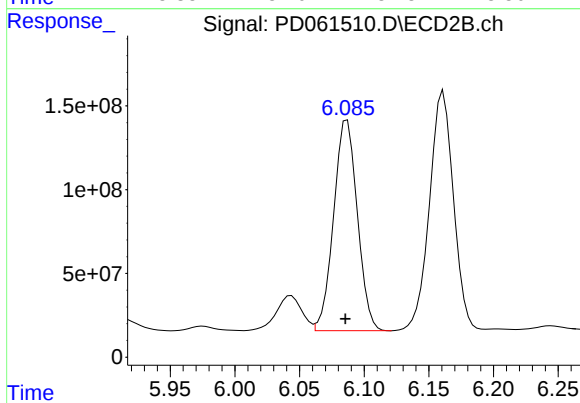

#25 Chlordane-3


R.T.: 6.087 min
Delta R.T.: 0.001 min
Response: 1602619185
Conc: 938.13 ng/ml

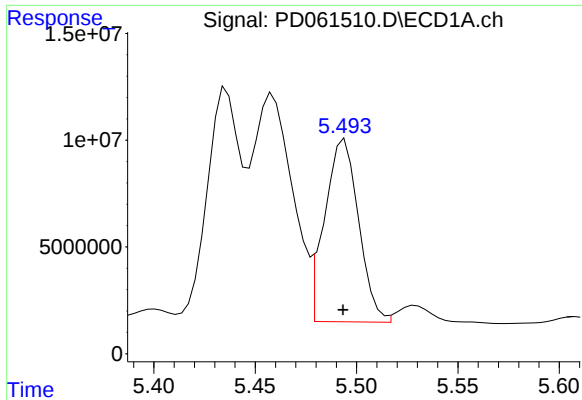

#26 Chlordane-4


R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 99819274
Conc: 969.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

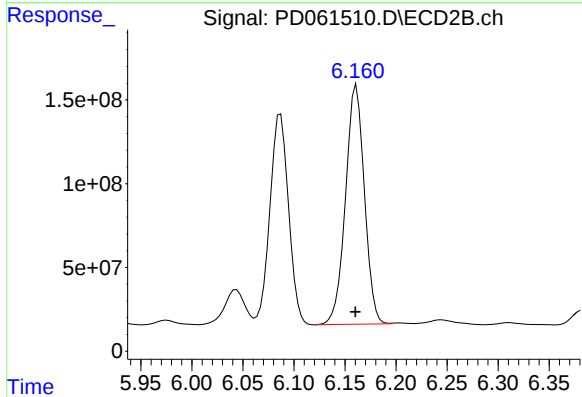


#26 Chlordane-4

R.T.: 6.161 min
Delta R.T.: 0.001 min
Response: 1837600951
Conc: 933.85 ng/ml

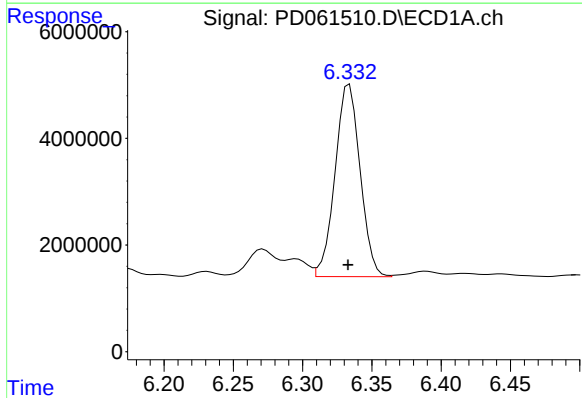


#27 Chlordane-5

R.T.: 6.334 min
Delta R.T.: 0.001 min
Response: 45377556
Conc: 950.65 ng/ml

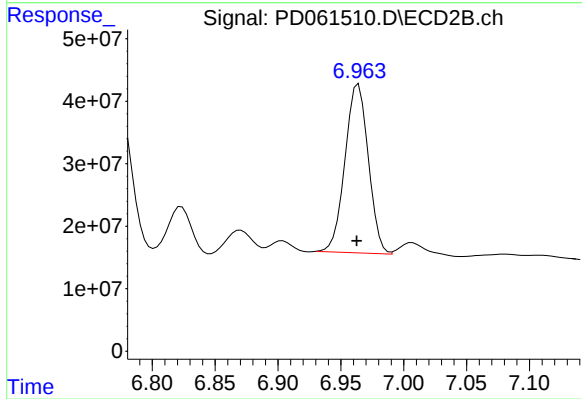

#27 Chlordane-5


R.T.: 6.964 min
Delta R.T.: 0.001 min
Response: 348717889
Conc: 948.73 ng/ml

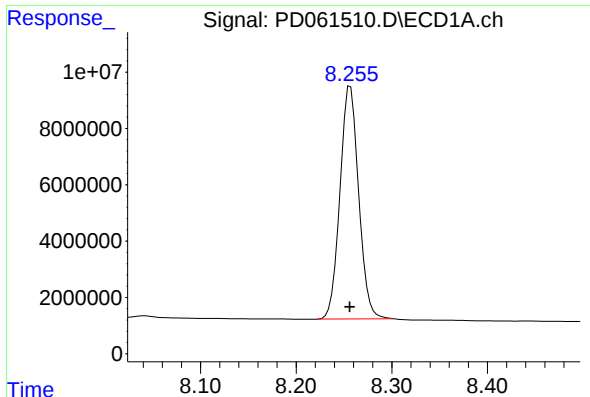

#28 Decachlorobiphenyl

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 112586322
Conc: 91.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

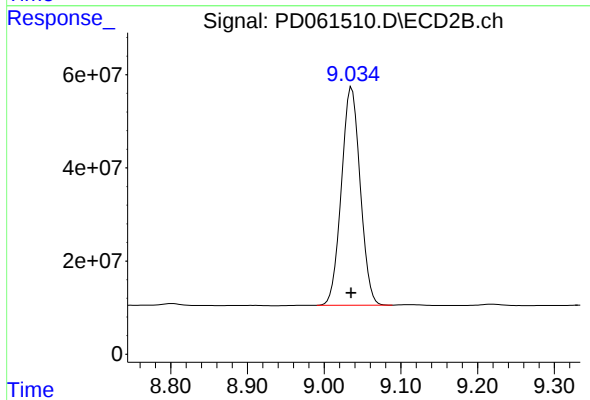

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 799898748
Conc: 91.27 ng/ml